

Data Path : V:\HPCHEM1\BNA M\DATA\BM112115\
Data File : BM003242.D
Acq On : 21 Nov 2015 10:55
Operator : UM/I2
Sample : PB86663BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant Time: Nov 23 12:24:53 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 04:42:03 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/23/2015 7:03:35 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	12823	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	50370	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.38	164	26483	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.12	188	48719m	0.40	ng/ul	0.00
18) Chrysene-d12	21.33	240	43239	0.40	ng/ul	0.00
22) Perylene-d12	23.59	264	41174m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.20	96	79189	5.78	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.12	152	20875	0.30	ng/ul	0.00
16) Fluoranthene-d10	19.17	212	36884	0.31	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} U.M
11/25/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112115\
 Data File : BM003242.D
 Acq On : 21 Nov 2015 10:55
 Operator : UM/IZ
 Sample : PB86663BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK63

Quant Time: Nov 23 12:23:31 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 04:42:03 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 7:03:35 PM

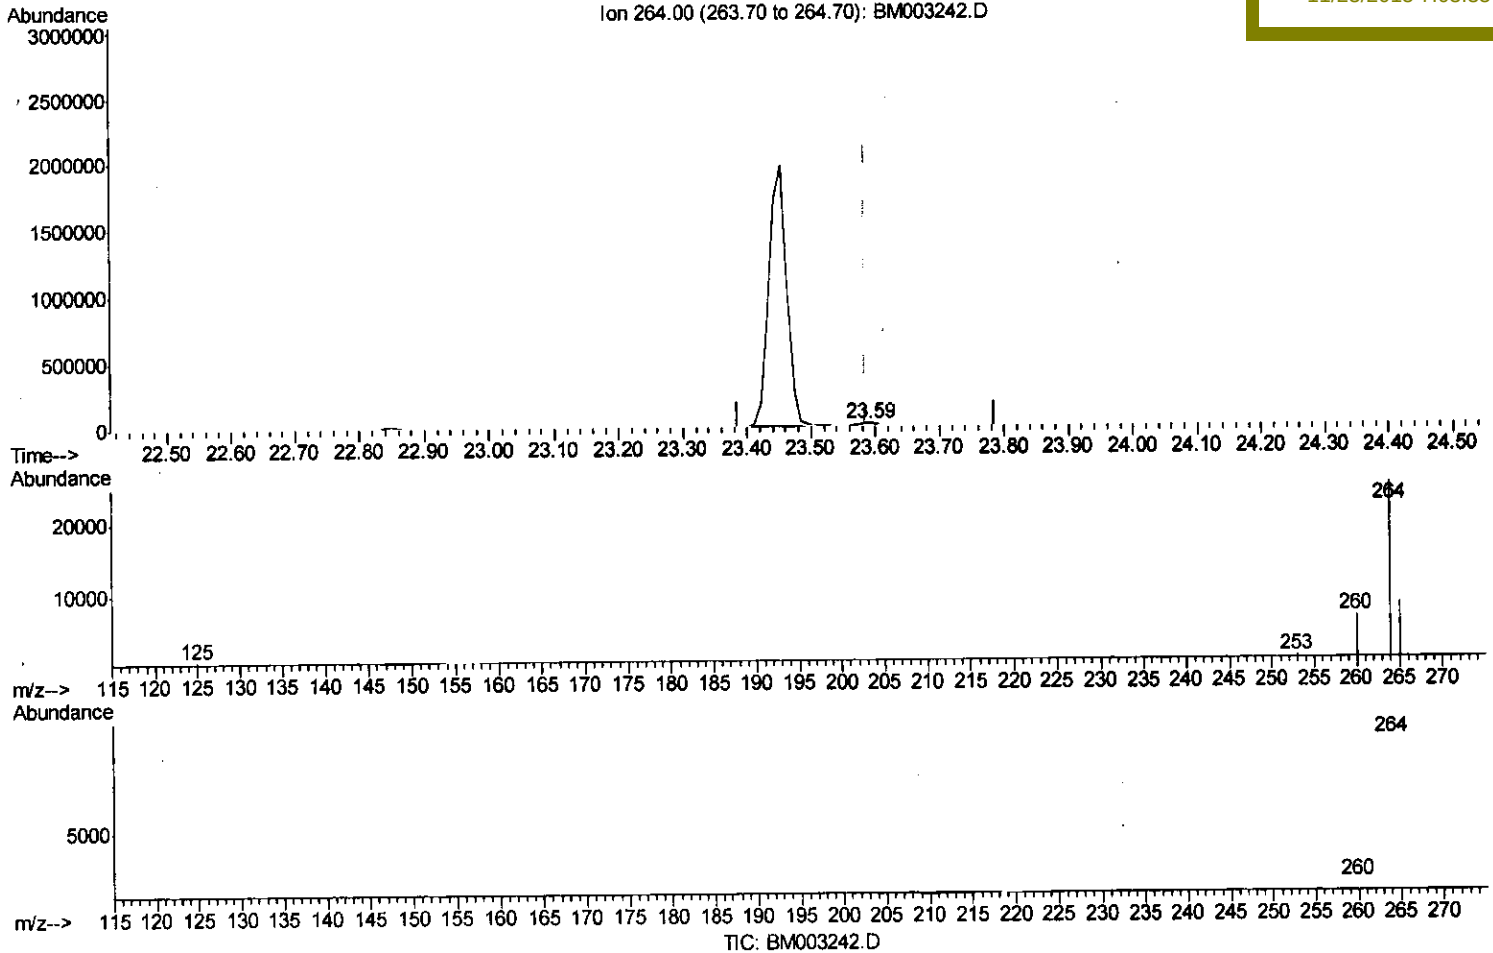

(22) Perylene-d12 (I)

23.588min (+0.003) 0.40ng/ul m

response 41174

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	25.72
265.00	38.20	32.86
0.00	0.00	0.00

U.M
 11/25/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112115\
Data File : BM003242.D
Acq On : 21 Nov 2015 10:55
Operator : UM/I2
Sample : PB86663BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant Time: Nov 23 12:23:31 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 04:42:03 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/23/2015 7:03:35 PM

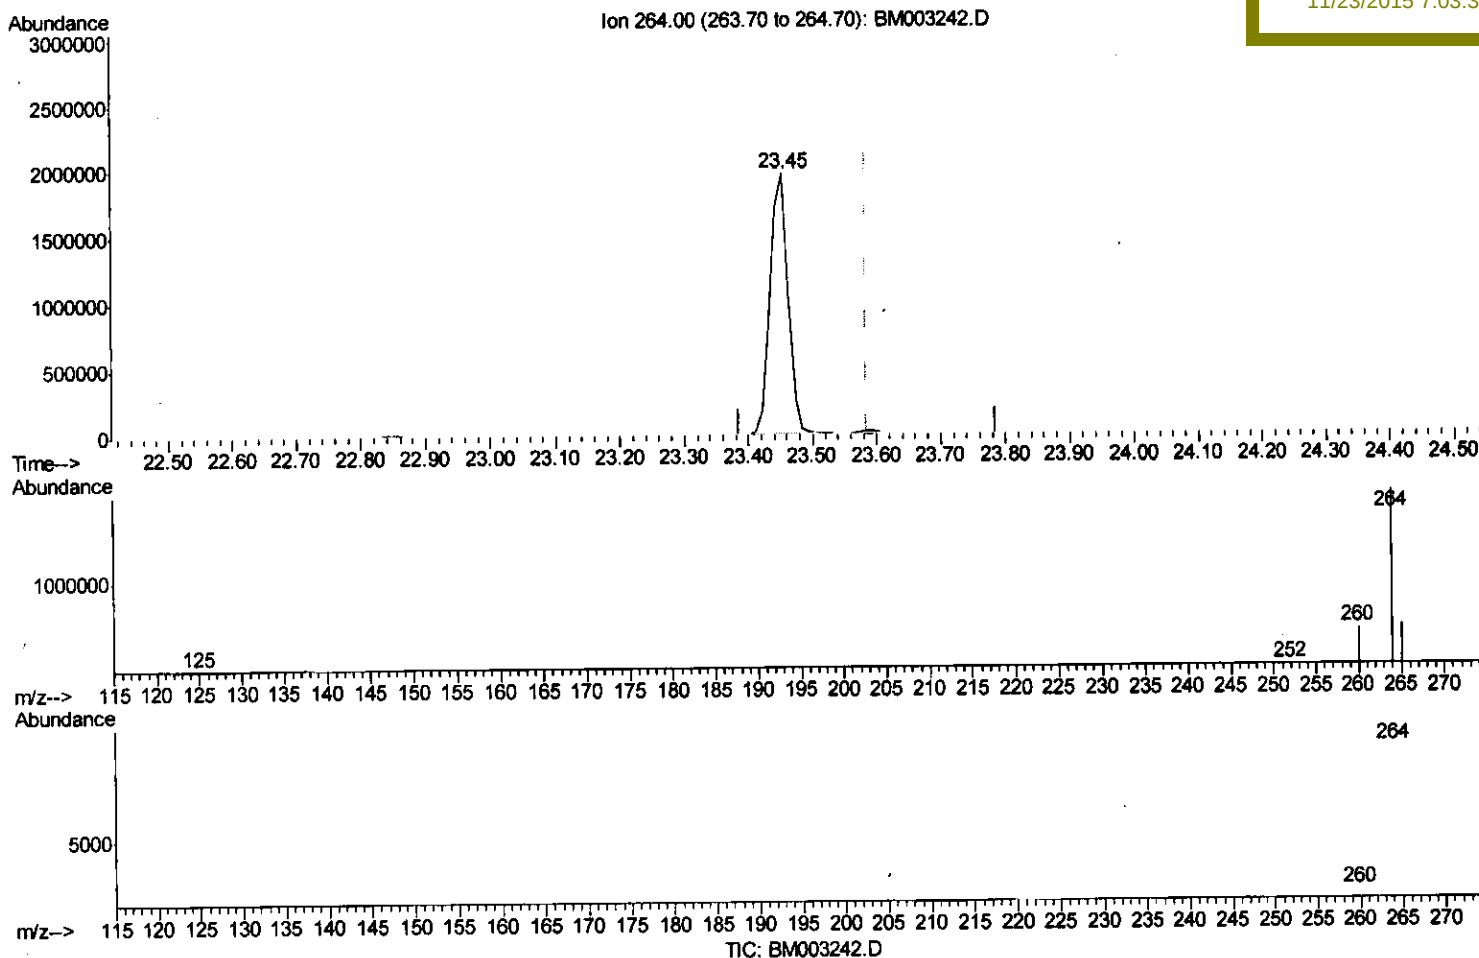

(22) Perylene-d12 (I)

23.453min (-0.132) 0.40ng/ul

response 3753765

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	20.89
265.00	38.20	22.57#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112115\
 Data File : BM003242.D
 Acq On : 21 Nov 2015 10:55
 Operator : UM/IZ
 Sample : PB86663BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK63

Quant Time: Nov 22 10:59:57 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 04:42:03 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 7:03:35 PM

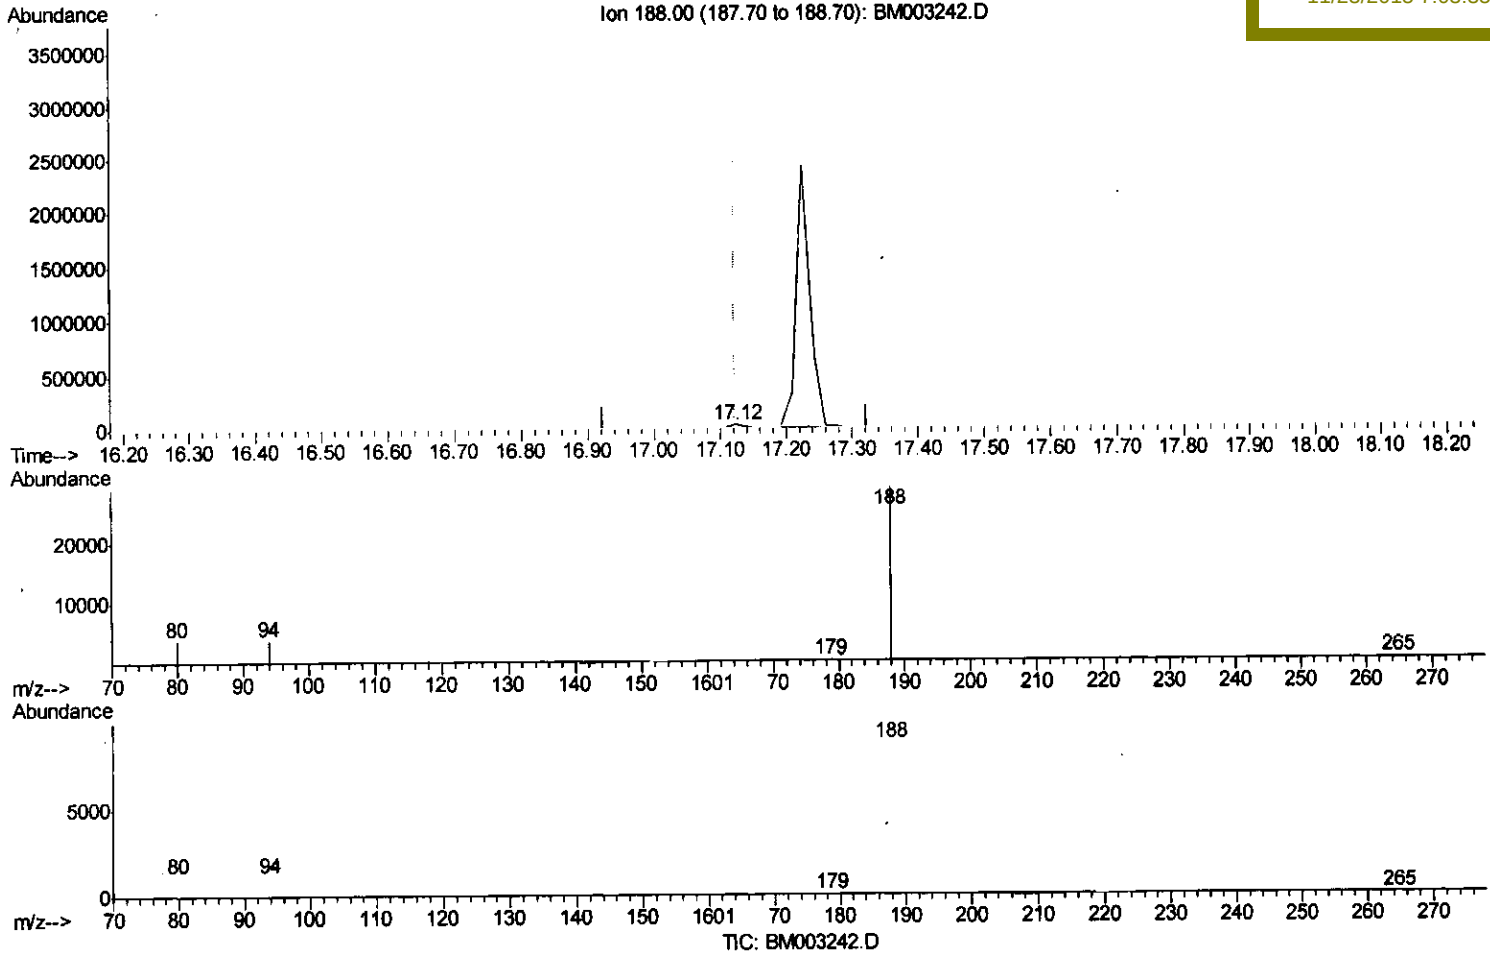

(12) Phenanthrene-d10 (I)

17.123min (-0.000) 0.40ng/ul m

response 48719

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	12.53
80.00	11.90	13.04
0.00	0.00	0.00

U.M
 11/25/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112115\
Data File : BM003242.D
Acq On : 21 Nov 2015 10:55
Operator : UM/IZ
Sample : PB86663BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant Time: Nov 22 10:59:57 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 04:42:03 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/23/2015 7:03:35 PM

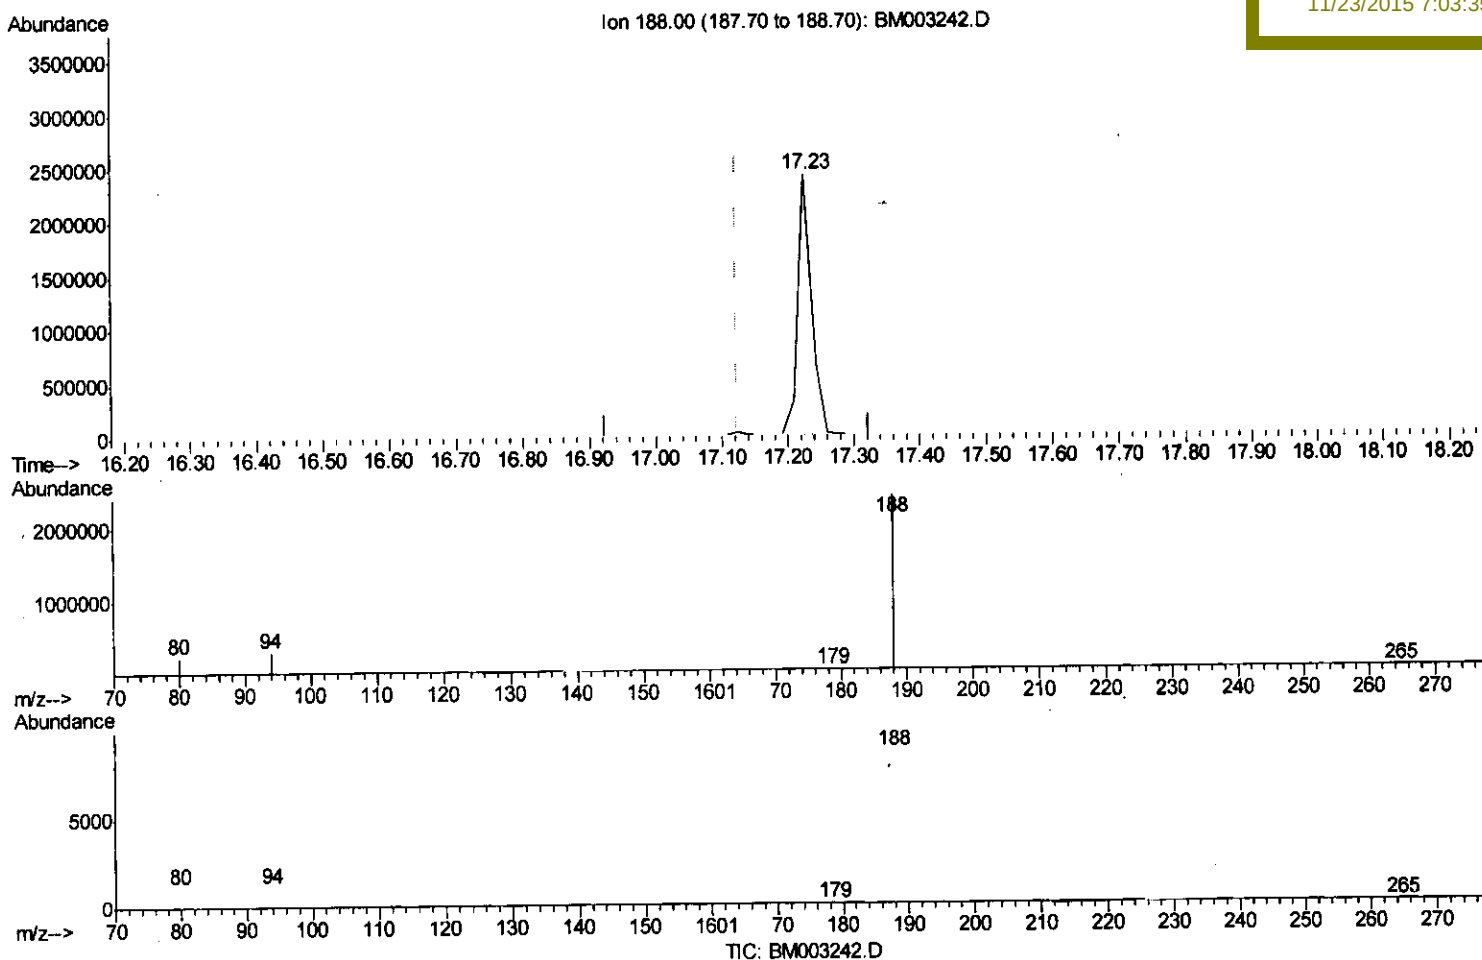

(12) Phenanthrene-d10 (I)

17.226min (+0.103) 0.40ng/ul

response 3498761

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	11.70
80.00	11.90	9.06#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM112115\
Data File : BM003242.D
Acq On : 21 Nov 2015 10:55
Operator : UM/IZ
Sample : PB86663BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant Time: Nov 23 12:24:53 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 04:42:03 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/23/2015 7:03:35 PM

