

Data Path : V:\HPCHEM1\BNA M\DATA\BM112115\
Data File : BM003261.D
Acq On : 21 Nov 2015 22:53
Operator : UM/IZ
Sample : PB86665BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Time: Nov 23 13:06:33 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 04:42:03 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/23/2015 7:04:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	14523	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	56798	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.38	164	30552	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.12	188	60409m	0.40	ng/ul	0.00
18) Chrysene-d12	21.33	240	59774	0.40	ng/ul	0.00
22) Perylene-d12	23.59	264	54540m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.20	96	82671	5.33	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.12	152	22010	0.29	ng/ul	0.00
16) Fluoranthene-d10	19.16	212	44282	0.30	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} U.M
11/25/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112115\
 Data File : BM003261.D
 Acq On : 21 Nov 2015 22:53
 Operator : UM/IZ
 Sample : PB86665BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Nov 22 05:01:27 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 04:42:03 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 7:04:22 PM

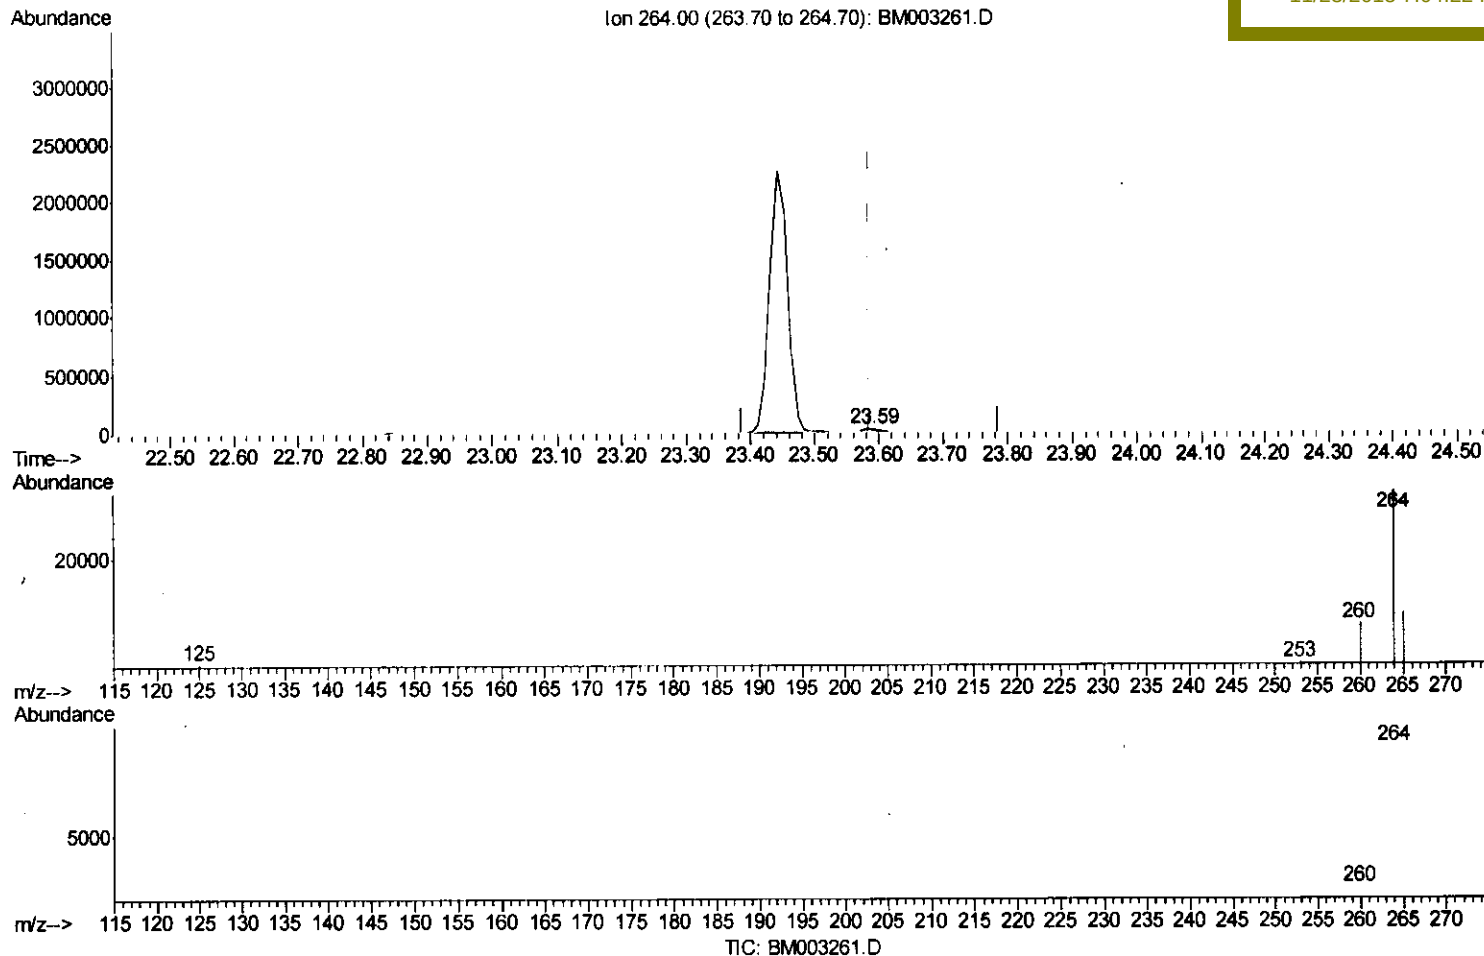

(22) Perylene-d12 (I)

23.588min (+0.003) 0.40ng/ul m

response 54540

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	24.93
265.00	38.20	31.15
0.00	0.00	0.00

U. m
 11/25/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112115\
 Data File : BM003261.D
 Acq On : 21 Nov 2015 22:53
 Operator : UM/IZ
 Sample : PB86665BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Nov 22 05:01:27 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 04:42:03 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 7:04:22 PM

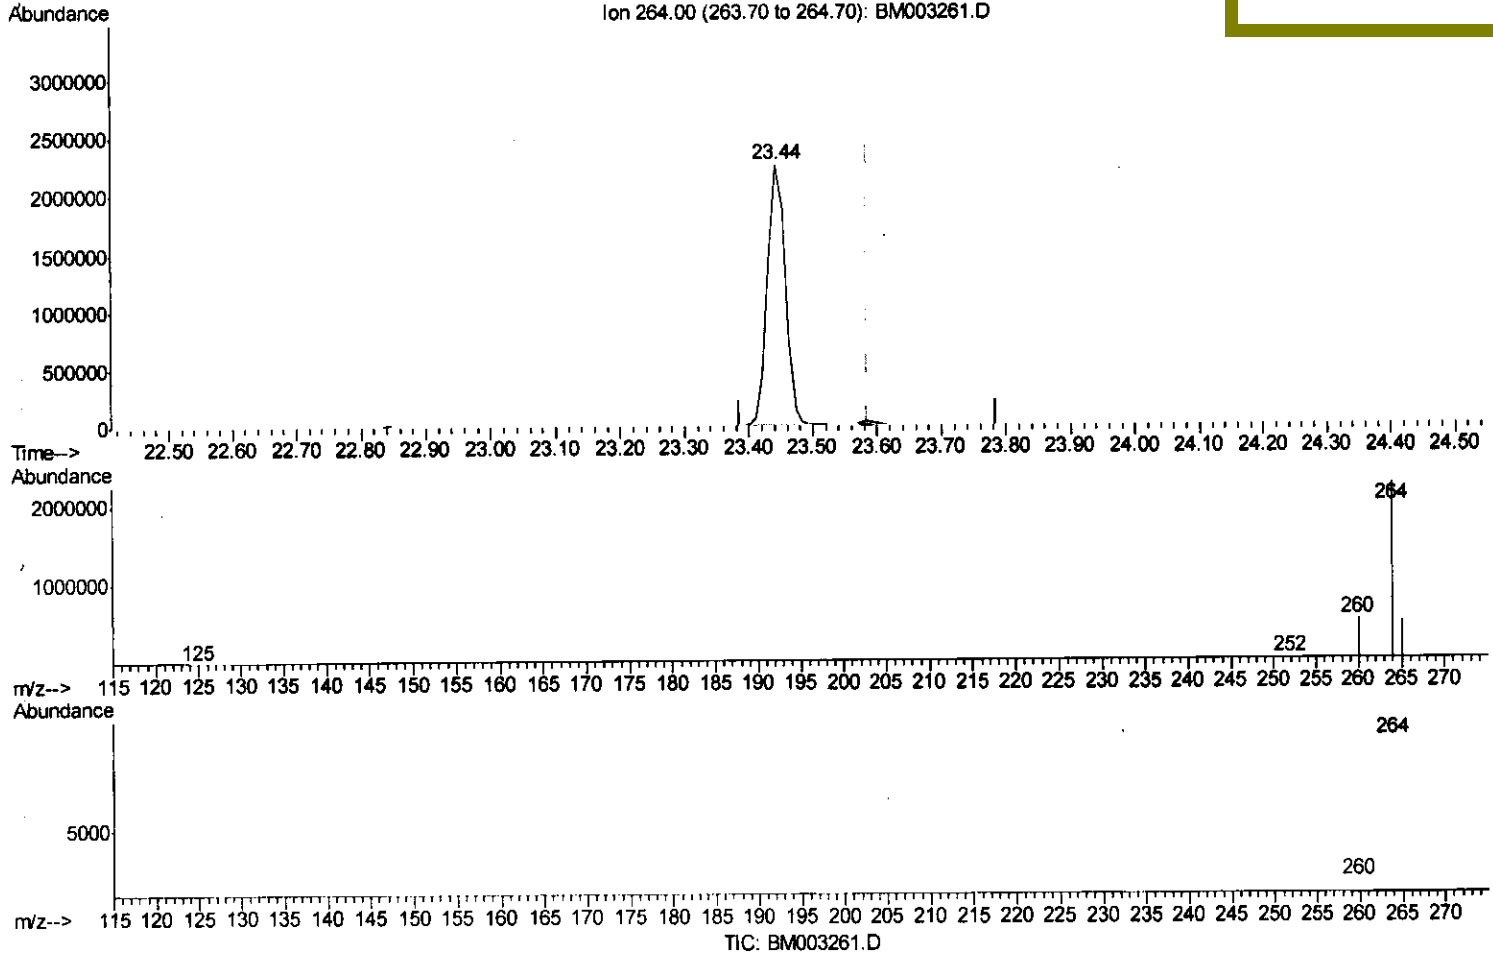

(22) Perylene-d12 (I)

23.442min (-0.143) 0.40ng/ul

response 4312874

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	22.62
265.00	38.20	21.22#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112115\
 Data File : BM003261.D
 Acq On : 21 Nov 2015 22:53
 Operator : UM/IZ
 Sample : PB86665BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Nov 22 05:03:07 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 04:42:03 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 7:04:22 PM

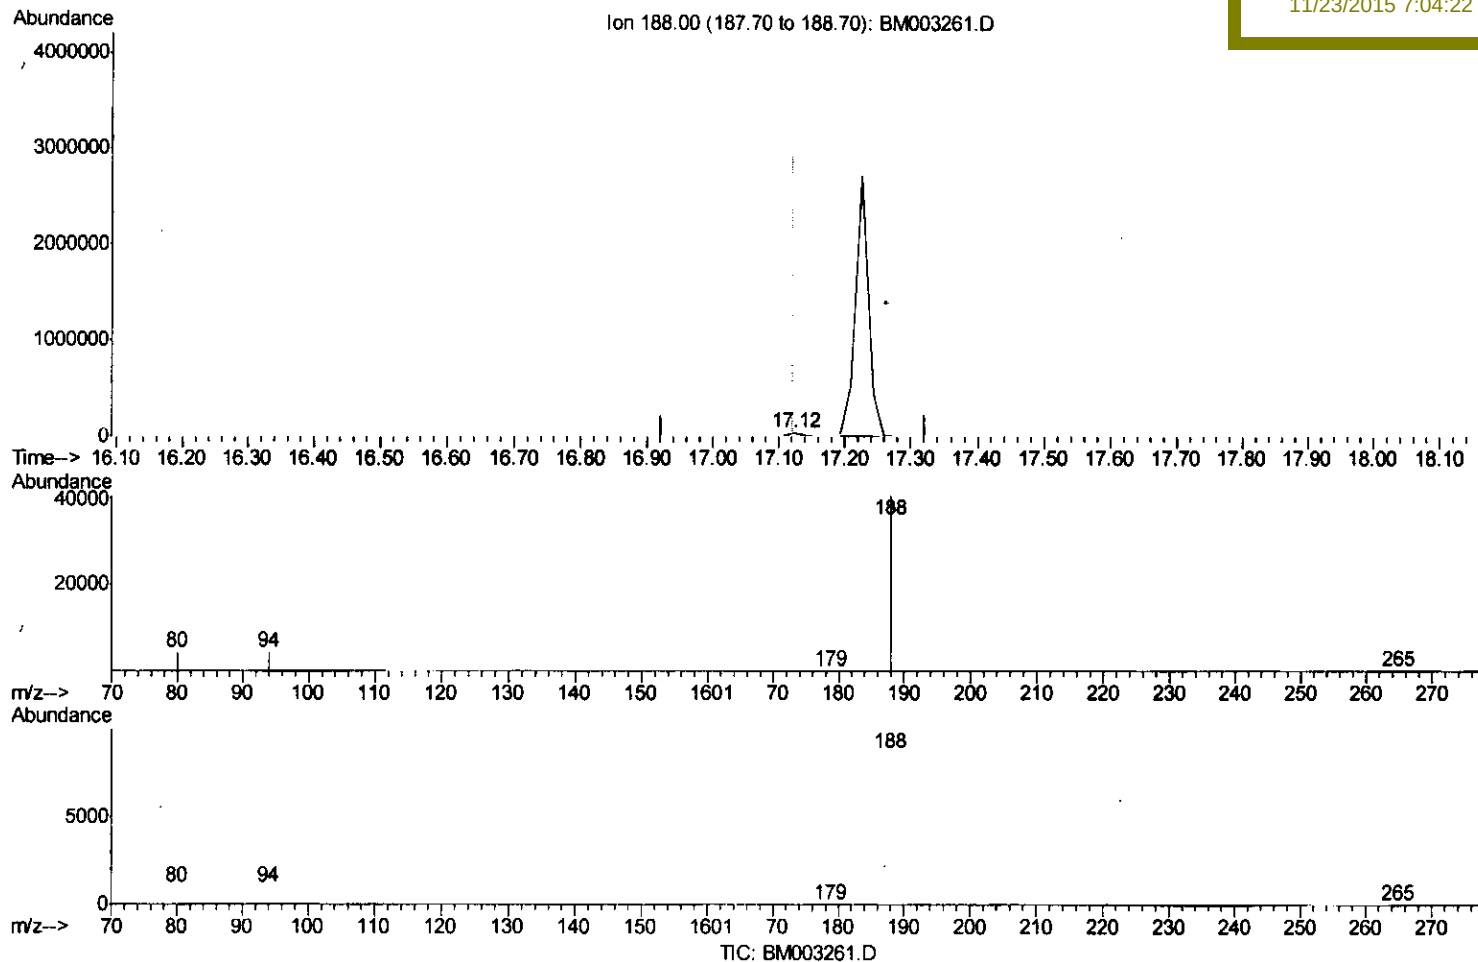

(12) Phenanthrene-d10 (I)

17.123min (-0.000) 0.40ng/ul m

response 60409

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	10.74
80.00	11.90	10.58
0.00	0.00	0.00

U.M
 11/25/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112115\
 Data File : BM003261.D
 Acq On : 21 Nov 2015 22:53
 Operator : UM/IZ
 Sample : PB86665BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Nov 22 04:46:47 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 04:42:03 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 7:04:22 PM

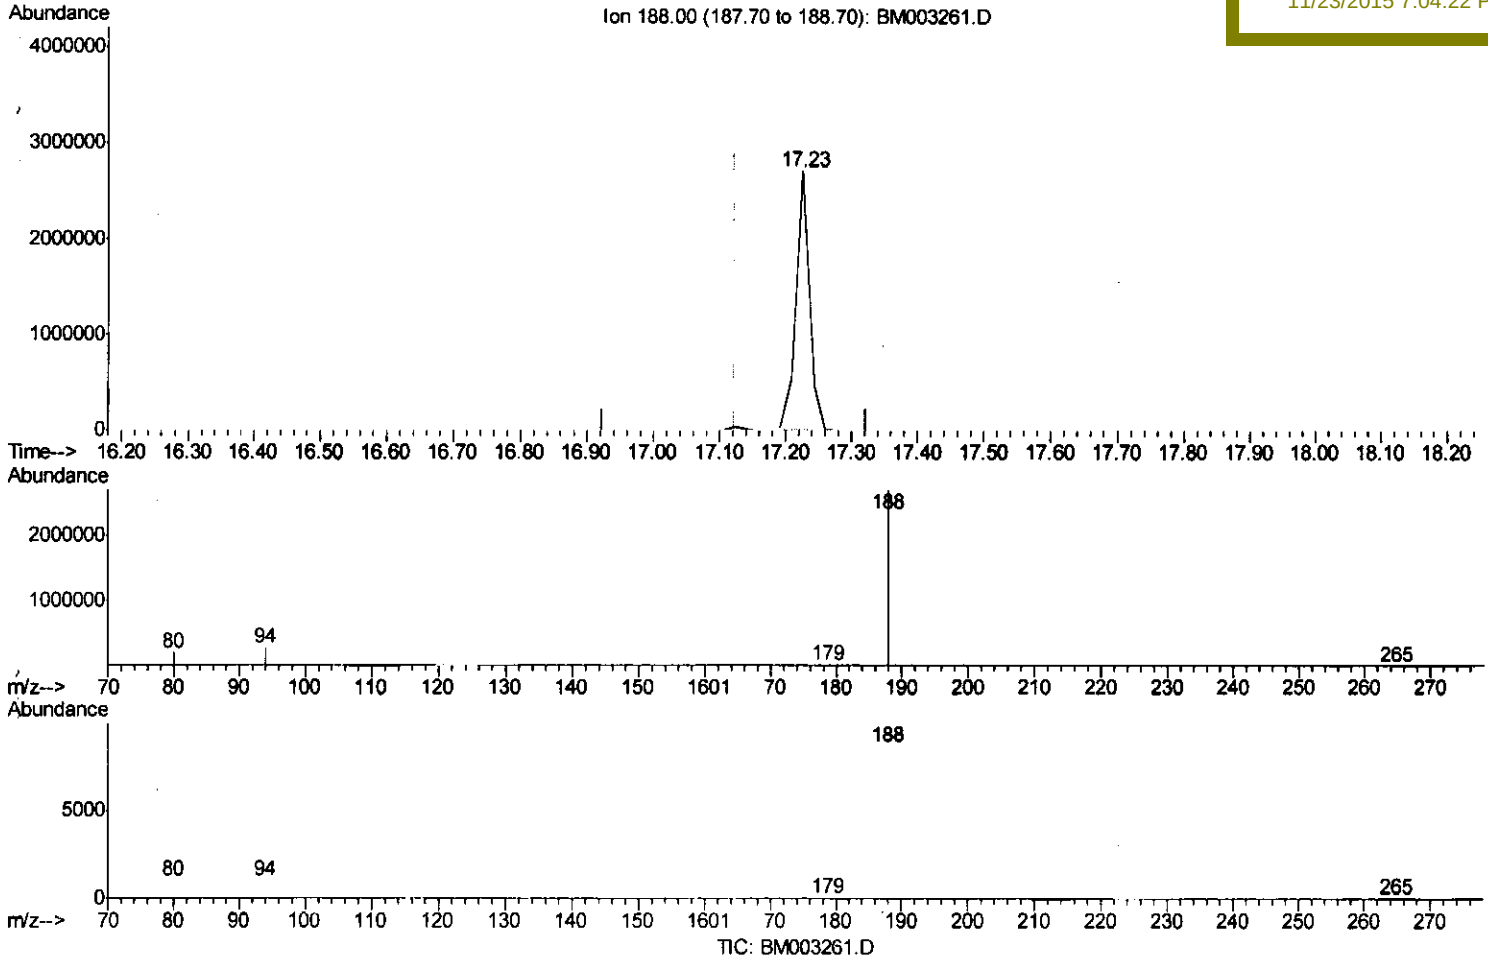

(12) Phenanthrene-d10 (I)

17.226min (+0.103) 0.40ng/ul

response 3841882

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	9.97
80.00	11.90	7.39#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112115\
Data File : BM003261.D
Acq On : 21 Nov 2015 22:53
Operator : UM/IZ
Sample : PB86665BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK65

Quant Time: Nov 22 05:03:07 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 04:42:03 2015
Response via : Initial Calibration

Manual Integration
APPROVED

Mmdadoda
11/23/2015 7:04:22 PM

