

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037669.D
 Acq On : 23 Nov 2022 08:16
 Operator : CG/JU
 Sample : N5591-12
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9824

Quant Time: Nov 24 01:48:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.125	152	8046	0.400	ng/ul	0.00
4) Naphthalene-d8	10.942	136	24261	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.743	164	14394	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.475	188	31988	0.400	ng/ul	0.00
17) Chrysene-d12	21.637	240	22512	0.400	ng/ul #	0.00
23) Perylene-d12	24.121	264	22683	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	43537	4.654	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.515	152	8912	0.222	ng/ul	0.00
18) Fluoranthene-d10	19.486	212	19163	0.258	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.728	166	3524	0.052	ng/ul#	15
20) Pyrene	19.853	202	4179	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.961	252	6921	0.077	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037669.D
Acq On : 23 Nov 2022 08:16
Operator : CG/JU
Sample : N5591-12
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9824

Quant Time: Nov 24 01:48:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration




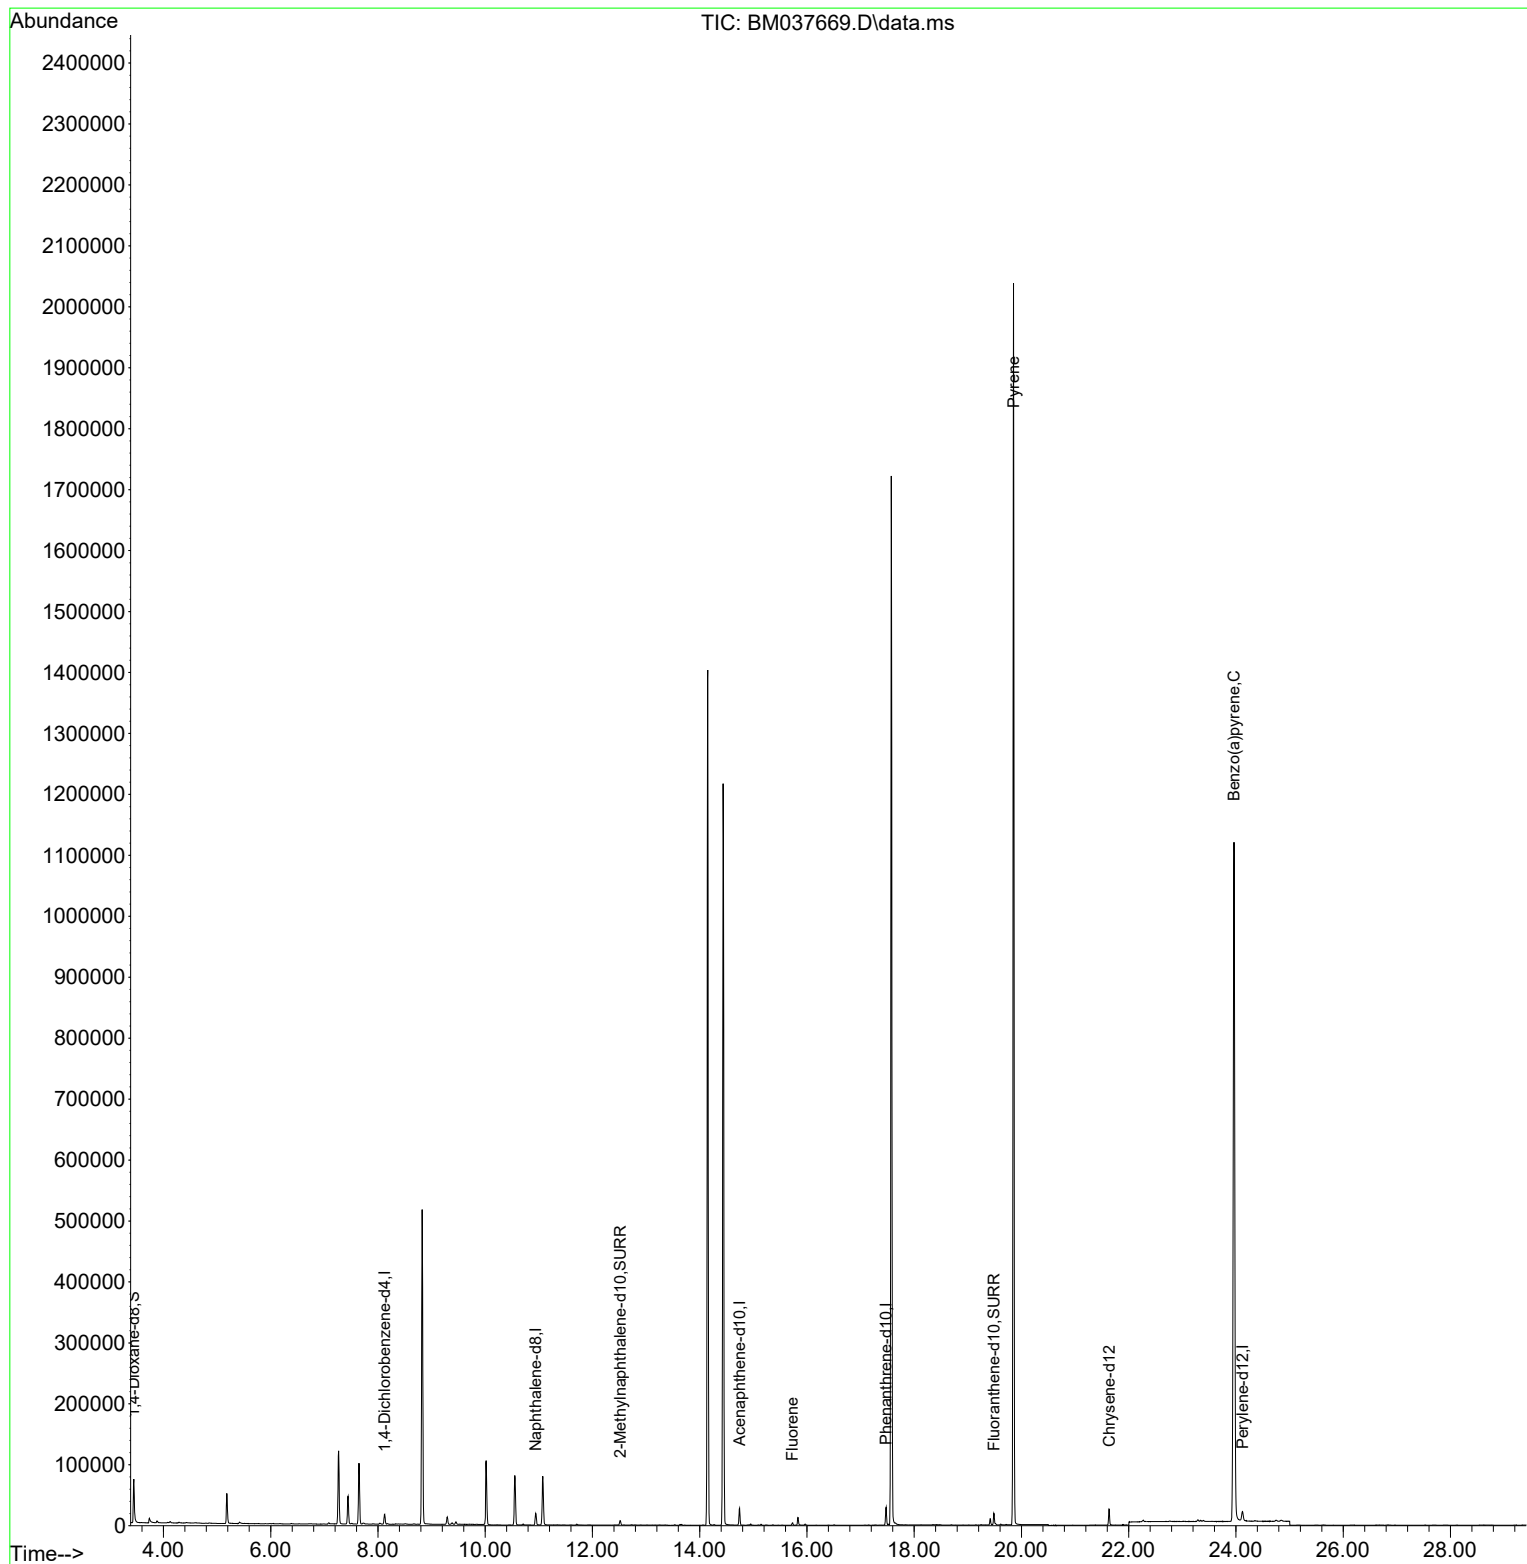


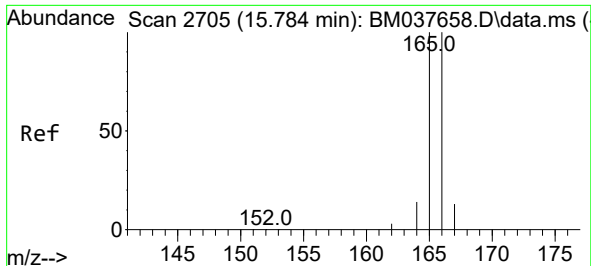

#12
Fluorene
Concen: 0.052 ng/ul
RT: 15.728 min Scan# 2693
Delta R.T. -0.058 min
Lab File: BM037669.D
Acq: 23 Nov 2022 08:16




Instrument :
BNA_M
ClientSampleId :
C9824


Tgt Ion:166 Resp: 3524
Ion Ratio Lower Upper
166 100
165 8.1 78.7 118.1#
167 31.0 11.3 16.9#

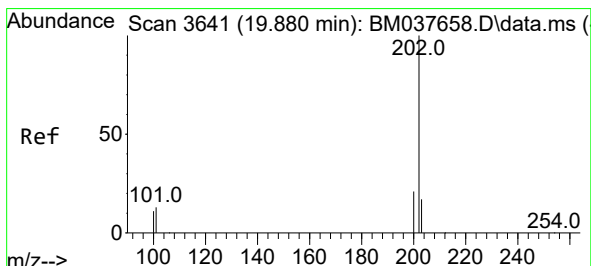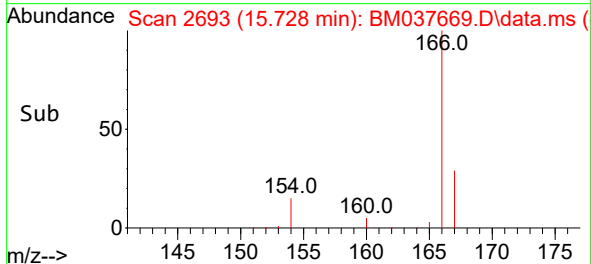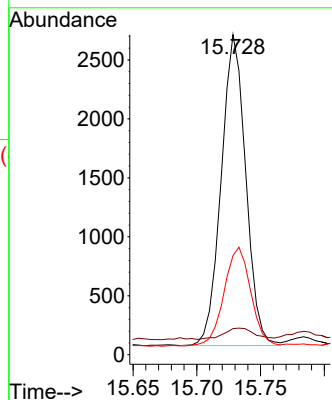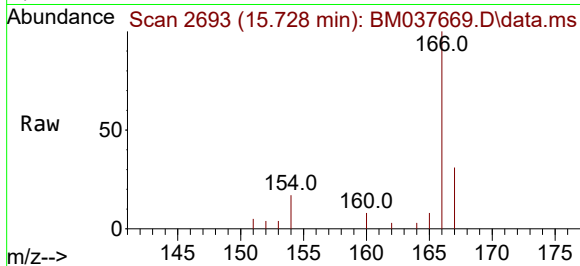

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.853 min Scan# 3635
Delta R.T. -0.031 min
Lab File: BM037669.D
Acq: 23 Nov 2022 08:16


Tgt Ion:202 Resp: 4179
Ion Ratio Lower Upper
202 100
101 154.1 10.1 15.1#
100 1127.0 8.0 12.0#

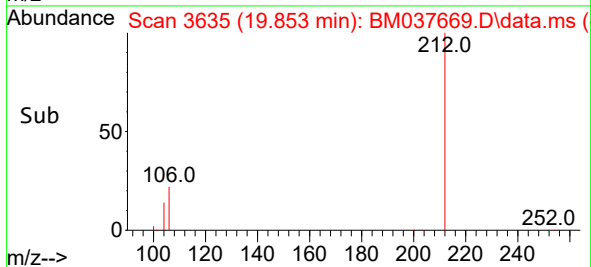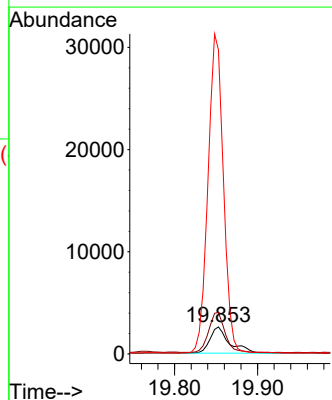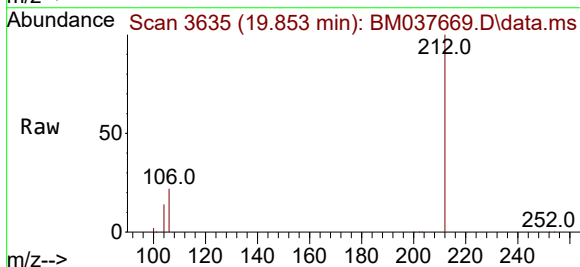

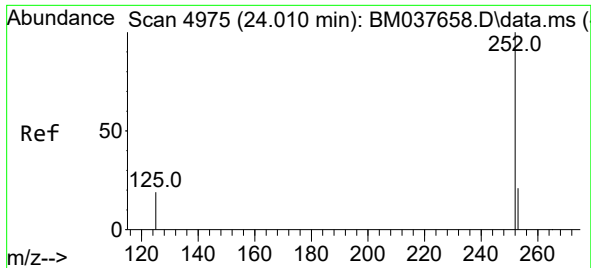

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.961 min Scan# 4975
Delta R.T. -0.053 min
Lab File: BM037669.D
Acq: 23 Nov 2022 08:16

Instrument :
BNA_M
ClientSampleId :
C9824

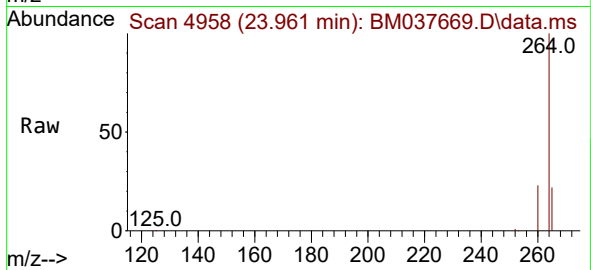

Tgt Ion:252 Resp: 6921
Ion Ratio Lower Upper
252 100
253 49.9 18.8 28.2#
125 46.9 10.5 15.7#

