

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037605.D
 Acq On : 21 Nov 2022 11:19
 Operator : CG/JU
 Sample : N5690-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE5

Quant Time: Nov 21 13:36:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	6756	0.400	ng/ul	0.00
4) Naphthalene-d8	10.953	136	19462	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.747	164	13616	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.479	188	25531	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.639	240	17981	0.400	ng/ul	# 0.00
23) Perylene-d12	24.127	264	19086	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	34832	4.434	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	4431	0.137	ng/ul	0.00
18) Fluoranthene-d10	19.495	212	21858	0.368	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1968	0.241	ng/ul#	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\  
Data File : BM037605.D  
Acq On    : 21 Nov 2022  11:19  
Operator  : CG/JU  
Sample    : N5690-01  
Misc      :  
ALS Vial  : 4    Sample Multiplier: 1
```

Quant Time: Nov 21 13:36:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

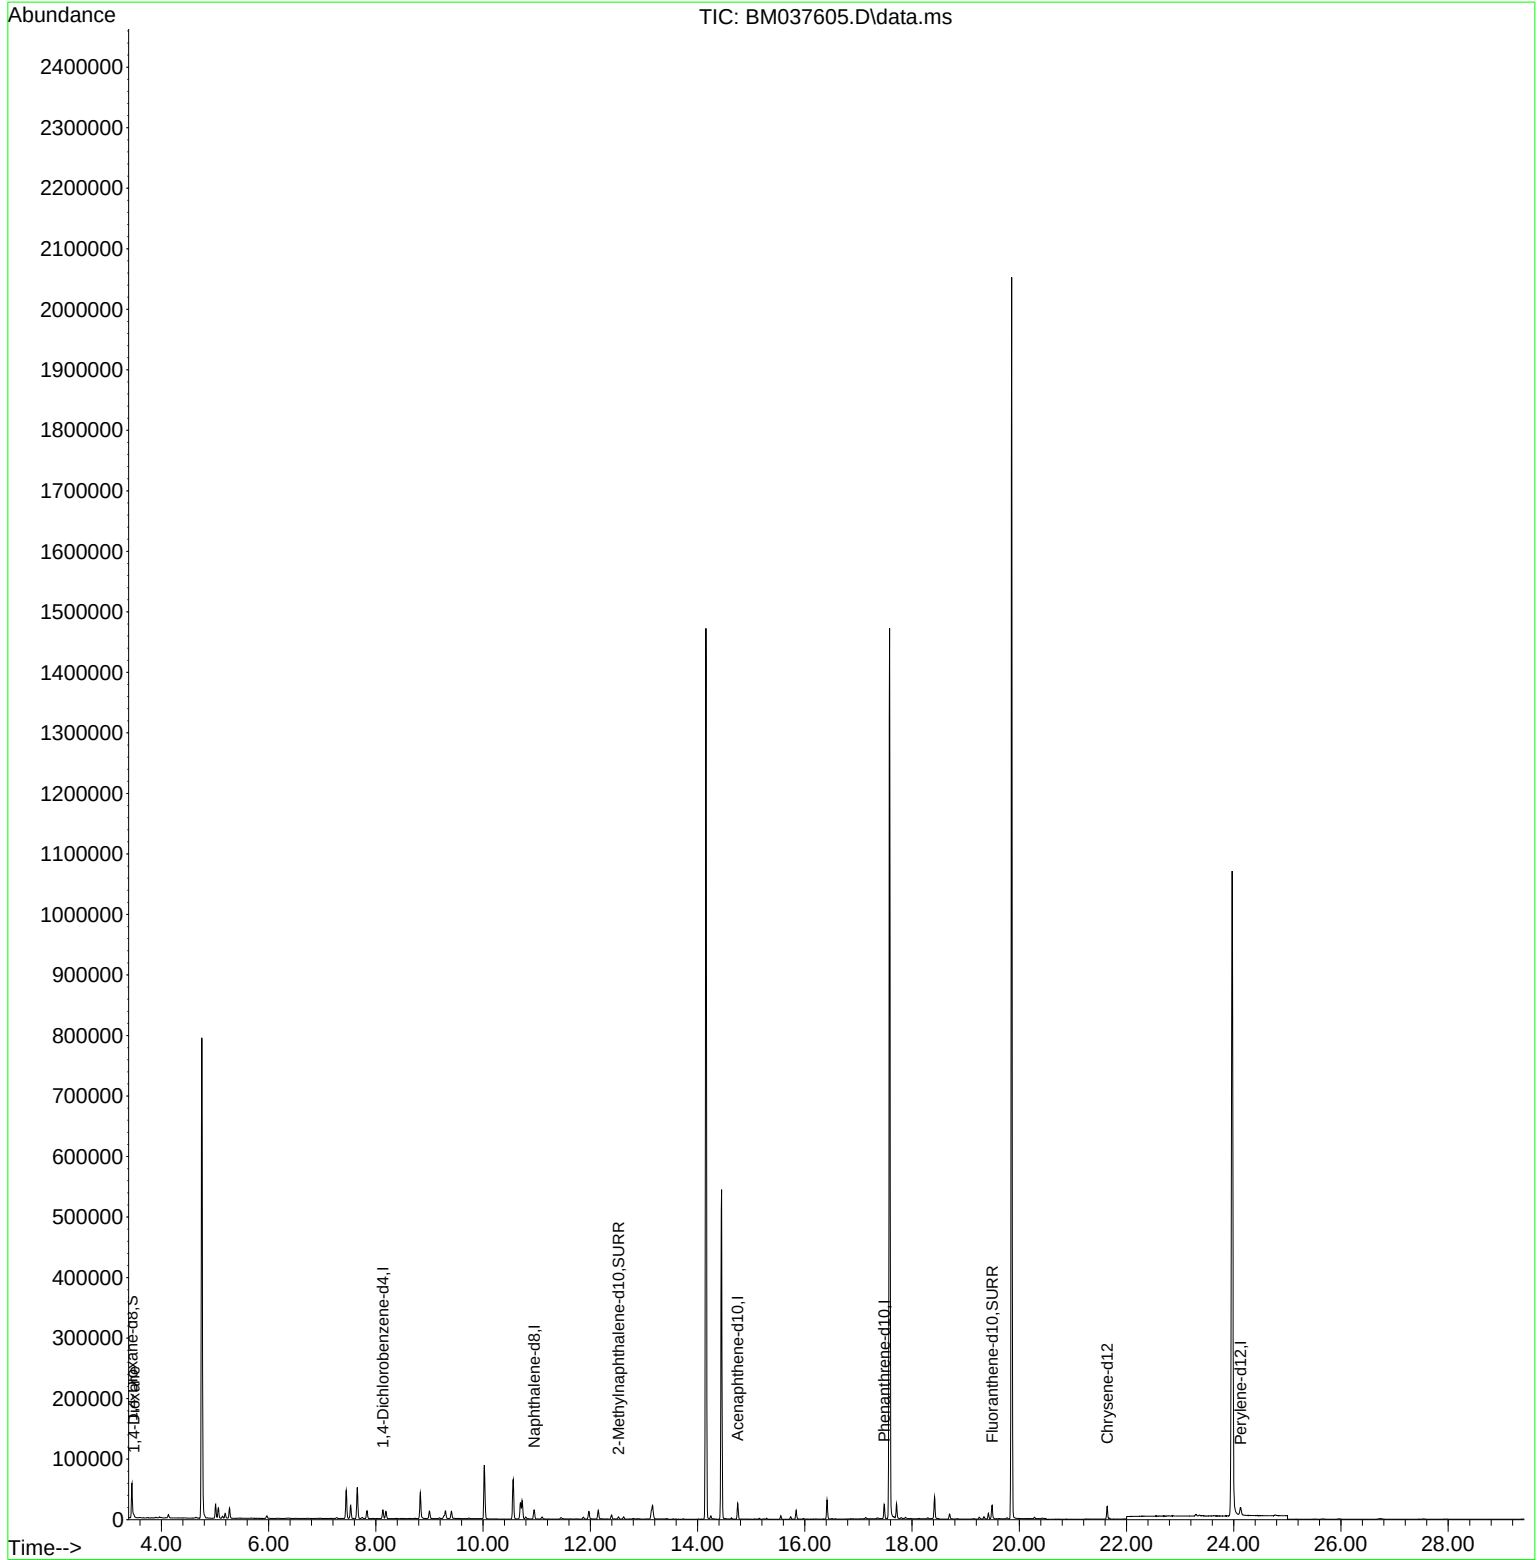

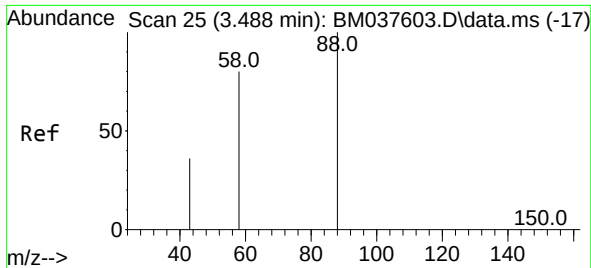

#2
 1,4-Dioxane
 Concen: 0.241 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BM037605.D
 Acq: 21 Nov 2022 11:19

Instrument :
 BNA_M
 ClientSampleId :
 BGCE5

Tgt Ion: 88 Resp: 1968

Ion	Ratio	Lower	Upper
88	100		
43	57.6	102.8	154.2#
58	63.8	67.3	100.9#

