

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037606.D
 Acq On : 21 Nov 2022 11:56
 Operator : CG/JU
 Sample : N5690-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE6

Quant Time: Nov 21 13:38:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	7414	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	21536	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	13277	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	27889	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	20140	0.400	ng/ul	# 0.00
23) Perylene-d12	24.127	264	22585	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	33031	3.832	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.524	152	9536	0.267	ng/ul	0.00
18) Fluoranthene-d10	19.493	212	22223	0.334	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1589	0.177	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037606.D
Acq On : 21 Nov 2022 11:56
Operator : CG/JU
Sample : N5690-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE6

Quant Time: Nov 21 13:38:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

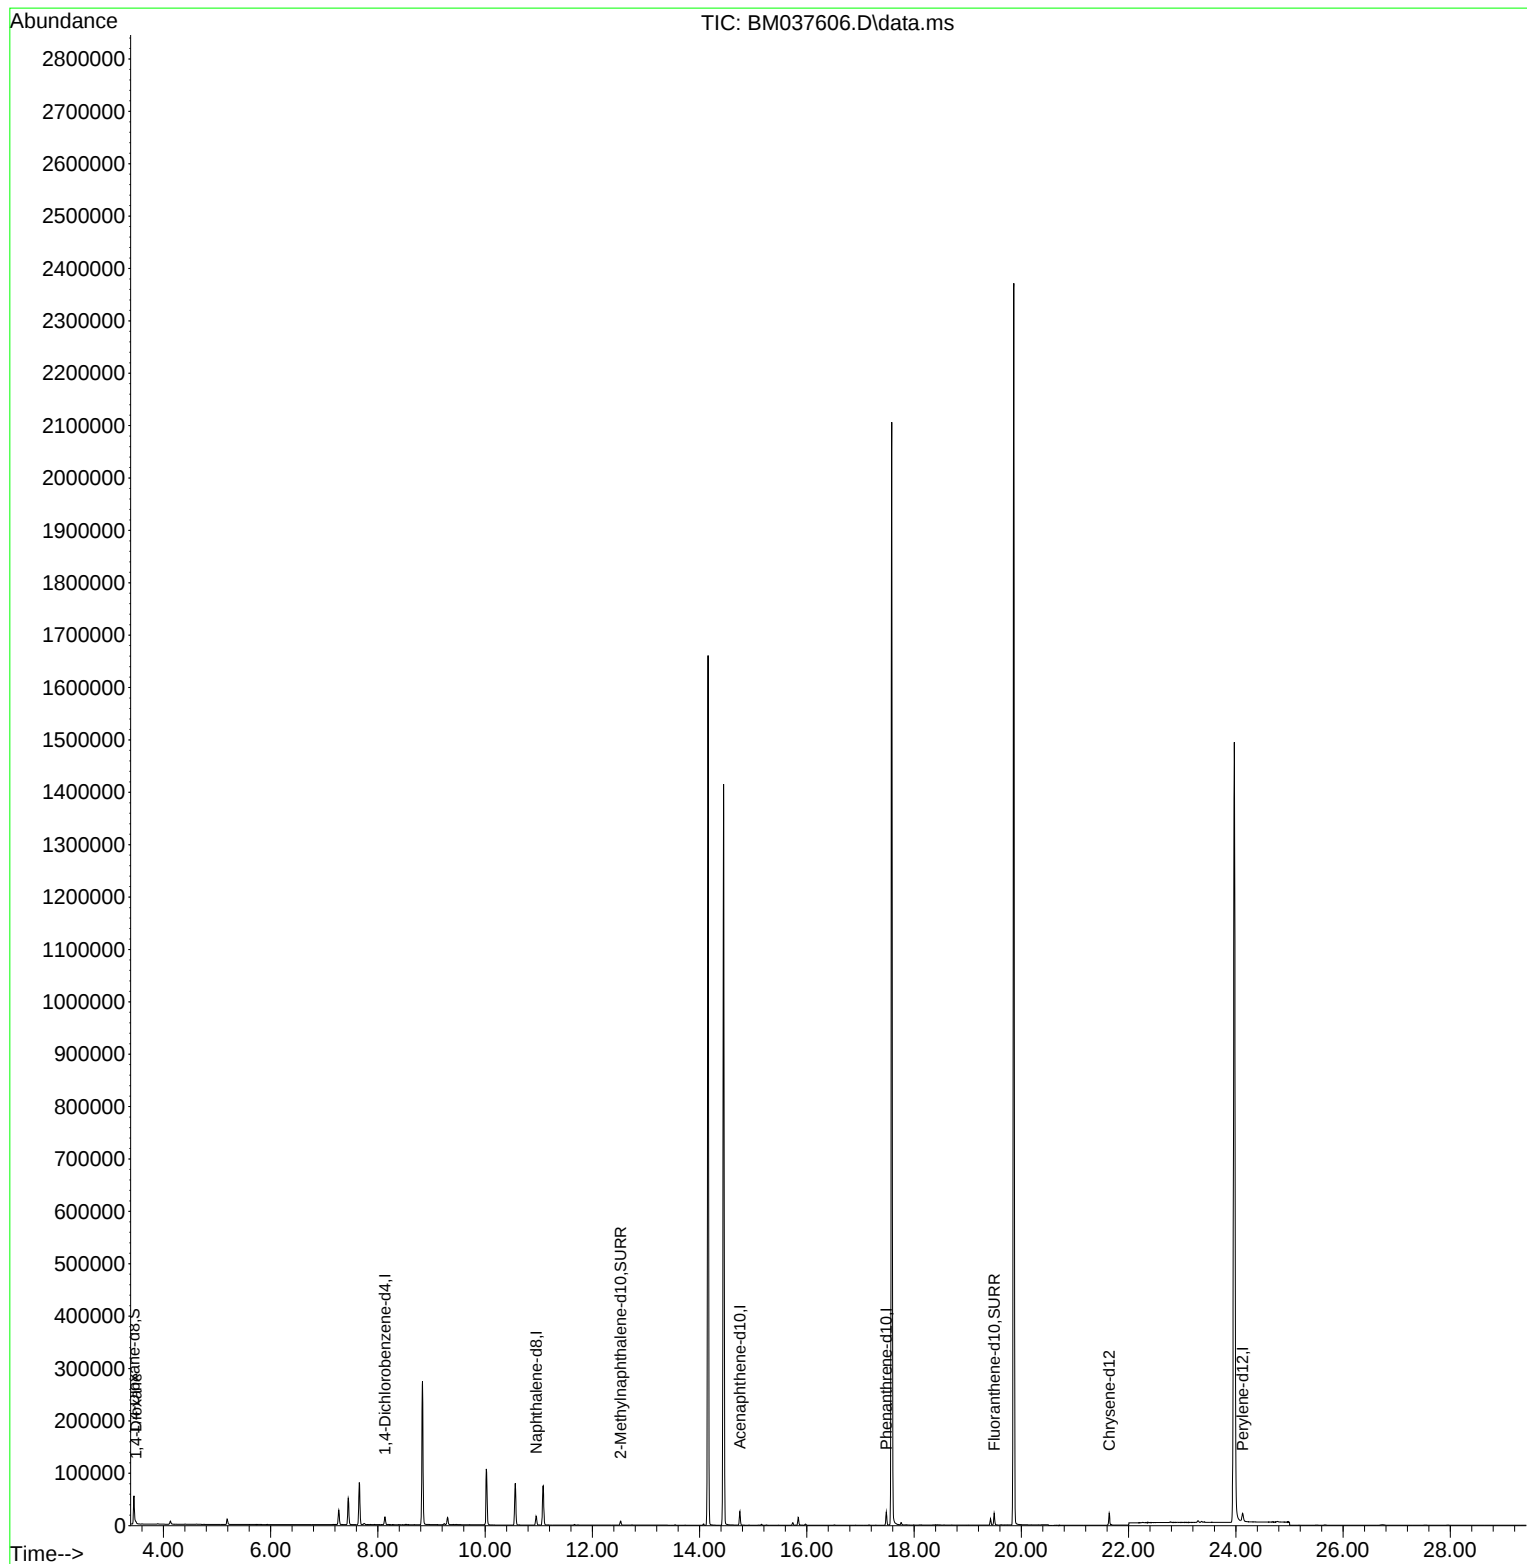

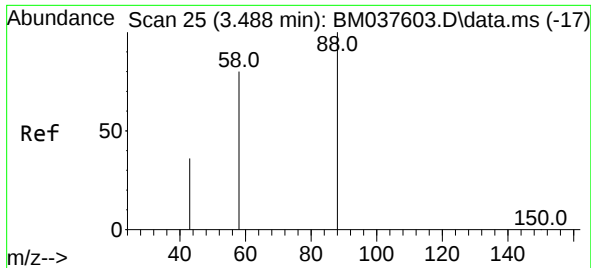

#2
 1,4-Dioxane
 Concen: 0.177 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BM037606.D
 Acq: 21 Nov 2022 11:56

Instrument :
 BNA_M
 ClientSampleId :
 BGCE6

Tgt Ion: 88	Resp: 1589
Ion Ratio	Lower Upper
88 100	
43 60.6	102.8 154.2#
58 60.2	67.3 100.9#

