

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037607.D
 Acq On : 21 Nov 2022 12:32
 Operator : CG/JU
 Sample : N5690-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE7

Quant Time: Nov 21 13:39:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	7555	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	22197	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	13660	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	28683	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	20569	0.400	ng/ul	# 0.00
23) Perylene-d12	24.127	264	21822	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	36373	4.141	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.524	152	9595	0.261	ng/ul	0.00
18) Fluoranthene-d10	19.493	212	24031	0.354	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	2159	0.236	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037607.D
Acq On : 21 Nov 2022 12:32
Operator : CG/JU
Sample : N5690-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE7


Quant Time: Nov 21 13:39:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

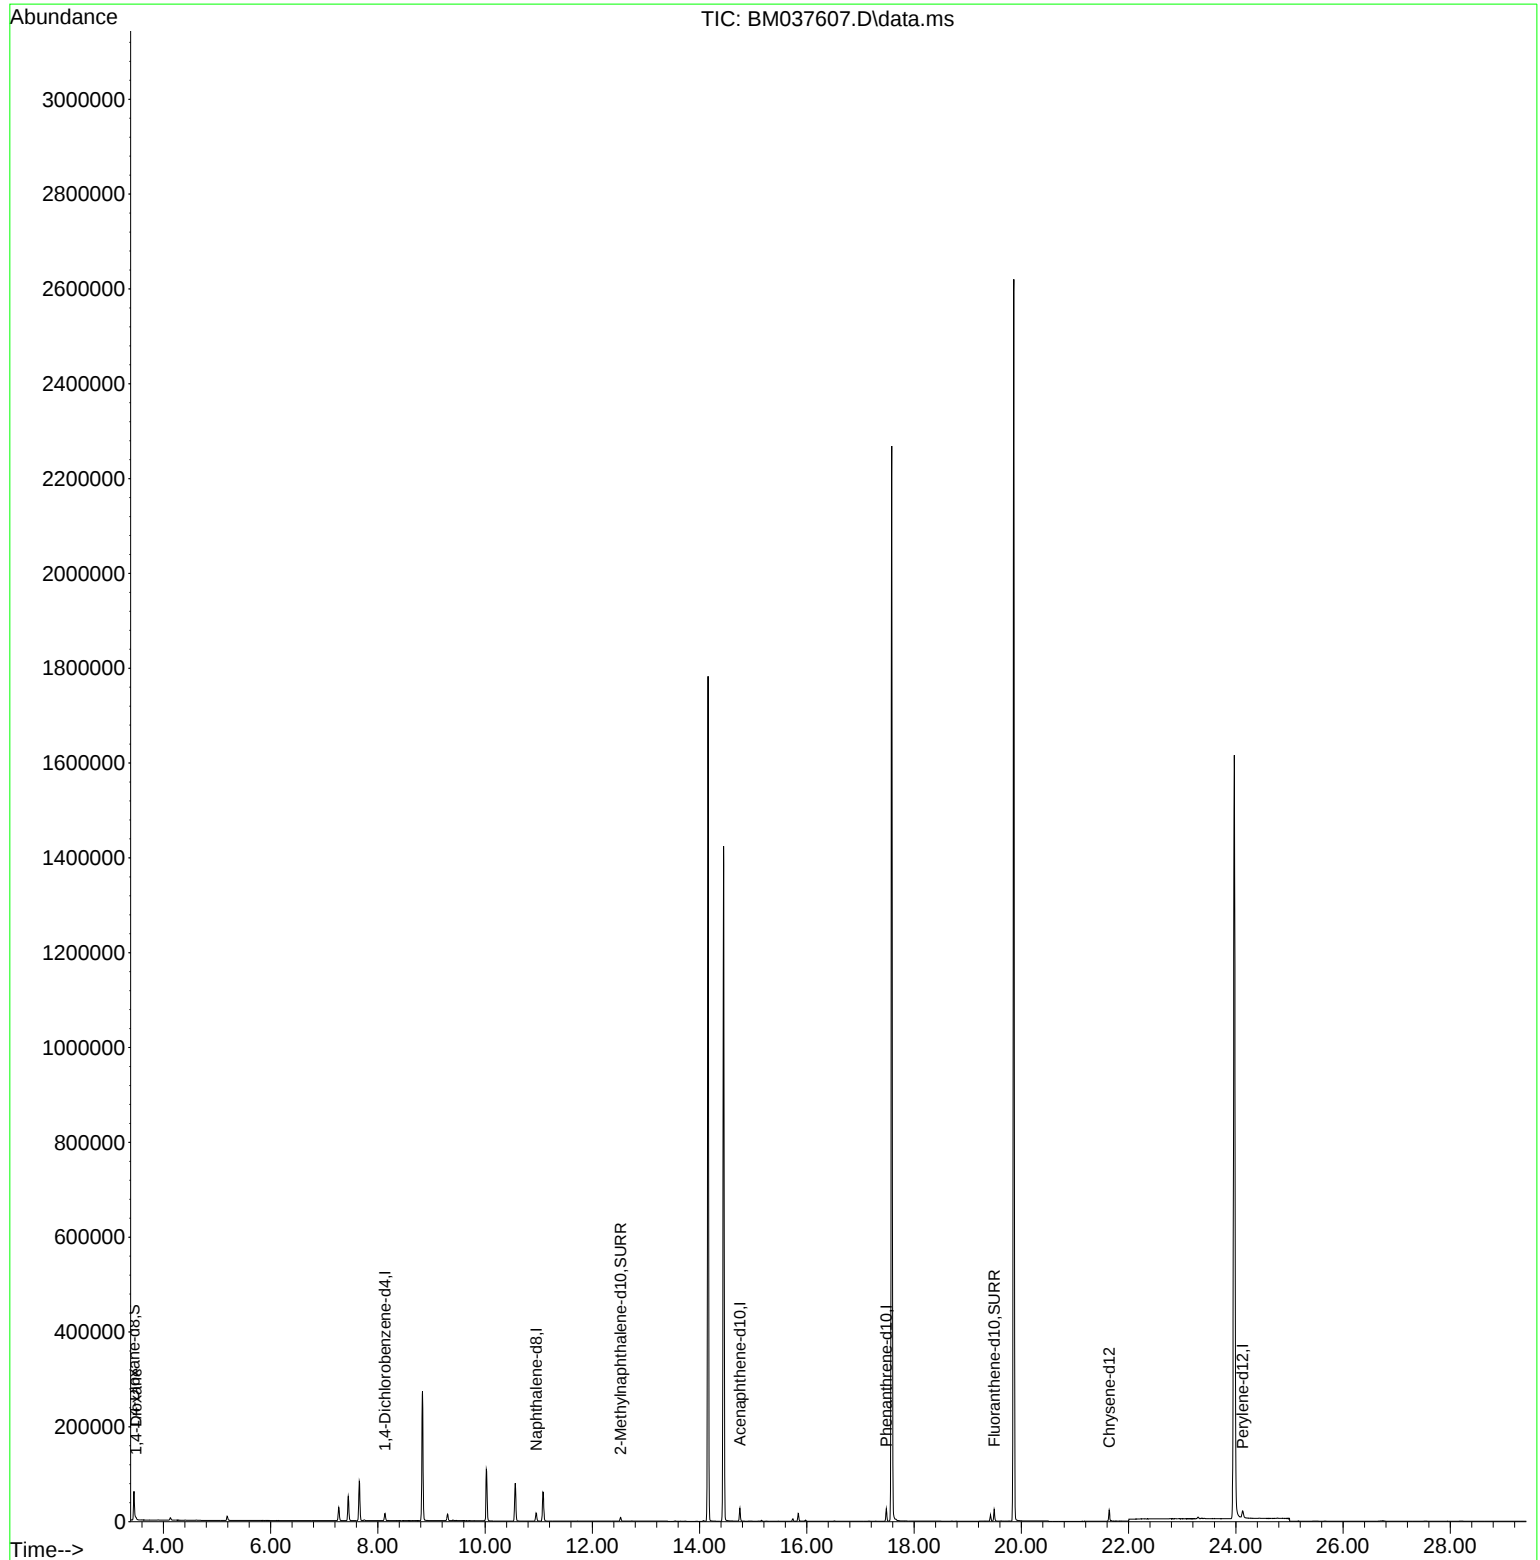

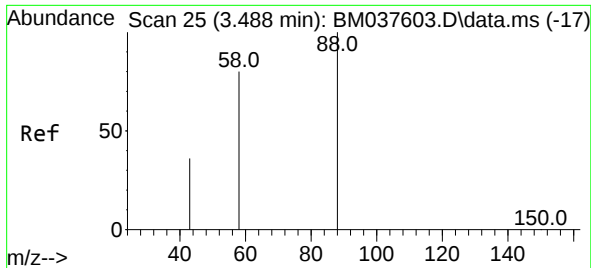

#2
 1,4-Dioxane
 Concen: 0.236 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BM037607.D
 Acq: 21 Nov 2022 12:32

Instrument :
 BNA_M
 ClientSampleId :
 BGCE7

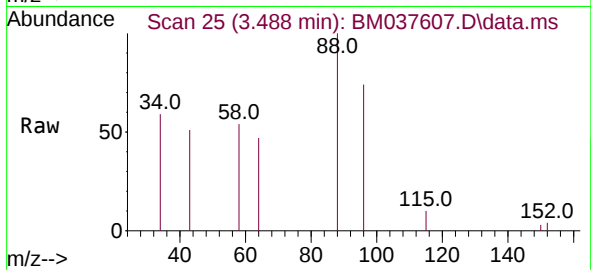

Tgt Ion:	88	Resp:	2159
Ion	Ratio	Lower	Upper
88	100		
43	51.0	102.8	154.2#
58	53.9	67.3	100.9#

