

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037608.D
 Acq On : 21 Nov 2022 13:09
 Operator : CG/JU
 Sample : N5690-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE2

Quant Time: Nov 21 13:49:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	6296	0.400	ng/ul	0.00
4) Naphthalene-d8	10.953	136	18514	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.752	164	11485	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.483	188	24158	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	16888	0.400	ng/ul	# 0.00
23) Perylene-d12	24.130	264	18719	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	30962	4.230	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	9110	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.495	212	22317	0.400	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1422	0.187	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037608.D
Acq On : 21 Nov 2022 13:09
Operator : CG/JU
Sample : N5690-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE2

Quant Time: Nov 21 13:49:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

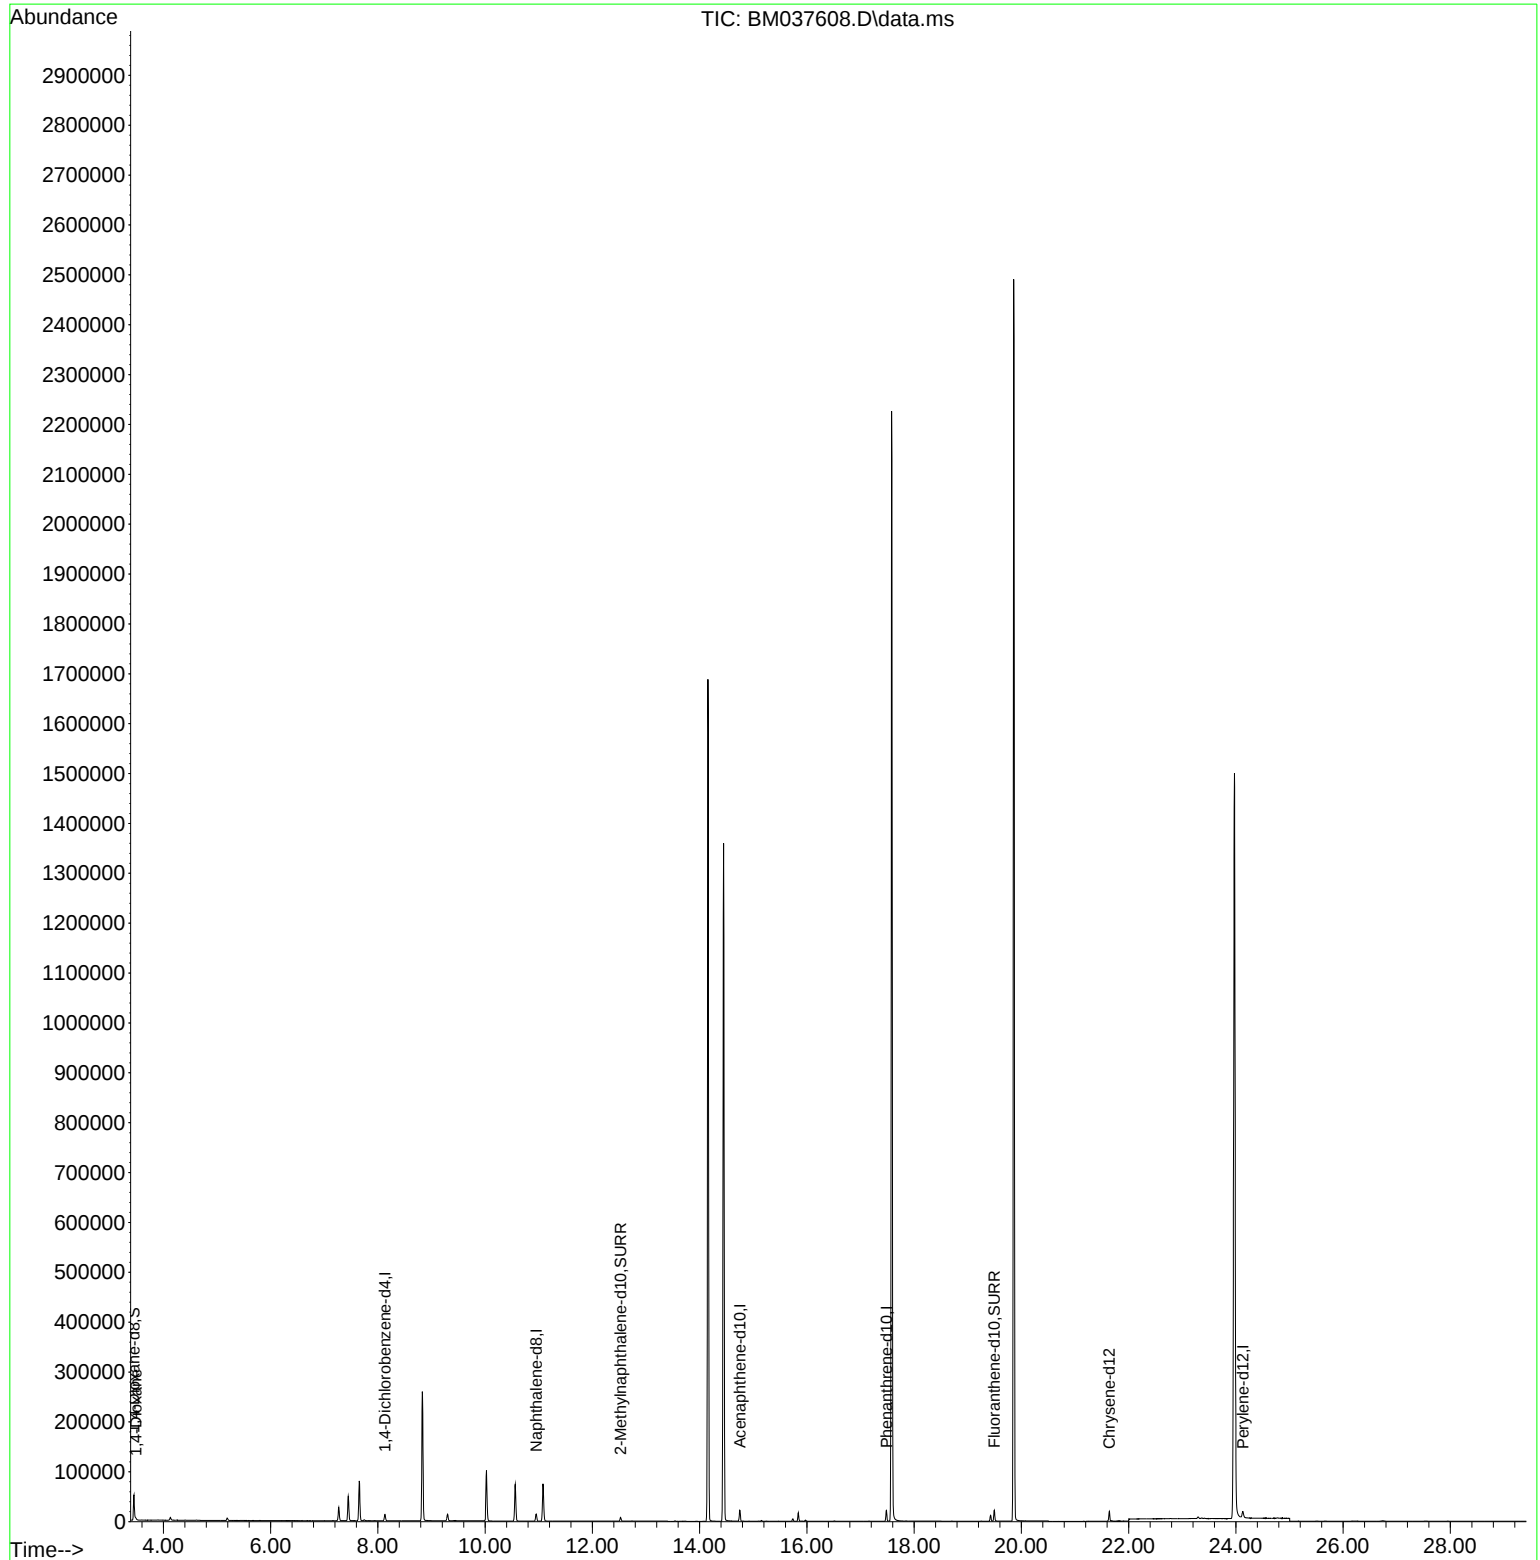

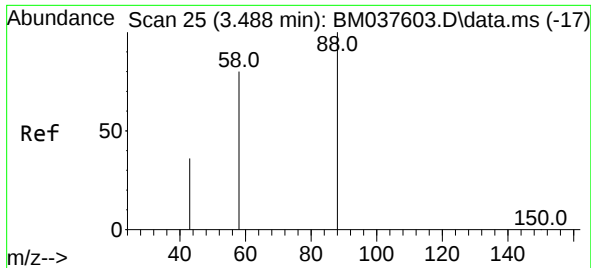

#2
 1,4-Dioxane
 Concen: 0.187 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BM037608.D
 Acq: 21 Nov 2022 13:09

Instrument :
 BNA_M
 ClientSampleId :
 BGCE2

Tgt Ion: 88 Resp: 1422
 Ion Ratio Lower Upper
 88 100
 43 64.2 102.8 154.2#
 58 60.8 67.3 100.9#

