

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037610.D
 Acq On : 21 Nov 2022 14:22
 Operator : CG/JU
 Sample : N5690-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE8

Quant Time: Nov 22 02:22:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	6258	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	18339	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.751	164	11541	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	24171	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	16938	0.400	ng/ul	# 0.00
23) Perylene-d12	24.130	264	18310	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	32204	4.426	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.524	152	8192	0.269	ng/ul	0.00
18) Fluoranthene-d10	19.493	212	20171	0.360	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1828	0.241	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037610.D
Acq On : 21 Nov 2022 14:22
Operator : CG/JU
Sample : N5690-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE8

Quant Time: Nov 22 02:22:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

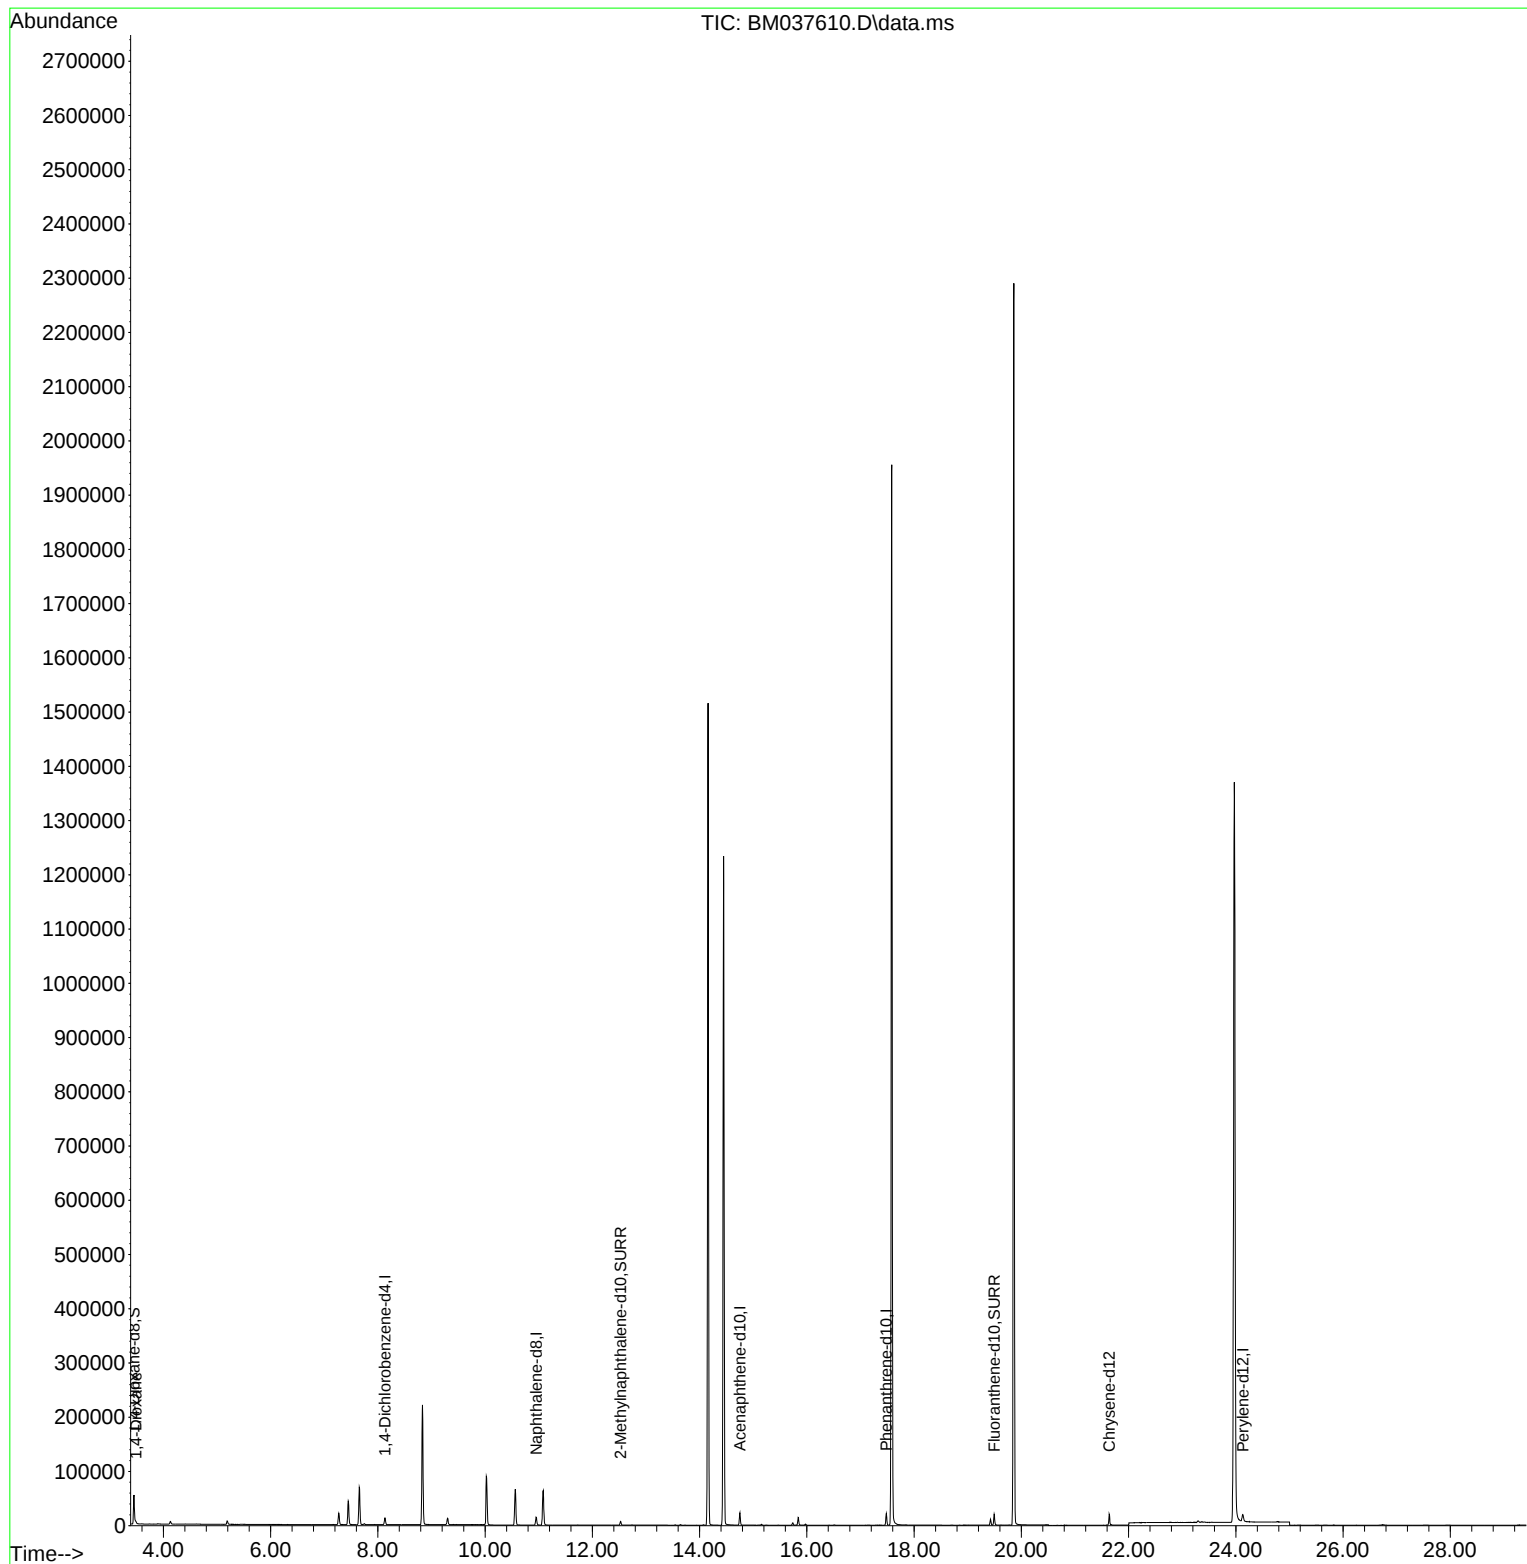

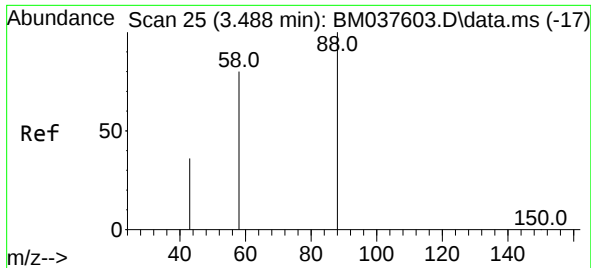

#2
 1,4-Dioxane
 Concen: 0.241 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM037610.D
 Acq: 21 Nov 2022 14:22

Instrument :
 BNA_M
 ClientSampleId :
 BGCE8

Tgt Ion: 88 Resp: 1828

Ion	Ratio	Lower	Upper
88	100		
43	60.9	102.8	154.2#
58	66.1	67.3	100.9#

