

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037611.D
 Acq On : 21 Nov 2022 14:59
 Operator : CG/JU
 Sample : N5690-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE9

Quant Time: Nov 22 02:23:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	7642	0.400	ng/ul	0.00
4) Naphthalene-d8	10.953	136	22634	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.752	164	13982	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.483	188	29271	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	21322	0.400	ng/ul	# 0.00
23) Perylene-d12	24.130	264	22730	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	33598	3.781	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	8810	0.235	ng/ul	0.00
18) Fluoranthene-d10	19.495	212	20950	0.297	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.493	88	2005	0.217	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037611.D
Acq On : 21 Nov 2022 14:59
Operator : CG/JU
Sample : N5690-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE9

Quant Time: Nov 22 02:23:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

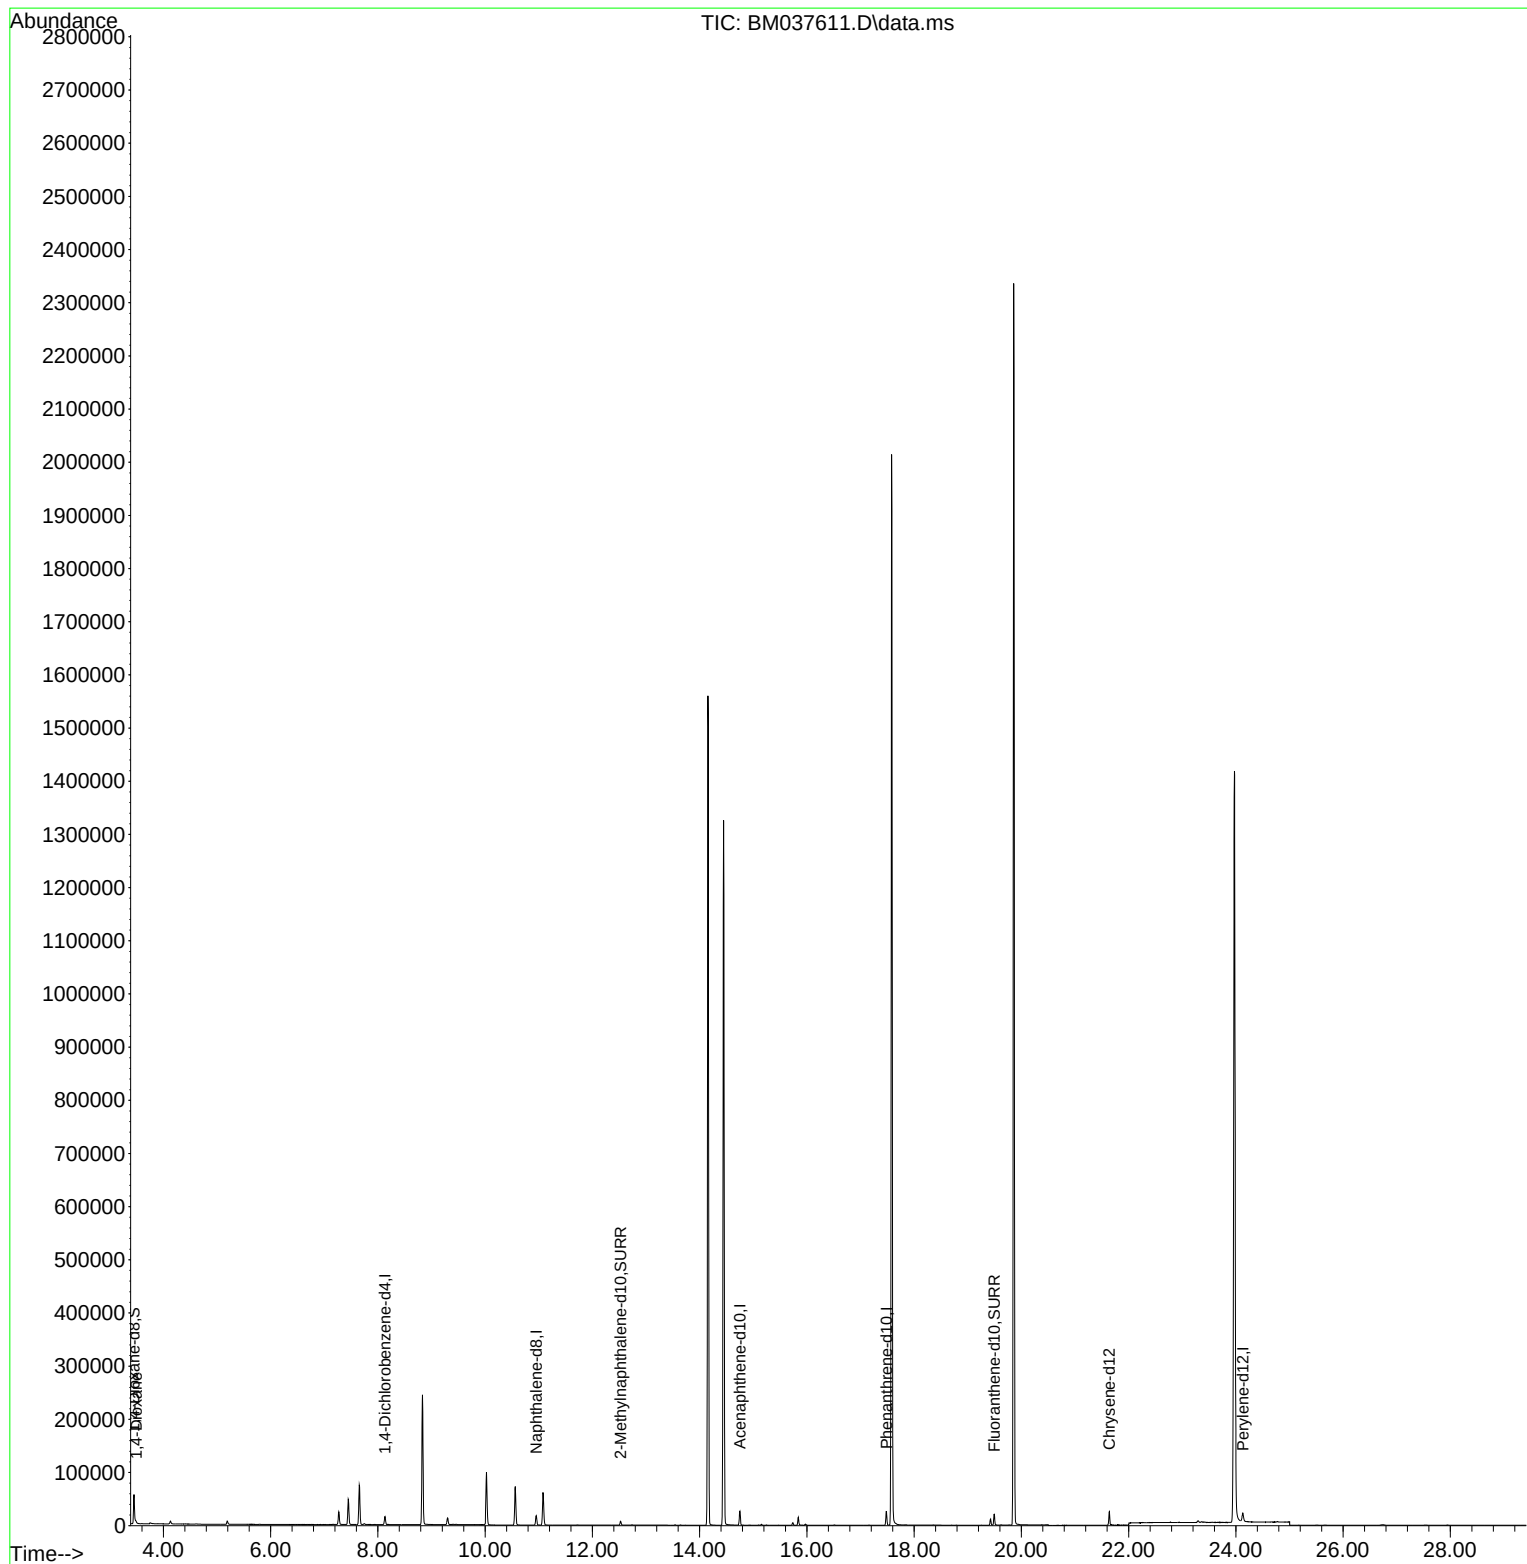

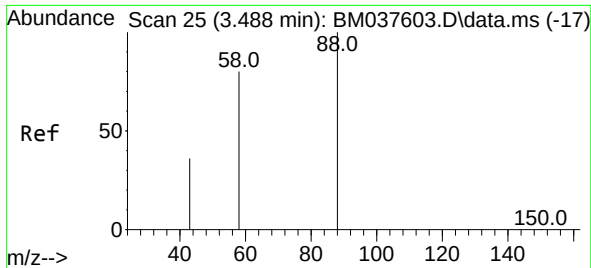

#2
 1,4-Dioxane
 Concen: 0.217 ng/ul
 RT: 3.493 min Scan# 20
 Delta R.T. 0.005 min
 Lab File: BM037611.D
 Acq: 21 Nov 2022 14:59

Instrument :
 BNA_M
 ClientSampleId :
 BGCE9

Tgt Ion: 88 Resp: 2005
 Ion Ratio Lower Upper
 88 100
 43 46.7 102.8 154.2#
 58 45.4 67.3 100.9#

