

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037614.D
 Acq On : 21 Nov 2022 16:50
 Operator : CG/JU
 Sample : N5690-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCC9

Quant Time: Nov 21 17:30:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	7452	0.400	ng/ul	0.00
4) Naphthalene-d8	10.953	136	22033	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.752	164	13620	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.483	188	28347	0.400	ng/ul	0.00
17) Chrysene-d12	21.642	240	20480	0.400	ng/ul	# 0.00
23) Perylene-d12	24.133	264	22346	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	37691	4.350	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	10455	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.495	212	25580	0.378	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.492	88	2134	0.237	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037614.D
Acq On : 21 Nov 2022 16:50
Operator : CG/JU
Sample : N5690-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCC9

Quant Time: Nov 21 17:30:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

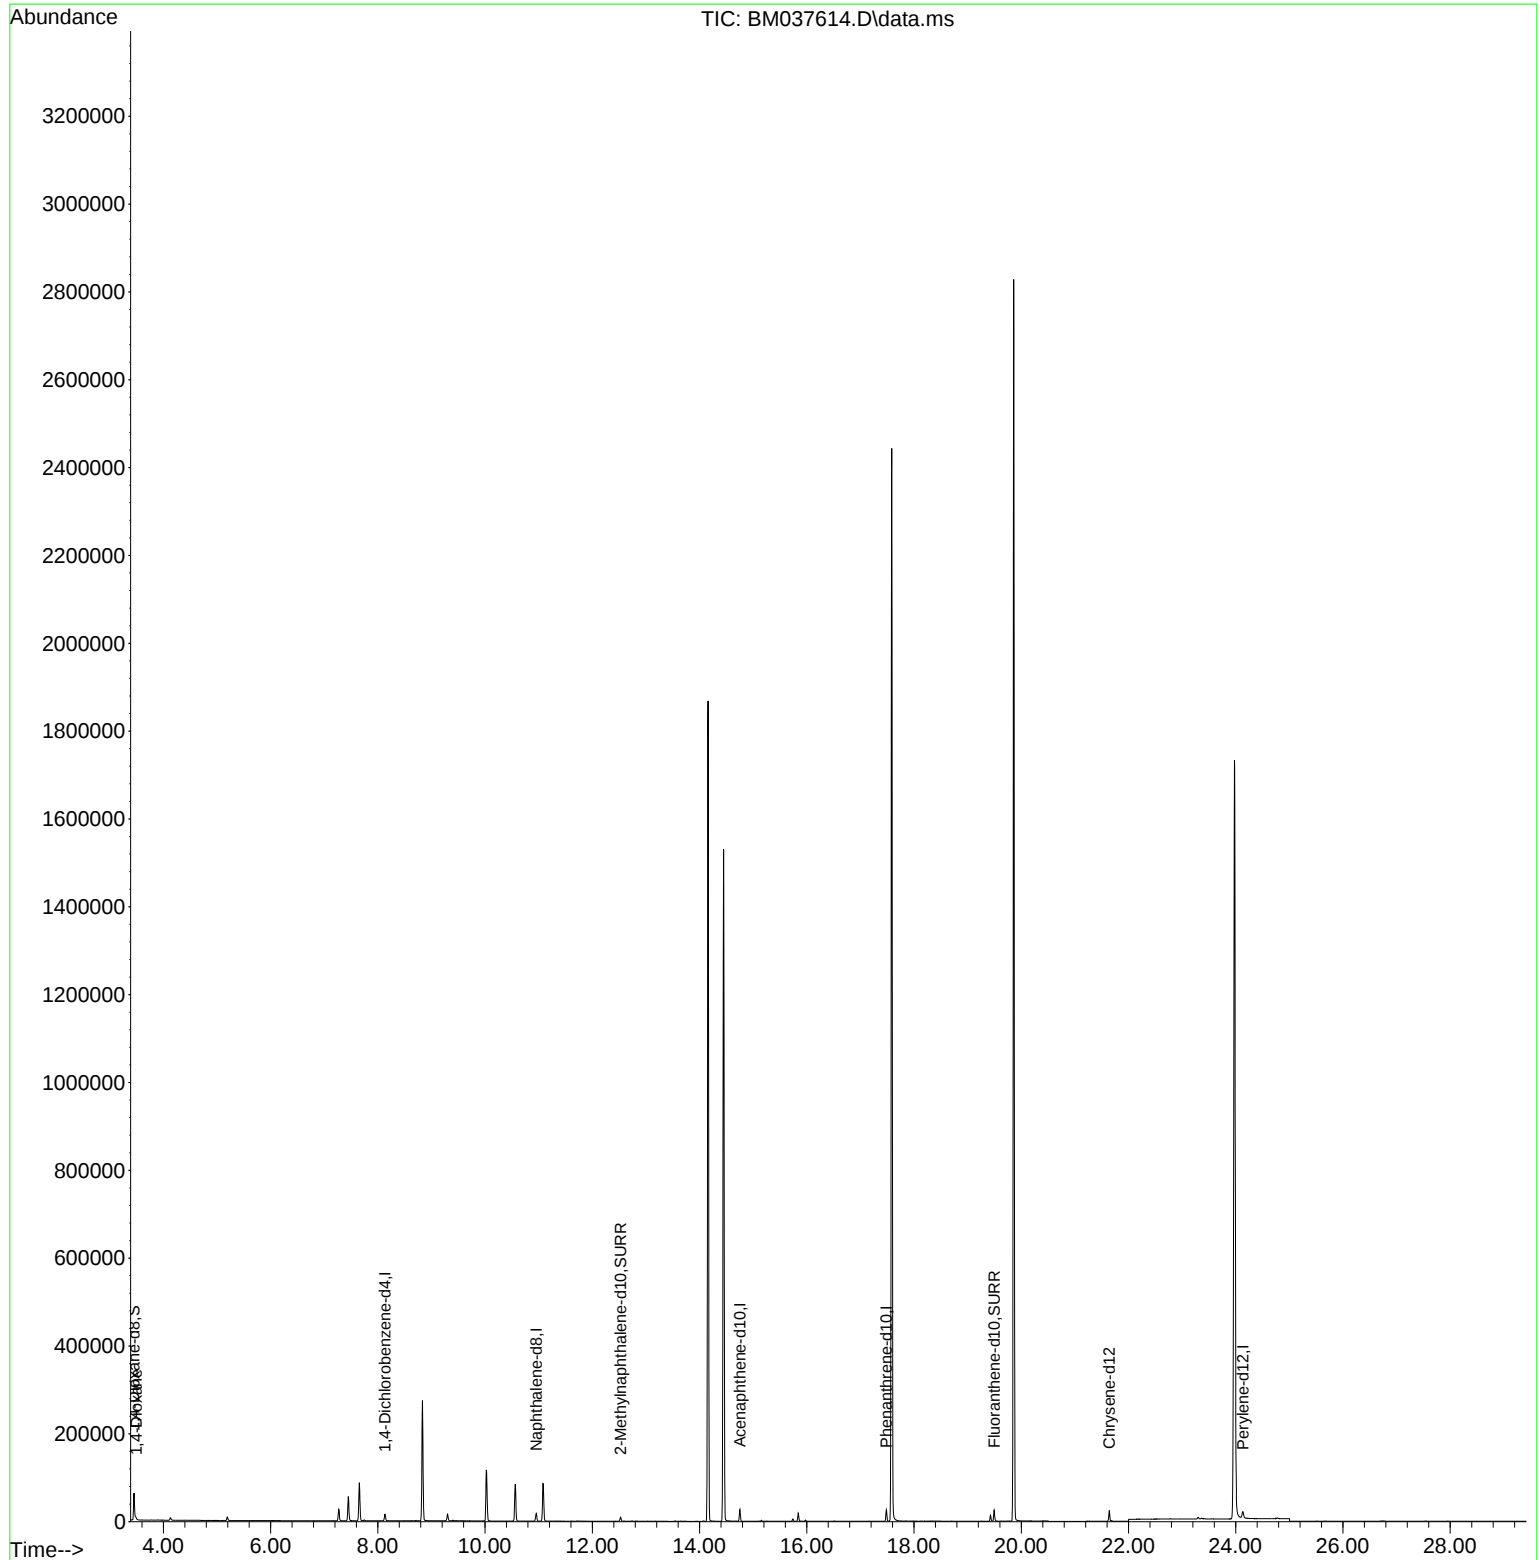

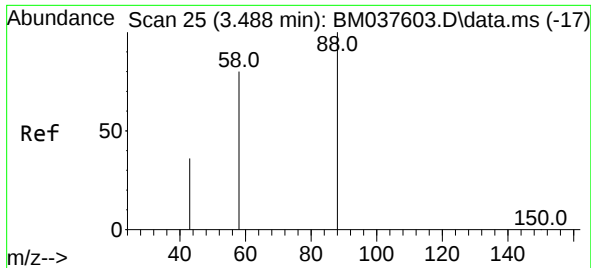

#2
 1,4-Dioxane
 Concen: 0.237 ng/ul
 RT: 3.492 min Scan# 20
 Delta R.T. 0.001 min
 Lab File: BM037614.D
 Acq: 21 Nov 2022 16:50

Instrument :
 BNA_M
 ClientSampleId :
 BGCC9

Tgt Ion: 88 Resp: 2134
 Ion Ratio Lower Upper
 88 100
 43 48.7 102.8 154.2#
 58 50.8 67.3 100.9#

