

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037617.D
 Acq On : 21 Nov 2022 18:42
 Operator : CG/JU
 Sample : N5690-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCG8

Quant Time: Nov 21 20:44:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.129	152	6807	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	20521	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.750	164	12646	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	26663	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	19205	0.400	ng/ul	# 0.00
23) Perylene-d12	24.130	264	20639	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	33814	4.273	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.524	152	9420	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.493	212	23281	0.367	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1726	0.210	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037617.D
Acq On : 21 Nov 2022 18:42
Operator : CG/JU
Sample : N5690-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCG8

Quant Time: Nov 21 20:44:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

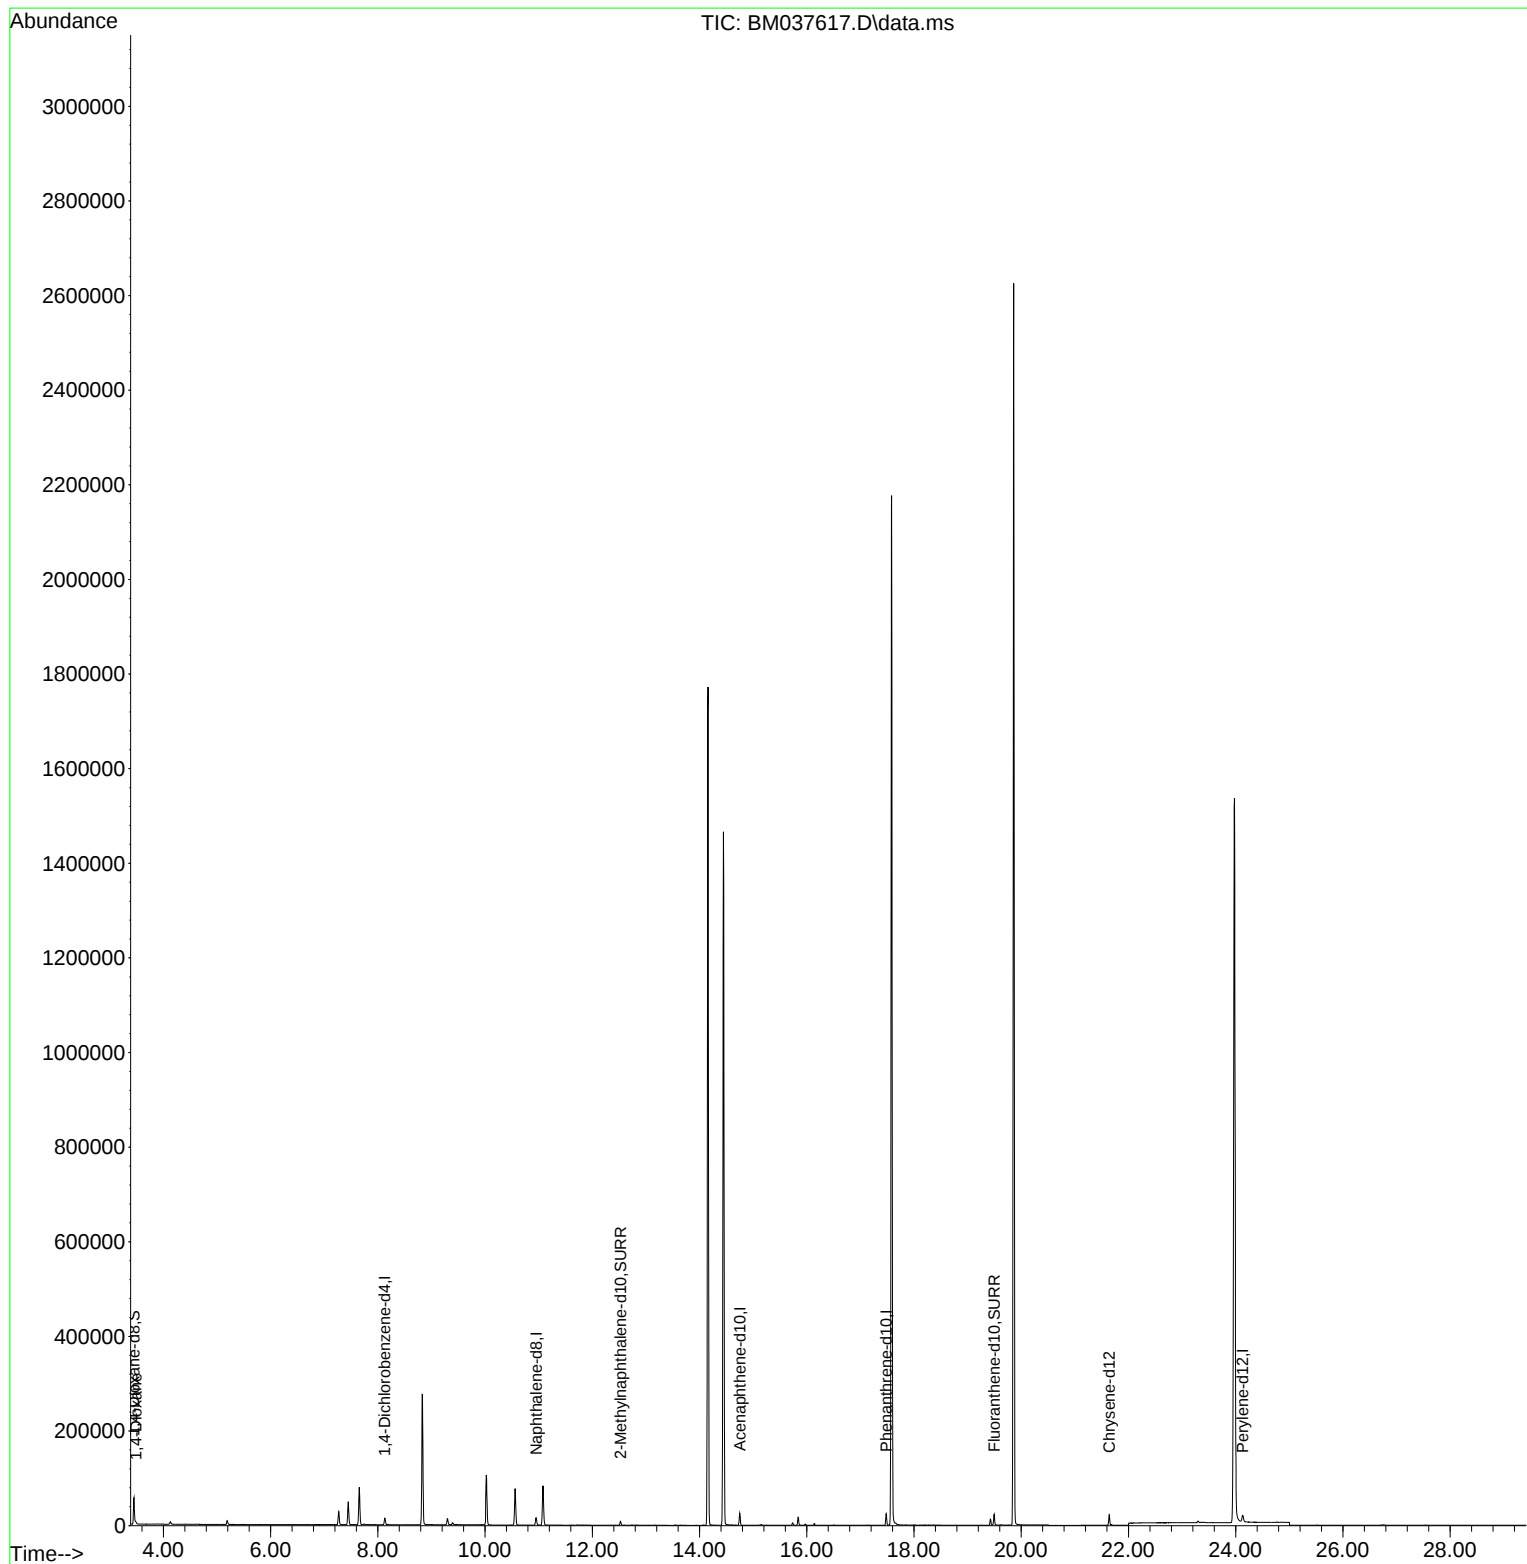

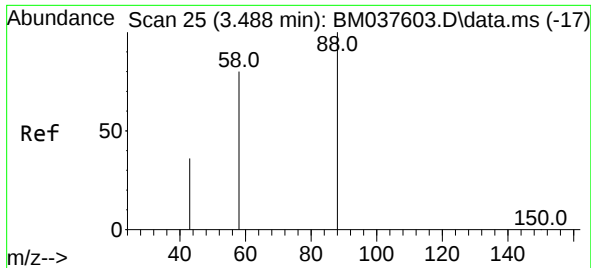

#2
 1,4-Dioxane
 Concen: 0.210 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BM037617.D
 Acq: 21 Nov 2022 18:42

Instrument :
 BNA_M
 ClientSampleId :
 BGCG8

Tgt Ion:	88	Resp:	1726
Ion	Ratio	Lower	Upper
88	100		
43	66.3	102.8	154.2#
58	68.1	67.3	100.9

