

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037618.D
 Acq On : 21 Nov 2022 19:18
 Operator : CG/JU
 Sample : N5690-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE4

Quant Time: Nov 21 20:45:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	7164	0.400	ng/ul	0.00
4) Naphthalene-d8	10.953	136	21466	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.747	164	13191	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.479	188	27151	0.400	ng/ul	0.00
17) Chrysene-d12	21.639	240	20354	0.400	ng/ul	# 0.00
23) Perylene-d12	24.130	264	22081	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	54464	6.539	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	12749	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.495	212	32847	0.488	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.492	88	2540	0.293	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037618.D
Acq On : 21 Nov 2022 19:18
Operator : CG/JU
Sample : N5690-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE4

Quant Time: Nov 21 20:45:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

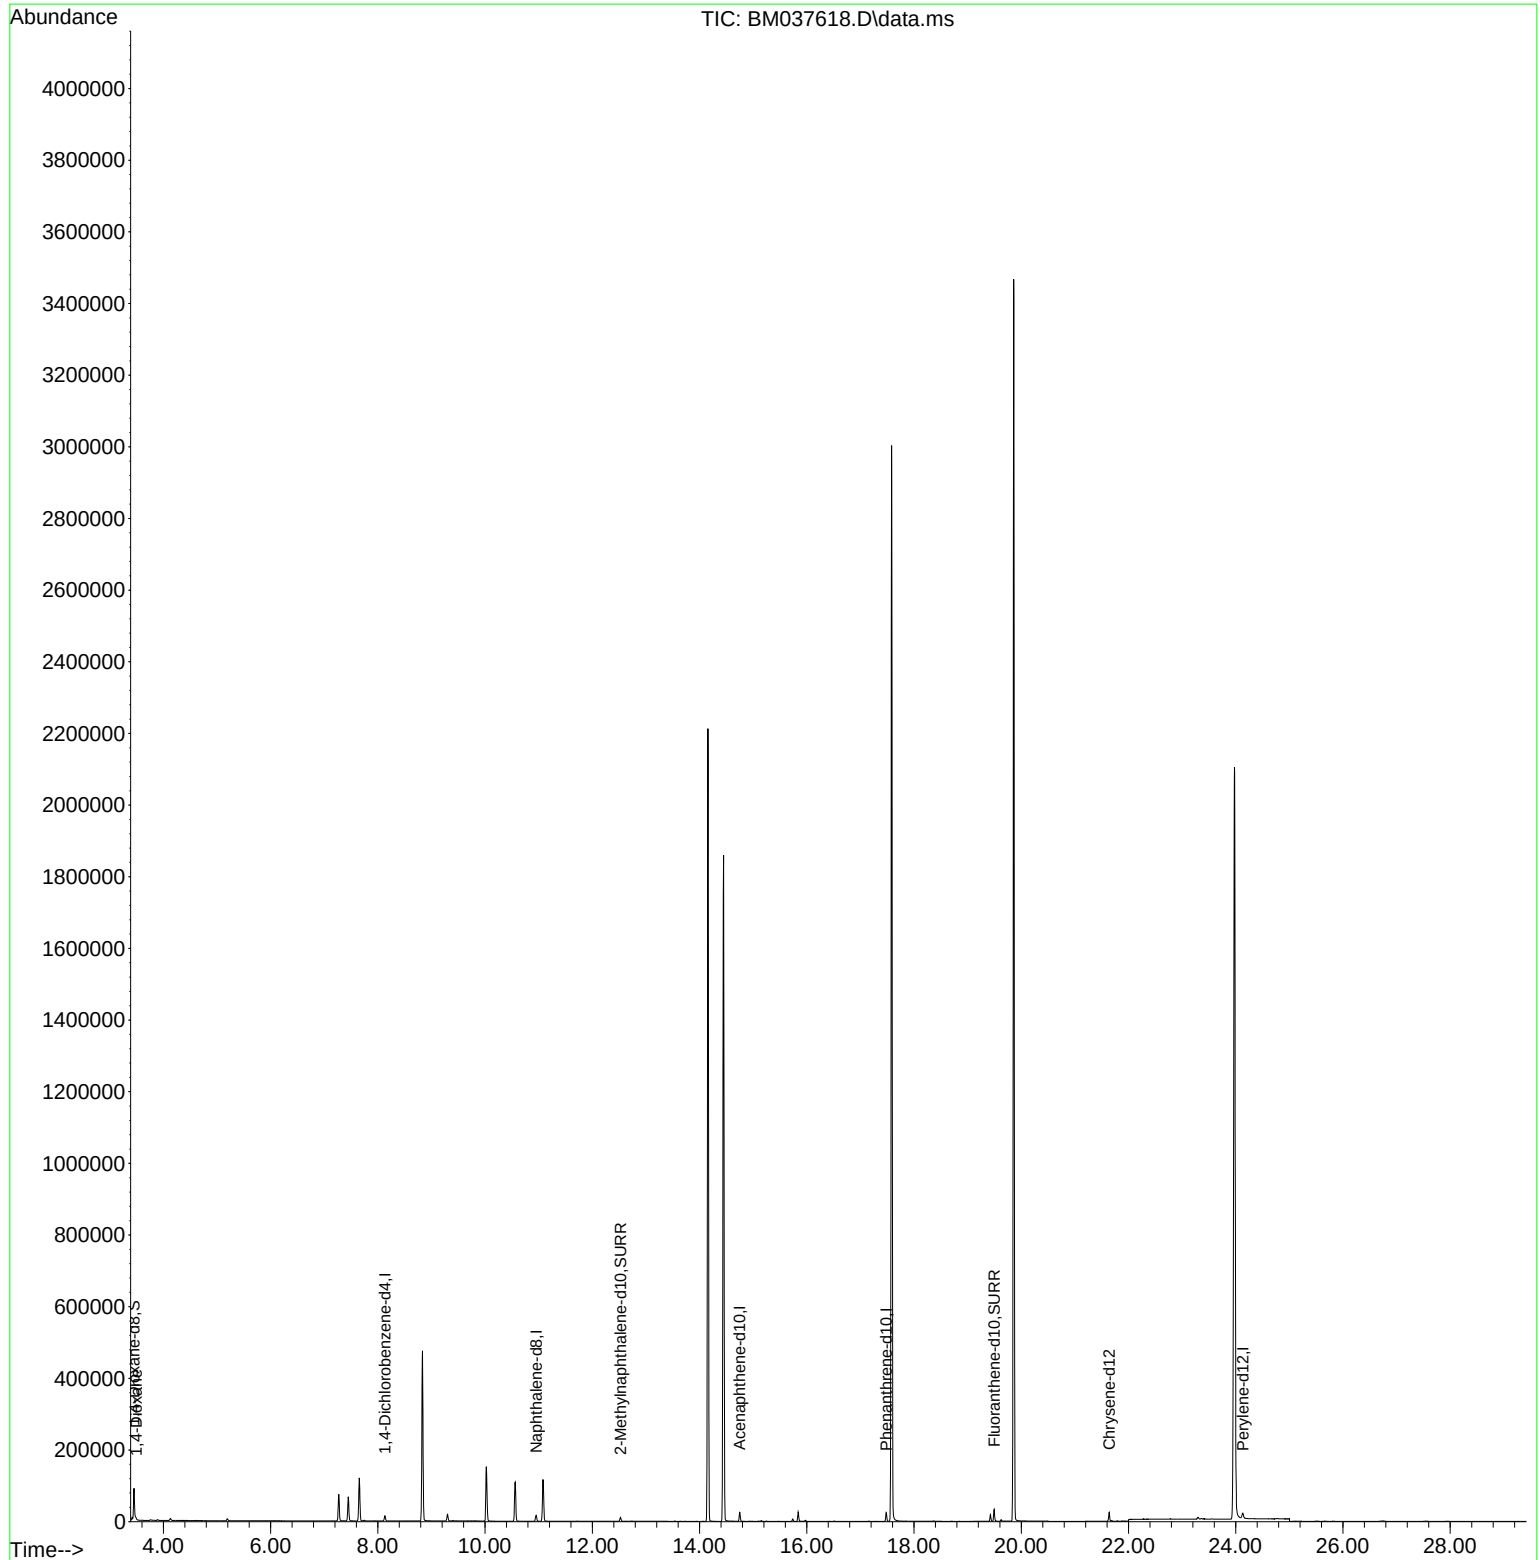

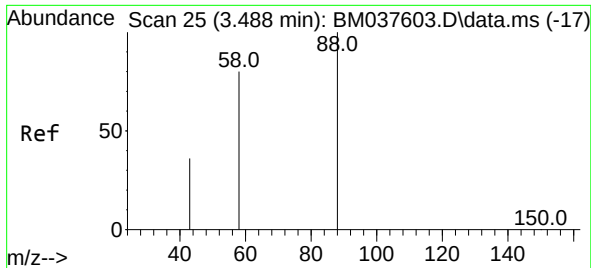

#2

1,4-Dioxane

Concen: 0.293 ng/ul

RT: 3.492 min Scan# 20

Delta R.T. 0.001 min

Lab File: BM037618.D

Acq: 21 Nov 2022 19:18

Instrument :

BNA_M

ClientSampleId :

BGCE4

Tgt Ion: 88 Resp: 2540

Ion Ratio Lower Upper

88 100

43 49.0 102.8 154.2#

58 52.6 67.3 100.9#

