

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037619.D
 Acq On : 21 Nov 2022 19:55
 Operator : CG/JU
 Sample : N5690-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCF4

Quant Time: Nov 21 20:46:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.133	152	7117	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	20989	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	13149	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	27557	0.400	ng/ul	0.00
17) Chrysene-d12	21.640	240	19934	0.400	ng/ul	# 0.00
23) Perylene-d12	24.130	264	21159	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	32514	3.929	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.524	152	9464	0.272	ng/ul	0.00
18) Fluoranthene-d10	19.493	212	24952	0.379	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.492	88	2222	0.258	ng/ul#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037619.D
Acq On : 21 Nov 2022 19:55
Operator : CG/JU
Sample : N5690-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCF4

Quant Time: Nov 21 20:46:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

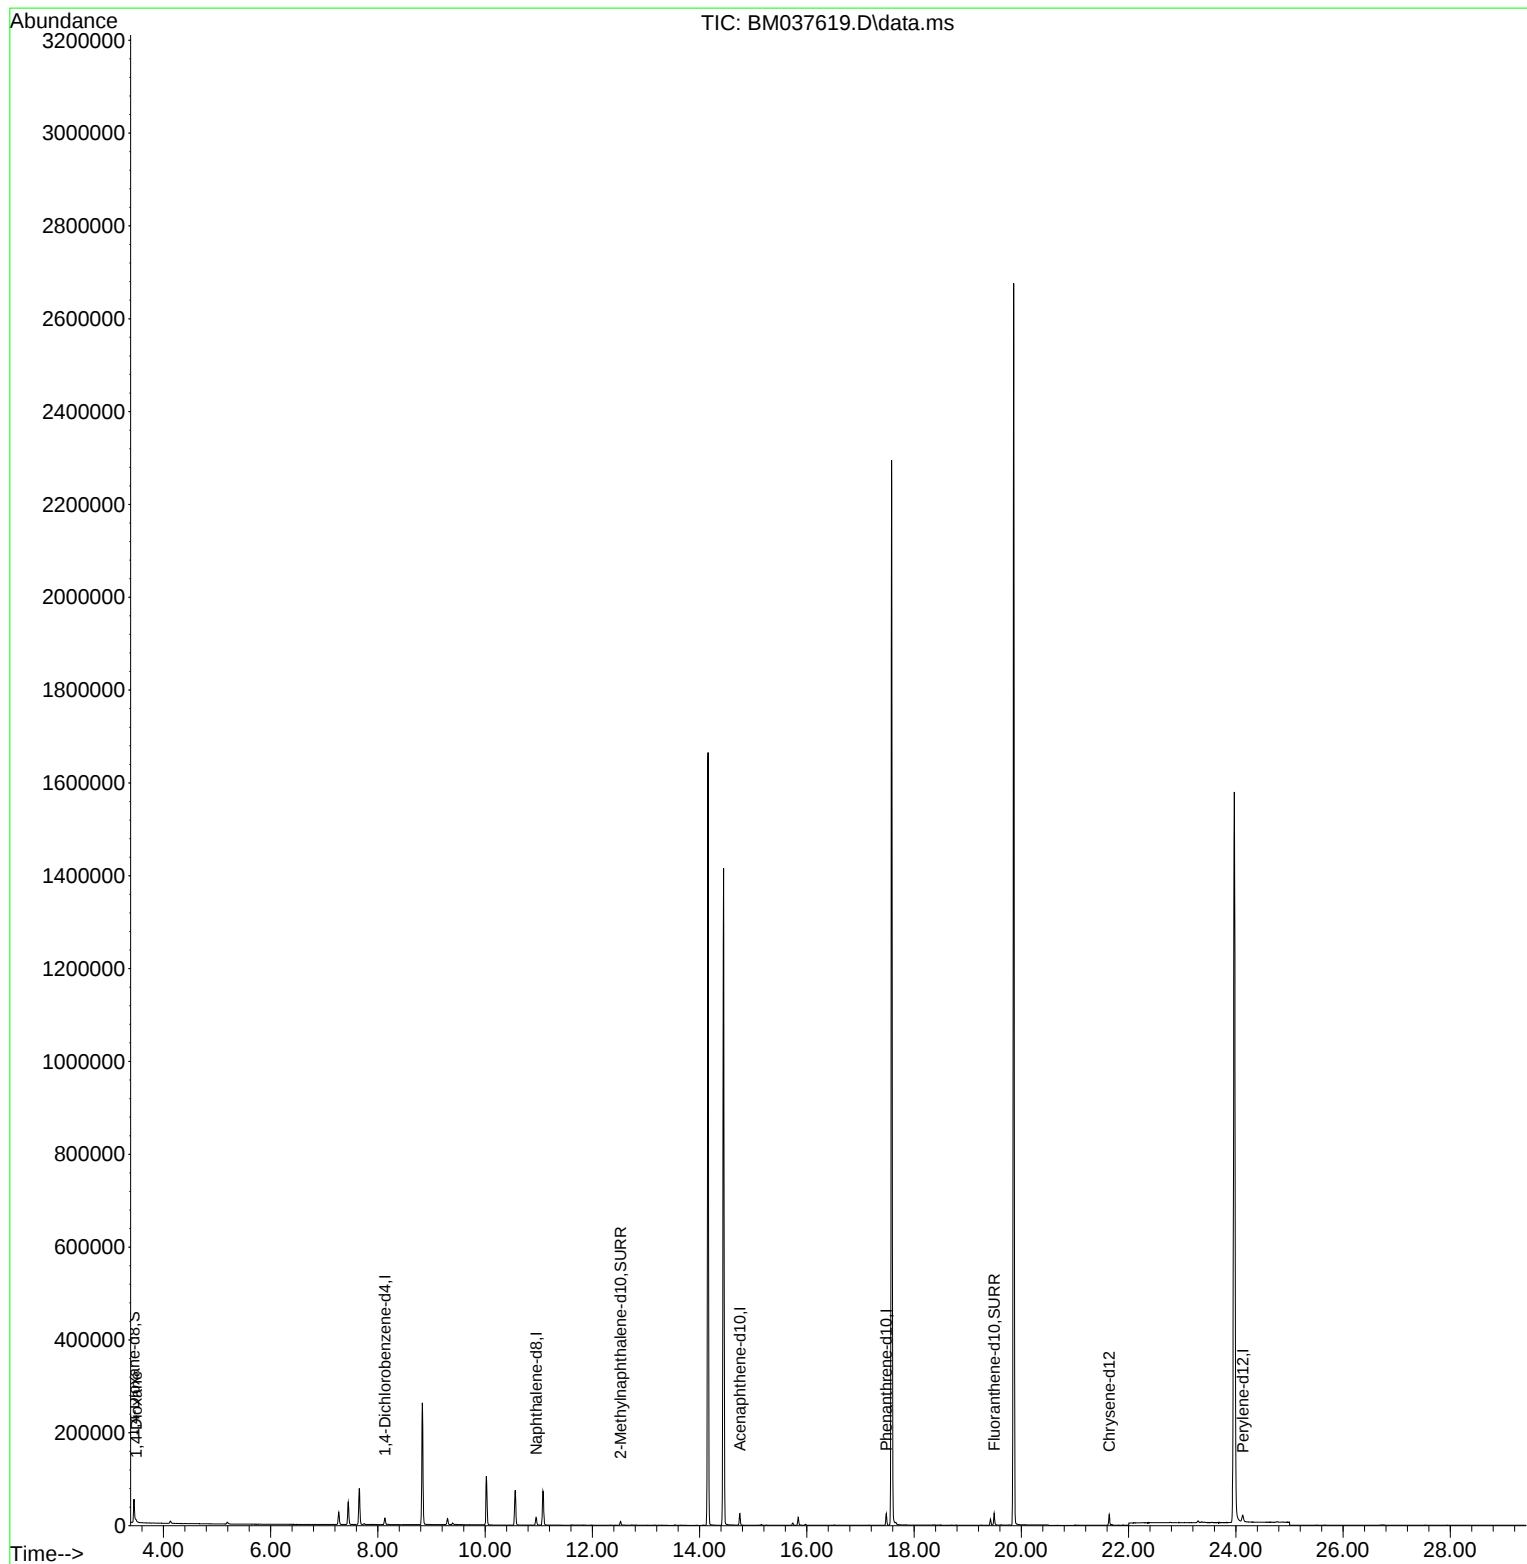

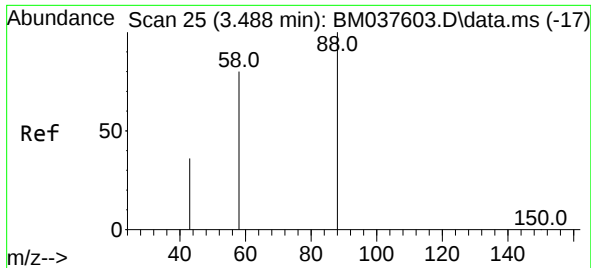

#2
 1,4-Dioxane
 Concen: 0.258 ng/ul
 RT: 3.492 min Scan# 20
 Delta R.T. 0.001 min
 Lab File: BM037619.D
 Acq: 21 Nov 2022 19:55

Instrument :
 BNA_M
 ClientSampleId :
 BGCF4

Tgt Ion: 88 Resp: 2222
 Ion Ratio Lower Upper
 88 100
 43 27.1 102.8 154.2#
 58 22.6 67.3 100.9#

