

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037623.D
 Acq On : 21 Nov 2022 22:58
 Operator : CG/JU
 Sample : N5690-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCG5

Quant Time: Nov 22 00:11:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.129	152	6157	0.400	ng/ul	0.00
4) Naphthalene-d8	10.947	136	18405	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.747	164	11302	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.479	188	23346	0.400	ng/ul	0.00
17) Chrysene-d12	21.636	240	18516	0.400	ng/ul	# 0.00
23) Perylene-d12	24.124	264	20178	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	30661	4.283	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	9060	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.495	212	22954	0.375	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1517	0.204	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037623.D
Acq On : 21 Nov 2022 22:58
Operator : CG/JU
Sample : N5690-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCG5


Quant Time: Nov 22 00:11:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

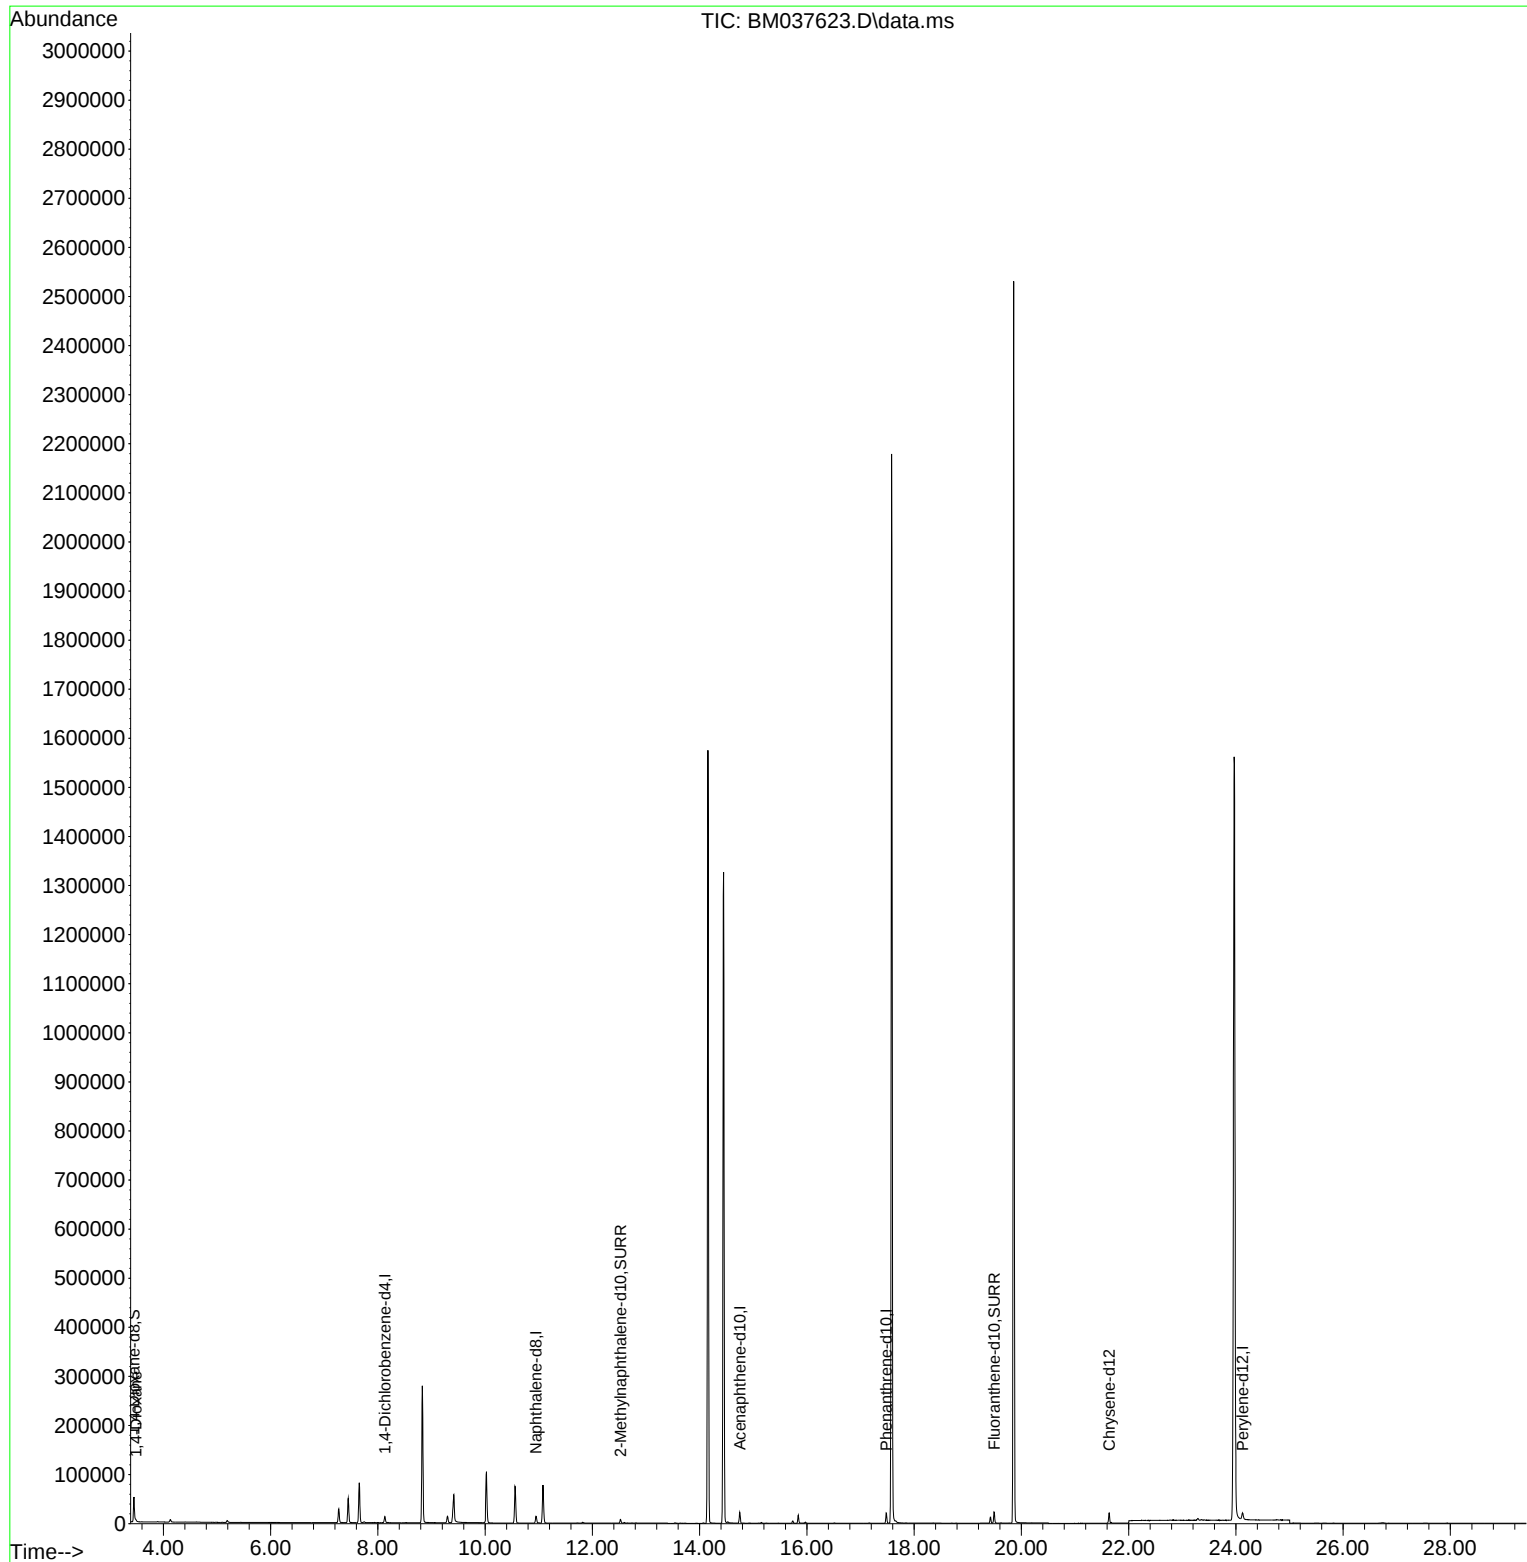

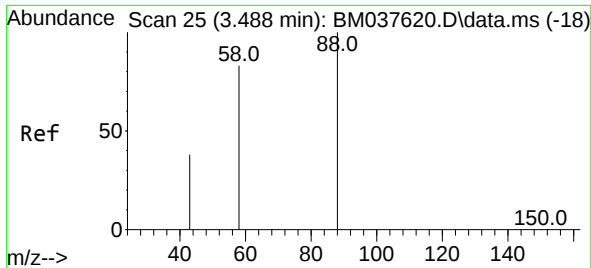

#2
 1,4-Dioxane
 Concen: 0.204 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM037623.D
 Acq: 21 Nov 2022 22:58

Instrument :
 BNA_M
 ClientSampleId :
 BGCG5

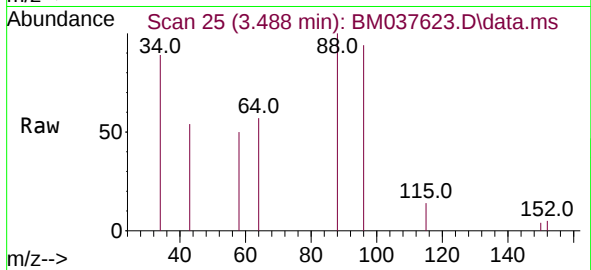

Tgt Ion:	88	Resp:	1517
Ion	Ratio	Lower	Upper
88	100		
43	54.4	102.8	154.2#
58	50.0	67.3	100.9#

