

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037624.D
 Acq On : 21 Nov 2022 23:34
 Operator : CG/JU
 Sample : N5690-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCG6

Quant Time: Nov 22 00:12:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.129	152	6368	0.400	ng/ul	0.00
4) Naphthalene-d8	10.953	136	18895	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.747	164	11662	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.483	188	24205	0.400	ng/ul	0.00
17) Chrysene-d12	21.636	240	17003	0.400	ng/ul	# 0.00
23) Perylene-d12	24.127	264	18176	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	35420	4.784	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.526	152	9555	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.490	212	24414	0.435	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1760	0.228	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037624.D
Acq On : 21 Nov 2022 23:34
Operator : CG/JU
Sample : N5690-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCG6

Quant Time: Nov 22 00:12:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

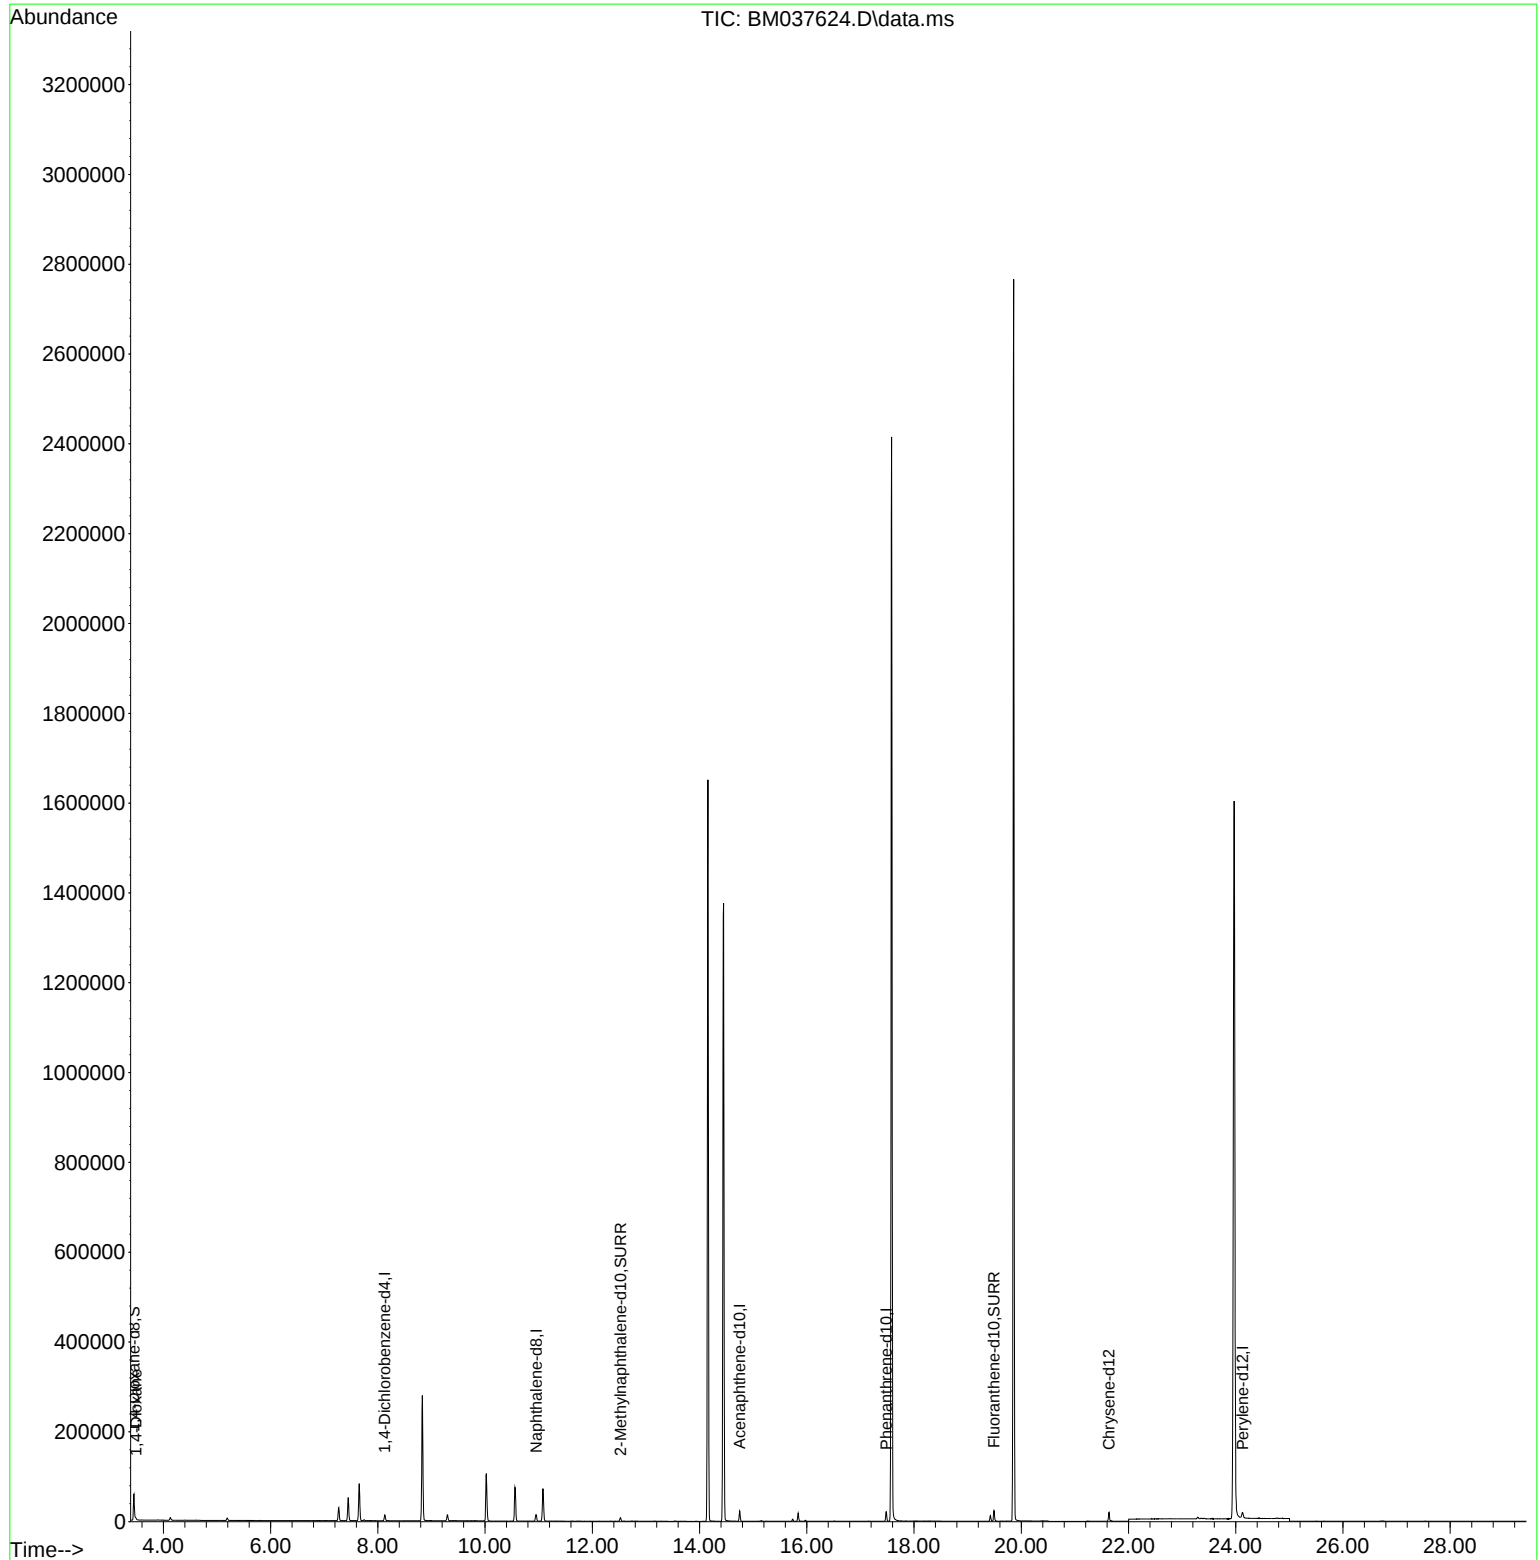

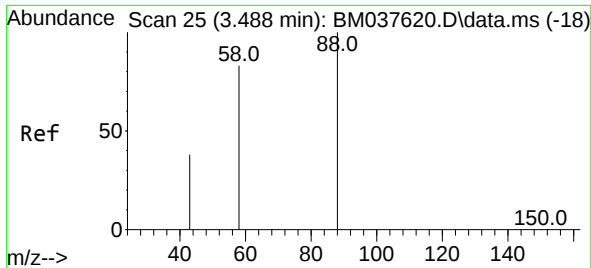

#2
 1,4-Dioxane
 Concen: 0.228 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM037624.D
 Acq: 21 Nov 2022 23:34

Instrument :
 BNA_M
 ClientSampleId :
 BGCG6

Tgt Ion: 88 Resp: 1760
 Ion Ratio Lower Upper
 88 100
 43 66.0 102.8 154.2#
 58 65.5 67.3 100.9#

