

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037657.D
 Acq On : 23 Nov 2022 00:25
 Operator : CG/JU
 Sample : N5593-09
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD8

Quant Time: Nov 23 01:27:22 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.125	152	7396	0.400	ng/ul	0.00
4) Naphthalene-d8	10.946	136	22284	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.746	164	12878	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.478	188	28217	0.400	ng/ul	0.00
17) Chrysene-d12	21.634	240	21867	0.400	ng/ul	# 0.00
23) Perylene-d12	24.119	264	23397	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.450	96	38181	4.440	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.519	152	10854	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.489	212	28294	0.392	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1325	0.148	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037657.D
Acq On : 23 Nov 2022 00:25
Operator : CG/JU
Sample : N5593-09
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD8


Quant Time: Nov 23 01:27:22 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

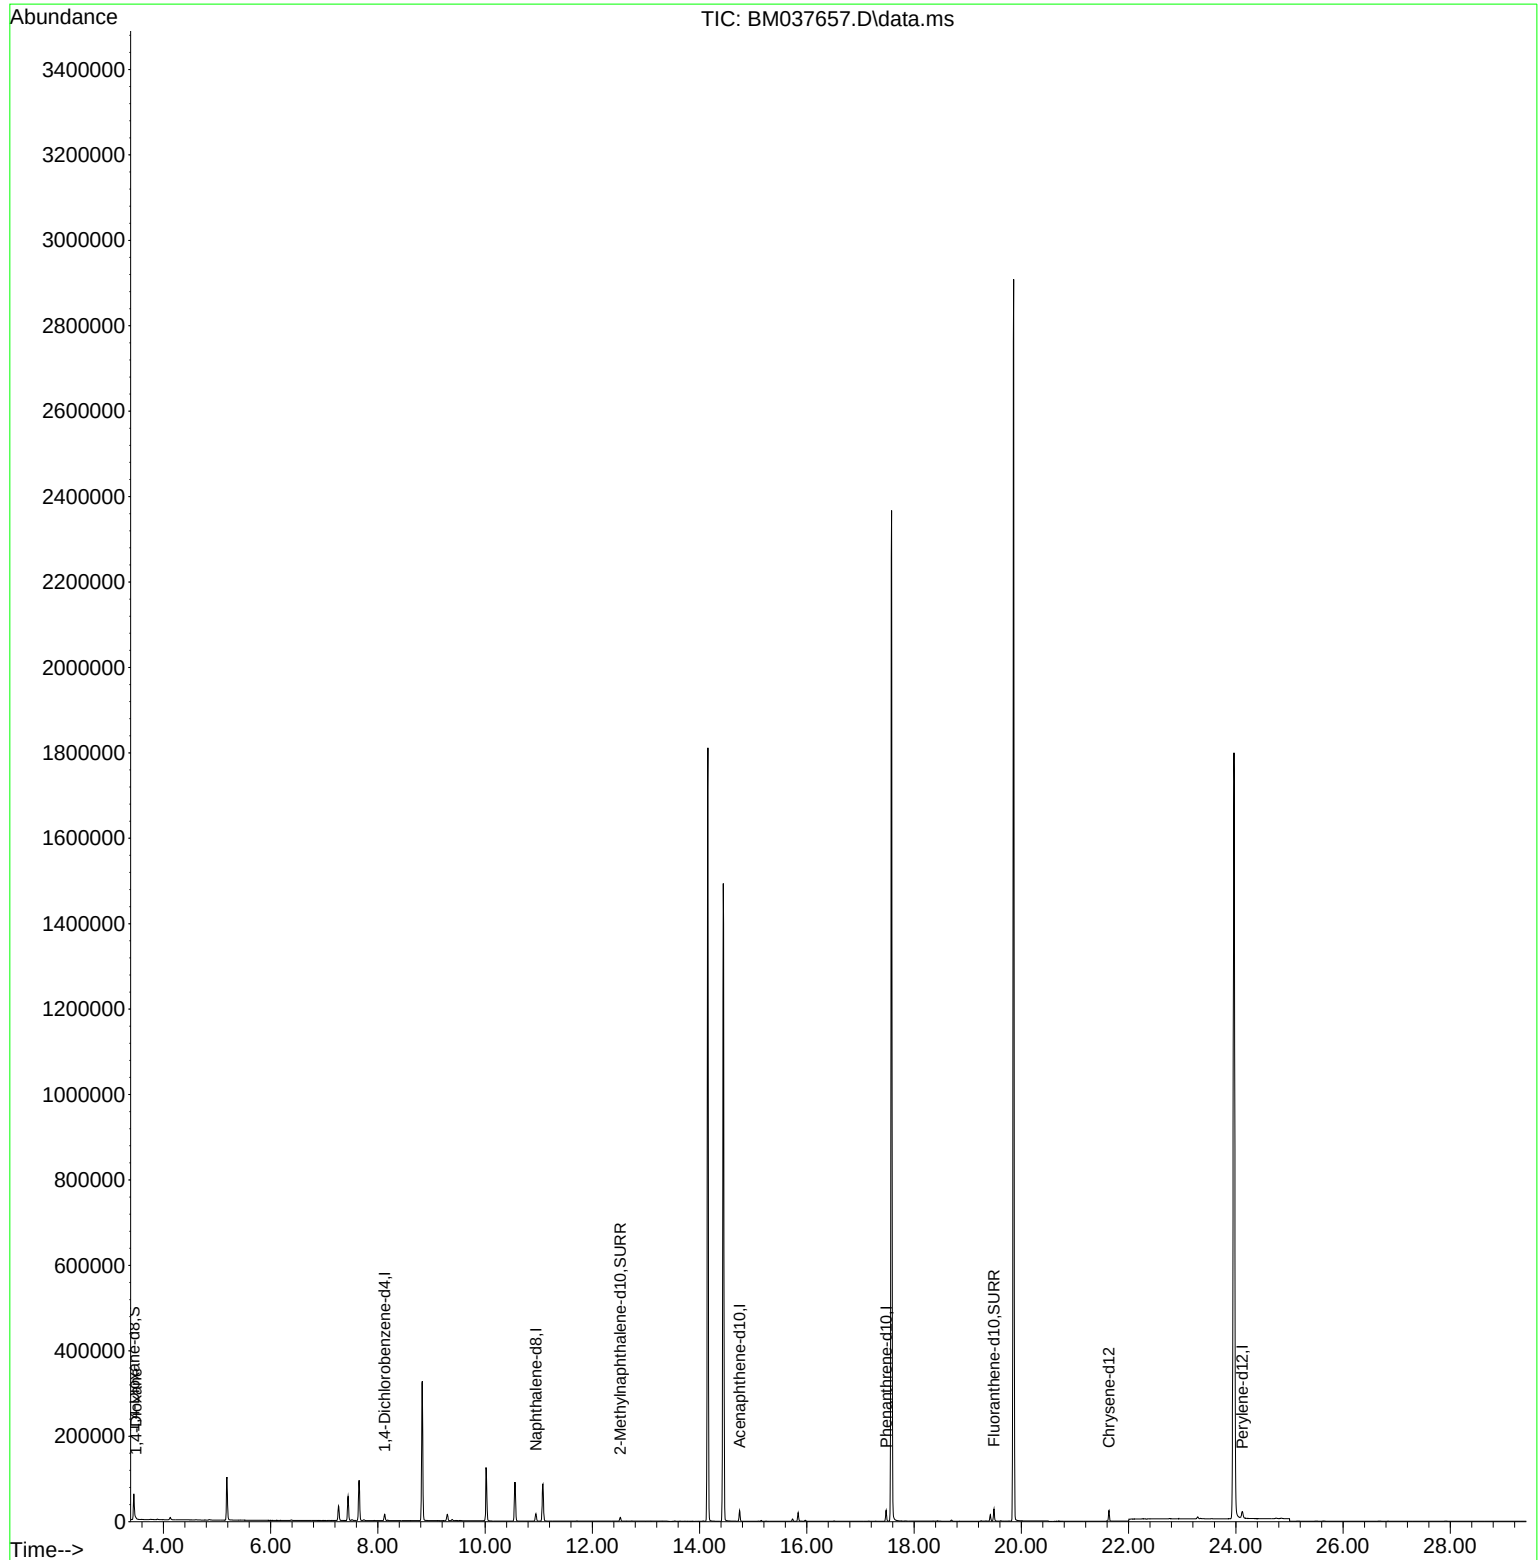

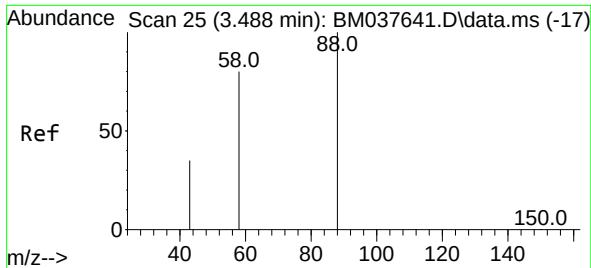

#2
 1,4-Dioxane
 Concen: 0.148 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM037657.D
 Acq: 23 Nov 2022 00:25

Instrument :
 BNA_M
 ClientSampleId :
 H0AD8

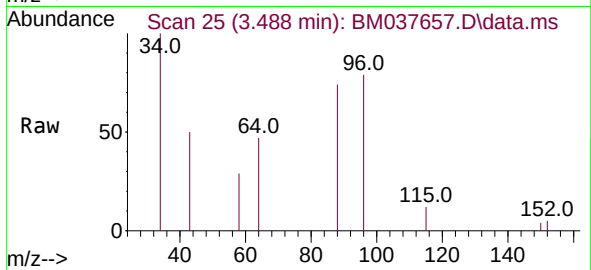

Tgt Ion: 88 Resp: 1325

Ion	Ratio	Lower	Upper
88	100		
43	66.8	102.8	154.2#
58	38.8	67.3	100.9#

