

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037661.D
 Acq On : 23 Nov 2022 03:27
 Operator : CG/JU
 Sample : N5593-10
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD9

Quant Time: Nov 23 04:25:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.125	152	7242	0.400	ng/ul	0.00
4) Naphthalene-d8	10.942	136	21325	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.743	164	12543	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.475	188	28022	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.636	240	21389	0.400	ng/ul	# 0.00
23) Perylene-d12	24.124	264	22748	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	31285	3.716	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.520	152	11311	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.490	212	28599	0.405	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.484	88	37854	4.320	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037661.D
Acq On : 23 Nov 2022 03:27
Operator : CG/JU
Sample : N5593-10
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD9


Quant Time: Nov 23 04:25:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

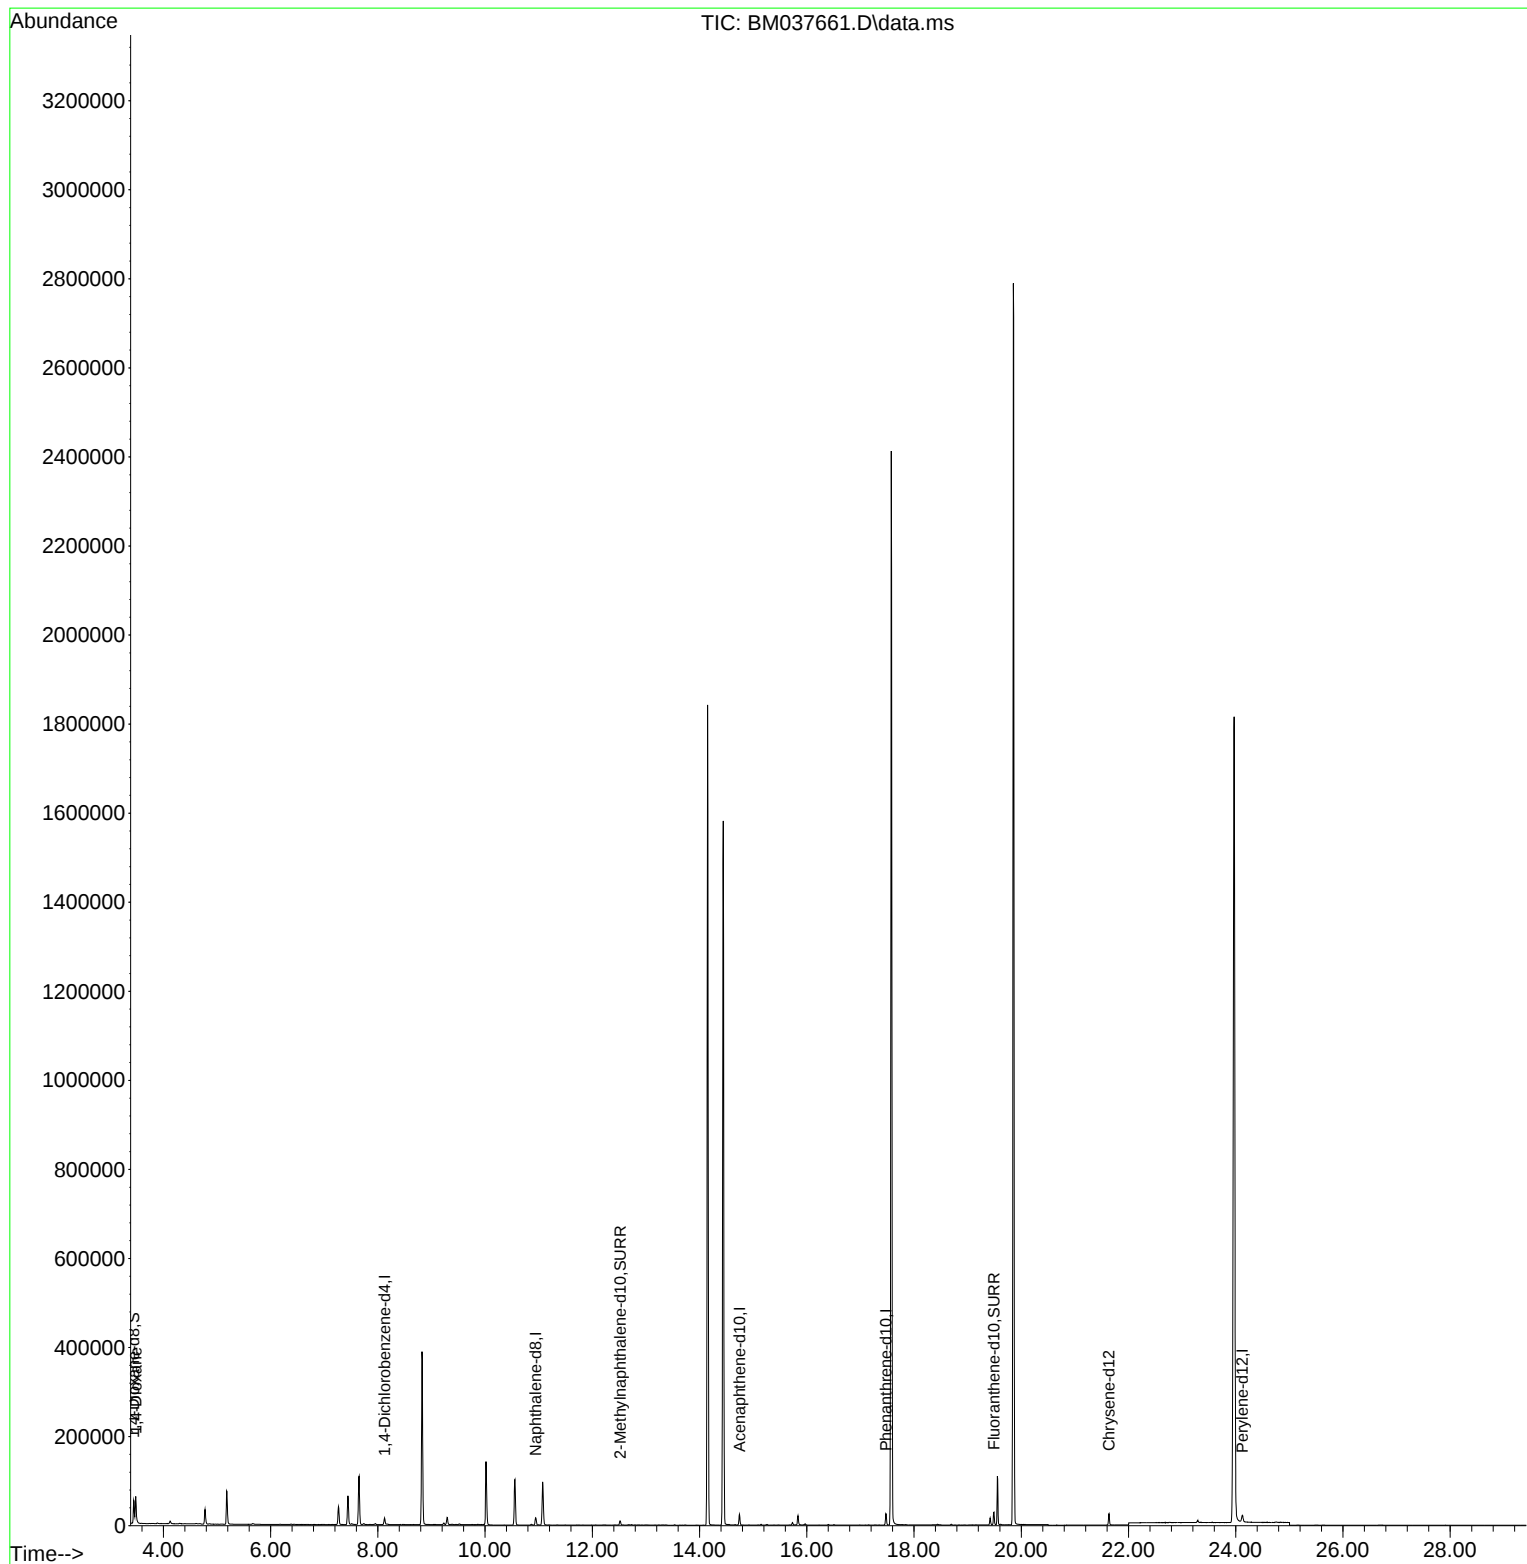

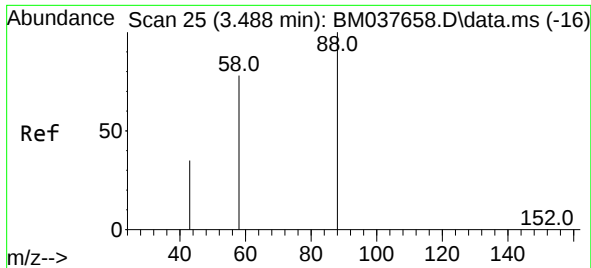

#2
 1,4-Dioxane
 Concen: 4.320 ng/ul
 RT: 3.484 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BM037661.D
 Acq: 23 Nov 2022 03:27

Instrument :
 BNA_M
 ClientSampleId :
 H0AD9

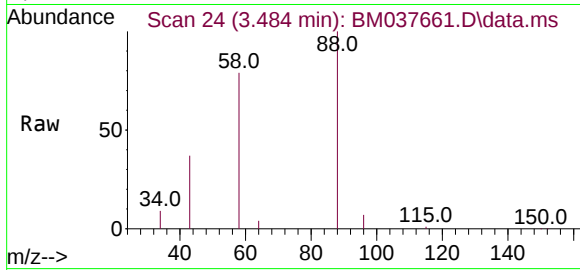

Tgt Ion: 88 Resp: 37854
 Ion Ratio Lower Upper
 88 100
 43 37.4 102.8 154.2#
 58 78.5 67.3 100.9

