

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037662.D
 Acq On : 23 Nov 2022 04:03
 Operator : CG/JU
 Sample : N5593-11
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AE0

Quant Time: Nov 23 05:26:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.125	152	7521	0.400	ng/ul	0.00
4) Naphthalene-d8	10.942	136	22508	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.743	164	13394	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.475	188	28954	0.400	ng/ul	0.00
17) Chrysene-d12	21.636	240	20295	0.400	ng/ul	# 0.00
23) Perylene-d12	24.121	264	20779	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	46644	5.334	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.520	152	12779	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.490	212	28711	0.428	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.484	88	38230	4.201	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037662.D
Acq On : 23 Nov 2022 04:03
Operator : CG/JU
Sample : N5593-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AE0


Quant Time: Nov 23 05:26:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

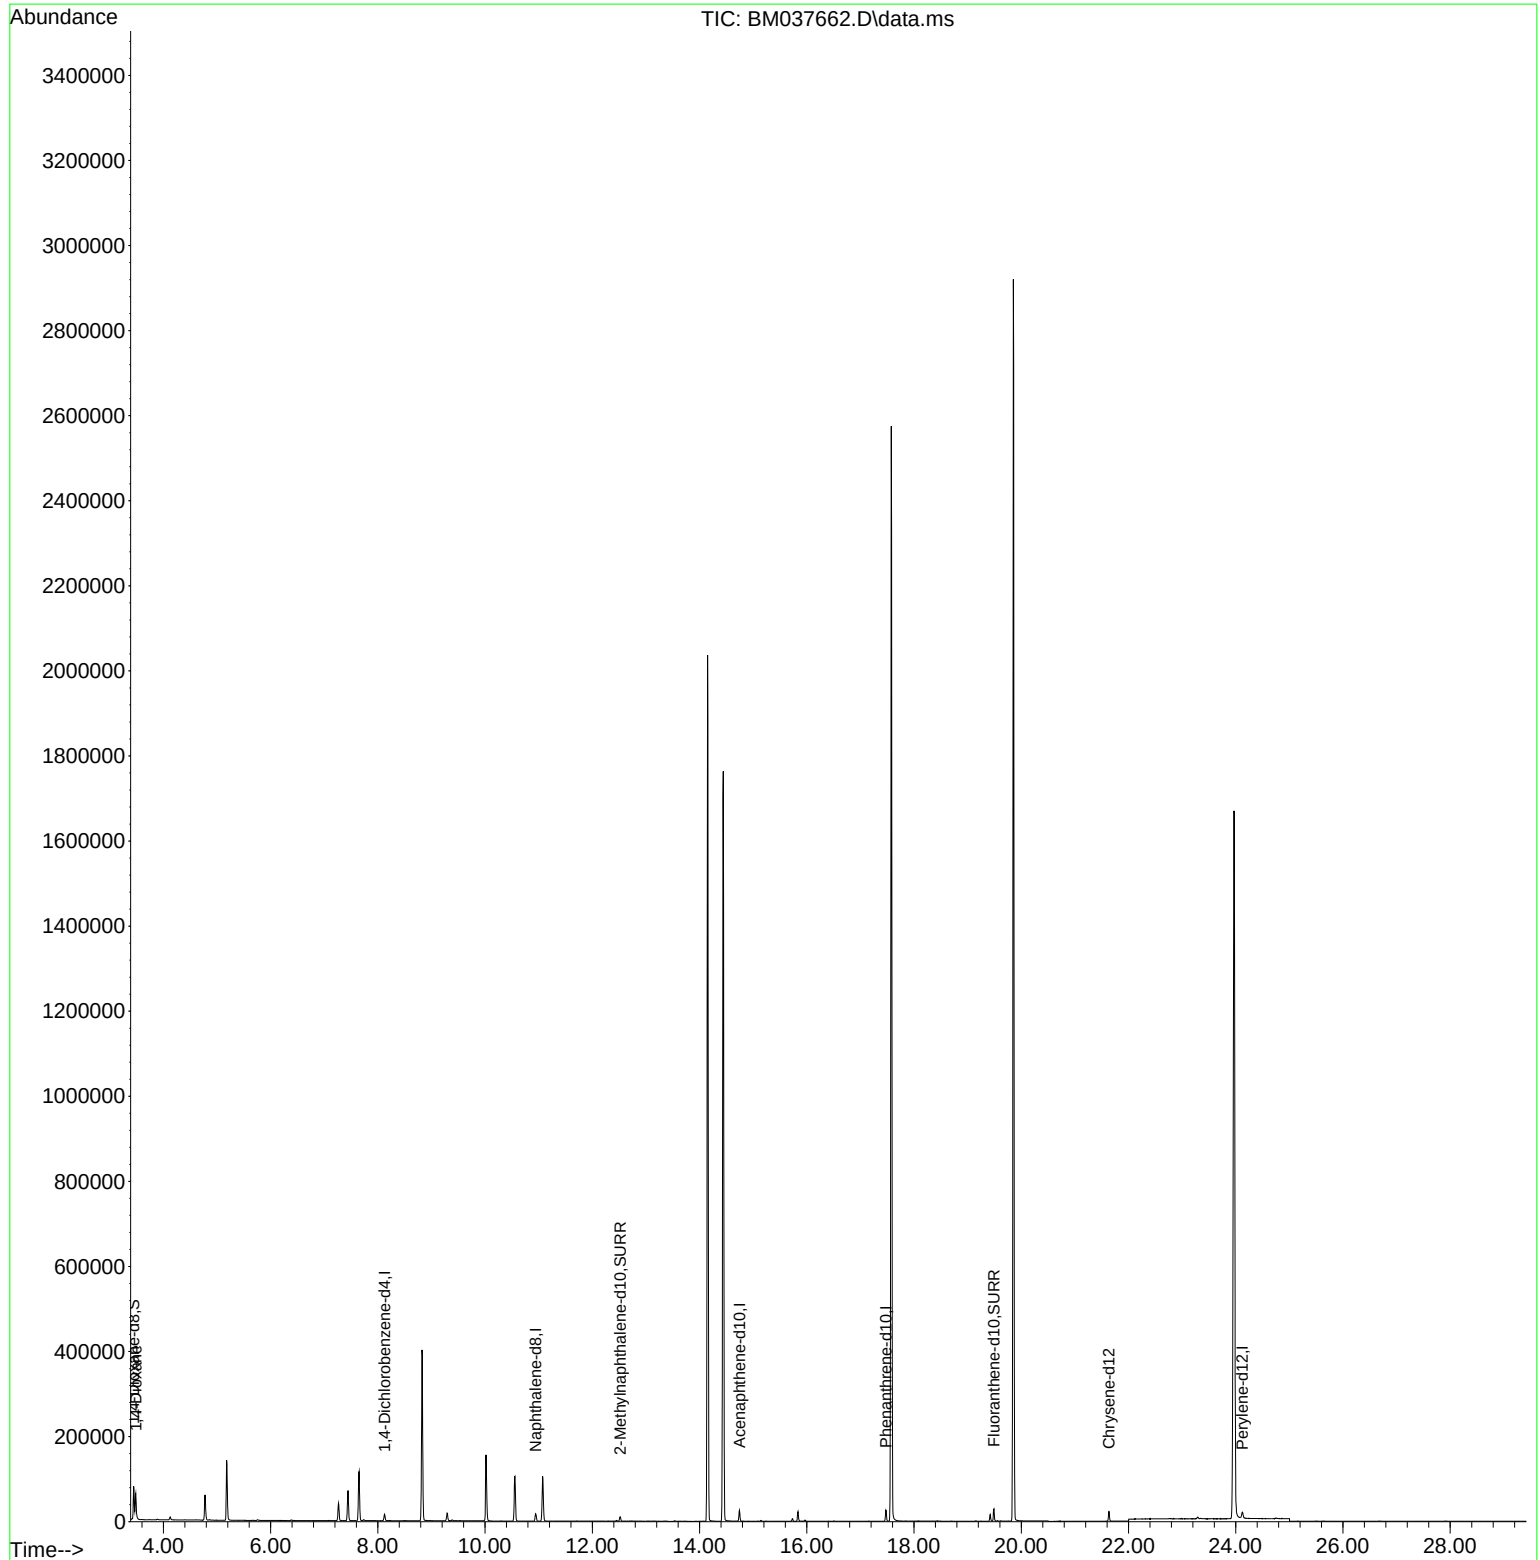

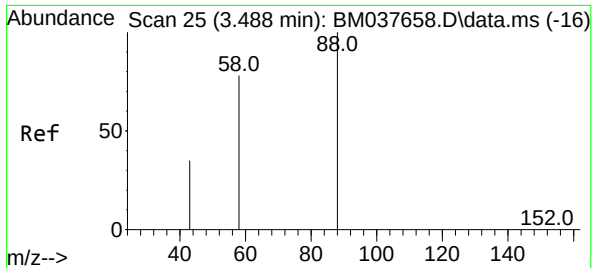

#2
 1,4-Dioxane
 Concen: 4.201 ng/ul
 RT: 3.484 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BM037662.D
 Acq: 23 Nov 2022 04:03

Instrument :
 BNA_M
 ClientSampleId :
 H0AE0

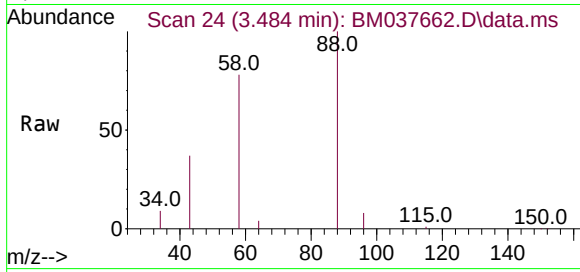

Tgt Ion: 88 Resp: 38230
 Ion Ratio Lower Upper
 88 100
 43 36.5 102.8 154.2#
 58 78.2 67.3 100.9

