

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037663.D
 Acq On : 23 Nov 2022 04:39
 Operator : CG/JU
 Sample : N5593-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC9

Quant Time: Nov 23 05:27:07 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.125	152	7272	0.400	ng/ul	0.00
4) Naphthalene-d8	10.942	136	21824	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.743	164	12855	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.475	188	27930	0.400	ng/ul	0.00
17) Chrysene-d12	21.636	240	19655	0.400	ng/ul	# 0.00
23) Perylene-d12	24.124	264	20199	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	42995	5.085	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.520	152	11877	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.490	212	27451	0.423	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.488	88	1285	0.146	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037663.D
Acq On : 23 Nov 2022 04:39
Operator : CG/JU
Sample : N5593-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AC9

Quant Time: Nov 23 05:27:07 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

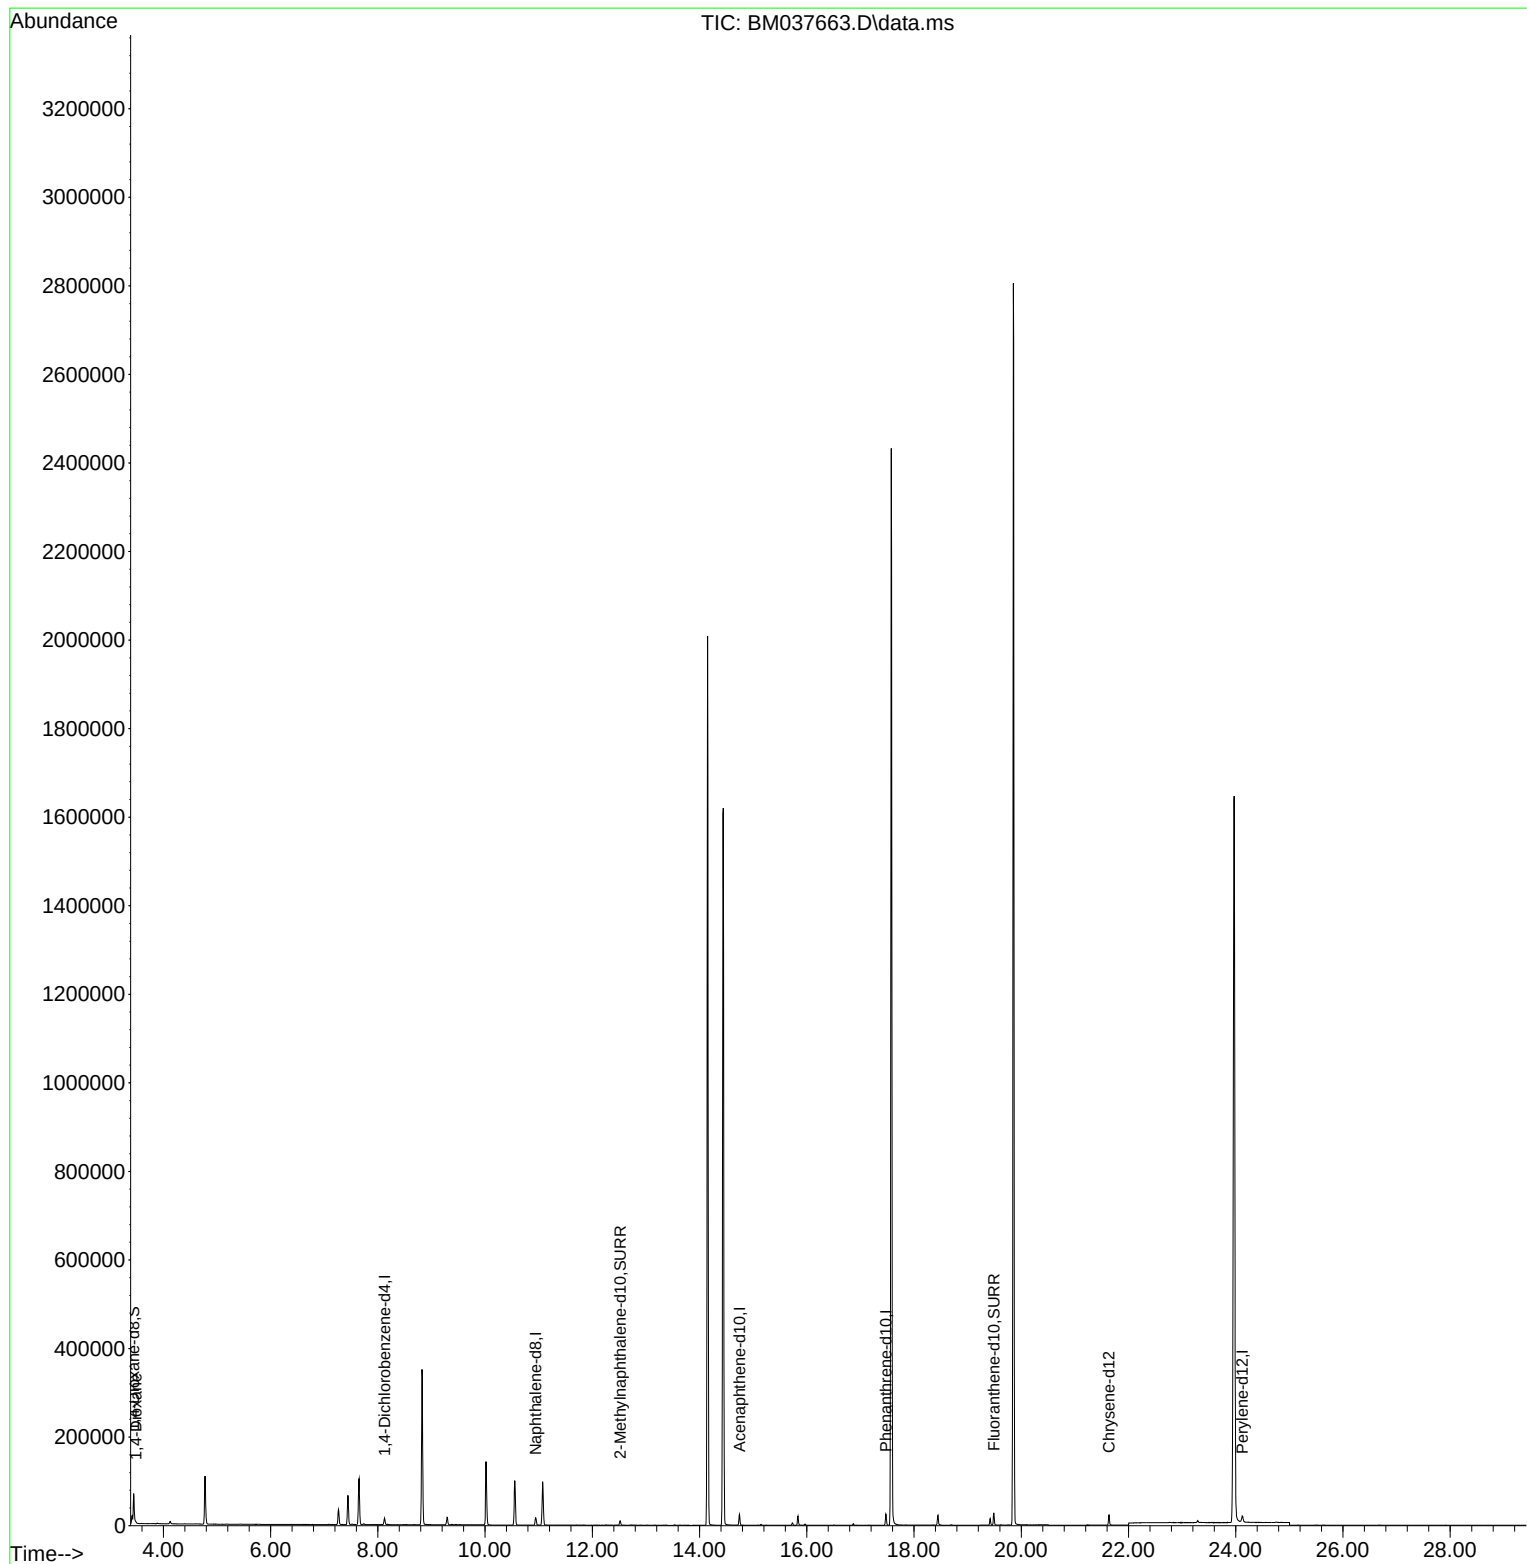

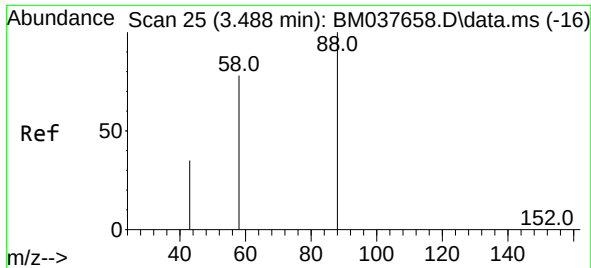

#2
 1,4-Dioxane
 Concen: 0.146 ng/ul
 RT: 3.488 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM037663.D
 Acq: 23 Nov 2022 04:39

Instrument :
 BNA_M
 ClientSampleId :
 H0AC9

Tgt Ion:	88	Resp:	1285
Ion	Ratio	Lower	Upper
88	100		
43	79.7	102.8	154.2#
58	58.8	67.3	100.9#

