

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
 Data File : BM037666.D
 Acq On : 23 Nov 2022 06:28
 Operator : CG/JU
 Sample : N5593-04
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD2

Quant Time: Nov 23 07:18:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 22:36:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.124	152	8444	0.400	ng/ul	0.00
4) Naphthalene-d8	10.946	136	26107	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.741	164	16057	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.477	188	33697	0.400	ng/ul	0.00
17) Chrysene-d12	21.637	240	23850	0.400	ng/ul	# 0.00
23) Perylene-d12	24.121	264	22564	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	47633	4.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.519	152	14092	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.489	212	33349	0.423	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.484	88	127674	12.495	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112122\
Data File : BM037666.D
Acq On : 23 Nov 2022 06:28
Operator : CG/JU
Sample : N5593-04
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD2

Quant Time: Nov 23 07:18:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 22:36:32 2022
Response via : Initial Calibration

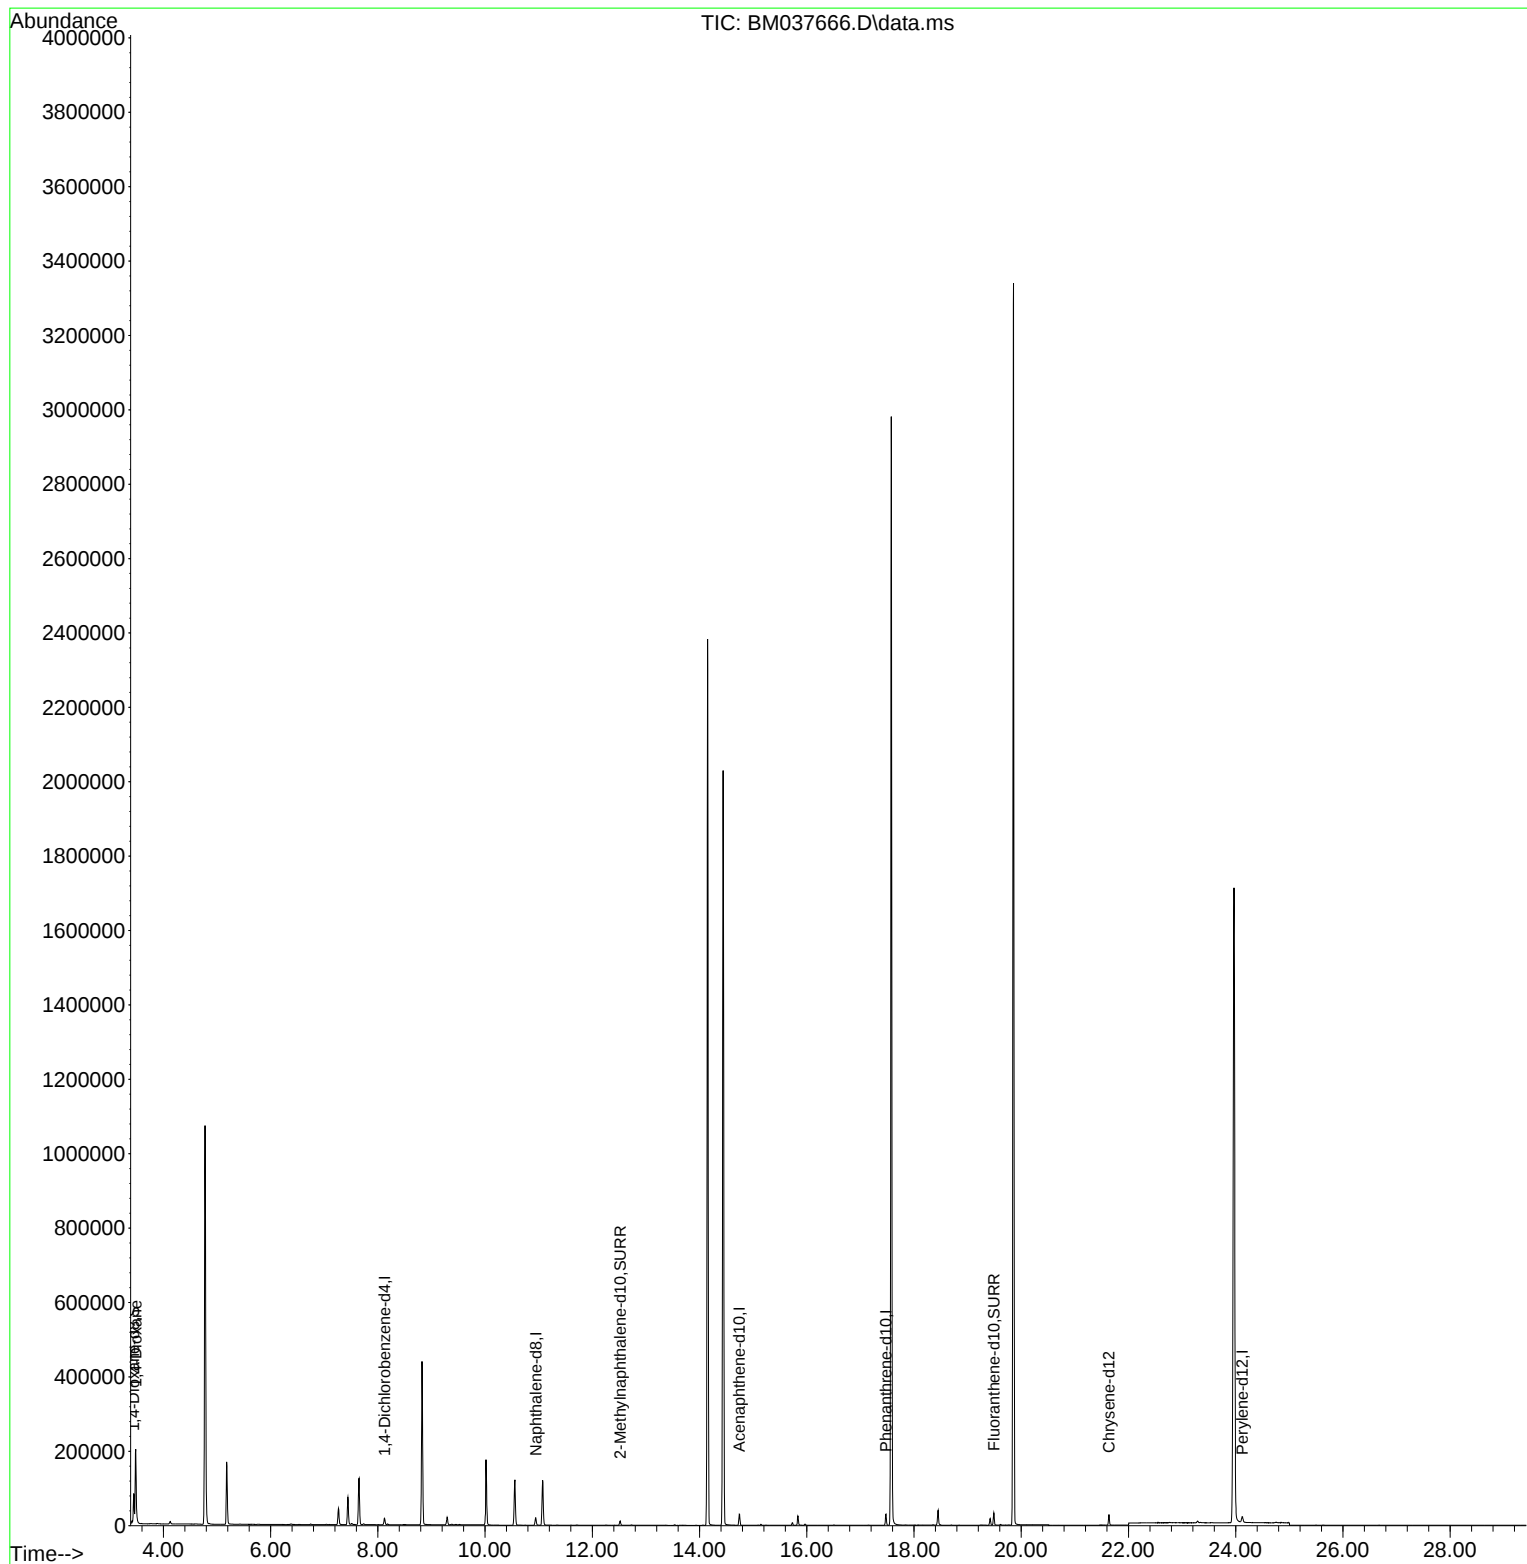

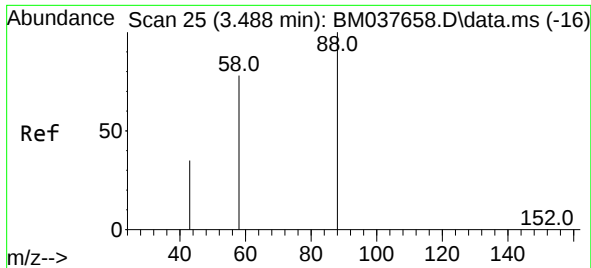

#2
 1,4-Dioxane
 Concen: 12.495 ng/ul
 RT: 3.484 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BM037666.D
 Acq: 23 Nov 2022 06:28

Instrument :
 BNA_M
 ClientSampleId :
 H0AD2

Tgt Ion:	88	Resp:	127674
Ion	Ratio	Lower	Upper
88	100		
43	34.8	102.8	154.2#
58	78.1	67.3	100.9

