
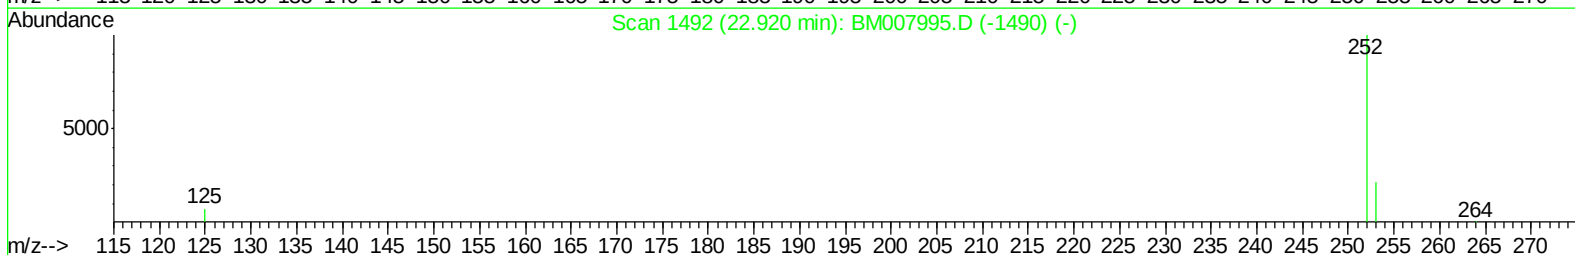
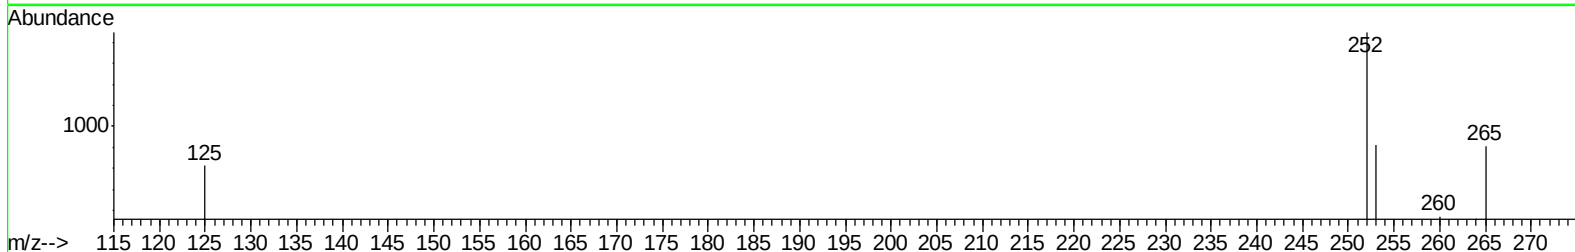


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM007999.D
Acq On : 22 Nov 2016 18:00
Operator : UM/SJ
Sample : H5695-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Nov 23 00:54:05 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 16:05:09 2016
Response via : Initial Calibration

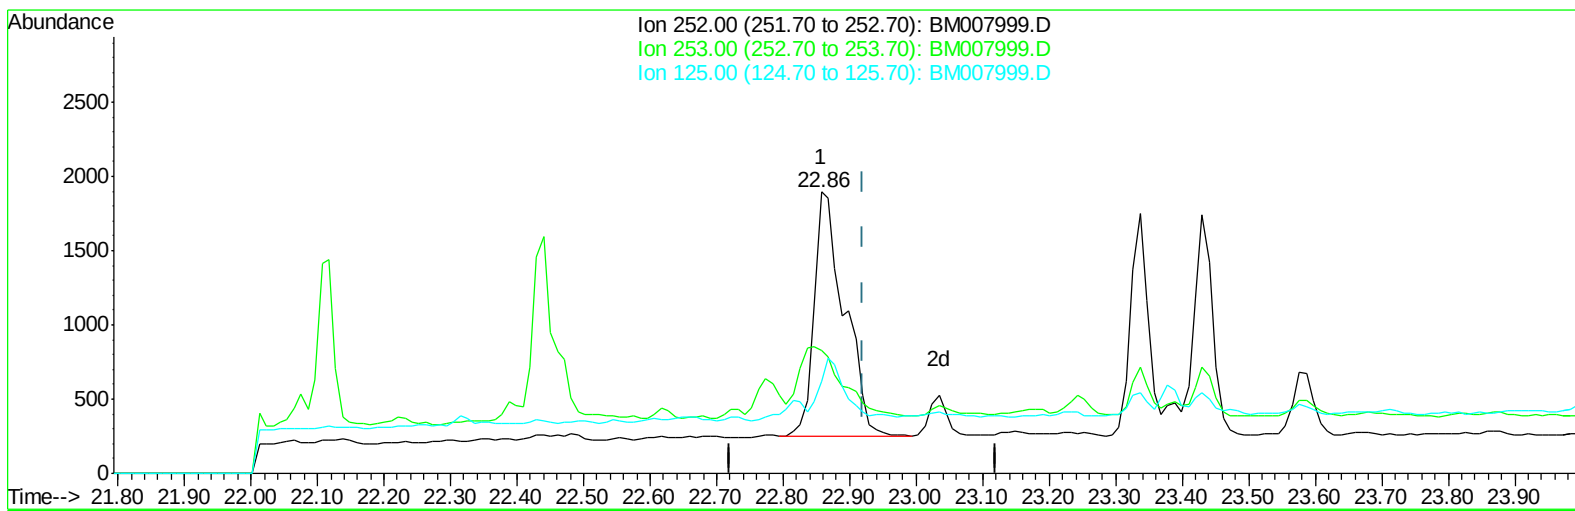

TIC: BM007999.D

(22) Benzo(k)fluoranthene

22.857min (-0.063) 0.45ng/ul

response 5261

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	43.72#
125.00	17.10	32.96#
0.00	0.00	0.00