
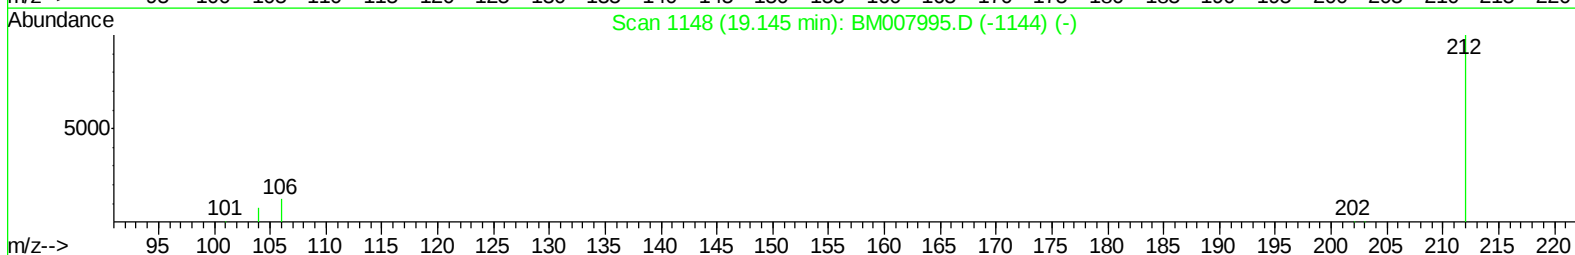
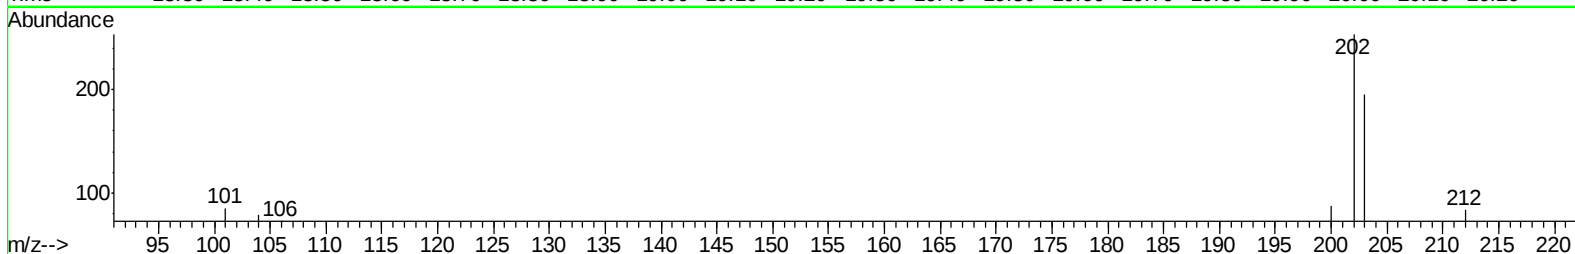


Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM112216\  
Data File : BM008001.D  
Acq On : 22 Nov 2016 19:11  
Operator : UM/SJ  
Sample : H5695-11  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 23 01:00:28 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM112116.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 22 16:05:09 2016  
Response via : Initial Calibration

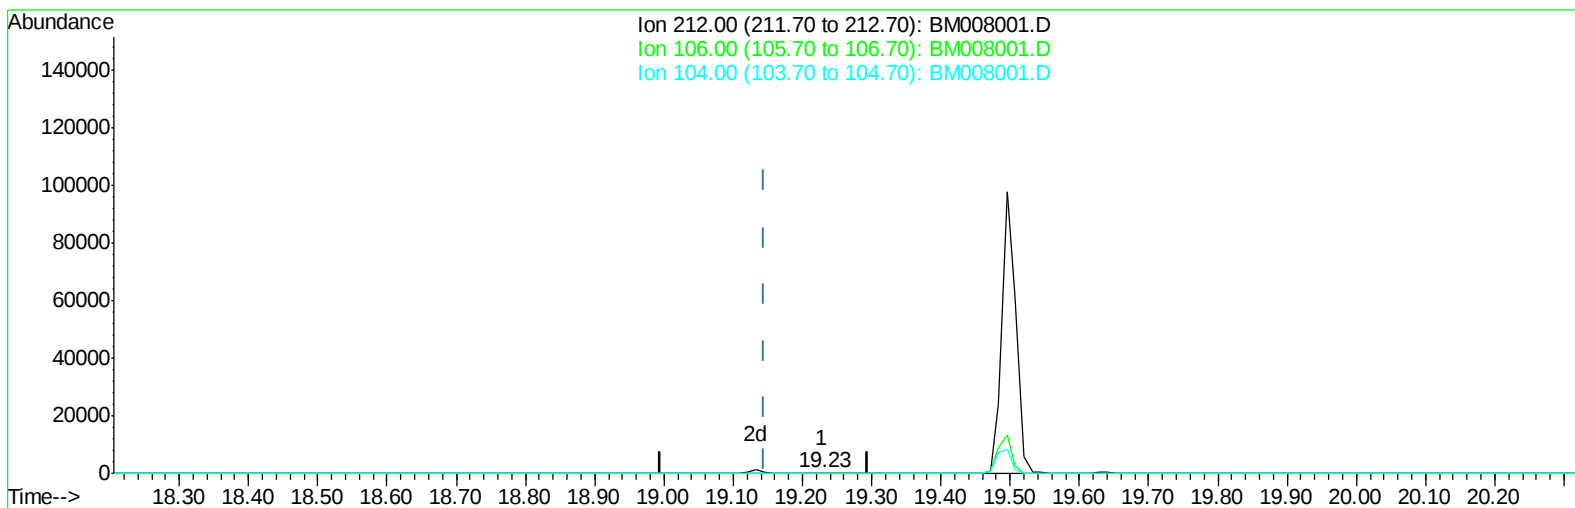

TIC: BM008001.D

(14) Fluoranthene-d10 (SURR)

19.229min (+0.084) 0.01ng/ul

response 60

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 100   |
| 106.00 | 18.30 | 0.00# |
| 104.00 | 15.60 | 0.00# |
| 0.00   | 0.00  | 0.00  |