
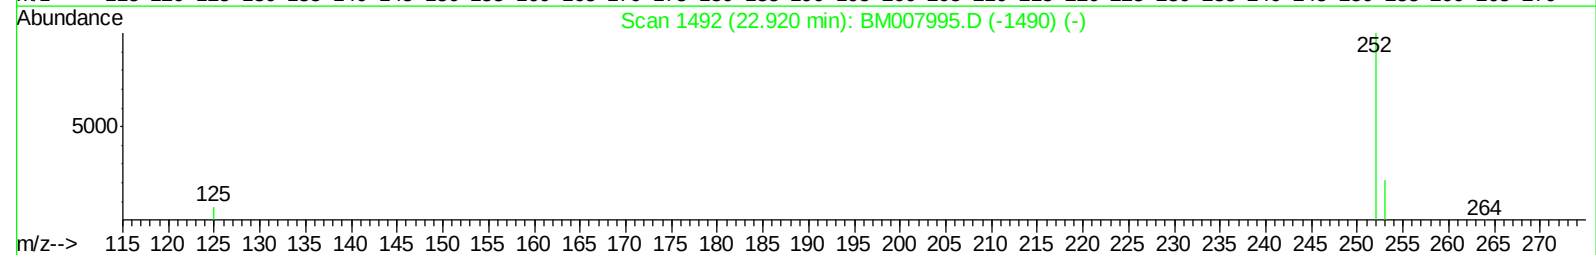
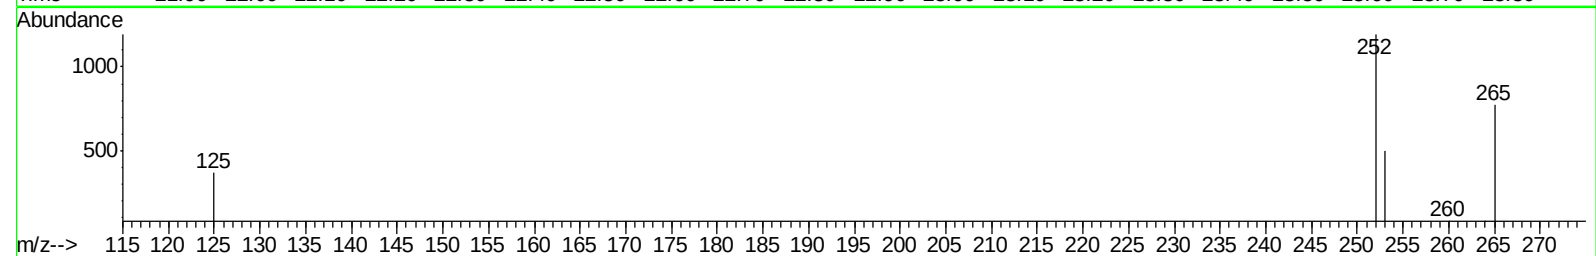


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM008002.D
Acq On : 22 Nov 2016 19:47
Operator : UM/SJ
Sample : H5695-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Nov 23 01:05:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 16:05:09 2016
Response via : Initial Calibration

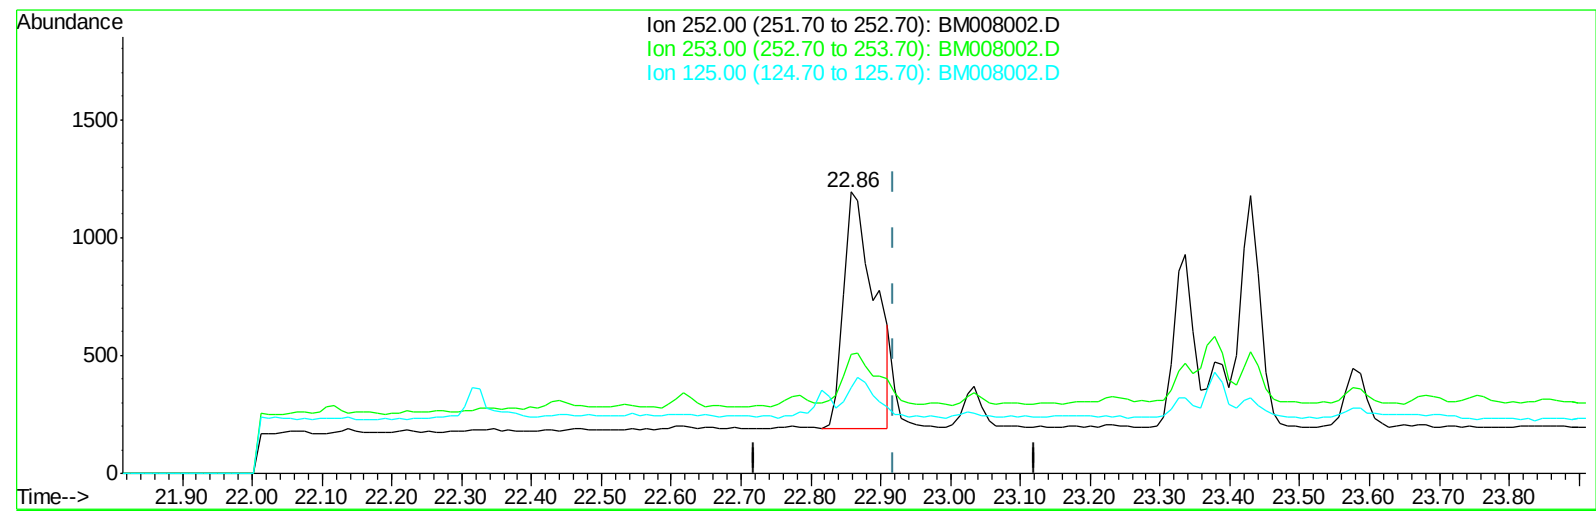

TIC: BM008002.D

(22) Benzo(k)fluoranthene
22.857min (-0.063) 0.30ng/ul
response 3103

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	42.13#
125.00	17.10	30.65#
0.00	0.00	0.00