
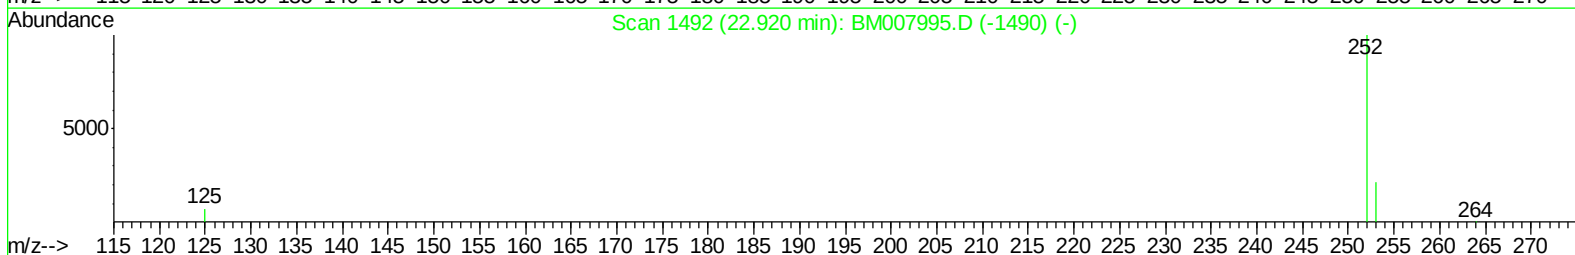
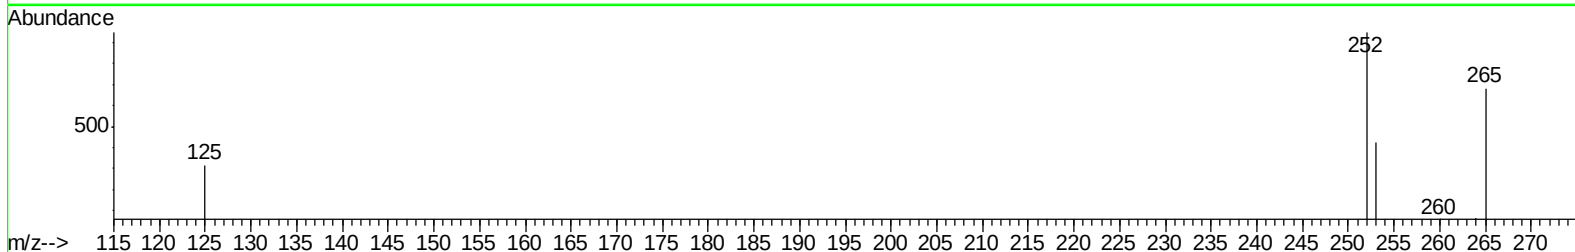


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM008008.D
Acq On : 22 Nov 2016 23:23
Operator : UM/SJ
Sample : H5694-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 23 01:21:41 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 16:05:09 2016
Response via : Initial Calibration

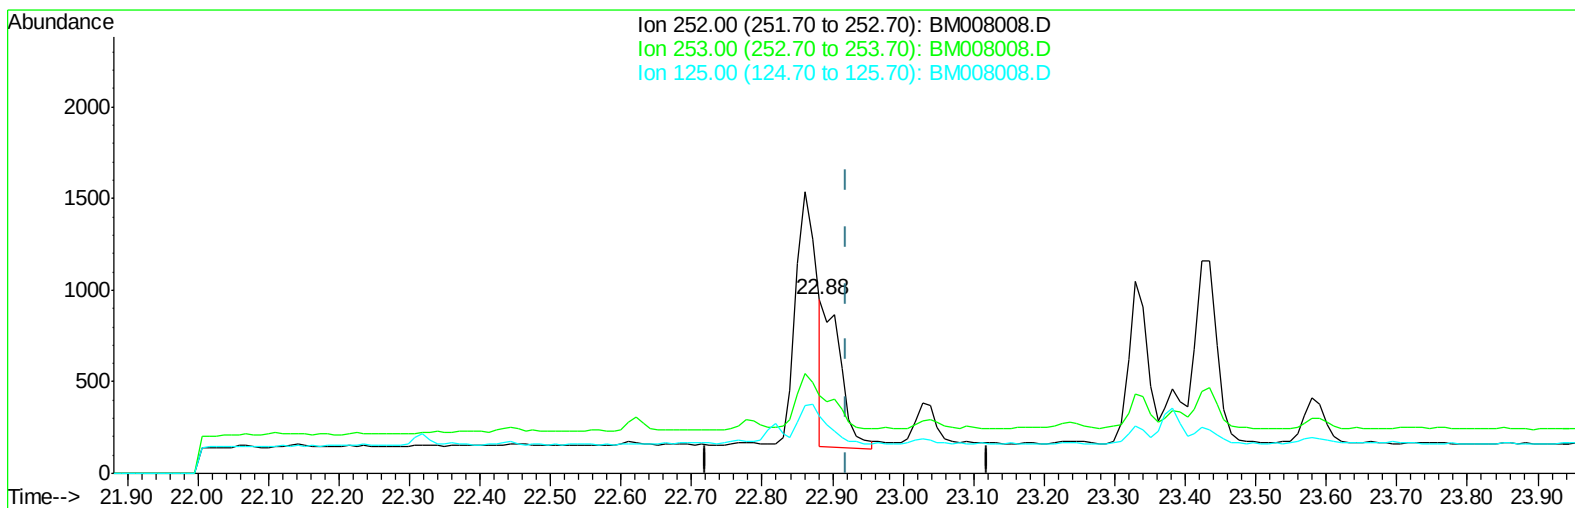

TIC: BM008008.D

(22) Benzo(k)fluoranthene

22.882min (-0.038) 0.15ng/ul m

response 1335

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	44.89#
125.00	17.10	33.19#
0.00	0.00	0.00