

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
 Data File : BM008004.D
 Acq On : 22 Nov 2016 20:59
 Operator : UM/SJ
 Sample : PB94816BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK16

Quant Time: Nov 23 00:49:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 22 16:05:09 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	652	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.50	136	2254	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1414	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.19	188	194378	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	2738	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	122945	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1002	0.31	ng/ul	-0.01
14) Fluoranthene-d10	19.13	212	2305	0.00	ng/ul	-0.01
Target Compounds						
9) Fluorene	15.34	166	387	0.07	ng/ul#	33
17) Pyrene	19.50	202	380	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM008004.D
Acq On : 22 Nov 2016 20:59
Operator : UM/SJ
Sample : PB94816BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK16

Quant Time: Nov 23 00:49:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 16:05:09 2016
Response via : Initial Calibration




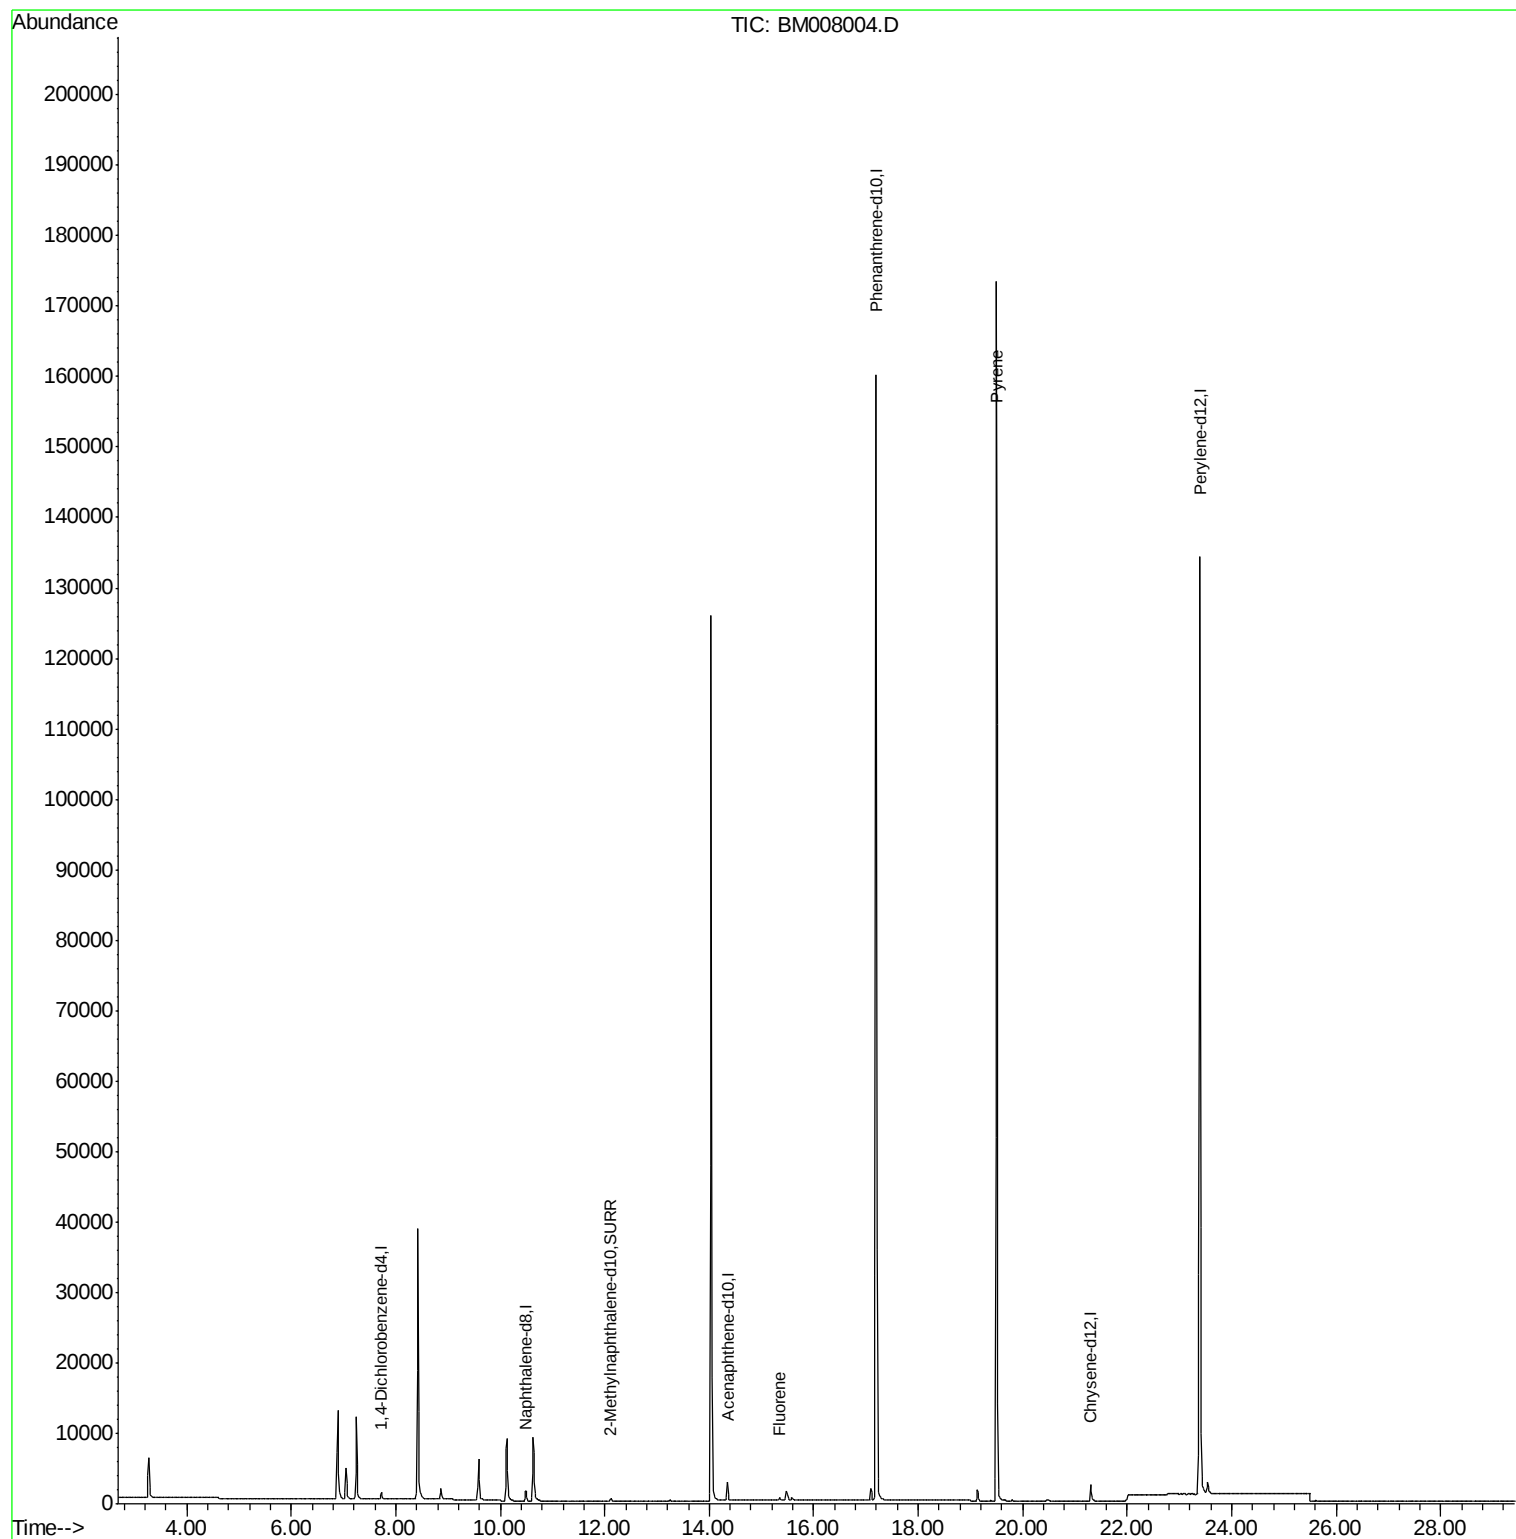


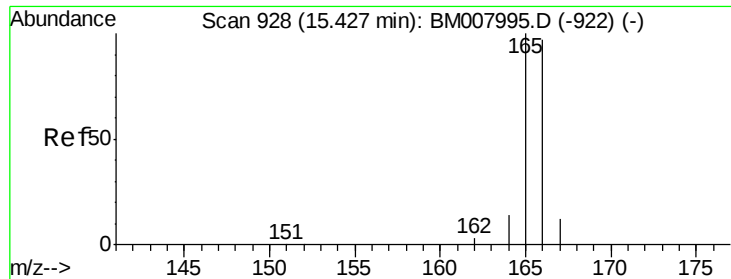

#9
Fluorene
 Concen: 0.07 ng/ul
 RT: 15.34 min Scan# 923
 Delta R.T. -0.09 min
 Lab File: BM008004.D
 Acq: 22 Nov 2016 20:59

Instrument :
 BNA_M
 ClientSampleId :
 SBLK16

Tgt Ion:166 Resp: 387
 Ion Ratio Lower Upper
 166 100
 165 23.3 73.4 110.2#
 167 38.0 14.6 22.0#

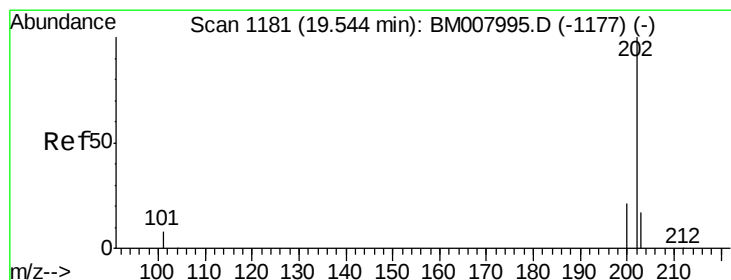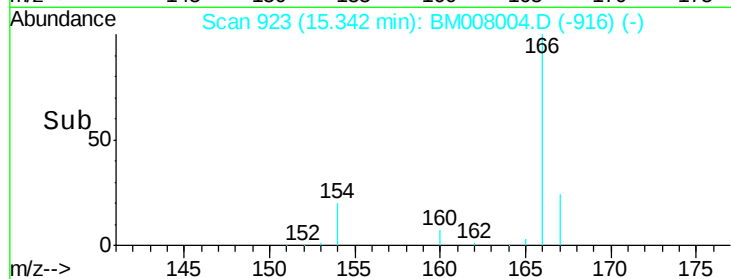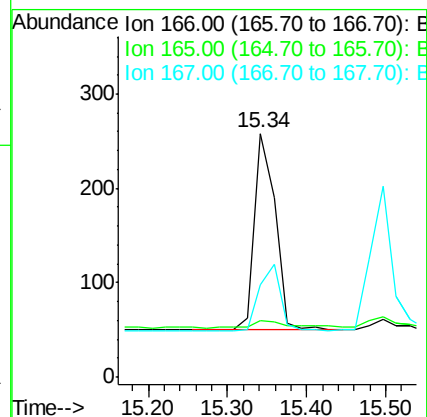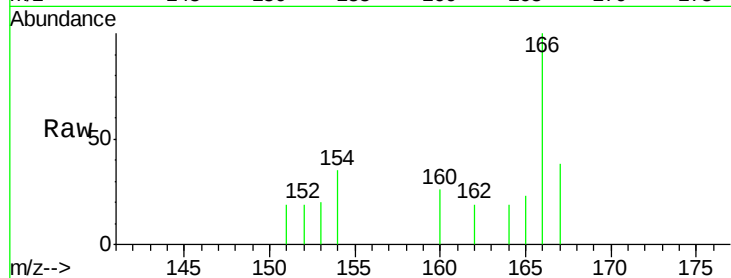

#17
Pyrene
 Concen: 0.04 ng/ul
 RT: 19.50 min Scan# 1177
 Delta R.T. -0.05 min
 Lab File: BM008004.D
 Acq: 22 Nov 2016 20:59

Tgt Ion:202 Resp: 380
 Ion Ratio Lower Upper
 202 100
 200 19.1 18.2 27.4
 203 146.9 15.6 23.4#

