

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
 Data File : BM008014.D
 Acq On : 23 Nov 2016 02:57
 Operator : UM/SJ
 Sample : H5699-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WC7

Quant Time: Nov 23 04:51:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 23 01:26:48 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	643	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	2158	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.35	164	1358	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	198156	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	2596	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	148433	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	957	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.14	212	2262	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.50	202	394	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM008014.D
Acq On : 23 Nov 2016 02:57
Operator : UM/SJ
Sample : H5699-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WC7

Quant Time: Nov 23 04:51:28 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:26:48 2016
Response via : Initial Calibration

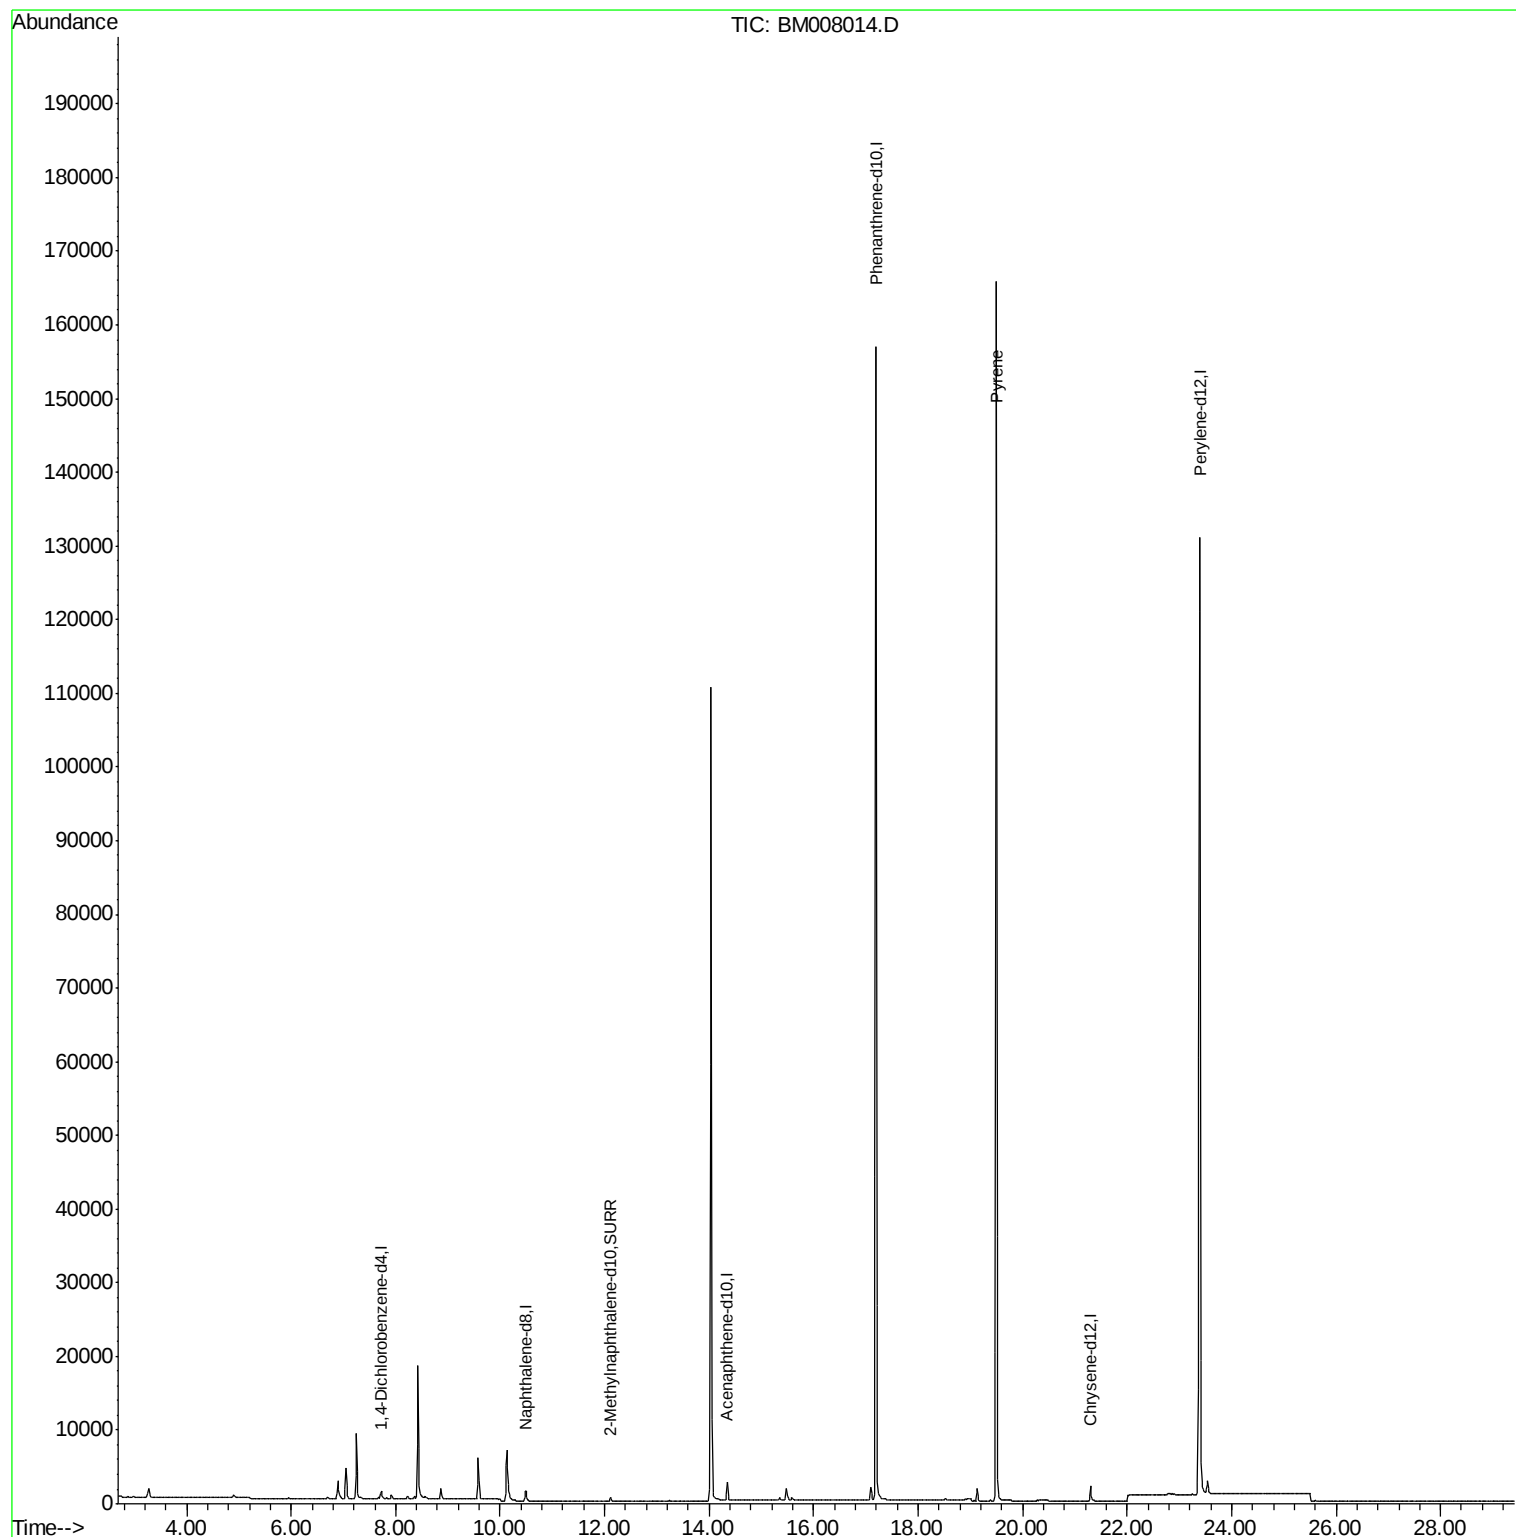

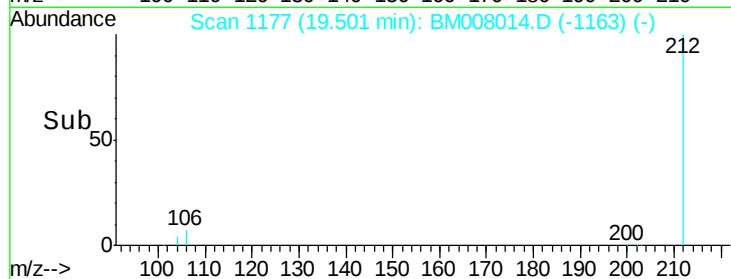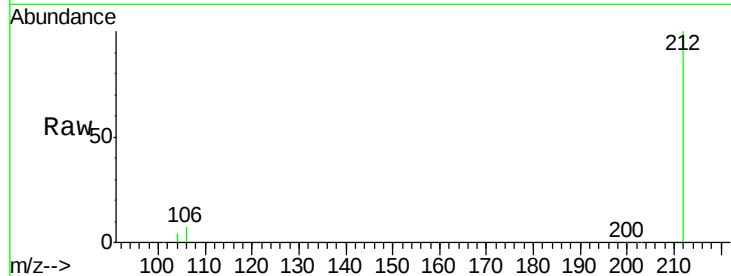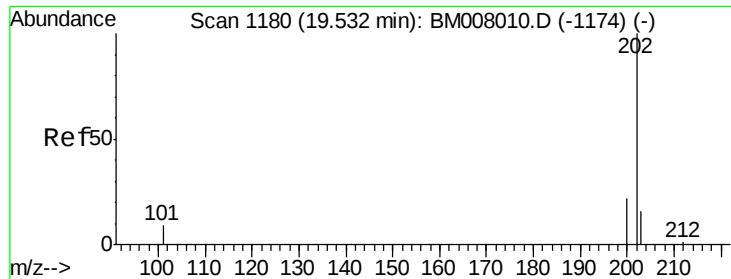

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.50 min Scan# 1177

Delta R.T. -0.03 min

Lab File: BM008014.D

Acq: 23 Nov 2016 02:57

Instrument :

BNA_M

ClientSampleId :

A4WC7

Tgt Ion: 202 Resp: 394

Ion Ratio Lower Upper

202 100

200 21.2 18.2 27.4

203 208.6 15.6 23.4#

