

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
 Data File : BM008015.D
 Acq On : 23 Nov 2016 03:32
 Operator : UM/SJ
 Sample : H5699-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WC9

Quant Time: Nov 23 04:51:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 23 01:26:48 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	697	0.40	ng/ul	0.00
2) Naphthalene-d8	10.49	136	2380	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1501	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	221500	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	2897	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	177913	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1087	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	2571	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.50	202	447	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM008015.D
Acq On : 23 Nov 2016 03:32
Operator : UM/SJ
Sample : H5699-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WC9

Quant Time: Nov 23 04:51:33 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:26:48 2016
Response via : Initial Calibration

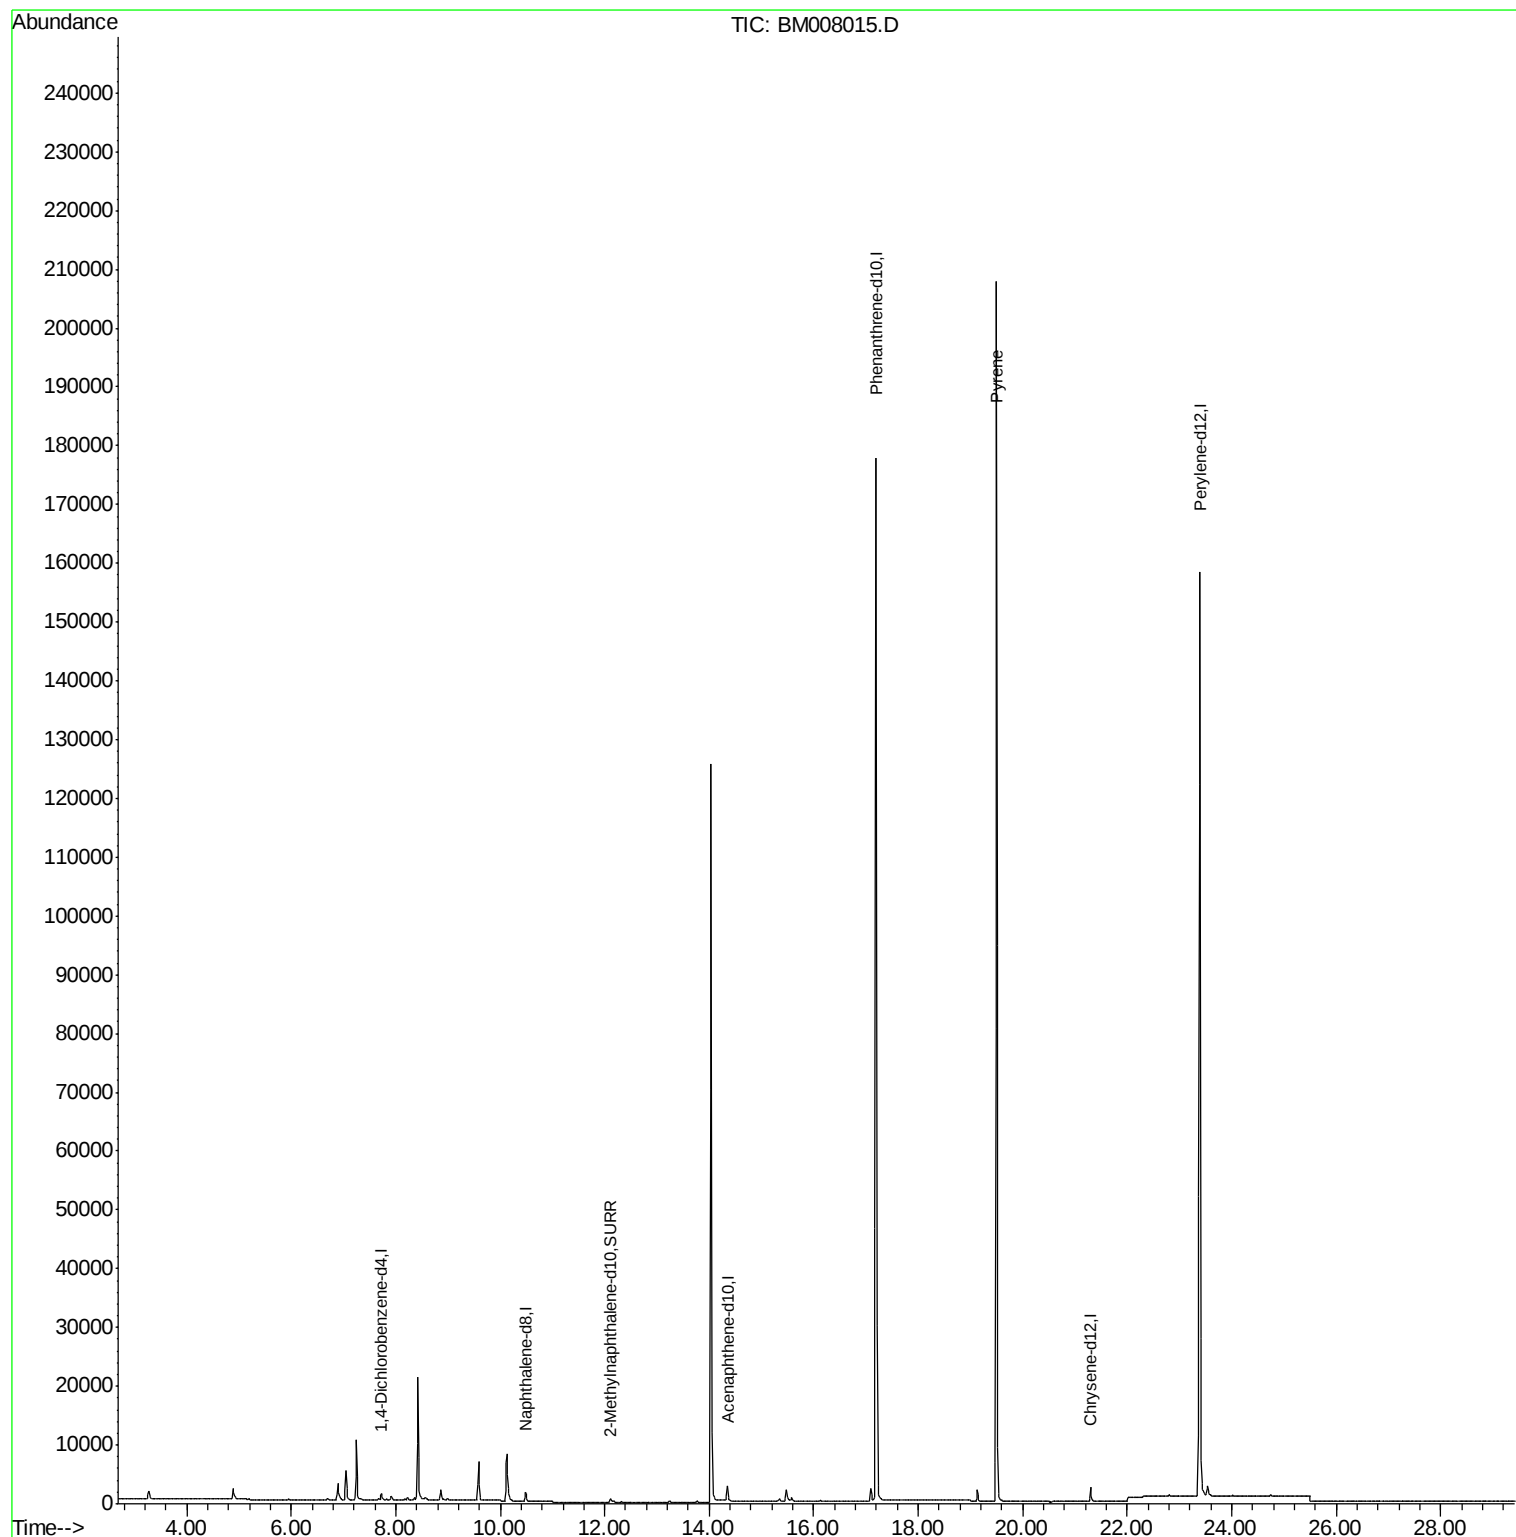

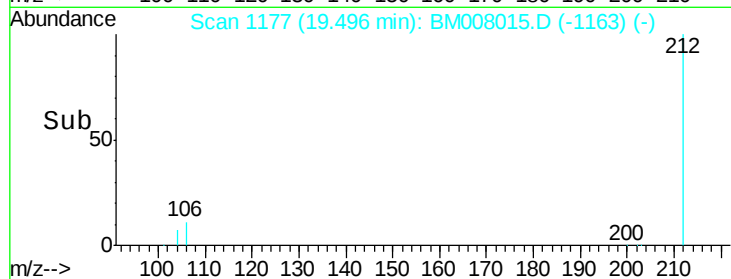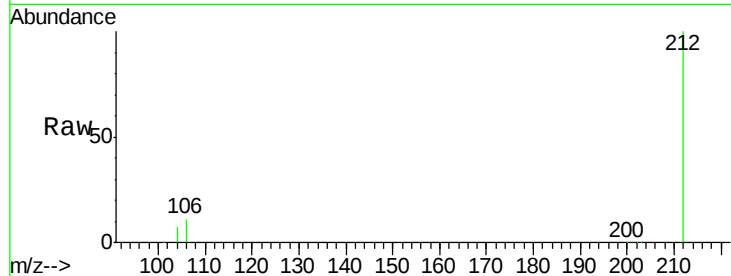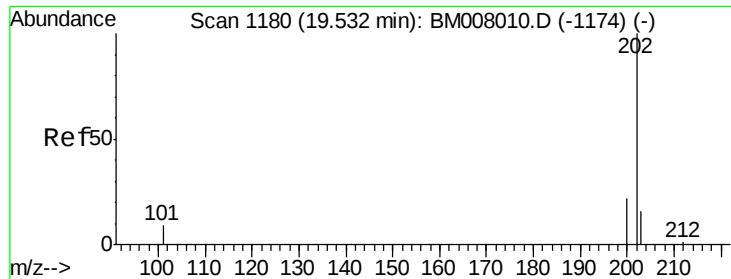

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.50 min Scan# 1177

Delta R.T. -0.04 min

Lab File: BM008015.D

Acq: 23 Nov 2016 03:32

Instrument :

BNA_M

ClientSampleId :

A4WC9

Tgt Ion: 202 Resp: 447

Ion Ratio Lower Upper

202 100

200 16.5 18.2 27.4#

203 170.7 15.6 23.4#

