

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112216\
 Data File : BM007994.D
 Acq On : 22 Nov 2016 14:57
 Operator : UM/SJ
 Sample : H5699-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WC9

Manual Integrations
 APPROVED

sohil
 11/23/2016 6:05:52 PM

Quant Time: Nov 22 15:55:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 22 15:01:04 2016
 Response via : Initial Calibration

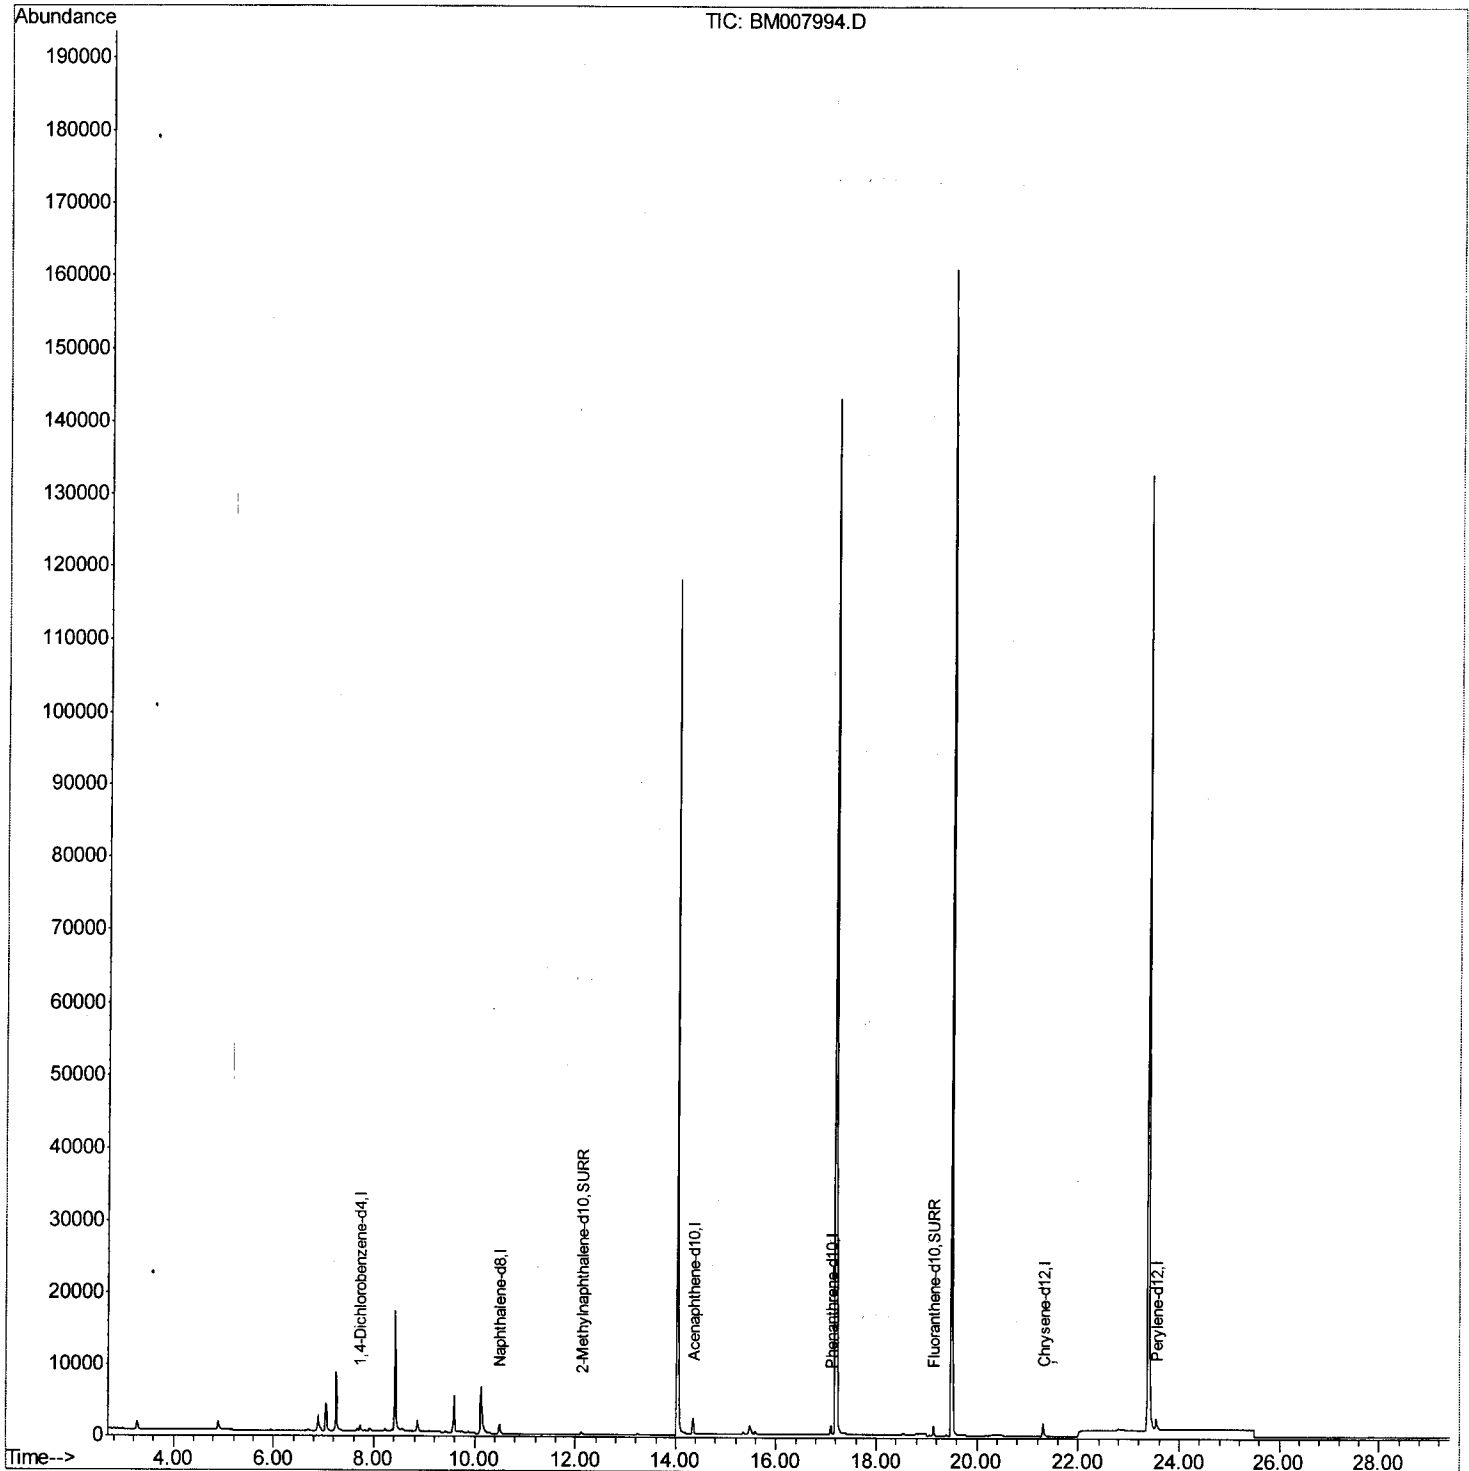

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112216\
 Data File : BM007994.D
 Acq On : 22 Nov 2016 14:57
 Operator : UM/SJ
 Sample : H5699-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 22 15:52:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 22 15:01:04 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WC9

Manual Integrations
 APPROVED

sohil
 11/23/2016 6:05:52 PM

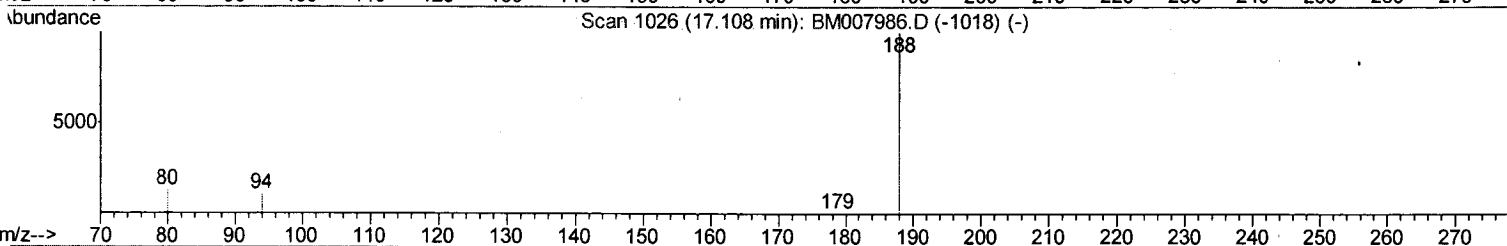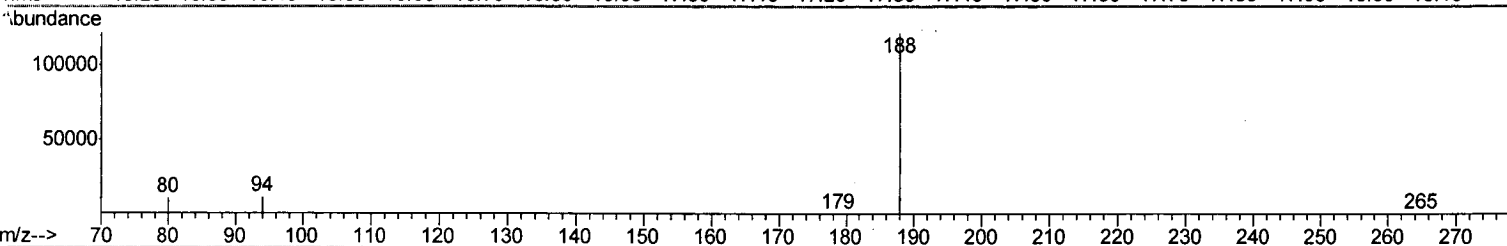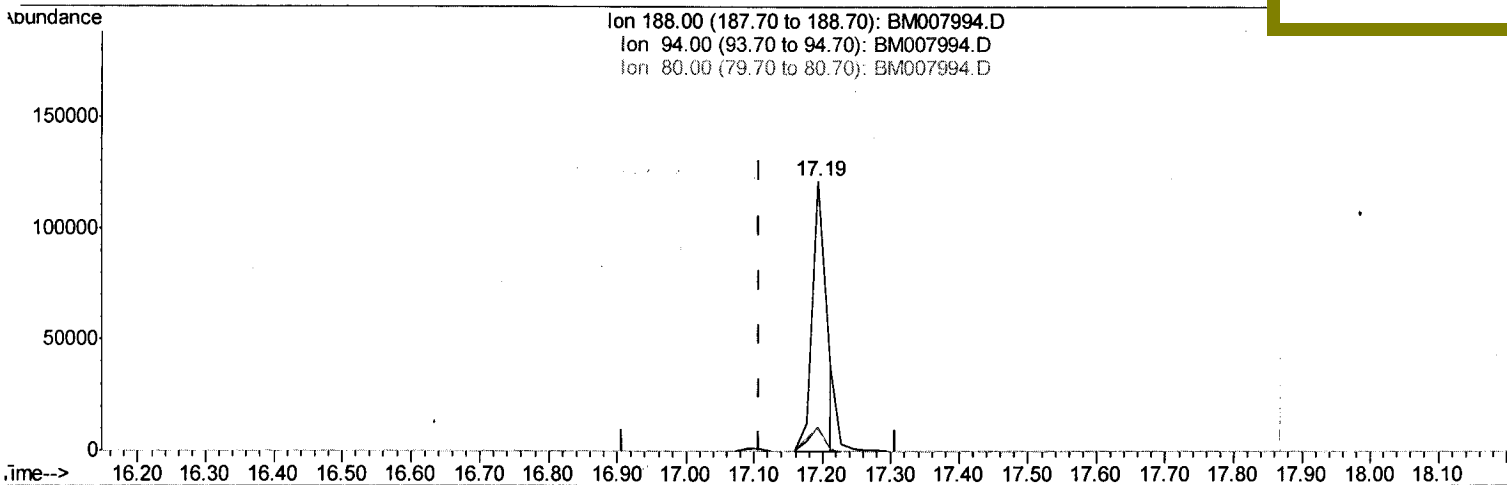

TIC: BM007994.D

(10) Phenanthrene-d10 (I)

17.193min (+0.085) 0.40ng/ul

response 178470

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.29
80.00	11.80	8.56#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112216\
 Data File : BM007994.D
 Acq On : 22 Nov 2016 14:57
 Operator : UM/SJ
 Sample : H5699-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WC9

Manual Integrations
 APPROVED

sohil
 11/23/2016 6:05:52 PM

Quant Time: Nov 22 15:52:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 22 15:01:04 2016
 Response via : Initial Calibration

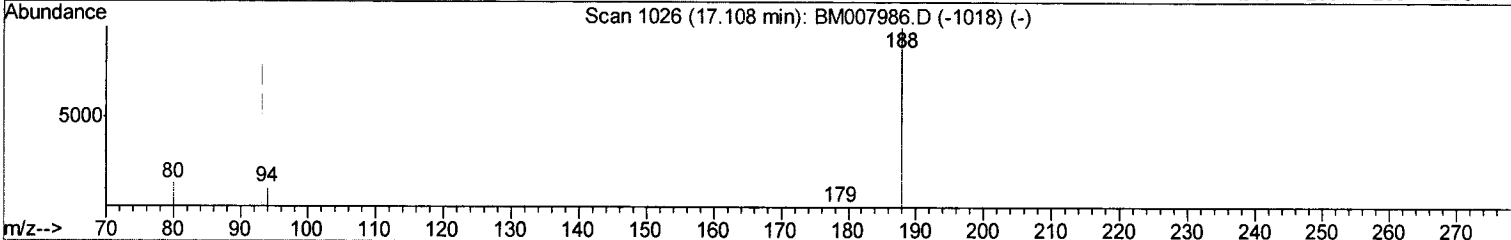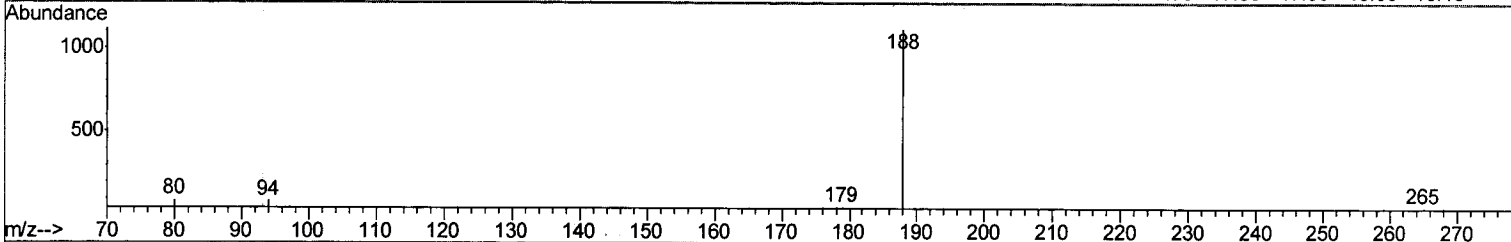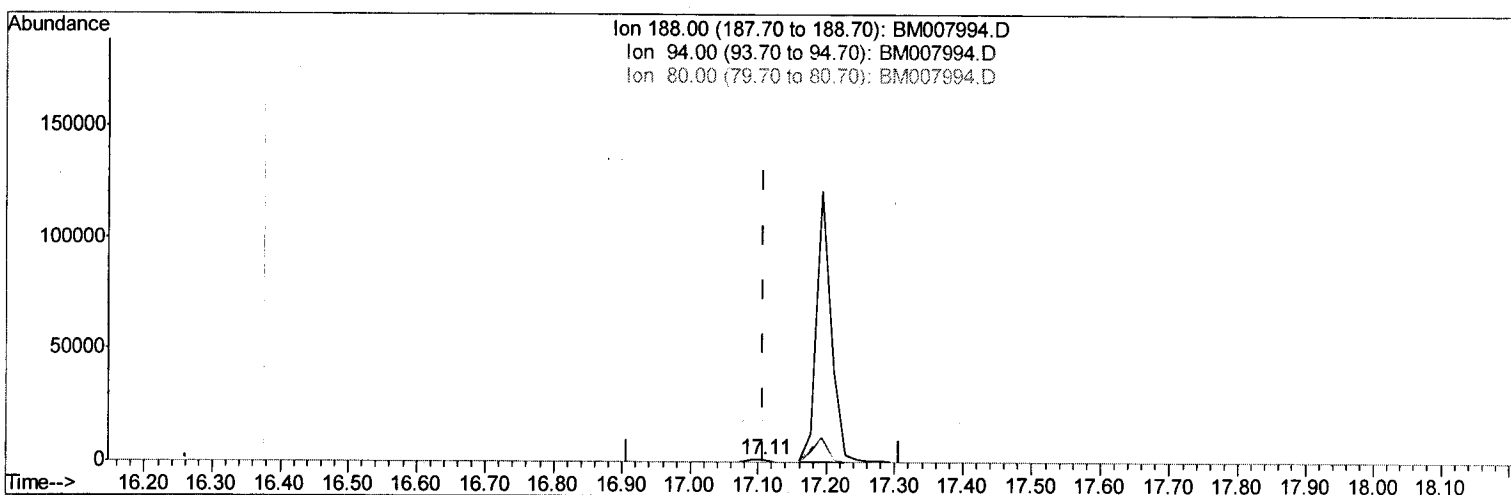

TIC: BM007994.D

(10) Phenanthrene-d10 (I)

17.107min (-0.000) 0.40ng/ul m

response 2471

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.14#
80.00	11.80	8.23#
0.00	0.00	0.00

SJ
 11/25/2016

Data Path : Z:\HPCHEM1\BNA_M\Data\BM112216\
Data File : BM007994.D
Acq On : 22 Nov 2016 14:57
Operator : UM/SJ
Sample : H5699-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WC9

Quant Time: Nov 22 15:55:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 15:01:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
11/23/2016 6:05:52 PM

Internal Standards	R.T.	QI	Ion	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152		581	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.50	136		1955	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164		1221	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.11	188		2471m	0.40	ng/ul	0.00
16) Chrysene-d12	21.31	240		2394	0.40	ng/ul	0.01
20) Perylene-d12	23.55	264		2675	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.12	152		904	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.14	212		2145	0.31	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ.
11/25/2016