

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
 Data File : BM007992.D
 Acq On : 22 Nov 2016 13:45
 Operator : UM/SJ
 Sample : H5622-21
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WL8

Manual Integrations
 APPROVED

sohil
 11/23/2016 6:05:57 PM

Quant Time: Nov 22 15:38:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 22 15:01:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	482	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.50	136	1647	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1073	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.11	188	2421m	0.40	ng/ul	0.00
16) Chrysene-d12	21.30	240	2677	0.40	ng/ul	0.00
20) Perylene-d12	23.54	264	2012m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.10	152	761	0.33	ng/ul	-0.02
14) Fluoranthene-d10	19.14	212	2240	0.33	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.42	153	325	0.09	ng/ul	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112216\
Data File : BM007992.D
Acq On : 22 Nov 2016 13:45
Operator : UM/SJ
Sample : H5622-21
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4WL8

Manual Integrations
APPROVED

sohil
11/23/2016 6:05:57 PM

Quant Time: Nov 22 15:38:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 15:01:04 2016
Response via : Initial Calibration

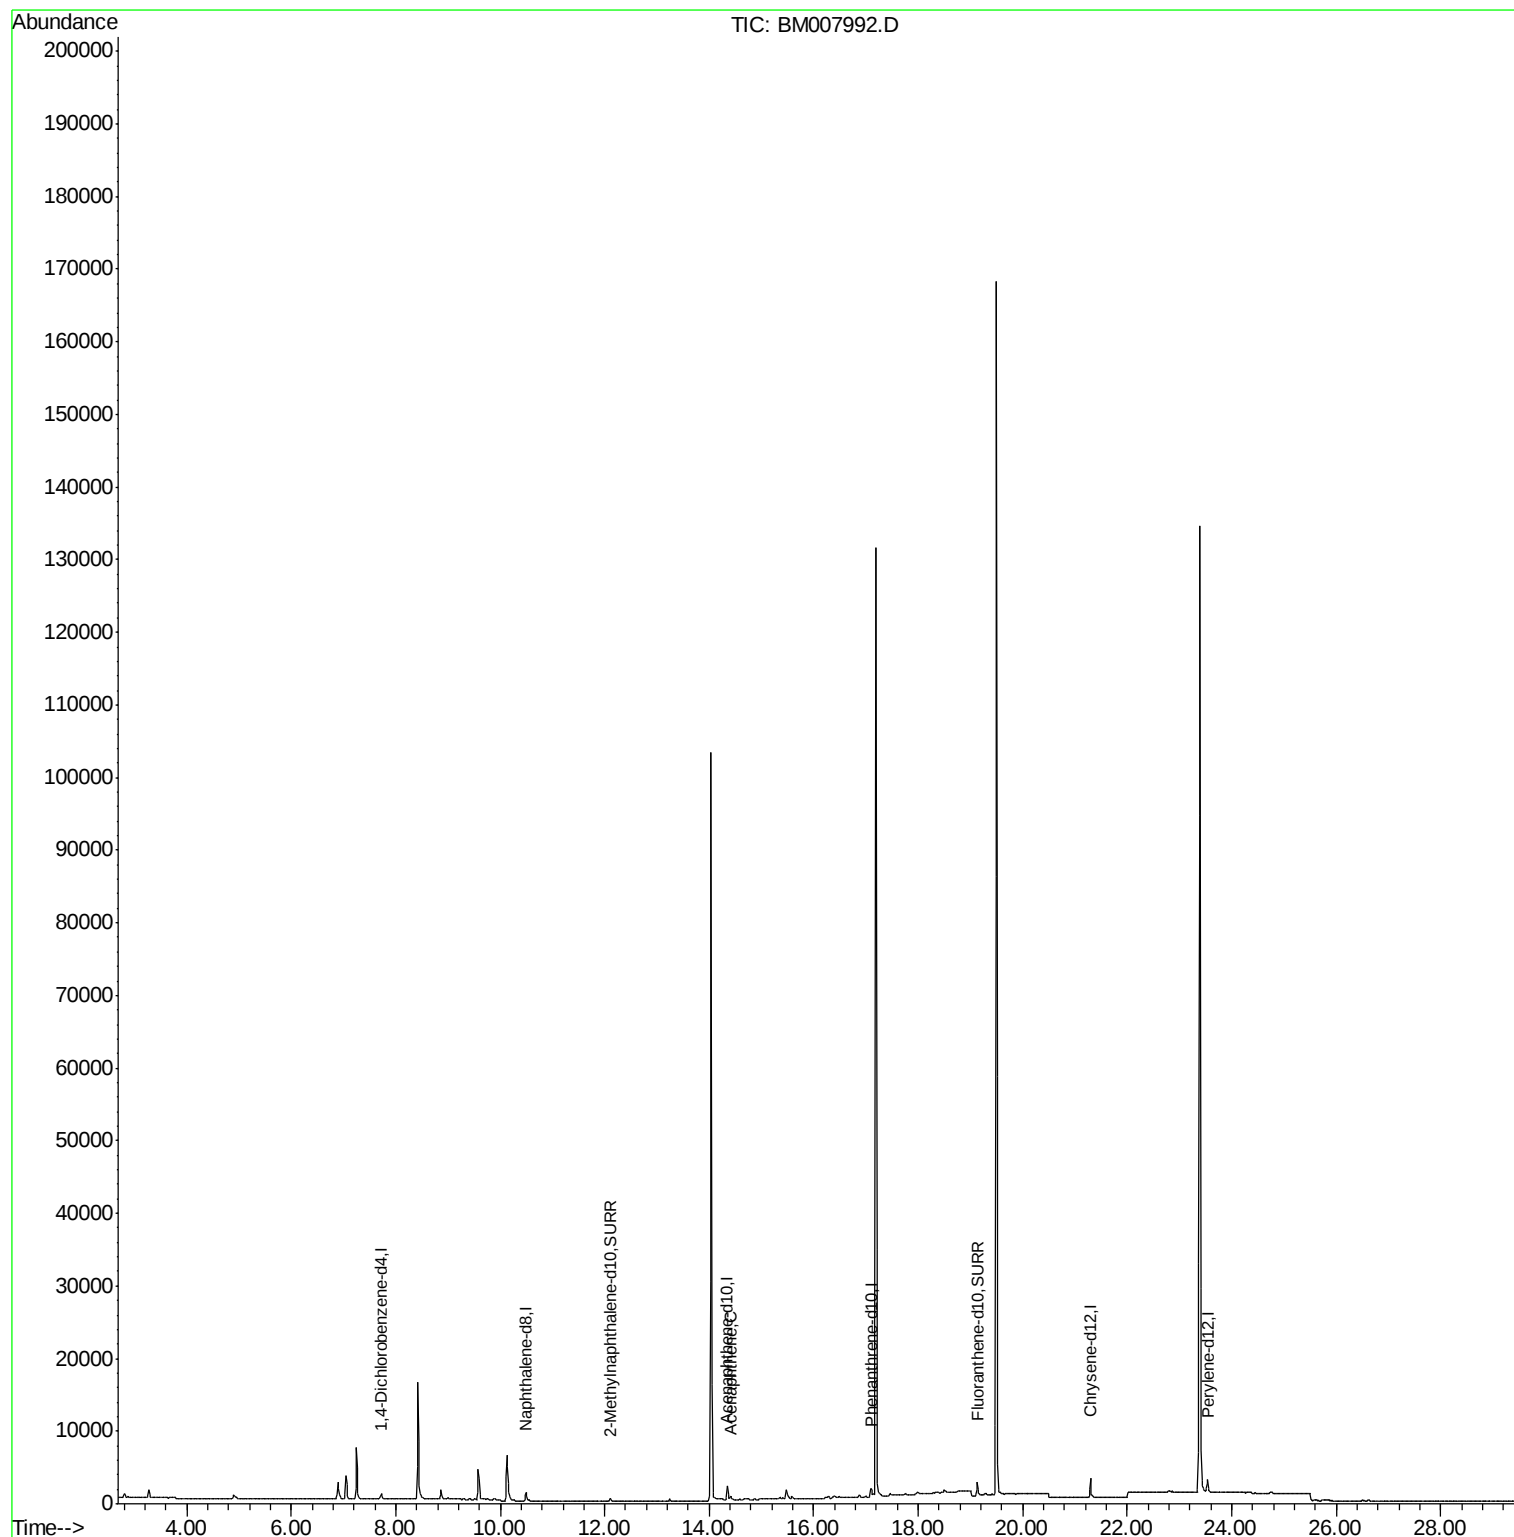

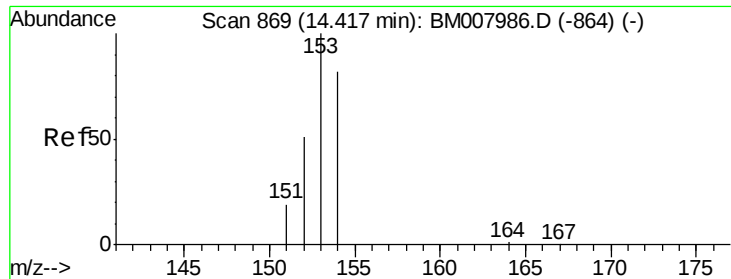

#8
 Acenaphthene
 Concen: 0.09 ng/ul
 RT: 14.42 min Scan# 869
 Delta R.T. -0.00 min
 Lab File: BM007992.D
 Acq: 22 Nov 2016 13:45

Instrument :
 BNA_M
 ClientSampleId :
 A4WL8

Tgt Ion	Ratio	Lower	Upper
153	100		
152	57.0	40.3	60.5
154	94.7	71.4	107.2

Manual Integrations
 APPROVED

sohil
 11/23/2016 6:05:57 PM

