

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112221\
 Data File : BM033217.D
 Acq On : 22 Nov 2021 15:24
 Operator : CG/JU
 Sample : M4677-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AA7

Quant Time: Nov 22 16:24:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 19 15:41:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.956	152	2770	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.751	136	8236	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	5156	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	11327	0.400	ng/ul	-0.01
17) Chrysene-d12	21.468	240	11354	0.400	ng/ul	0.00
23) Perylene-d12	23.805	264	11730	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	11690	4.488	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.334	152	4006	0.351	ng/ul	0.00
18) Fluoranthene-d10	19.327	212	12554	0.382	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	20946	7.151	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112221\
Data File : BM033217.D
Acq On : 22 Nov 2021 15:24
Operator : CG/JU
Sample : M4677-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AA7


Quant Time: Nov 22 16:24:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 15:41:12 2021
Response via : Initial Calibration

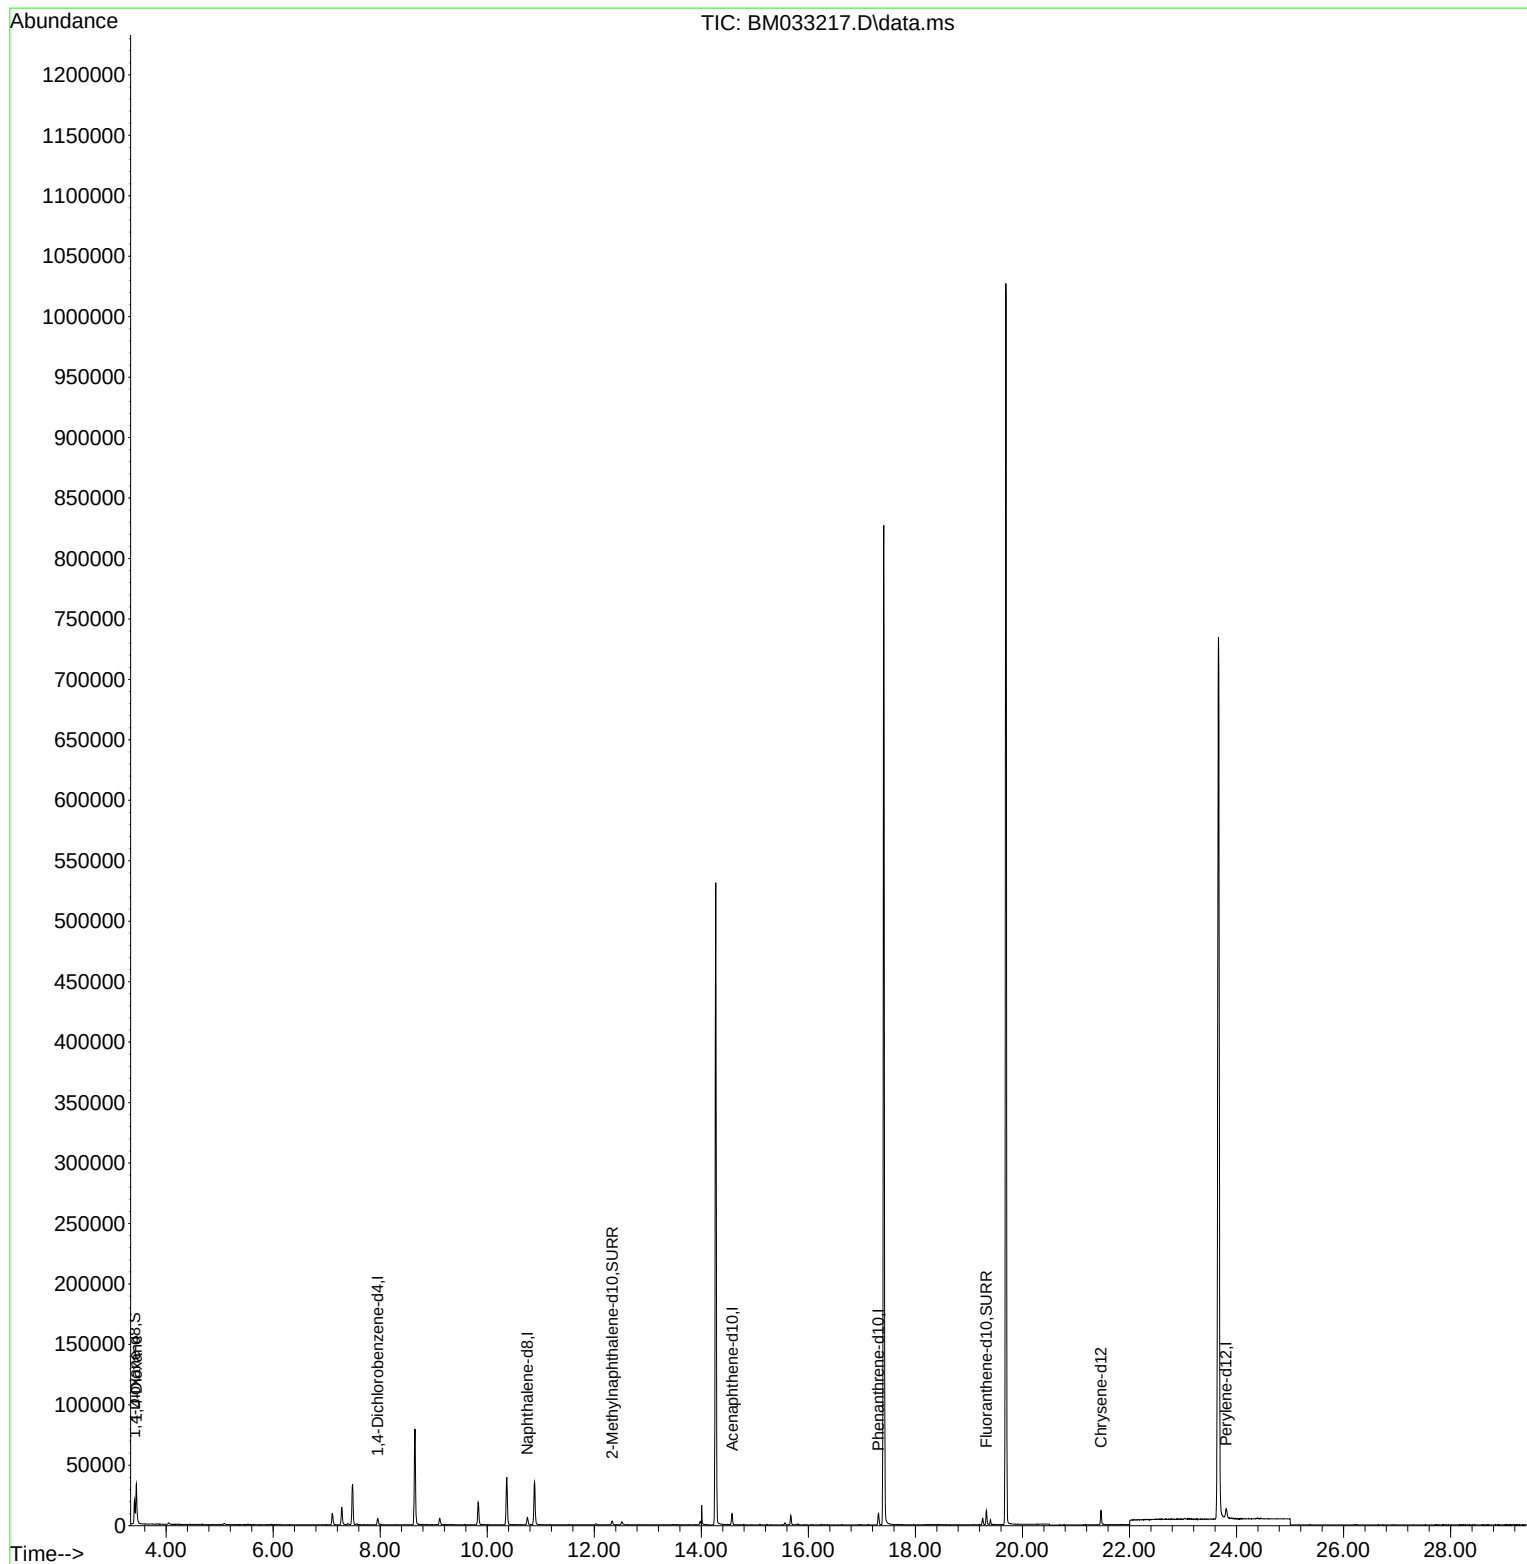

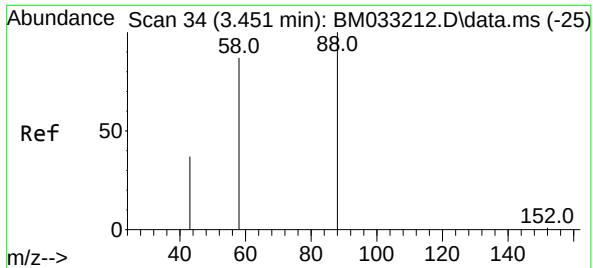

#2
 1,4-Dioxane
 Concen: 7.151 ng/ul
 RT: 3.444 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: BM033217.D
 Acq: 22 Nov 2021 15:24

Instrument :
 BNA_M
 ClientSampleId :
 H0AA7

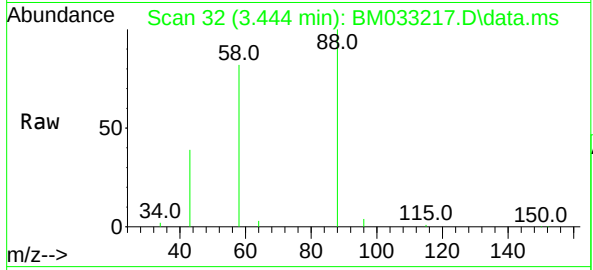

Tgt Ion: 88 Resp: 20946

Ion	Ratio	Lower	Upper
88	100		
43	39.5	35.8	53.8
58	82.3	55.8	83.8

