

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008038.D
 Acq On : 23 Nov 2016 17:40
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF5

Quant Time: Nov 24 02:59:21 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	548	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	1823	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1122	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	154876	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	2129	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	123547	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	759	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	1789	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.50	202	428	0.06	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008038.D
Acq On : 23 Nov 2016 17:40
Operator : UM/SJ
Sample : H5699-25
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WF5

Quant Time: Nov 24 02:59:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 02:56:32 2016
Response via : Initial Calibration

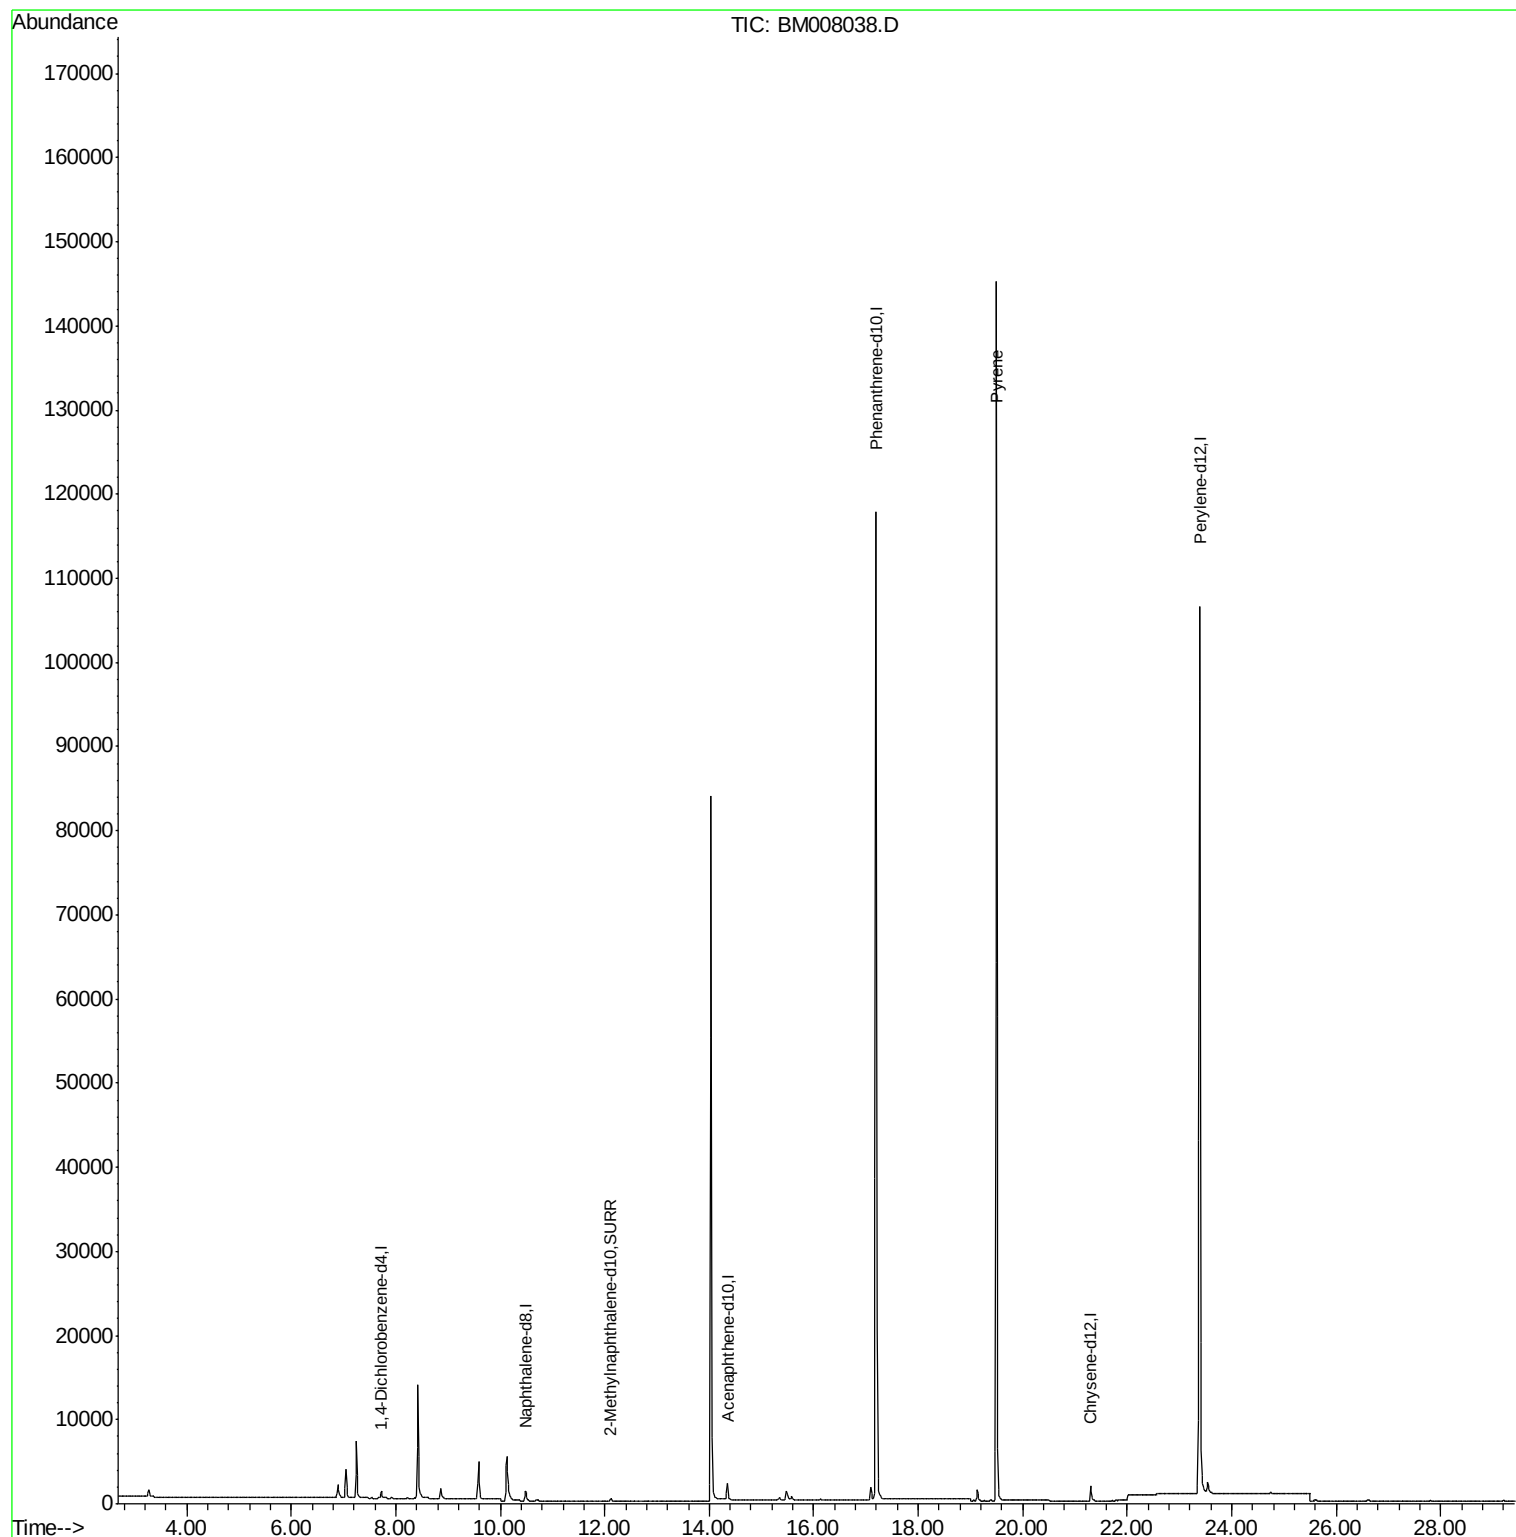

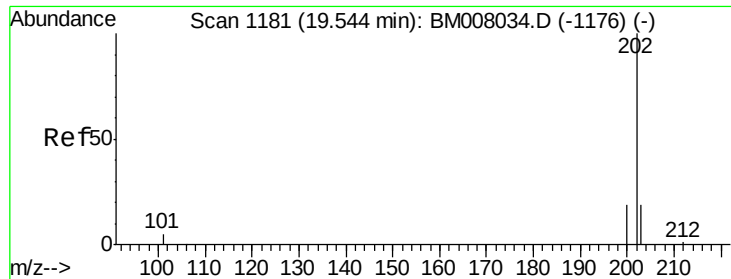

#17
 Pyrene
 Concen: 0.06 ng/ul
 RT: 19.50 min Scan# 1177
 Delta R.T. -0.05 min
 Lab File: BM008038.D
 Acq: 23 Nov 2016 17:40

Instrument :
 BNA_M
 ClientSampleId :
 A4WF5

Tgt Ion: 202 Resp: 428
 Ion Ratio Lower Upper
 202 100
 200 21.5 18.2 27.4
 203 170.1 15.6 23.4#

