

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008039.D
 Acq On : 23 Nov 2016 18:16
 Operator : UM/SJ
 Sample : H5699-26
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF7

Quant Time: Nov 24 02:59:27 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	512	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	1753	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1097	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	144423	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	2100	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	107440	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	690	0.28	ng/ul	0.01
14) Fluoranthene-d10	19.14	212	1631	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.49	202	335	0.05	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008039.D
Acq On : 23 Nov 2016 18:16
Operator : UM/SJ
Sample : H5699-26
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WF7

Quant Time: Nov 24 02:59:27 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 02:56:32 2016
Response via : Initial Calibration

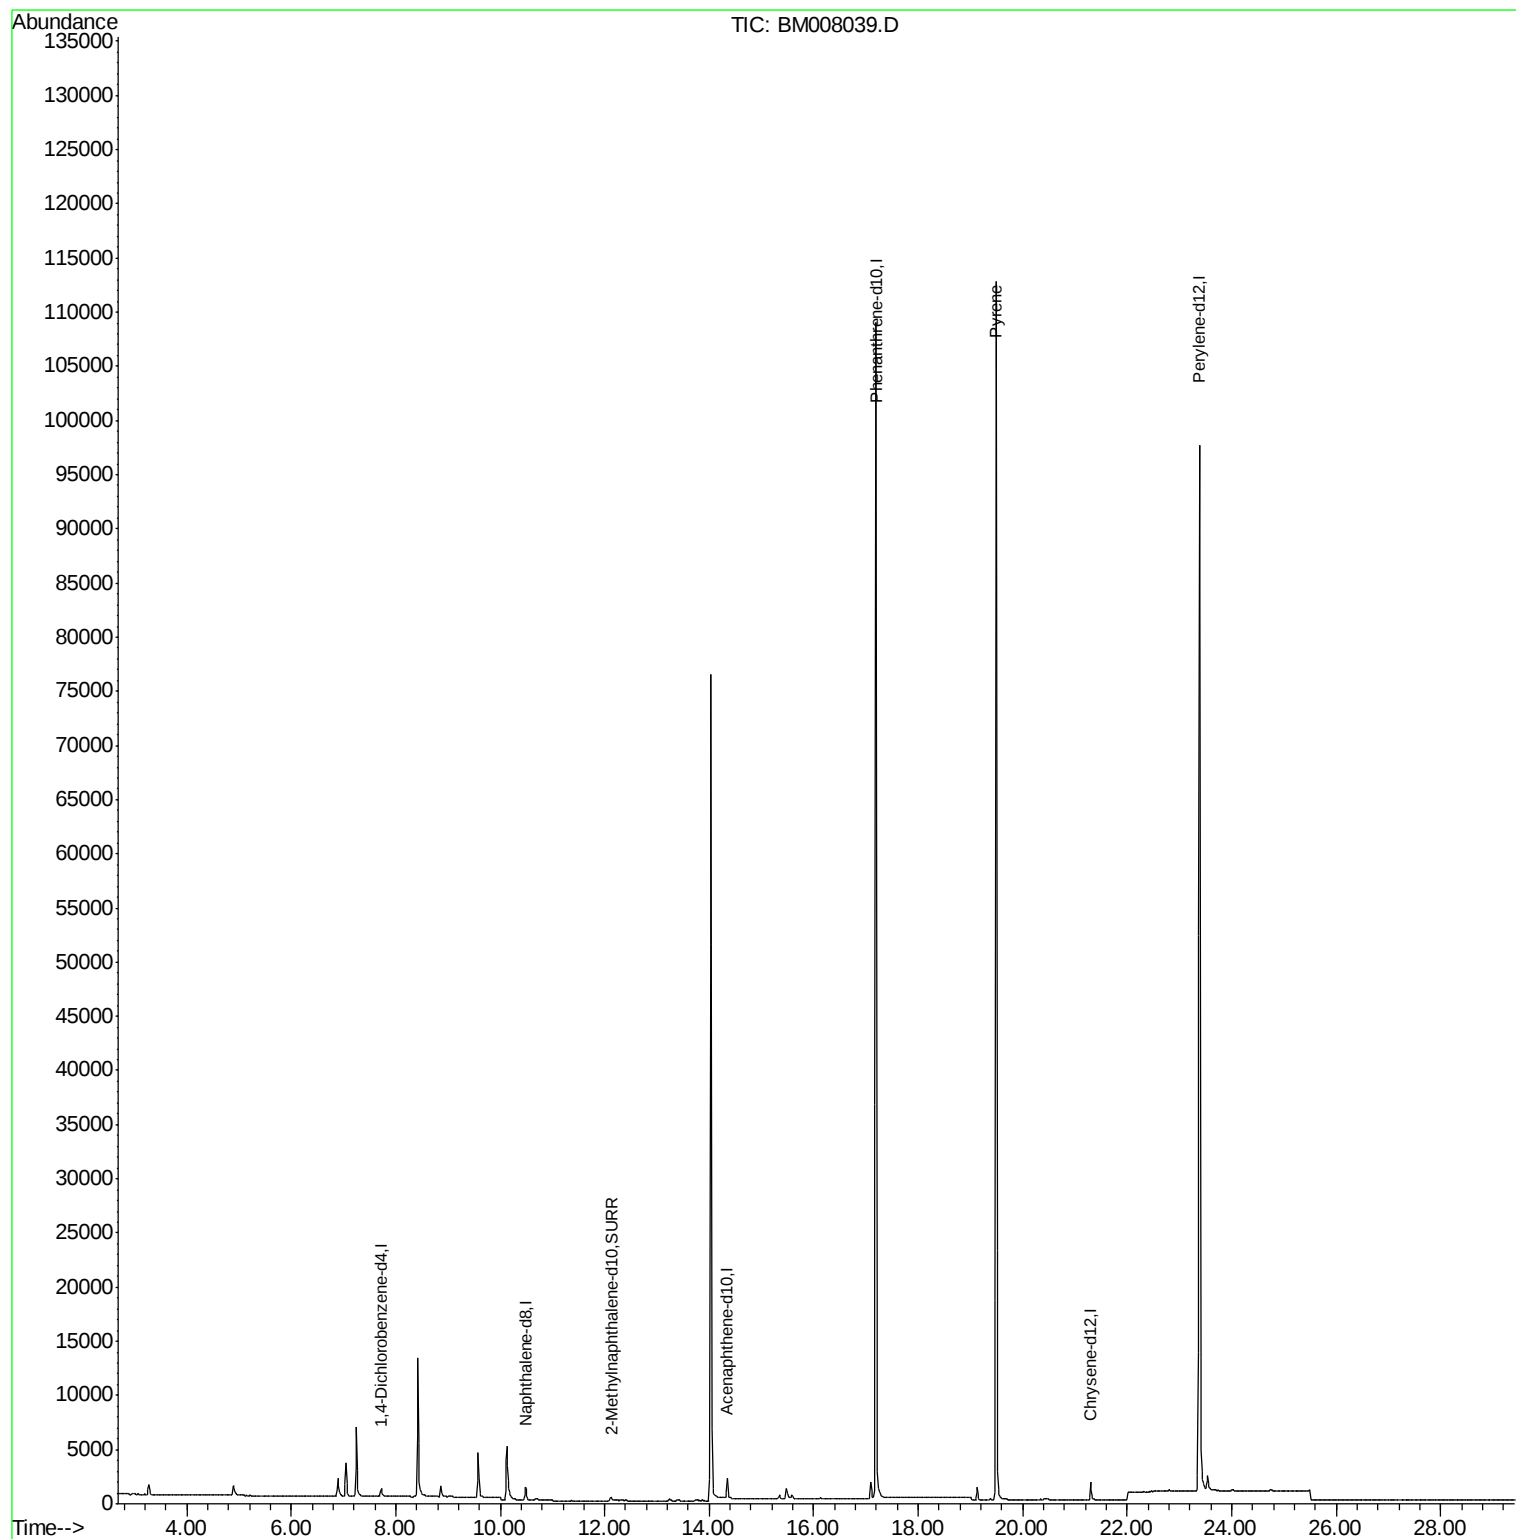

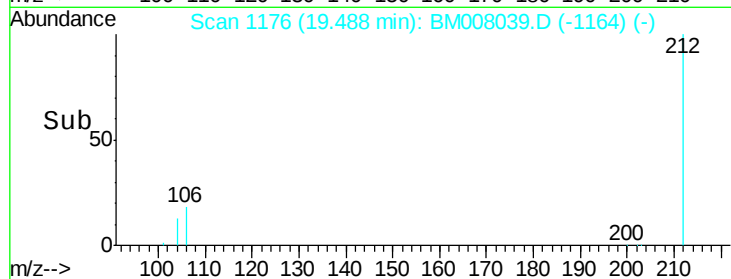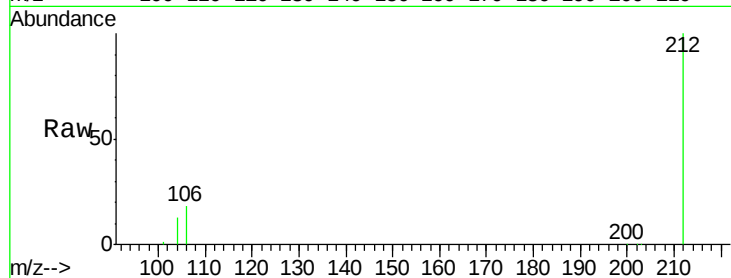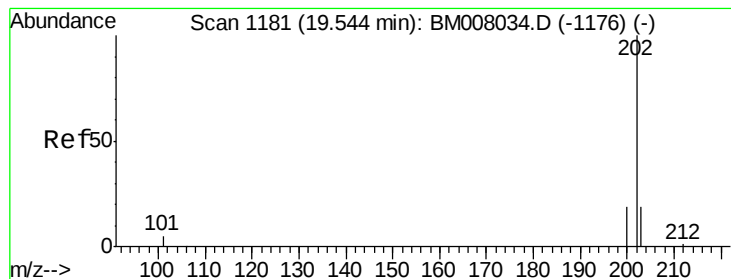

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.49 min Scan# 1176

Delta R.T. -0.06 min

Lab File: BM008039.D

Acq: 23 Nov 2016 18:16

Instrument :

BNA_M

ClientSampleId :

A4WF7

Tgt Ion: 202 Resp: 335

Ion Ratio Lower Upper

202 100

200 25.0 18.2 27.4

203 122.7 15.6 23.4#

