

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008040.D
 Acq On : 23 Nov 2016 18:52
 Operator : UM/SJ
 Sample : H5699-27
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF9

Quant Time: Nov 24 02:59:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	536	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.50	136	1782	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.35	164	1109	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	131002	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	2155	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	113795	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	581	0.23	ng/ul	0.01
14) Fluoranthene-d10	19.13	212	1597	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.50	202	286	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008040.D
Acq On : 23 Nov 2016 18:52
Operator : UM/SJ
Sample : H5699-27
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WF9

Quant Time: Nov 24 02:59:33 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 02:56:32 2016
Response via : Initial Calibration

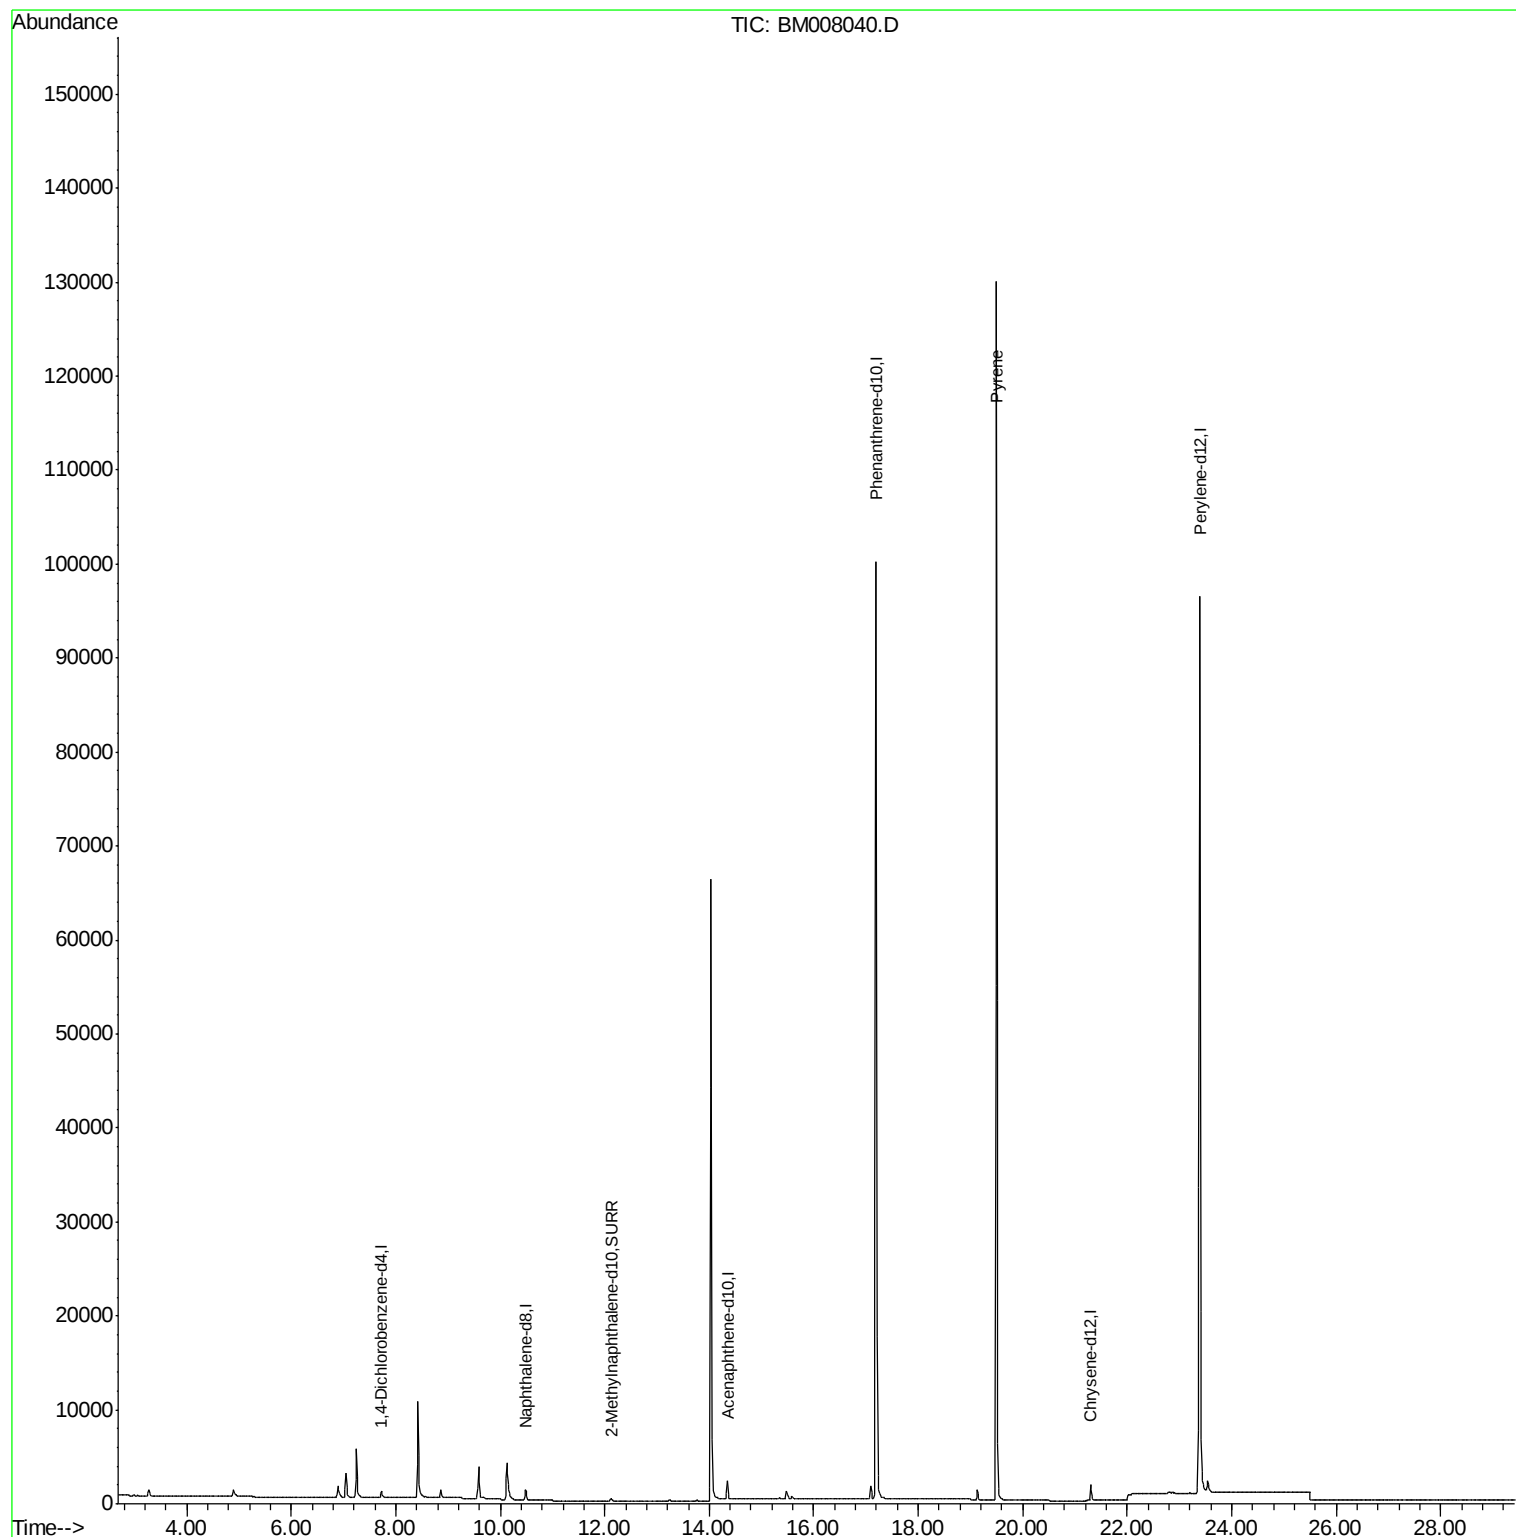

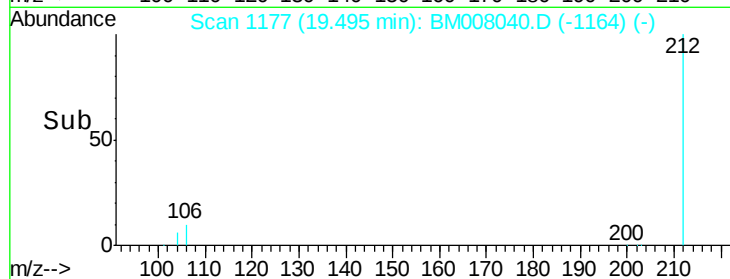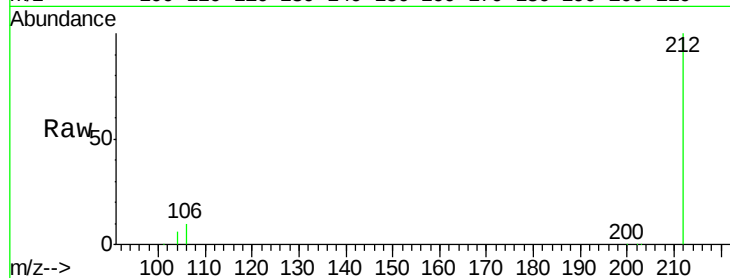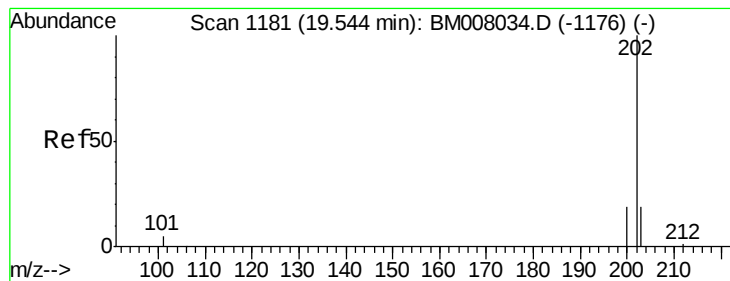

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.50 min Scan# 1177

Delta R.T. -0.05 min

Lab File: BM008040.D

Acq: 23 Nov 2016 18:52

Instrument :

BNA_M

ClientSampleId :

A4WF9

Tgt Ion: 202 Resp: 286

Ion Ratio Lower Upper

202 100

200 23.4 18.2 27.4

203 174.5 15.6 23.4#

