

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008042.D
 Acq On : 23 Nov 2016 20:04
 Operator : UM/SJ
 Sample : H5699-29
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG3

Quant Time: Nov 24 02:59:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	527	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	1793	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1114	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	182192	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	2120	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	134524	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	854	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.14	212	2082	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.49	202	384	0.05	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008042.D
Acq On : 23 Nov 2016 20:04
Operator : UM/SJ
Sample : H5699-29
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WG3

Quant Time: Nov 24 02:59:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 02:56:32 2016
Response via : Initial Calibration

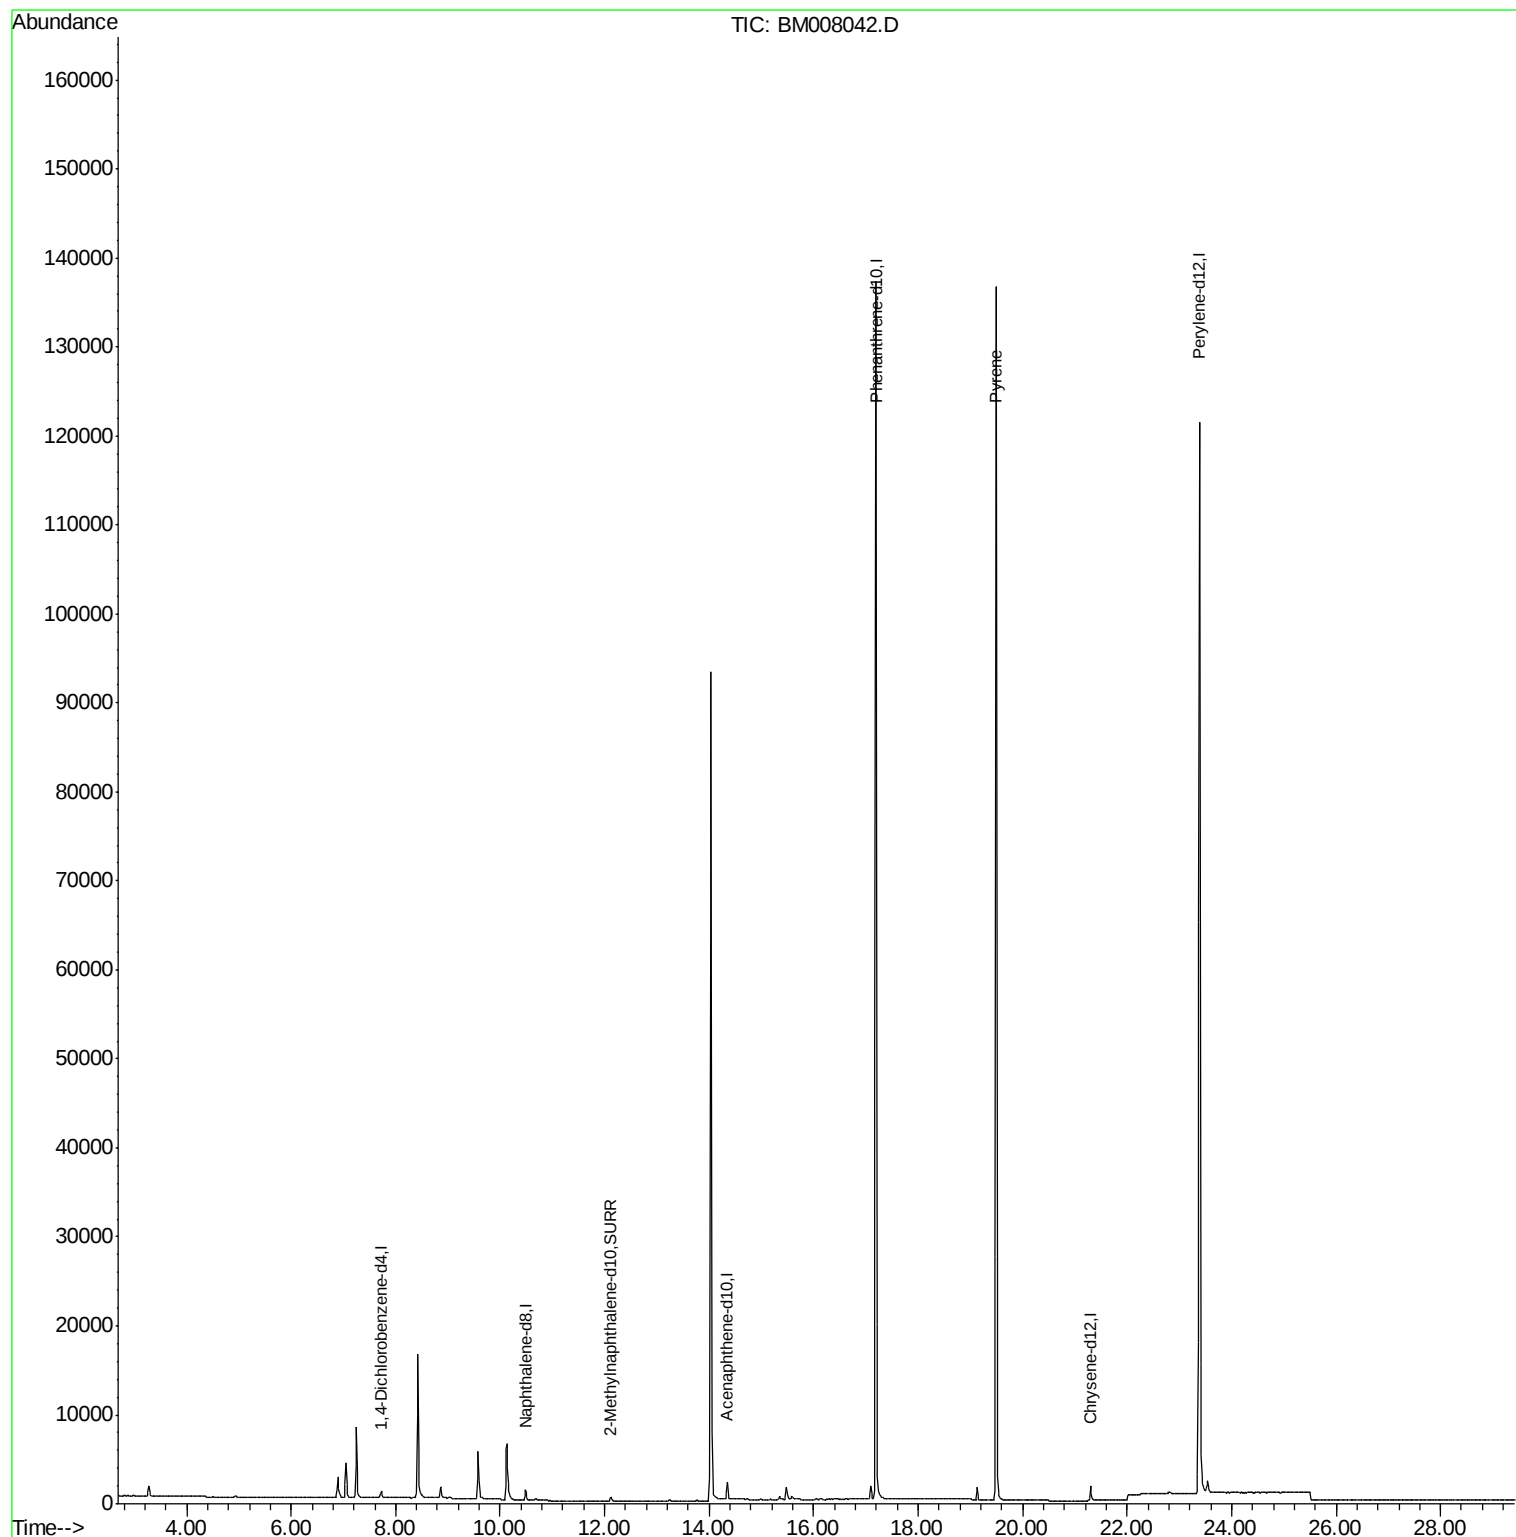

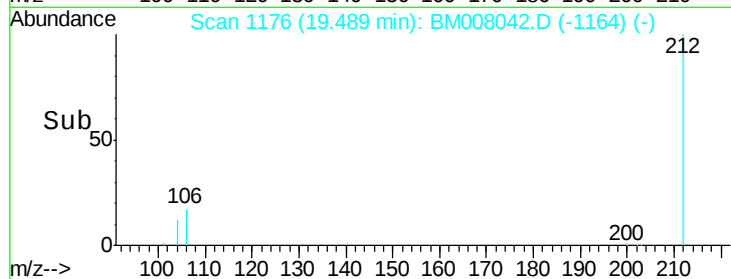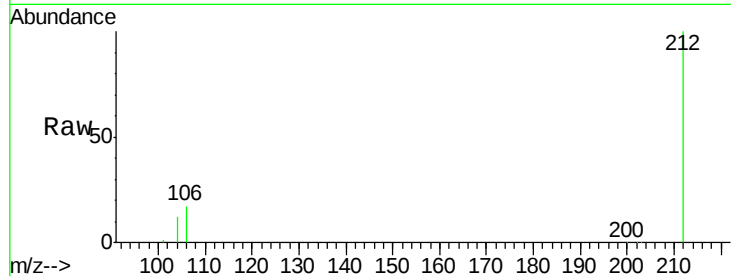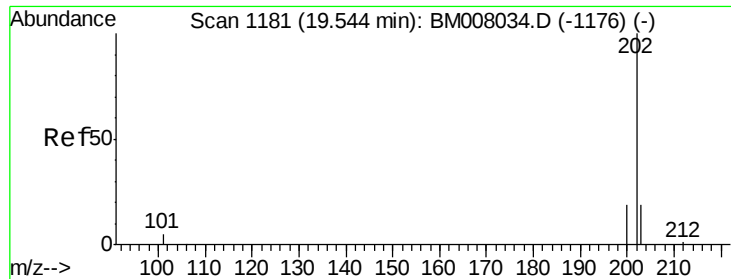

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.49 min Scan# 1176

Delta R.T. -0.06 min

Lab File: BM008042.D

Acq: 23 Nov 2016 20:04

Instrument :

BNA_M

ClientSampleId :

A4WG3

Tgt Ion: 202 Resp: 384

Ion Ratio Lower Upper

202 100

200 21.6 18.2 27.4

203 129.5 15.6 23.4#

