

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008048.D
 Acq On : 23 Nov 2016 23:38
 Operator : UM/SJ
 Sample : H5716-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WH7

Quant Time: Nov 24 03:00:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	514	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.50	136	1728	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.35	164	1062	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	98513	0.40	ng/ul	0.09
16) Chrysene-d12	21.31	240	2005	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	76596	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	405	0.17	ng/ul	0.01
14) Fluoranthene-d10	19.14	212	1220	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.49	202	227	0.03	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008048.D
Acq On : 23 Nov 2016 23:38
Operator : UM/SJ
Sample : H5716-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WH7

Quant Time: Nov 24 03:00:45 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 02:56:32 2016
Response via : Initial Calibration

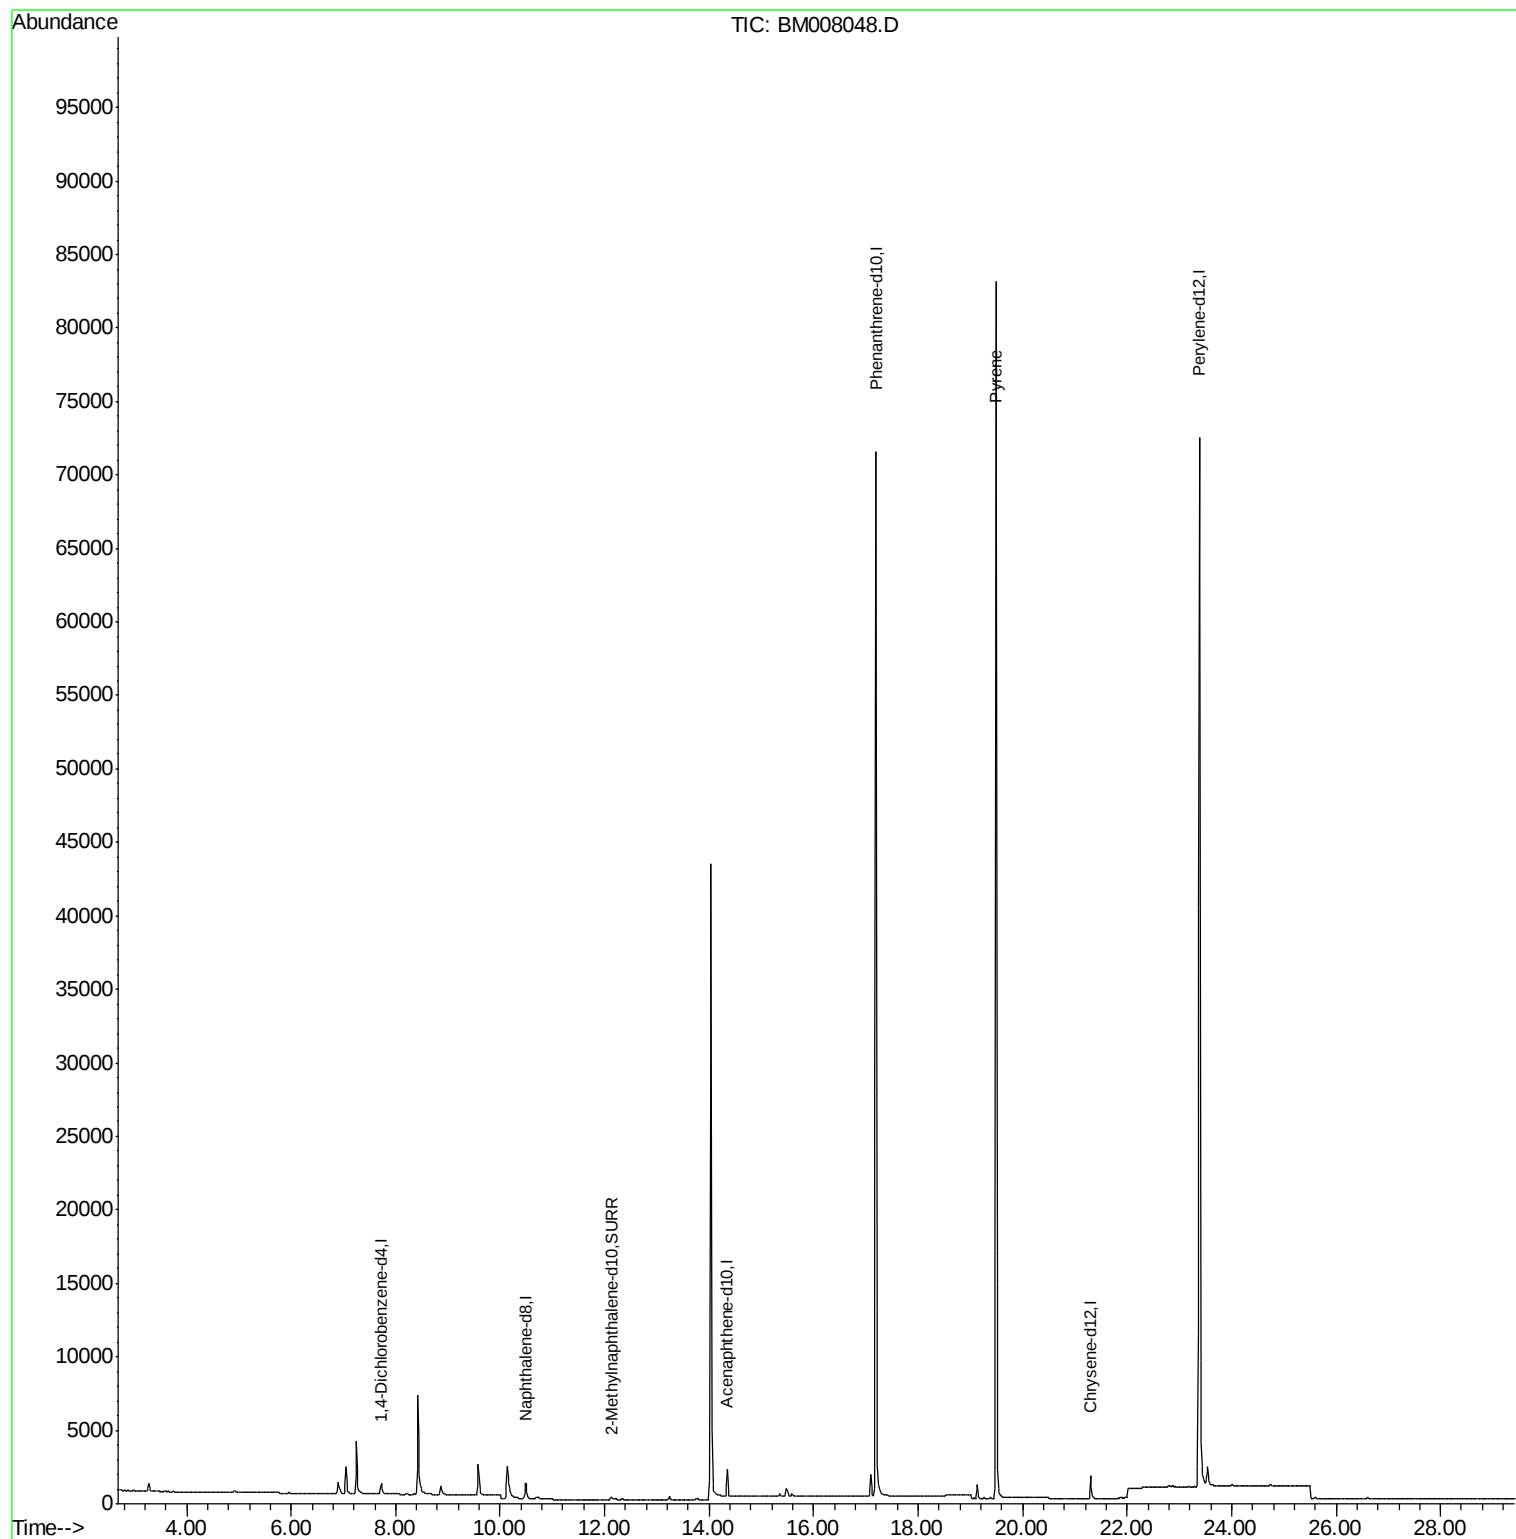

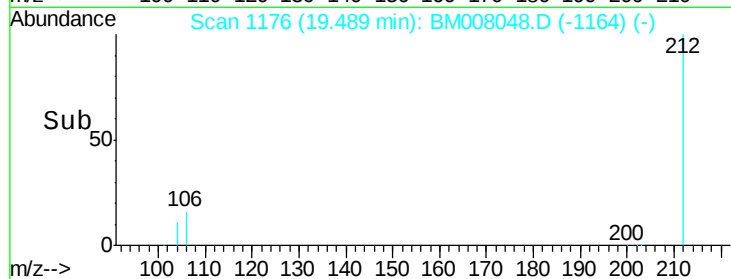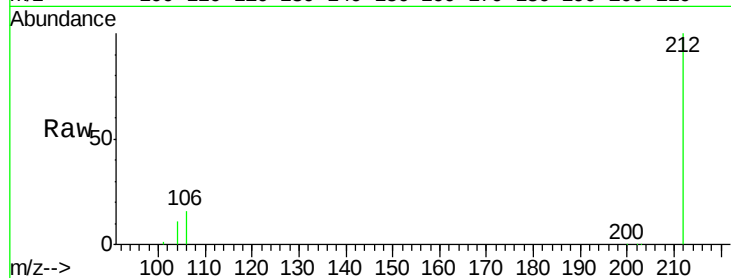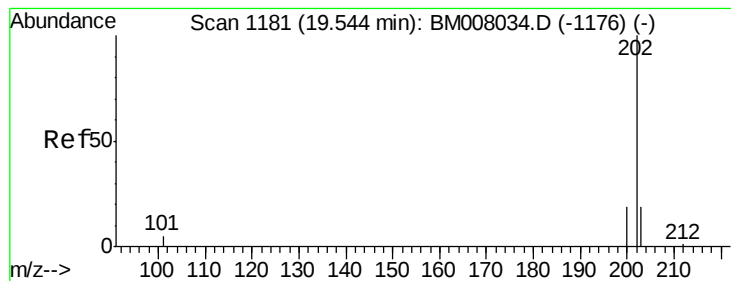

#17
 Pyrene
 Concen: 0.03 ng/ul
 RT: 19.49 min Scan# 1176
 Delta R.T. -0.06 min
 Lab File: BM008048.D
 Acq: 23 Nov 2016 23:38

Instrument :
 BNA_M
 ClientSampleId :
 A4WH7

Tgt Ion	Ratio	Lower	Upper
202	100		
200	29.1	18.2	27.4#
203	131.9	15.6	23.4#

