

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008050.D
 Acq On : 24 Nov 2016 00:50
 Operator : UM/SJ
 Sample : H5716-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WI0

Quant Time: Nov 24 04:13:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 04:11:15 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	518	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	1698	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1035	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	156421	0.40	ng/ul	0.09
16) Chrysene-d12	21.30	240	2058	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	126102	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	634	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	1854	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.50	202	336	0.05	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008050.D
Acq On : 24 Nov 2016 00:50
Operator : UM/SJ
Sample : H5716-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WI0

Quant Time: Nov 24 04:13:31 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 04:11:15 2016
Response via : Initial Calibration

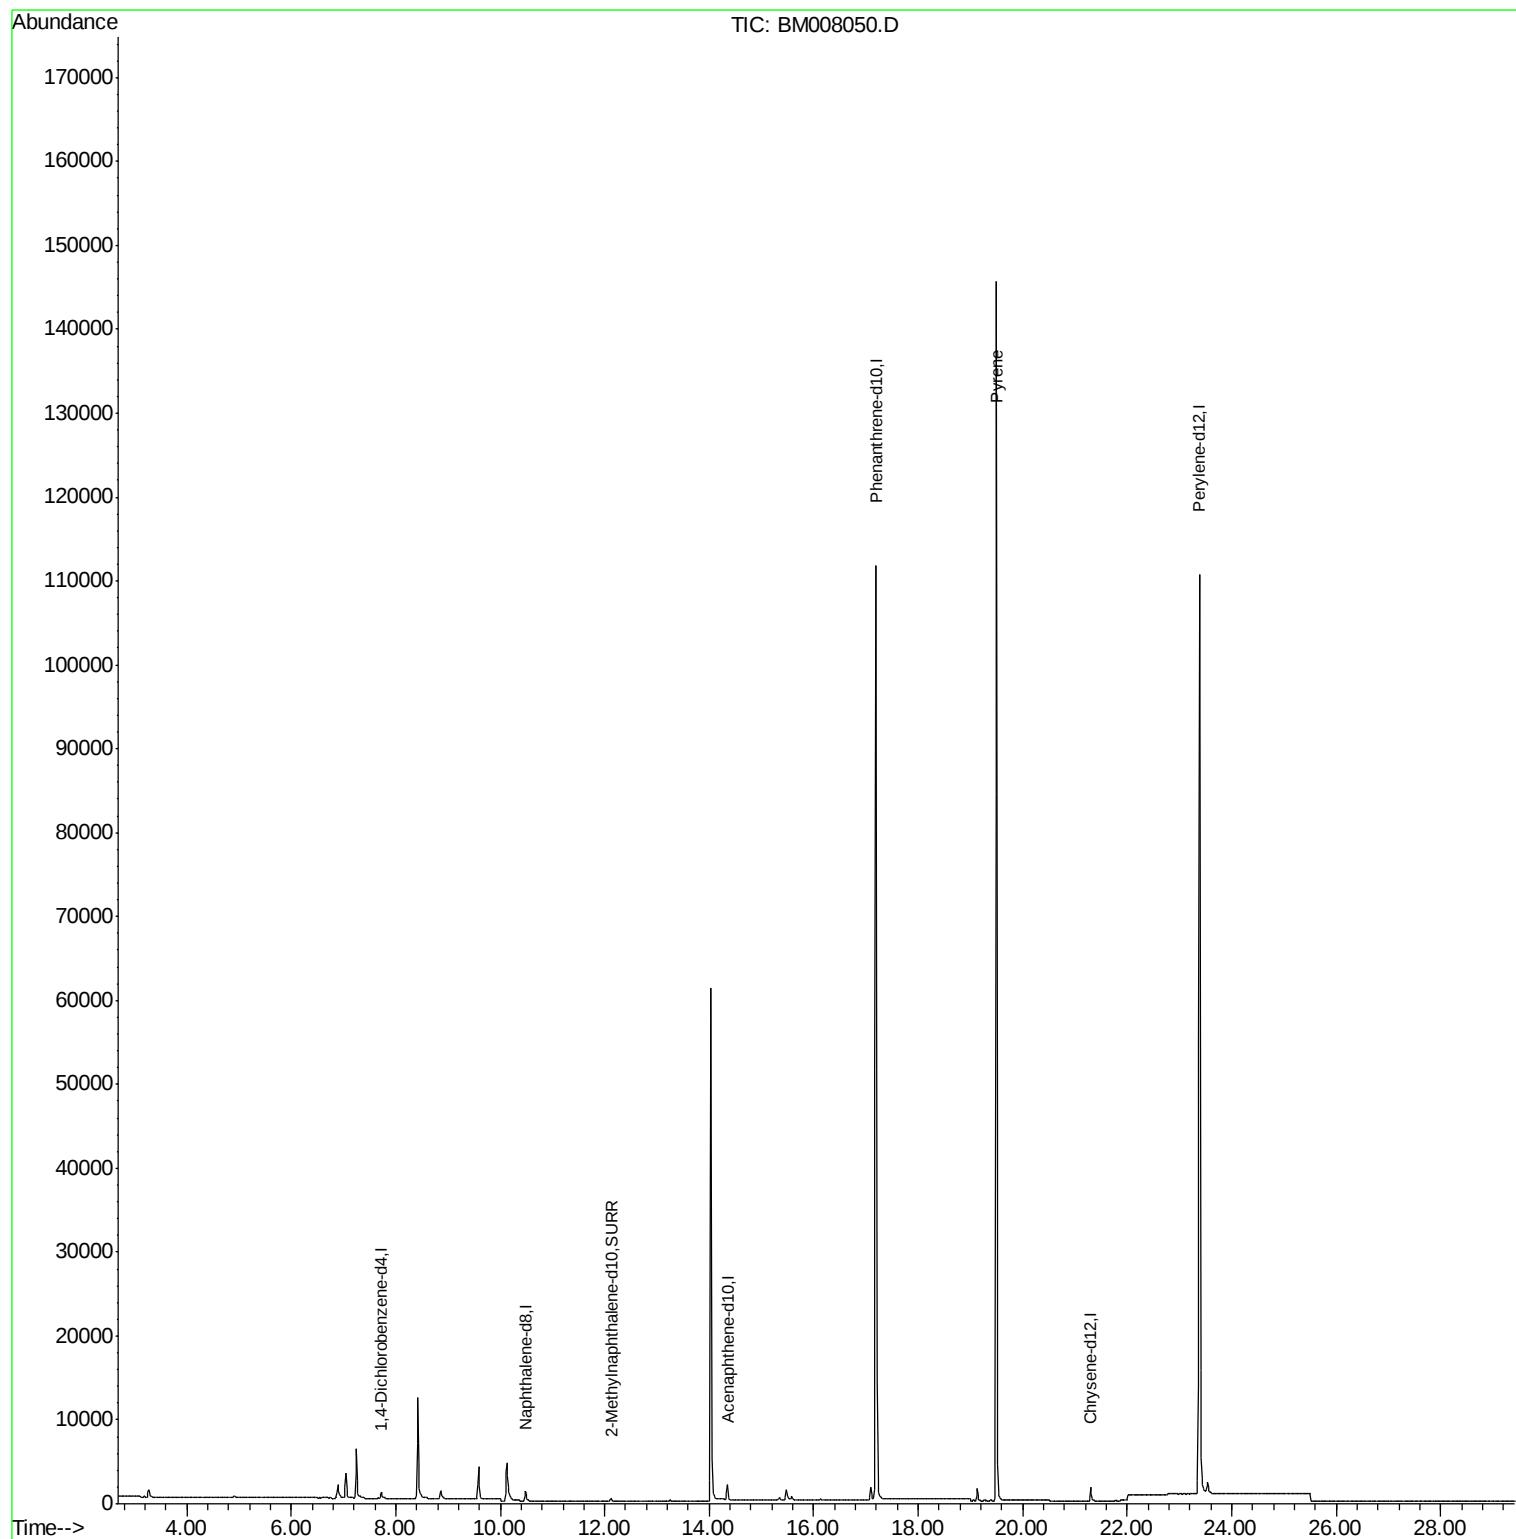

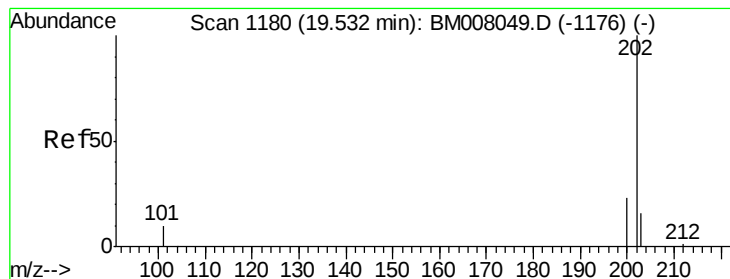

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.50 min Scan# 1177

Delta R.T. -0.04 min

Lab File: BM008050.D

Acq: 24 Nov 2016 00:50

Instrument :

BNA_M

ClientSampleId :

A4WI0


Tgt Ion: 202 Resp: 336

Ion Ratio Lower Upper

202 100

200 21.4 18.2 27.4

203 185.6 15.6 23.4#

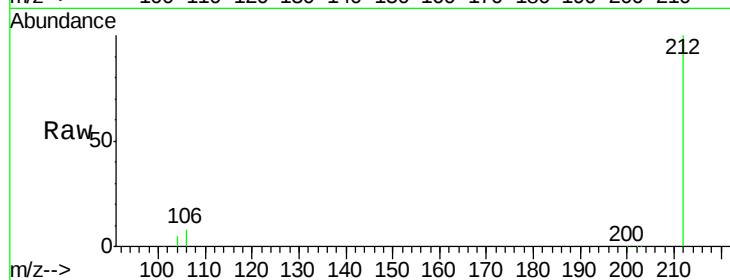

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

