

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008038.D
 Acq On : 23 Nov 2016 17:40
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WF5

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:26:29 PM

Quant Time: Nov 24 03:51:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration

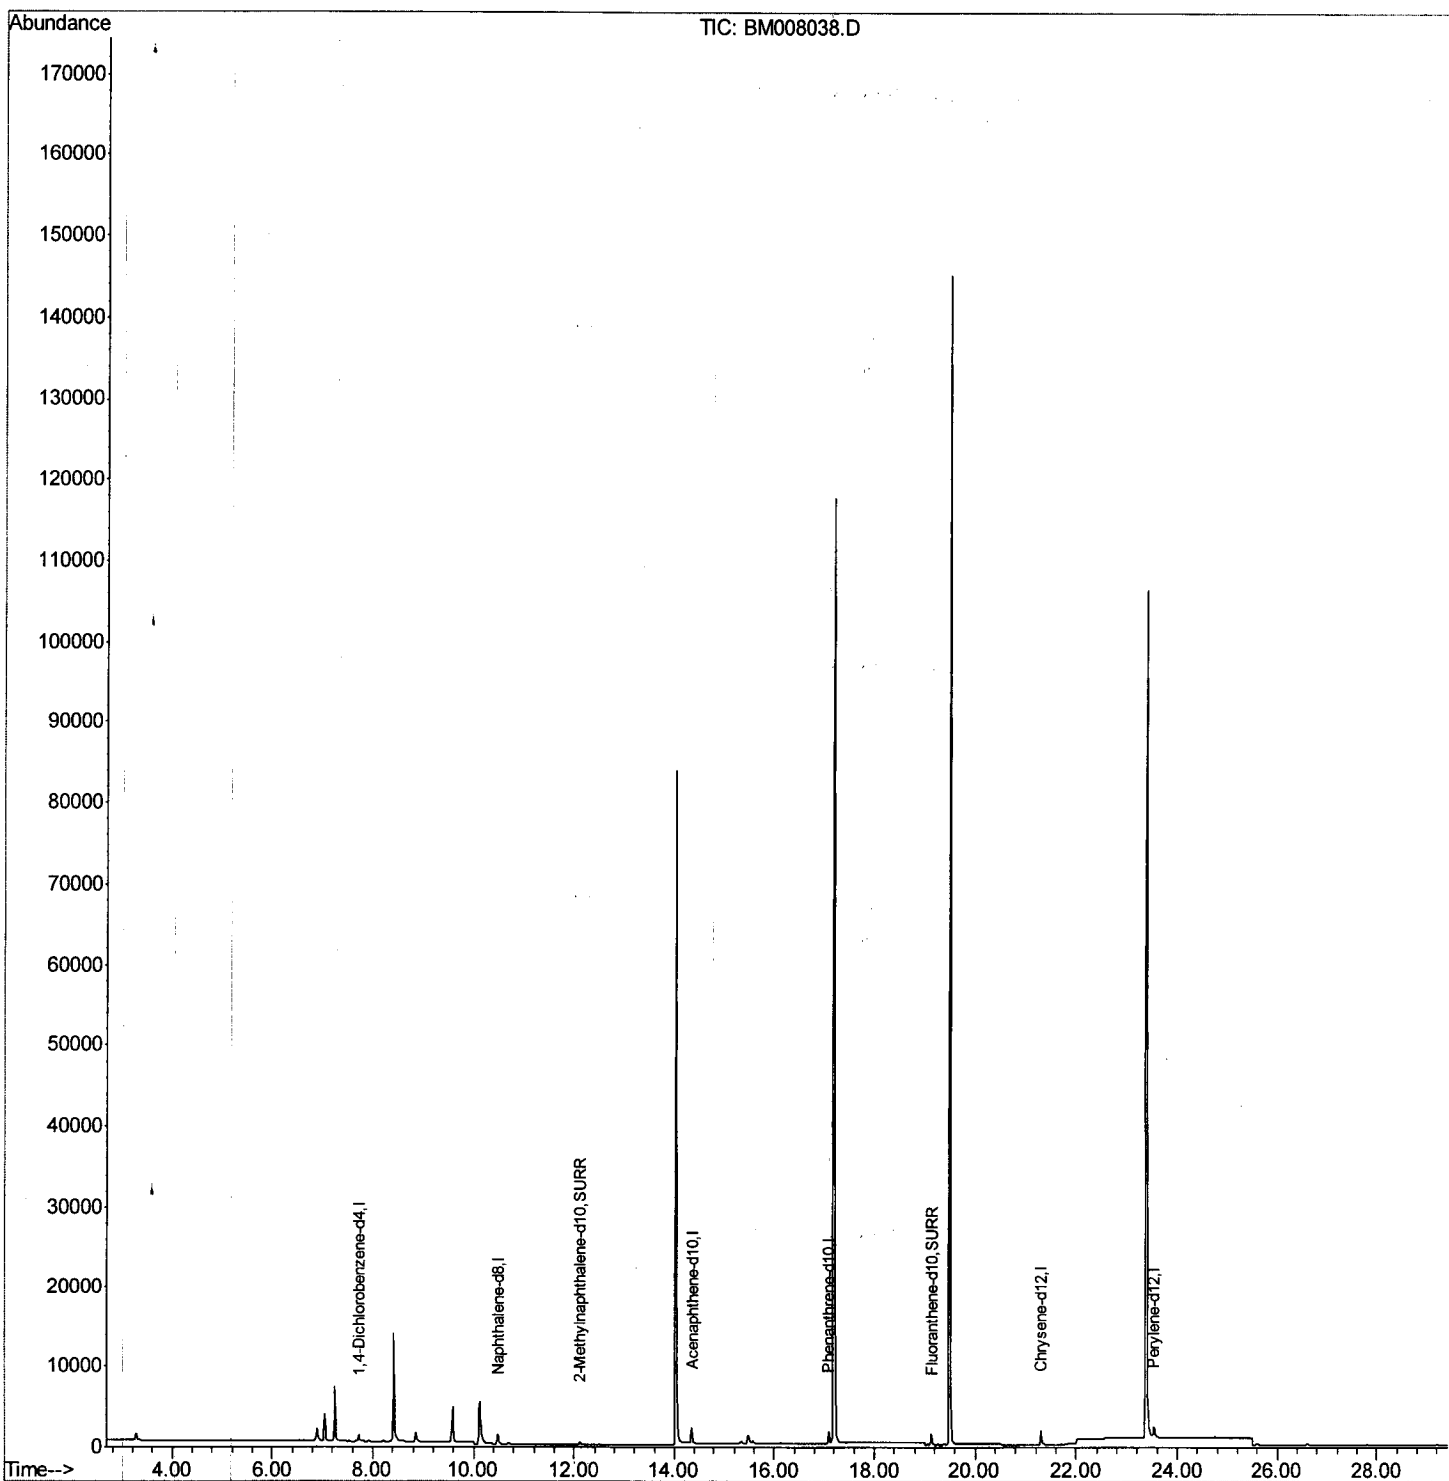

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008038.D
 Acq On : 23 Nov 2016 17:40
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF5

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:26:29 PM

Quant Time: Nov 24 02:59:21 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration

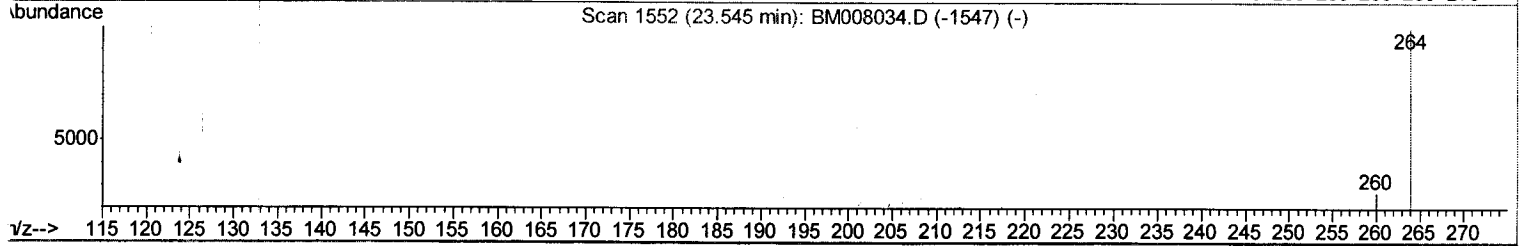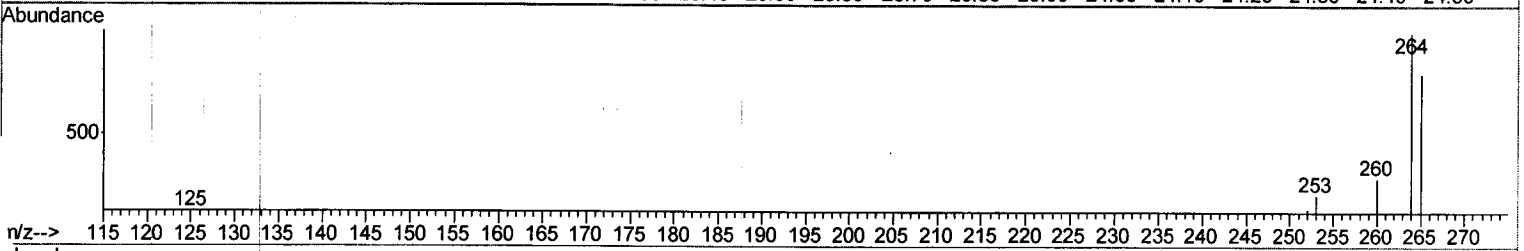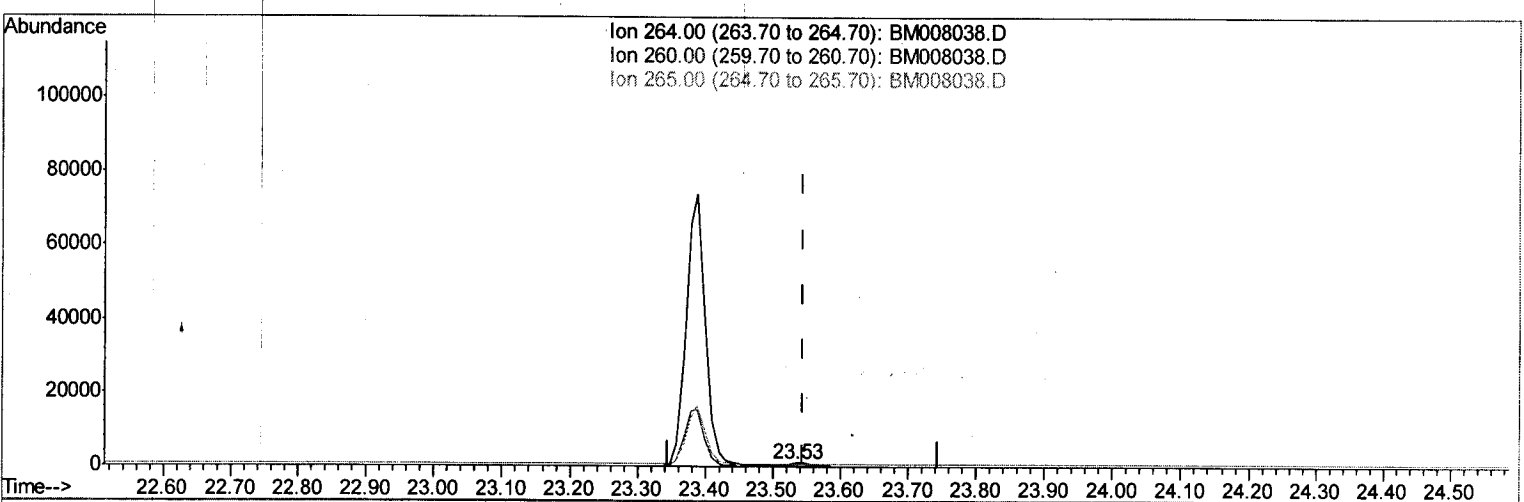

(20) Perylene-d12 (I)

23.535min (-0.011) 0.40ng/ul m

response 1589

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	29.61
265.00	103.50	80.53#
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008038.D
 Acq On : 23 Nov 2016 17:40
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF5

Quant Time: Nov 24 02:59:21 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:26:29 PM

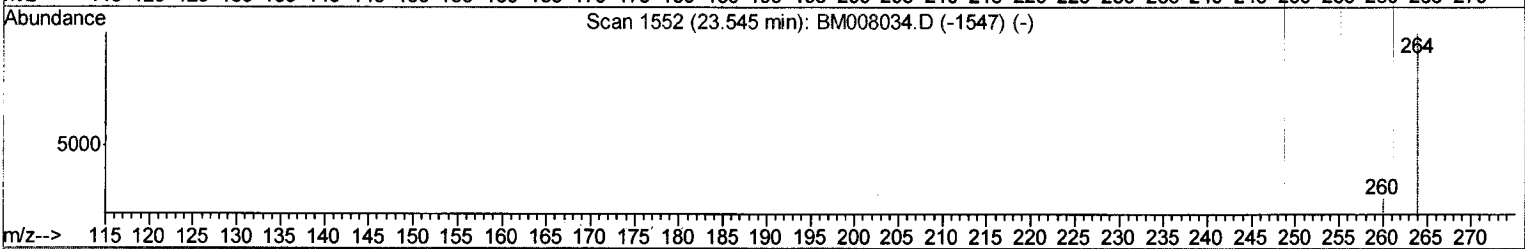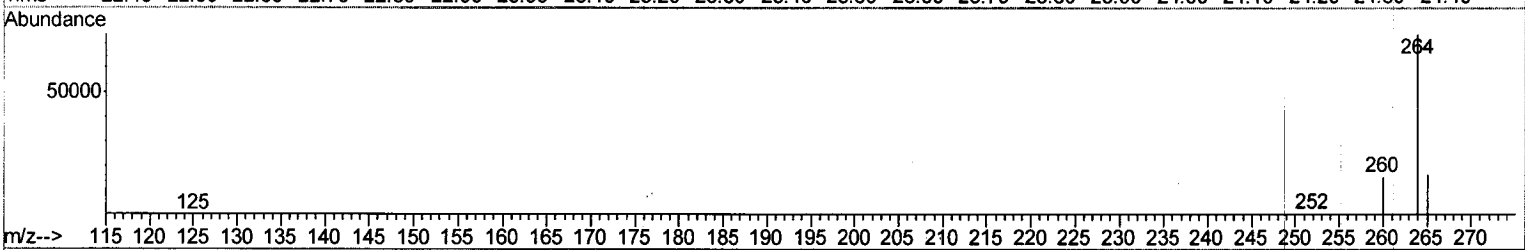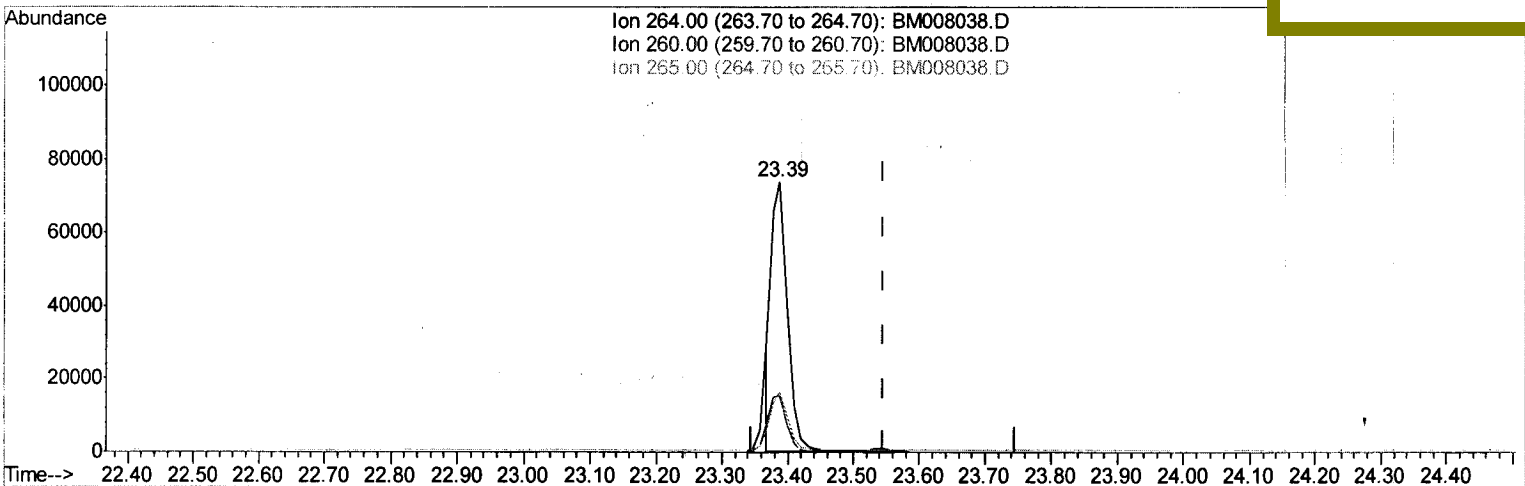

TIC: BM008038.D

(20) Perylene-d12 (I)

23.389min (-0.157) 0.40ng/ul

response 123547

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.93#
265.00	103.50	22.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008038.D
 Acq On : 23 Nov 2016 17:40
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WF5

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:26:29 PM

Quant Time: Nov 24 02:59:21 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration

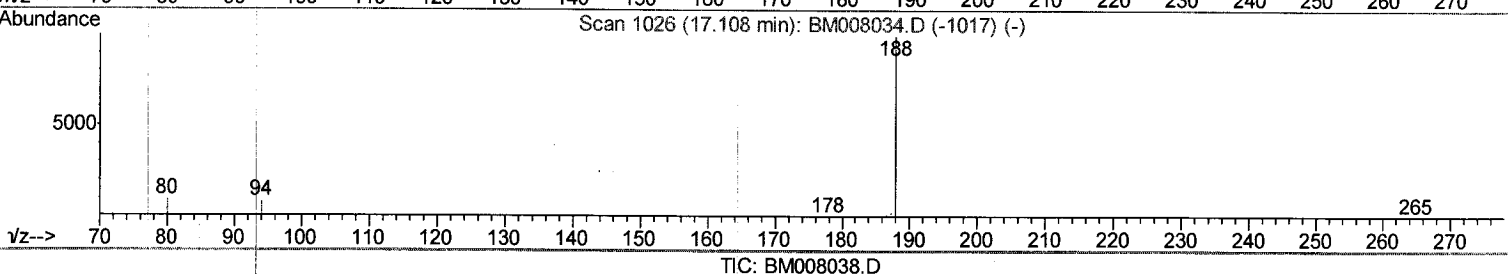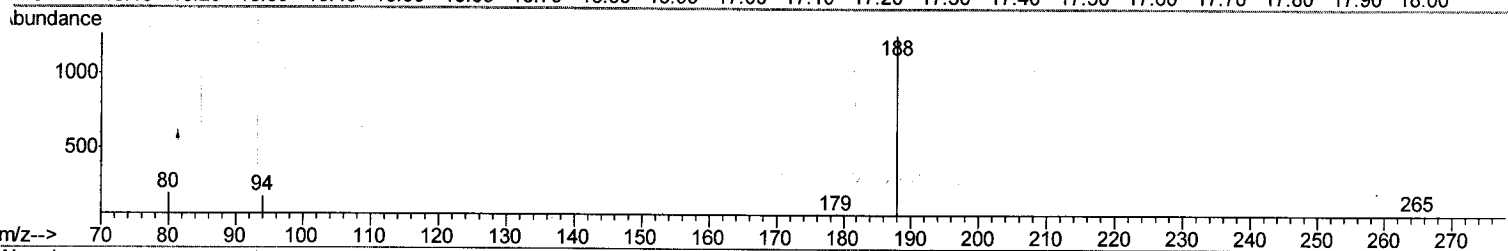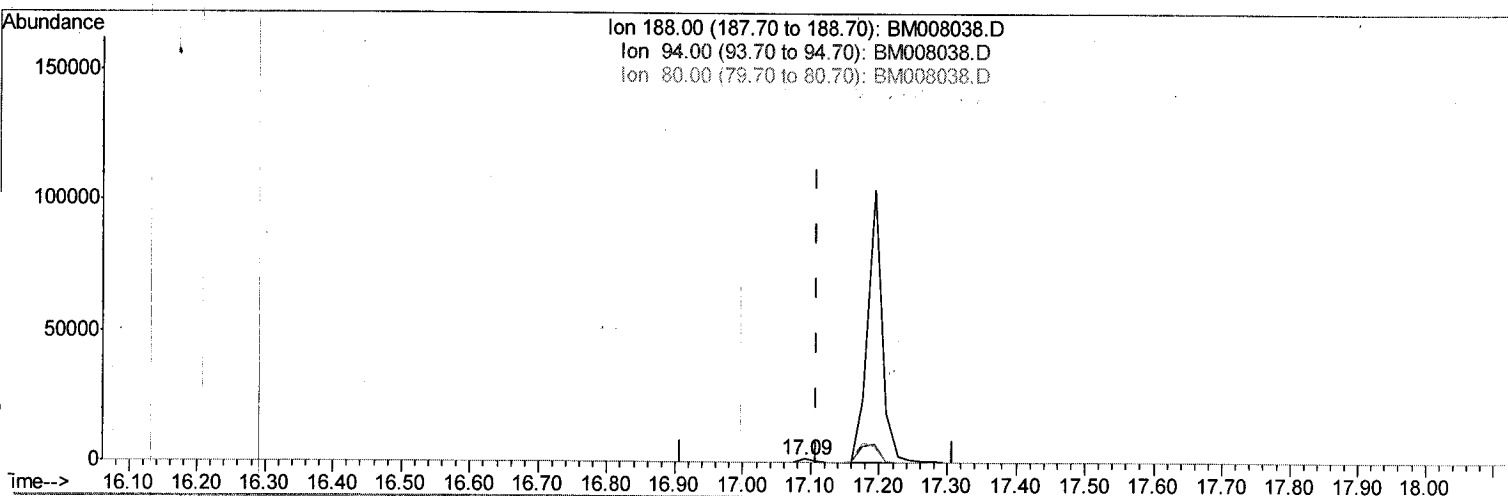

(10) Phenanthrene-d10 (I)

17.090min (-0.017) 0.40ng/ul m

response 2139

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.22#
80.00	11.80	14.71#
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008038.D
 Acq On : 23 Nov 2016 17:40
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF5

Quant Time: Nov 24 02:59:21 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 02:56:32 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:26:29 PM

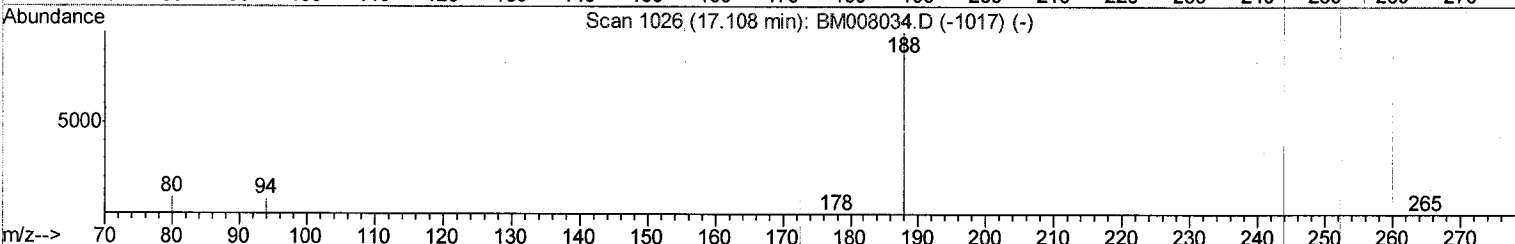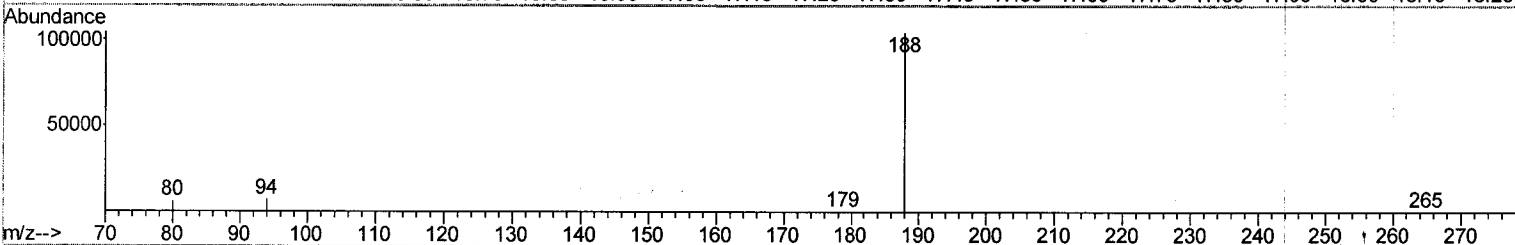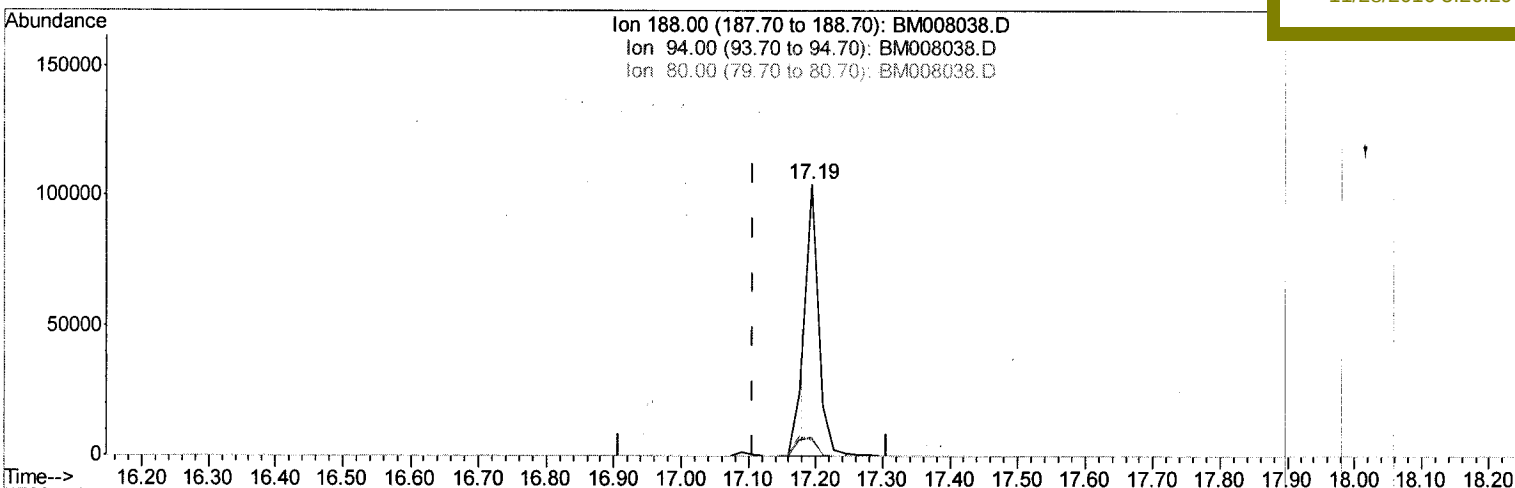

TIC: BM008038.D

(10) Phenanthrene-d10 (I)

17.193min (+0.086) 0.40ng/ul

response 154876

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.66#
80.00	11.80	5.84#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
Data File : BM008038.D
Acq On : 23 Nov 2016 17:40
Operator : UM/SJ
Sample : H5699-25
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WF5

Manual Integrations
APPROVED

Umangi
11/28/2016 5:26:29 PM

Quant Time: Nov 24 03:51:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 02:56:32 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	548	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	1823	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.35	164	1122	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	2139m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.30	240	2129	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	1589m	0.40	ng/ul	-0.01

S-J
11/29/16

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	759	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	1789	0.30	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed