

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:49:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

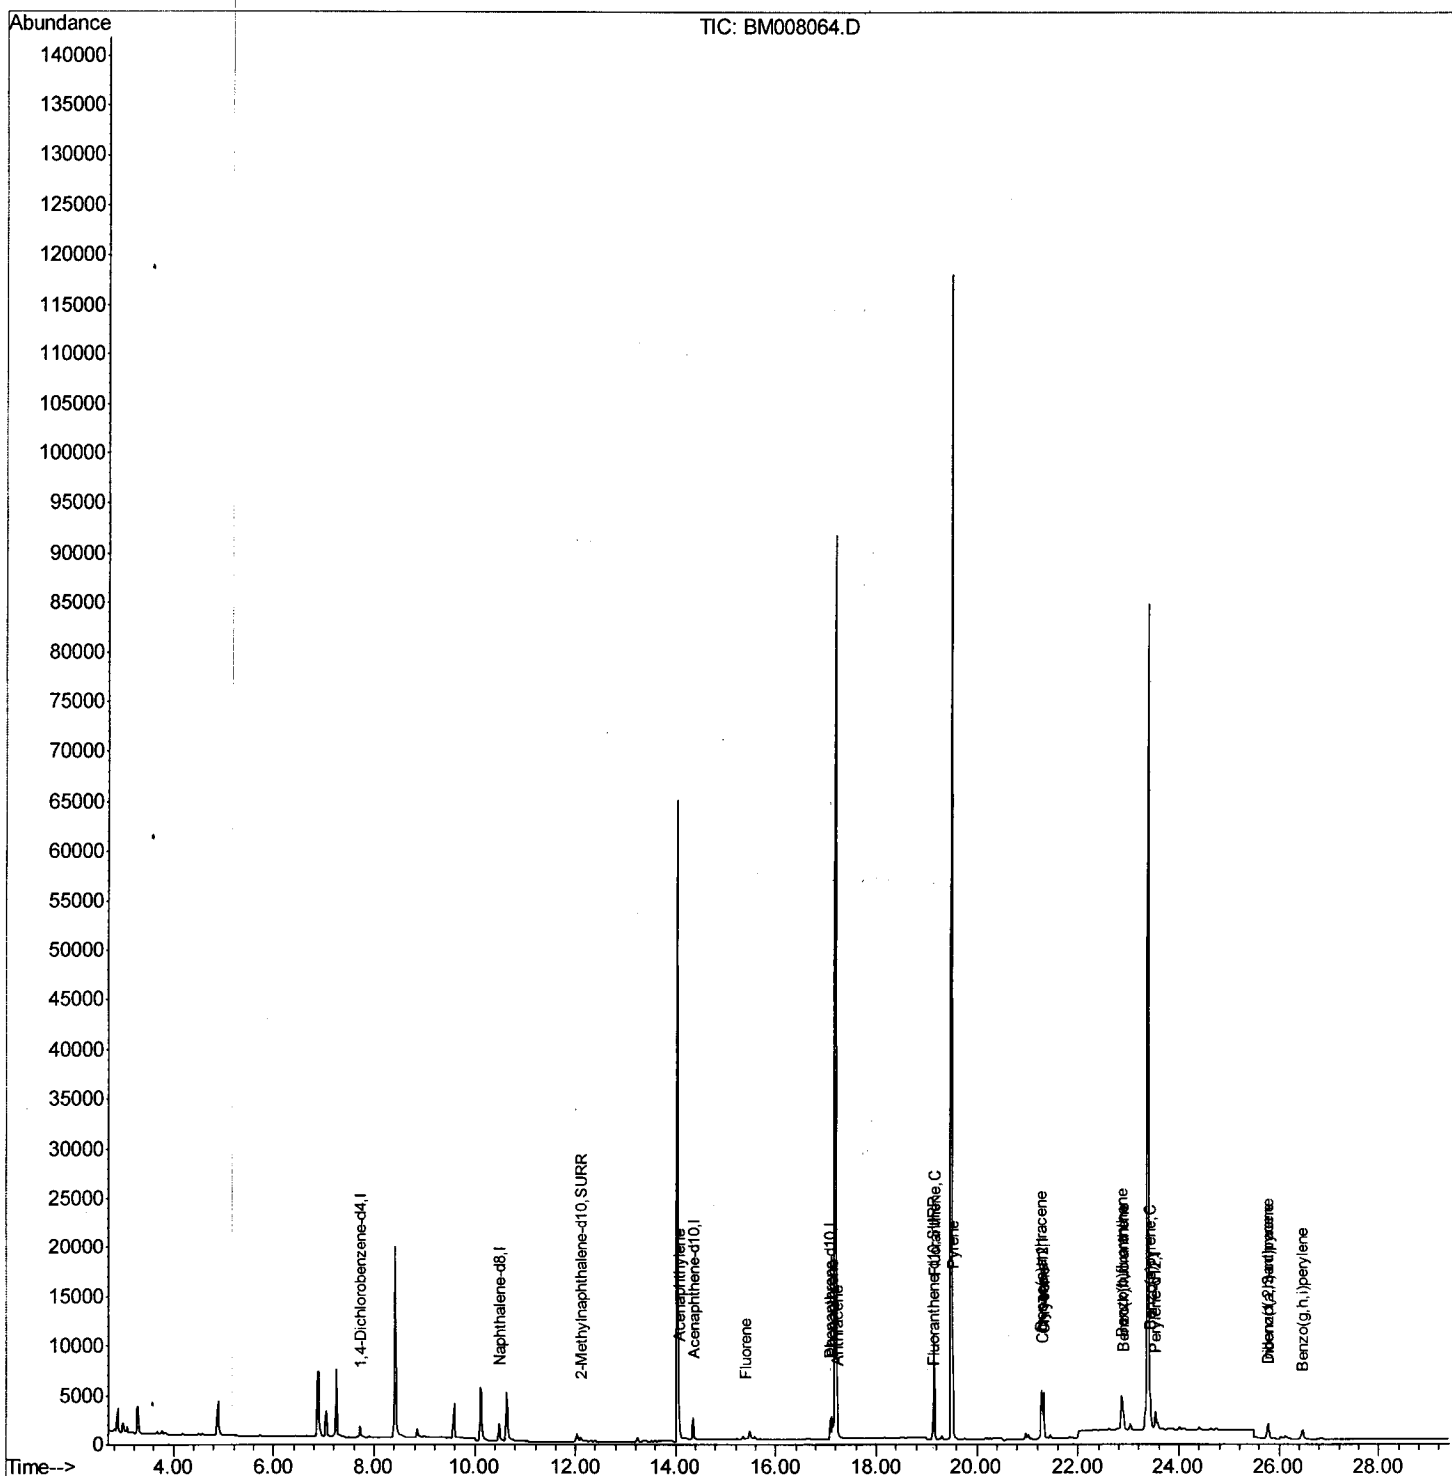

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

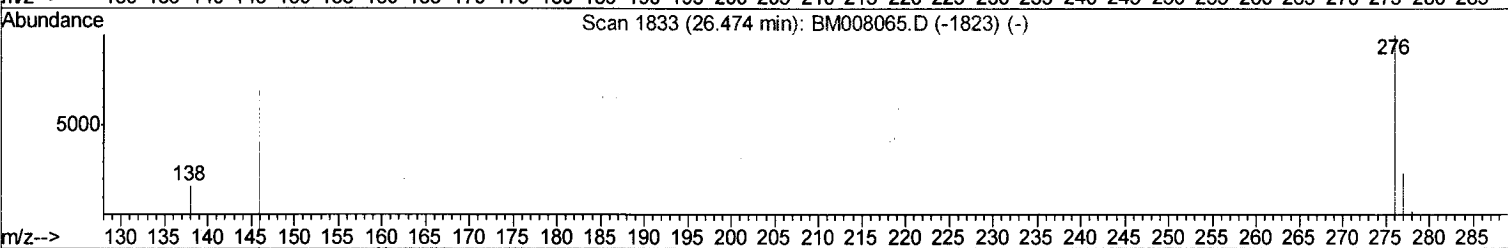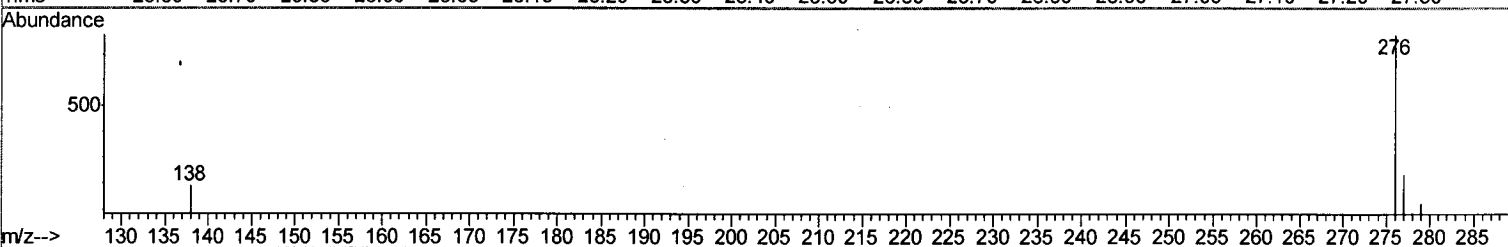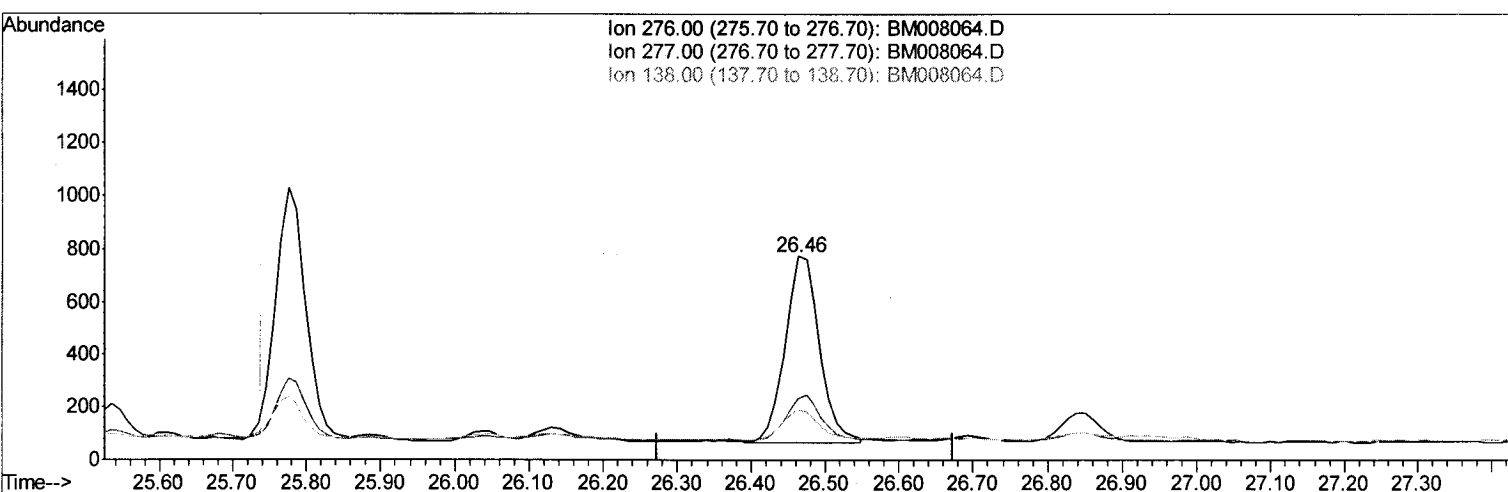

TIC: BM008064.D

(26) Benzo(g,h,i)perylene

26.464min (-0.010) 0.23ng/ul m

response 2297

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	30.49
138.00	25.60	24.81
0.00	0.00	0.00

S. J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

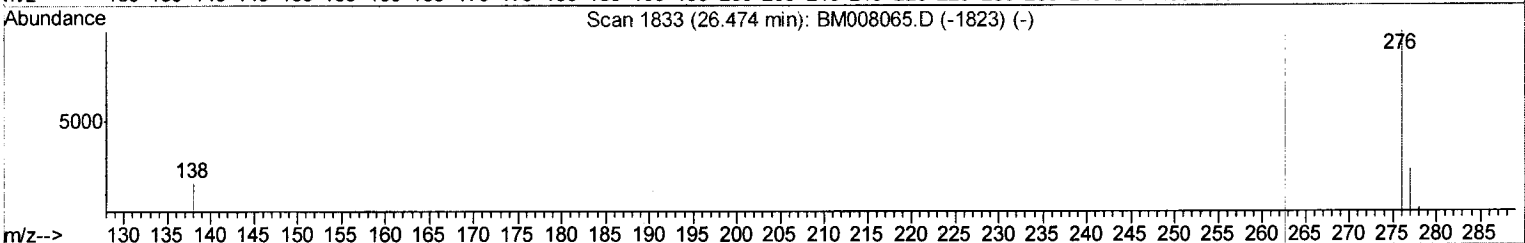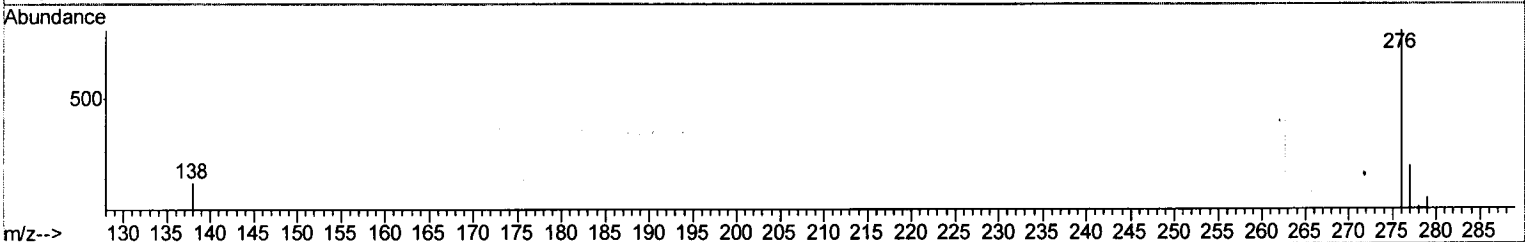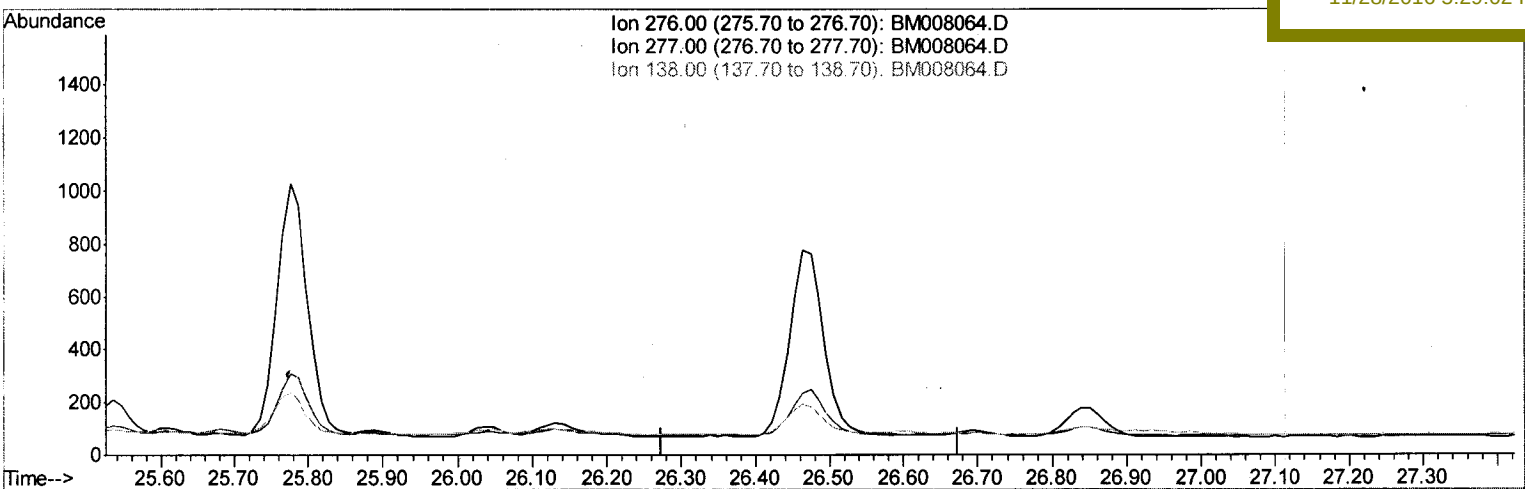

TIC: BM008064.D

(26) Benzo(g,h,i)perylene

26.474min (-26.474) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

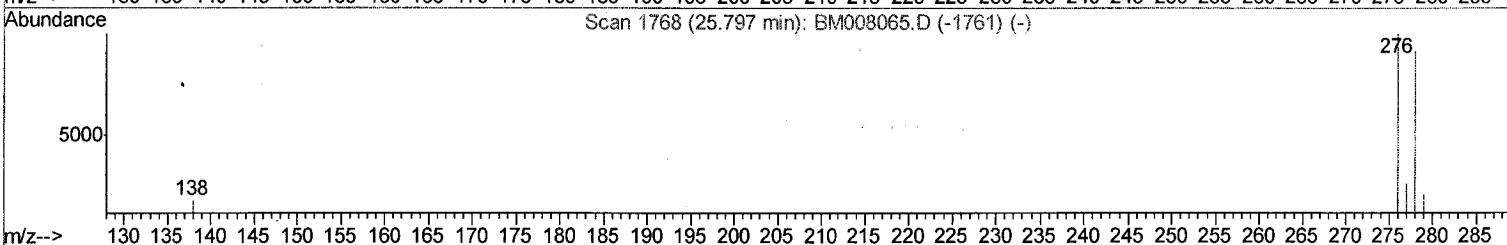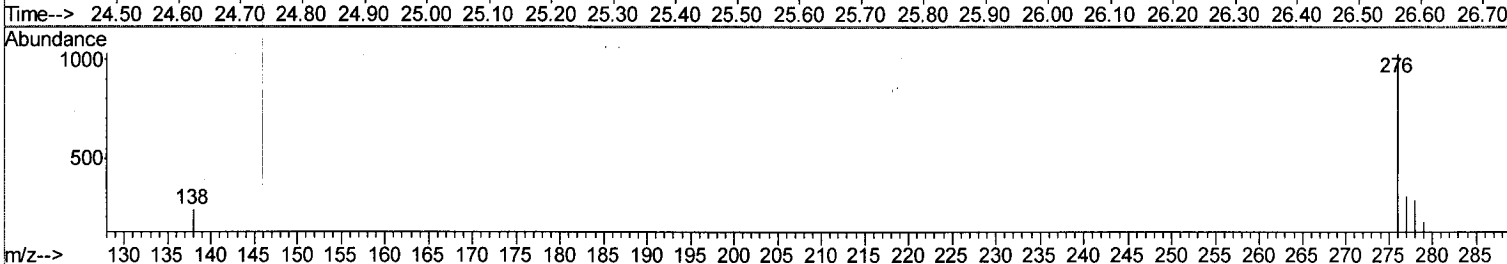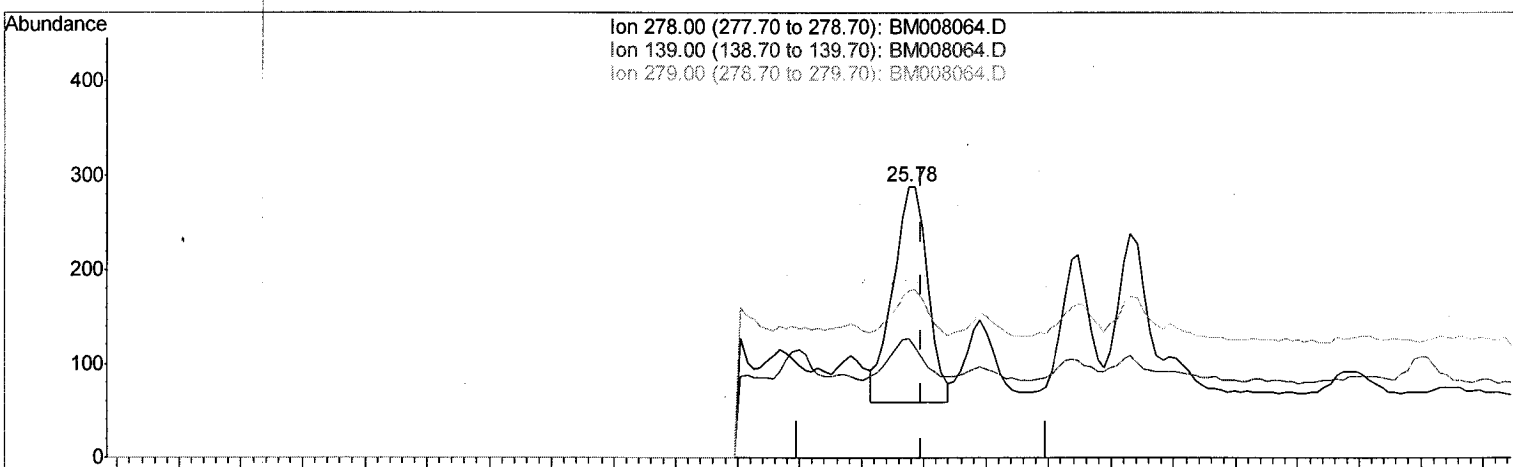

TIC: BM008064.D

(25) Dibenzo(a,h)anthracene

25.776min (-0.021) 0.10ng/ul m

response 892

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	44.10#
279.00	32.40	61.81#
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

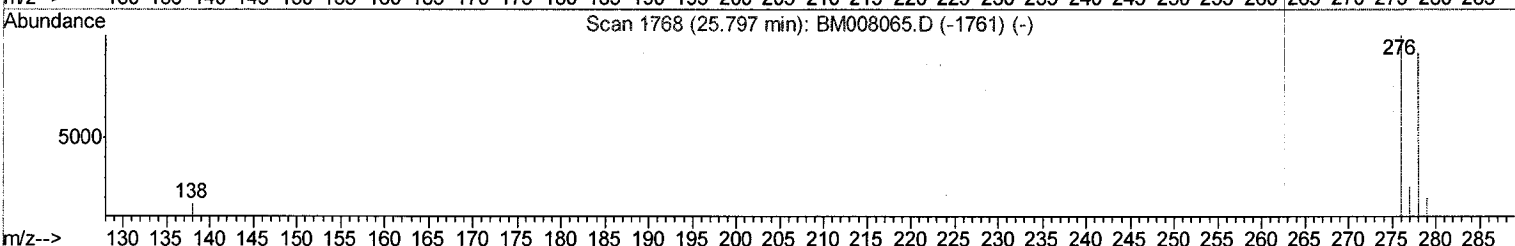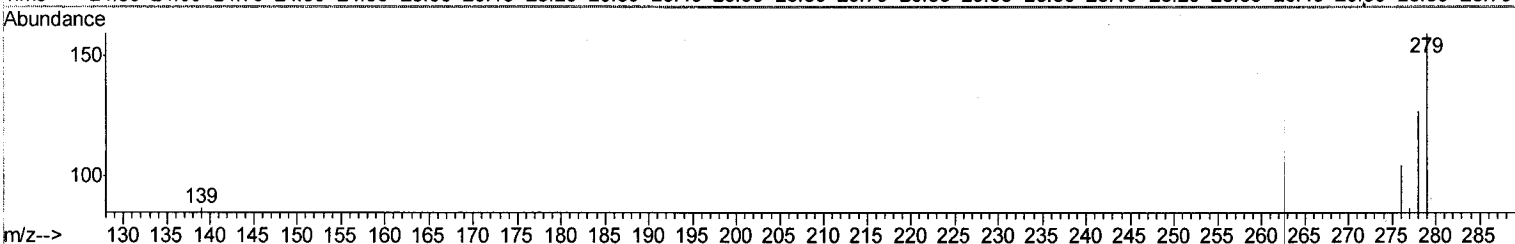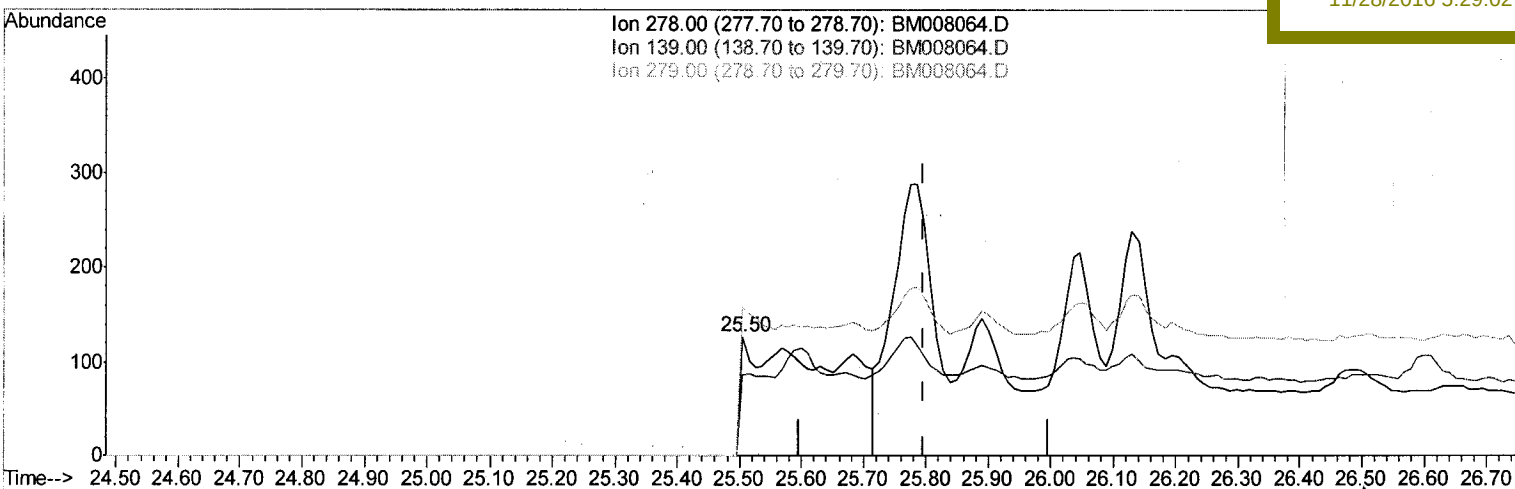

TIC: BM008064.D

(25) Dibenzo(a,h)anthracene

25.505min (-0.292) 0.15ng/ul

response 1324

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	68.50#
279.00	32.40	125.20#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

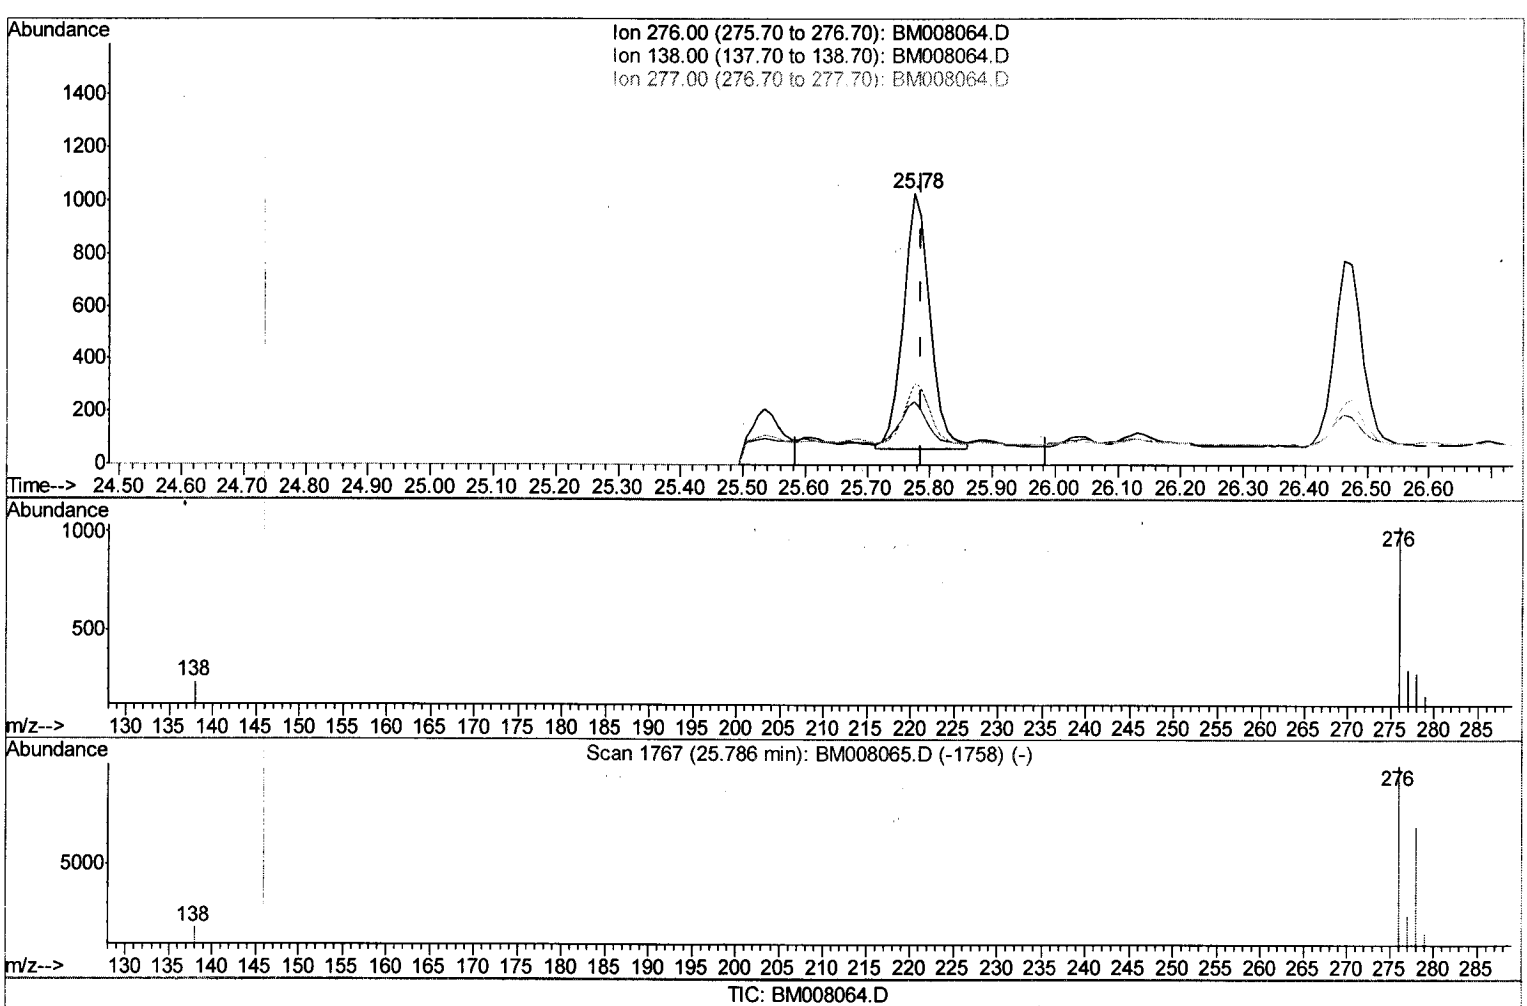

(24) Indeno(1,2,3-cd)pyrene

25.776min (-0.010) 0.25ng/ul m

response 2855

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	44.03#
0.00	0.00	0.00

S. J.
 11/29/16




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
Data File : BM008064.D
Acq On : 24 Nov 2016 09:08
Operator : UM/SJ
Sample : H5701-25
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 28 10:46:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 01:27:01 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4WG4

Manual Integrations
APPROVED

Umangi
11/28/2016 5:29:02 PM

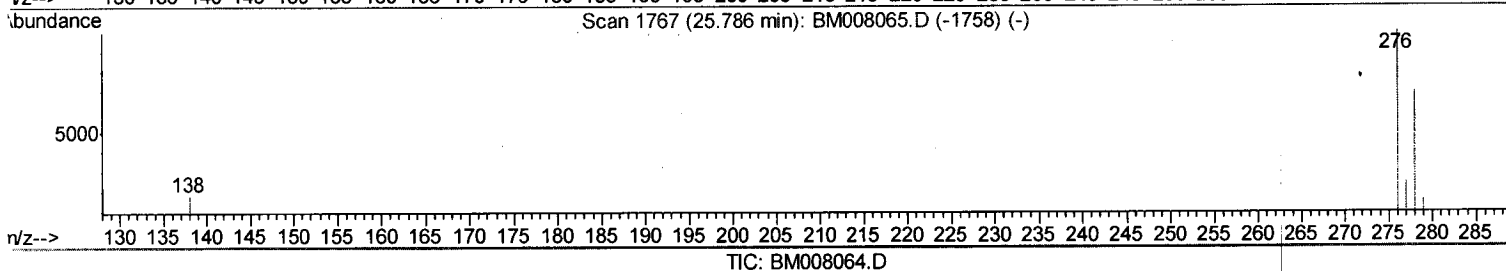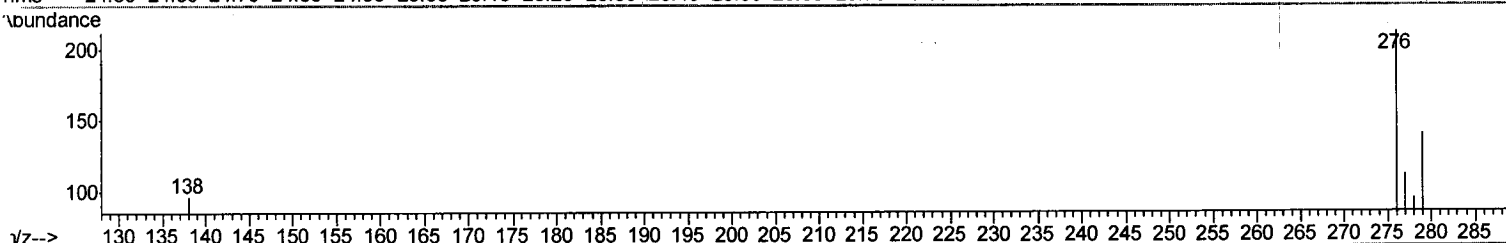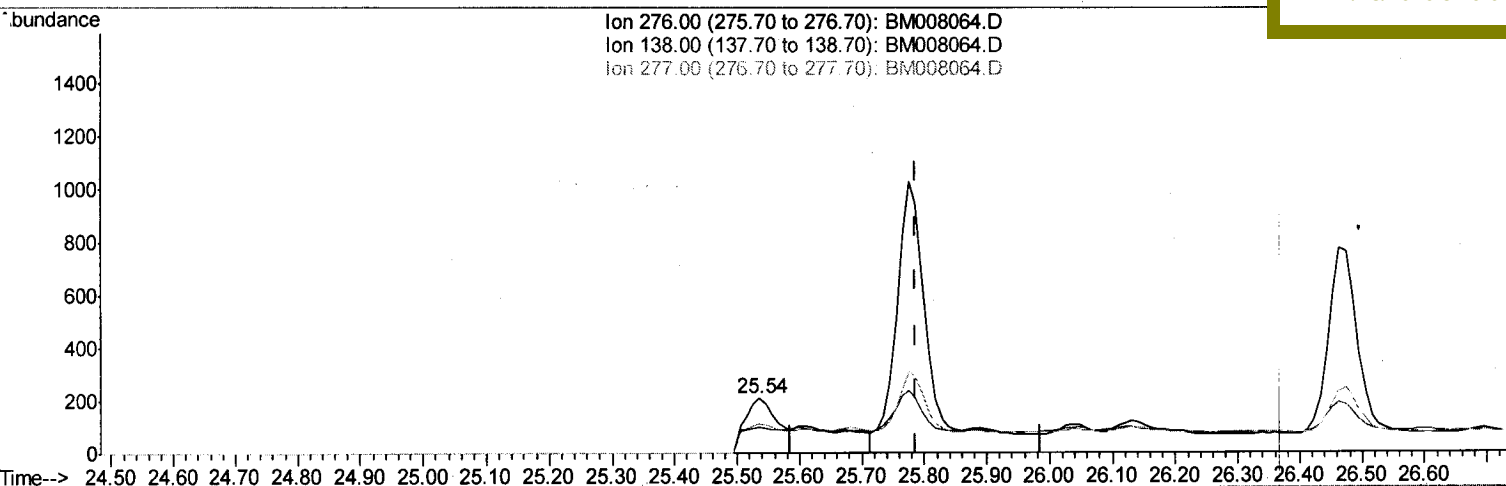

(24) Indeno(1,2,3-cd)pyrene

25.536min (-0.250) 0.13ng/ul

response 1449

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	86.75#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

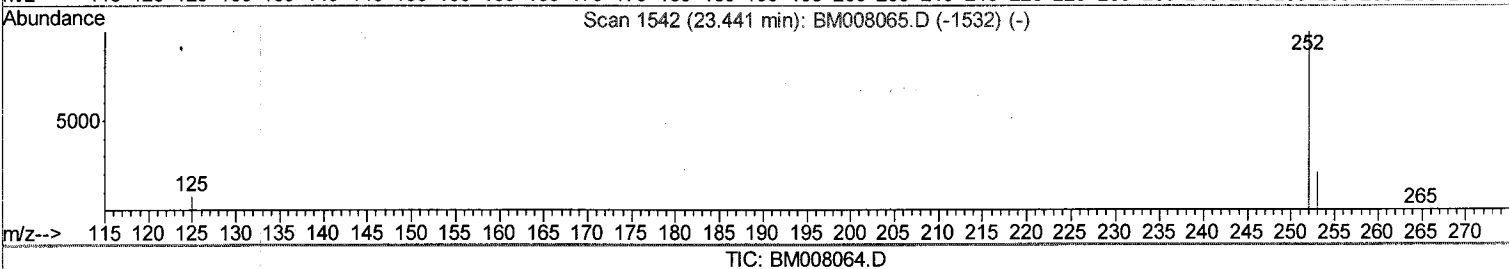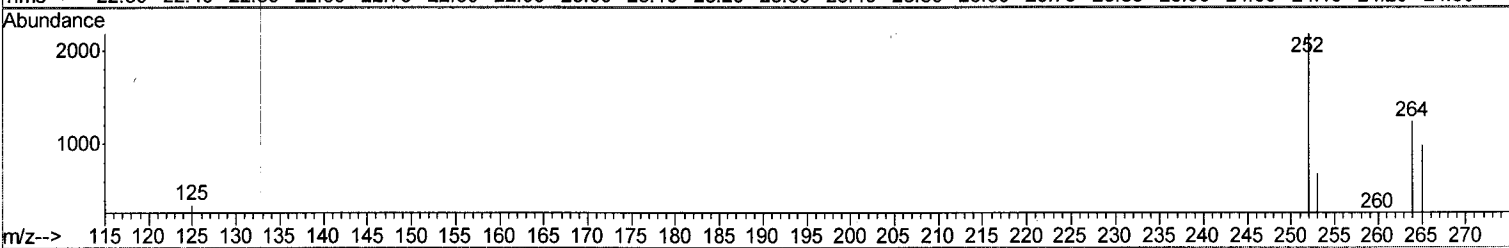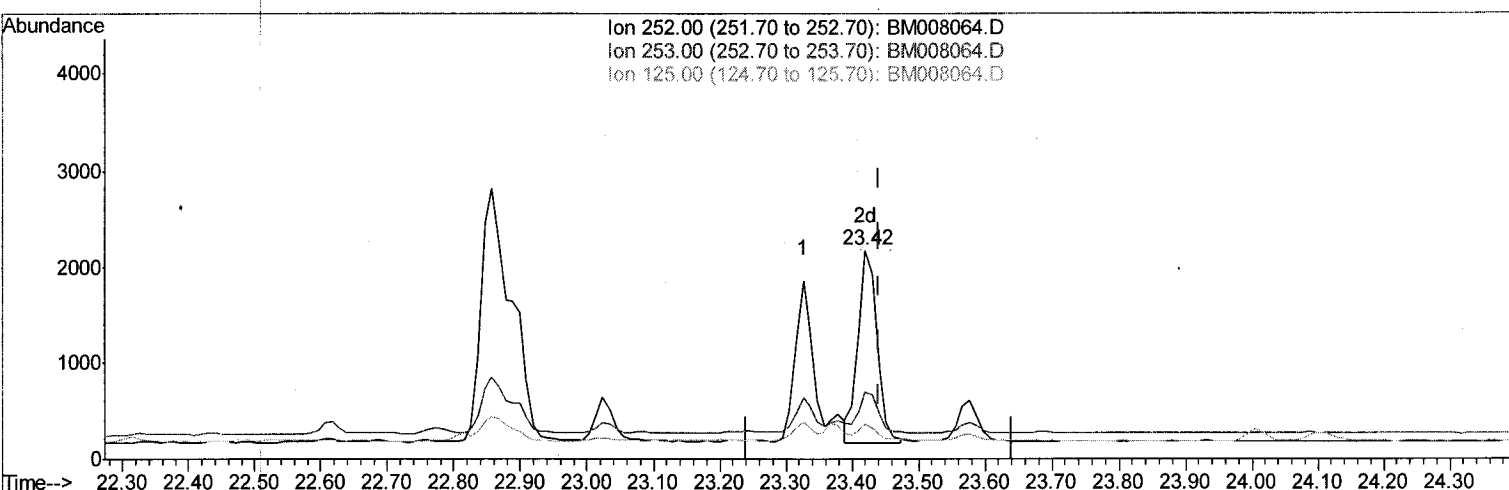

(23) Benzo(a)pyrene (C)

23.420min (-0.021) 0.44ng/ul m

response 3975

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	31.68
125.00	22.60	16.41#
0.00	0.00	0.00

S.S.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 A4WG4

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

Umangi
 11/28/2016 5:29:02 PM

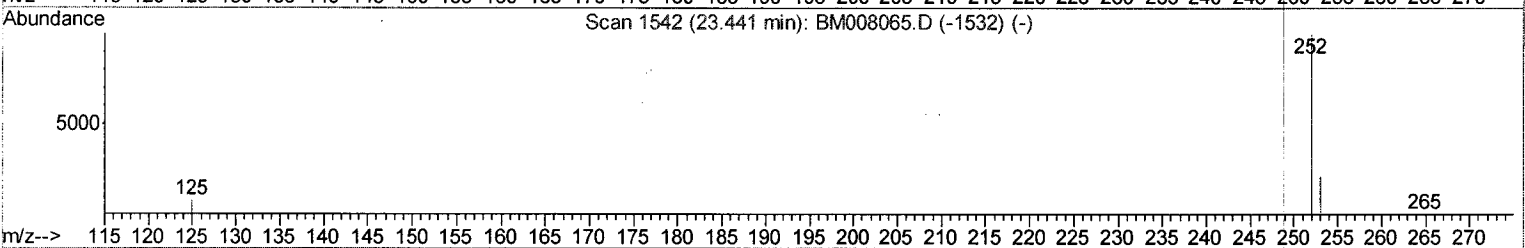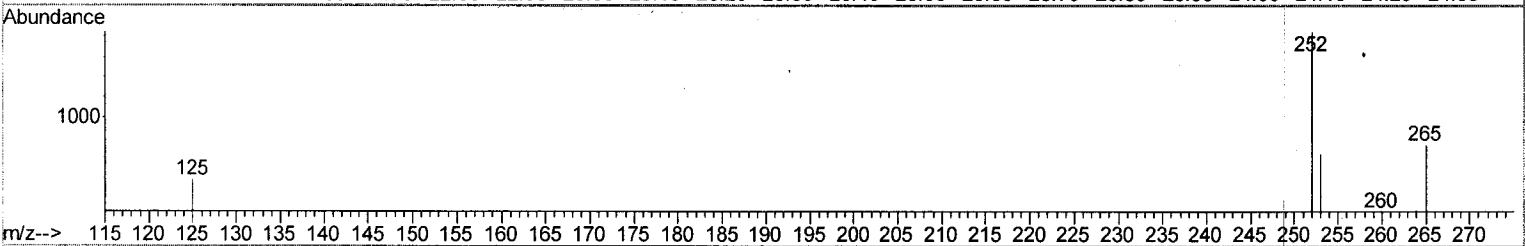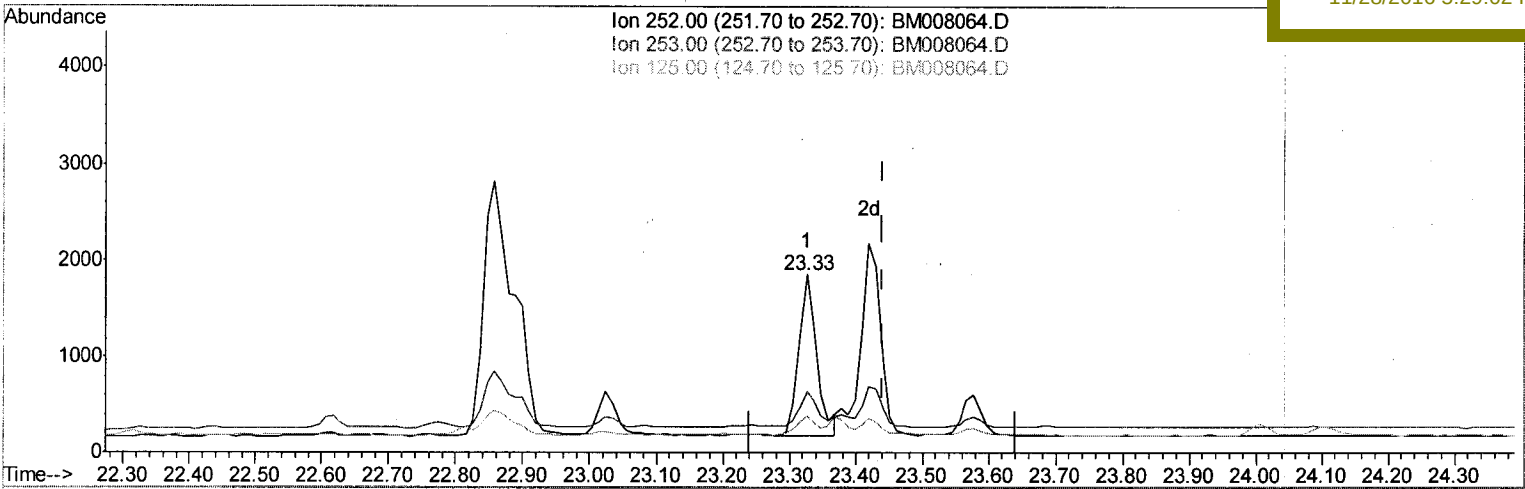

TIC: BM008064.D

(23) Benzo(a)pyrene (C)

23.326min (-0.115) 0.35ng/ul

response 3160

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	34.32
125.00	22.60	20.51
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

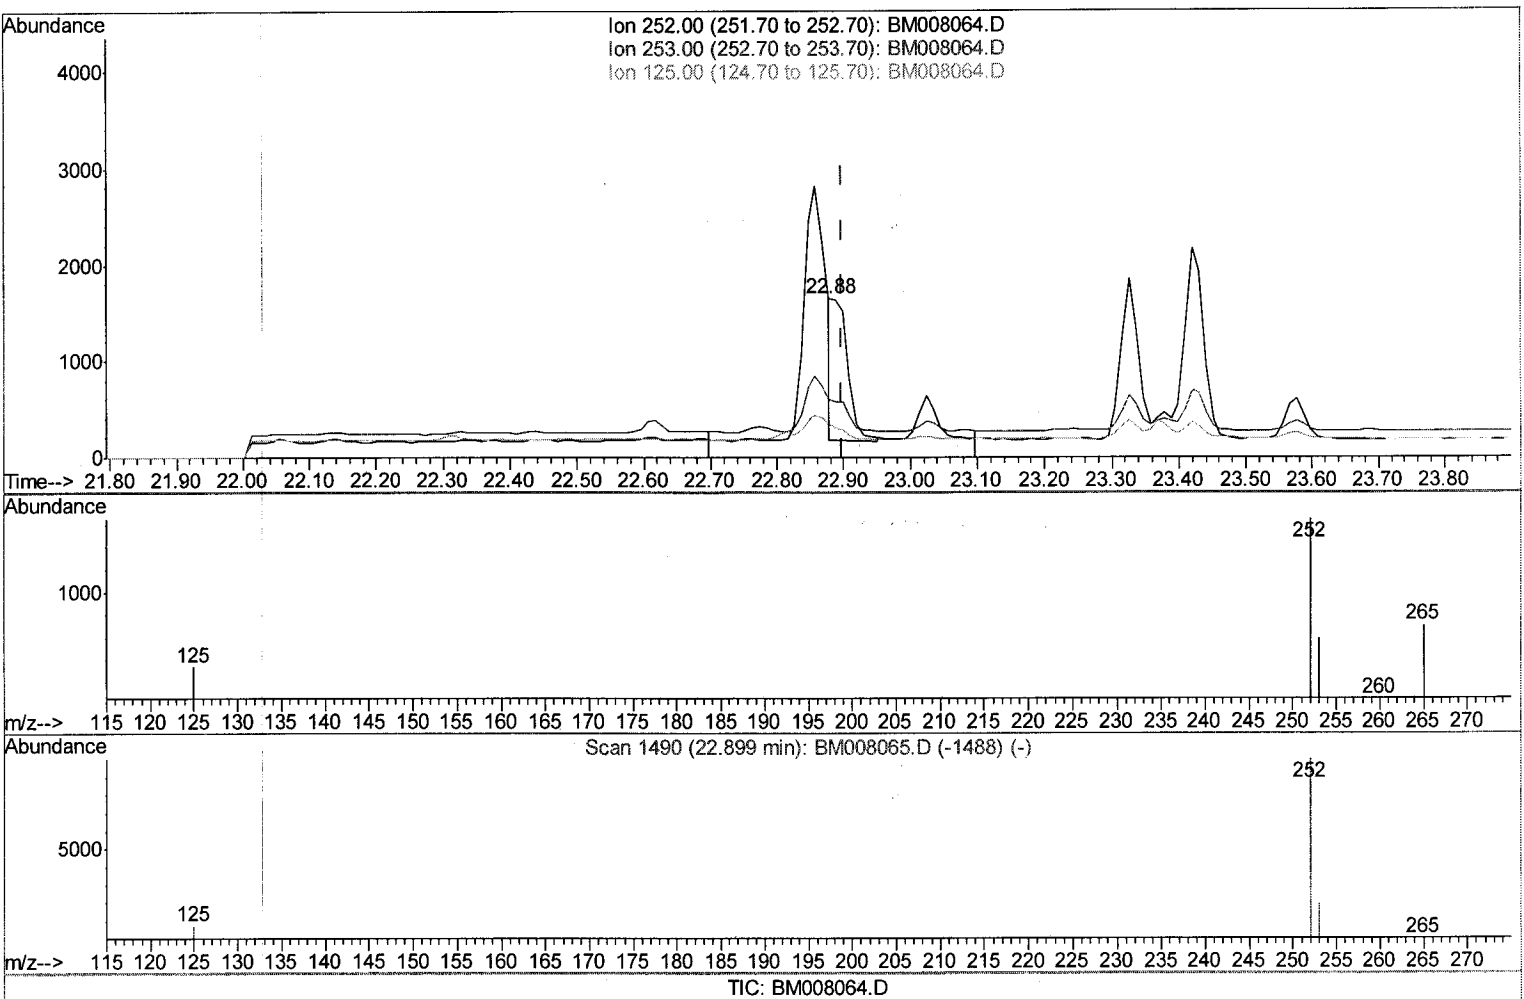

(22) Benzo(k)fluoranthene

22.878min (-0.021) 0.23ng/ul m

response 2352

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	36.30
125.00	17.10	20.69#
0.00	0.00	0.00

S. J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

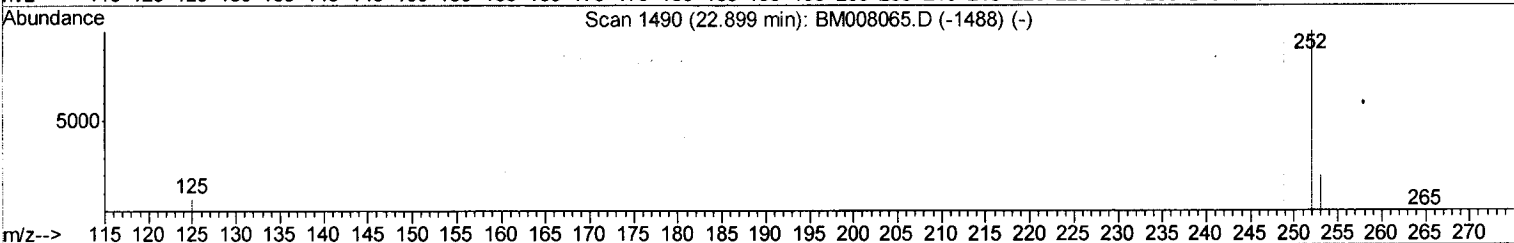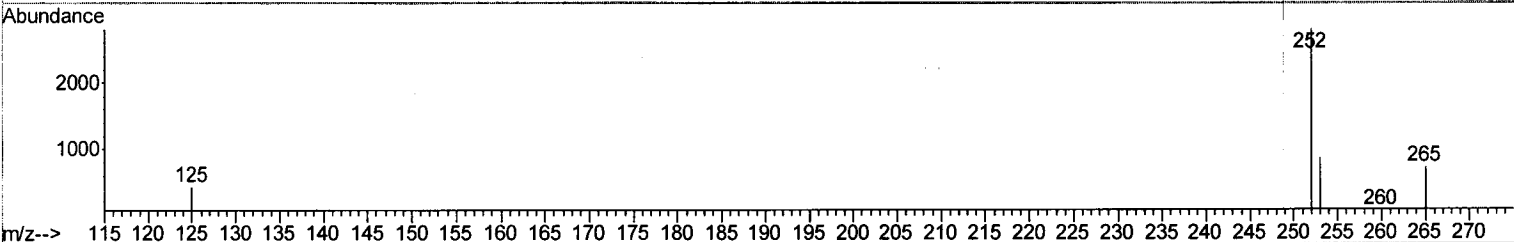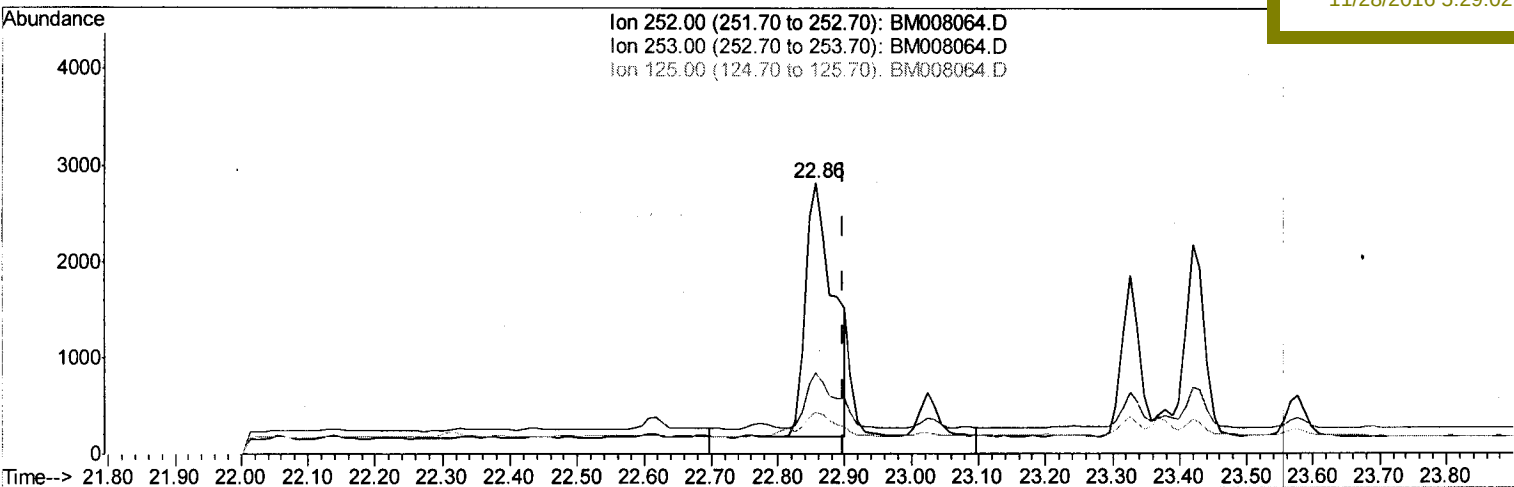

TIC: BM008064.D

(22) Benzo(k)fluoranthene

22.857min (-0.042) 0.77ng/ul

response 7695

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	30.12
125.00	17.10	15.31
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

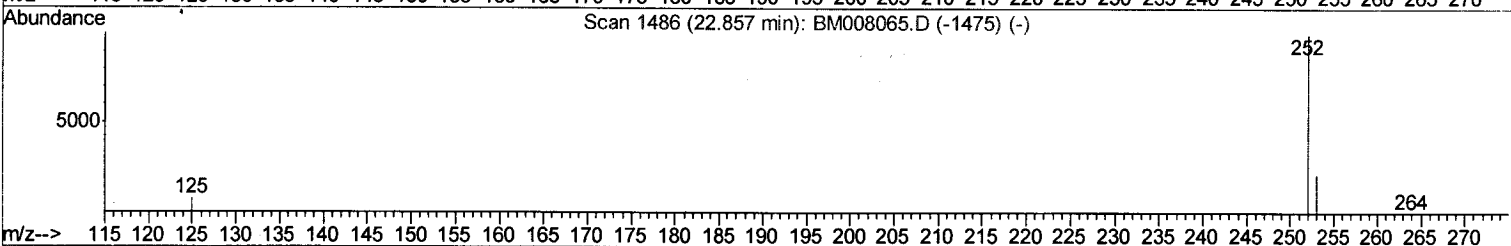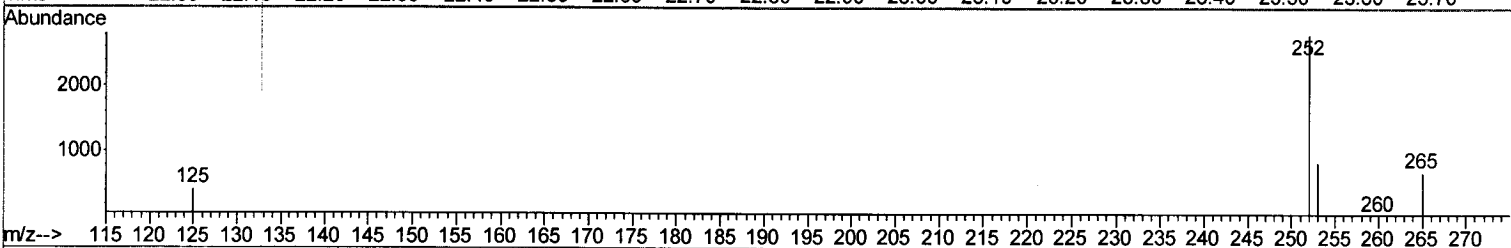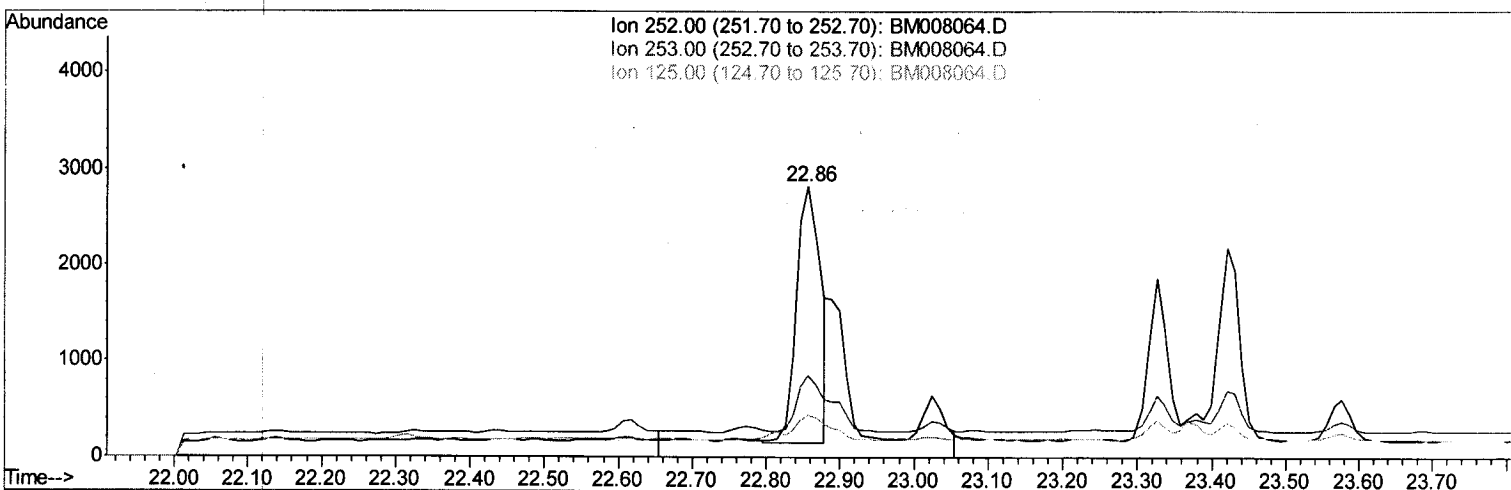

TIC: BM008064.D

(21) Benzo(b)fluoranthene

22.857min (+0.000) 0.62ng/ul m

response 6044

S.J.
 11/29/16

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	30.12
125.00	17.50	15.31
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 28 10:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

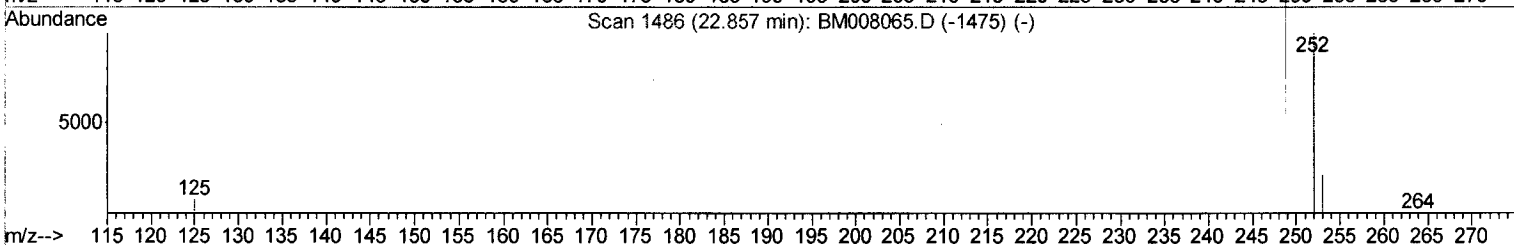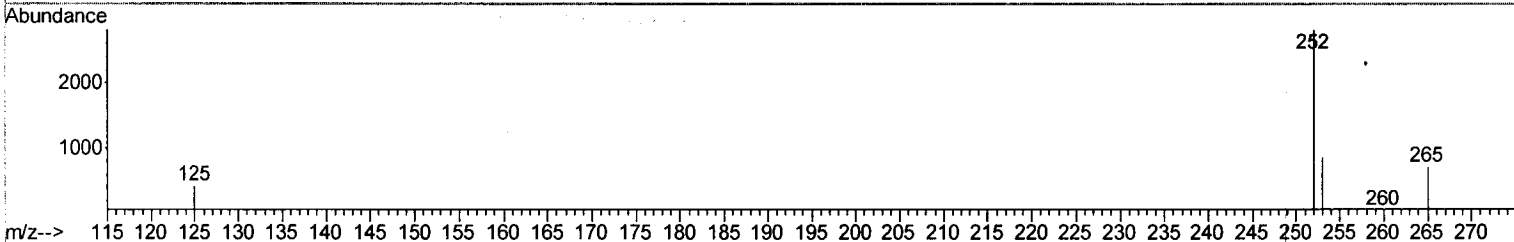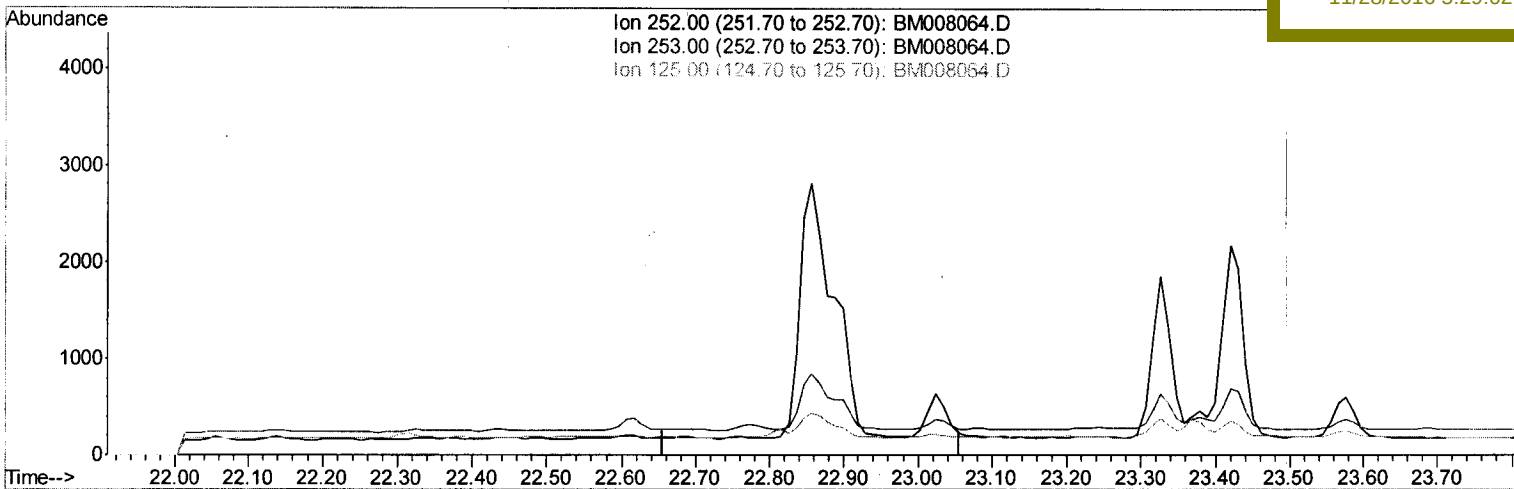

TIC: BM008064.D

(21) Benzo(b)fluoranthene

22.857min (-22.857) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	32.10	0.00
125.00	17.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:45:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

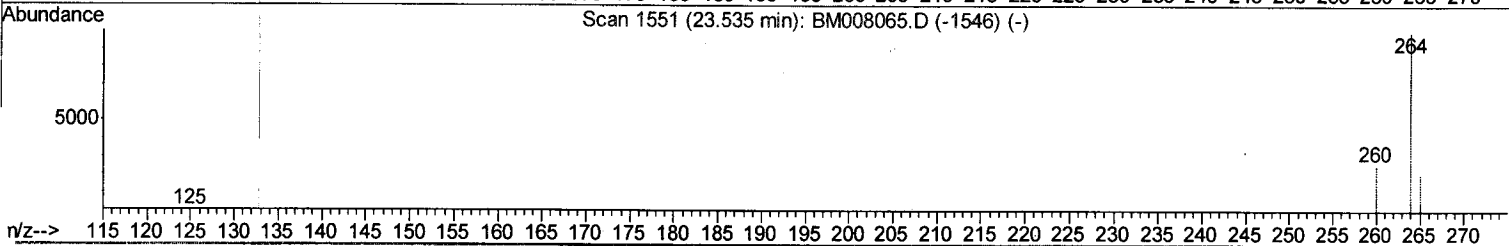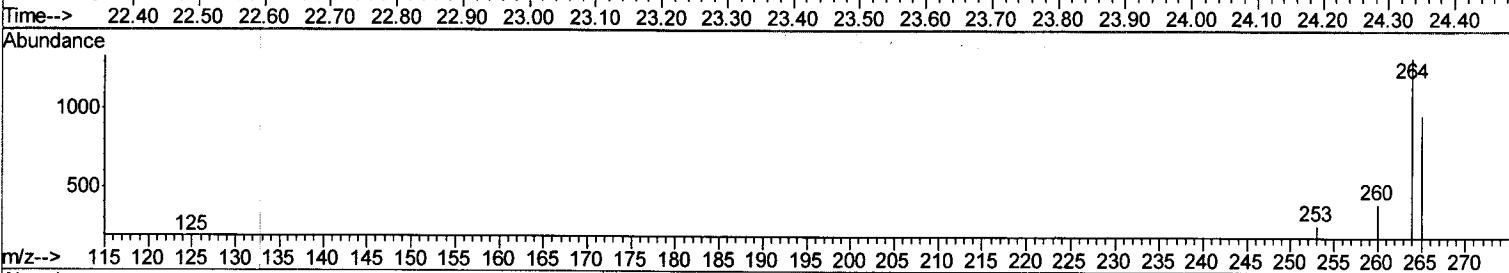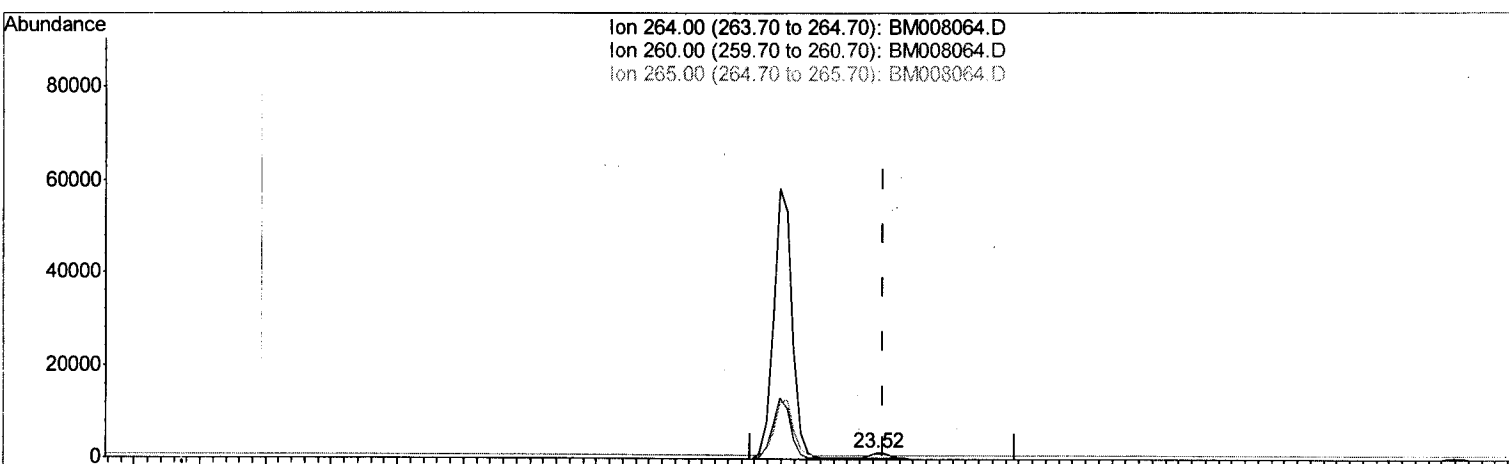

TIC: BM008064.D

(20) Perylene-d12 (I)

23.524min (-0.010) 0.40ng/ul m

response 2437

Ion Exp% Act%

264.00 100 100

260.00 30.10 30.13

265.00 103.50 72.18#

0.00 0.00 0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
Data File : BM008064.D
Acq On : 24 Nov 2016 09:08
Operator : UM/SJ
Sample : H5701-25
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 28 10:45:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 01:27:01 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4WG4

Manual Integrations
APPROVED

Umangi
11/28/2016 5:29:02 PM

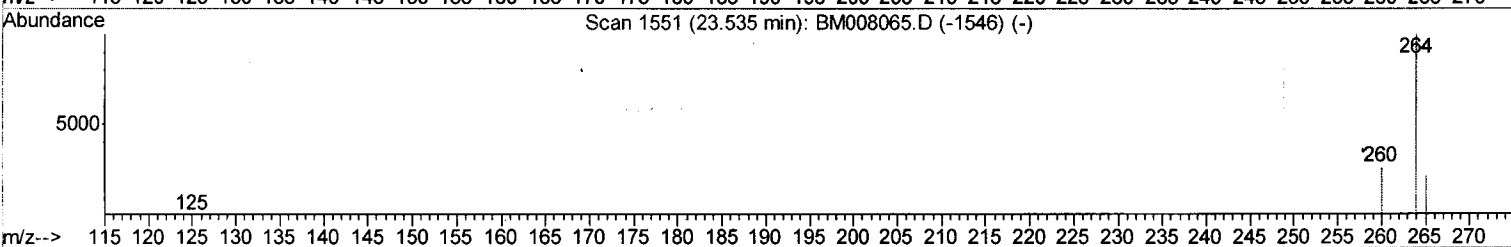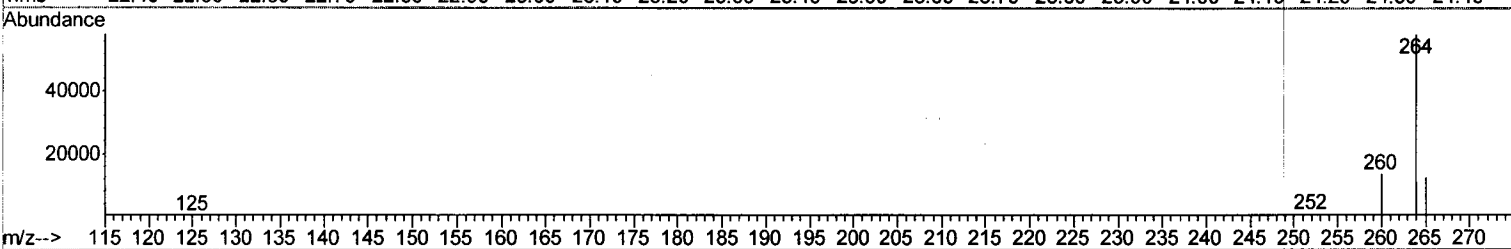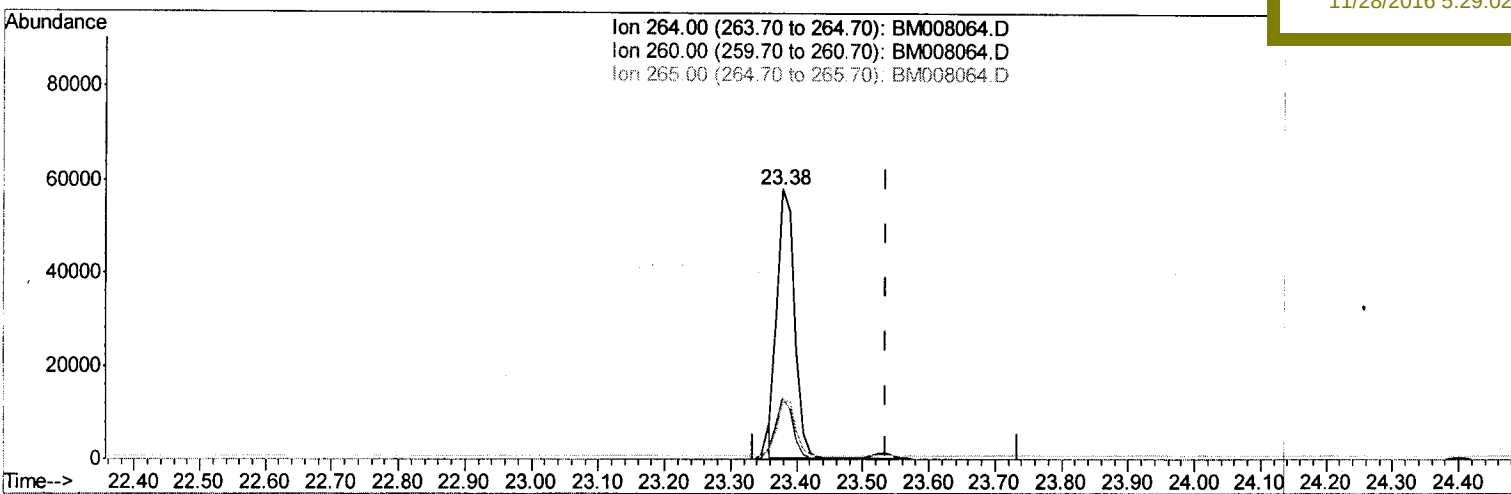

TIC: BM008064.D

(20) Perylene-d12 (I)

23.378min (-0.156) 0.40ng/ul

response 108008

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.80#
265.00	103.50	21.06#
0.00	0.00	0.00




```
Data Path   : Z:\HPCHEM1\BNA_M\Data\BM112316\  
Data File  : BM008064.D  
Acq On     : 24 Nov 2016   09:08  
Operator   : UM/SJ  
Sample     : H5701-25  
Misc       :  
ALS Vial   : 31      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
A4WG4

Manual Integrations
APPROVED

Umangi
11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:45:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 01:27:01 2016
Response via : Initial Calibration

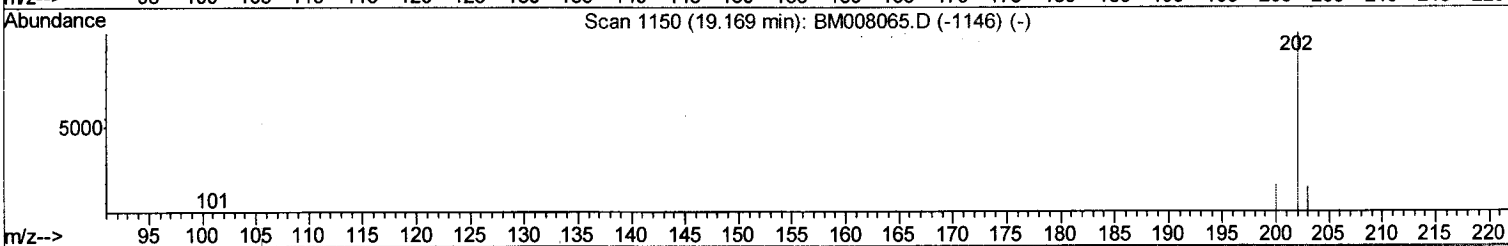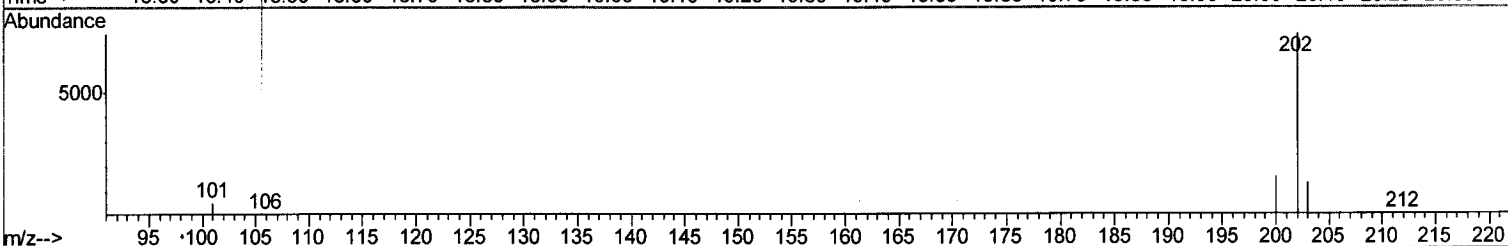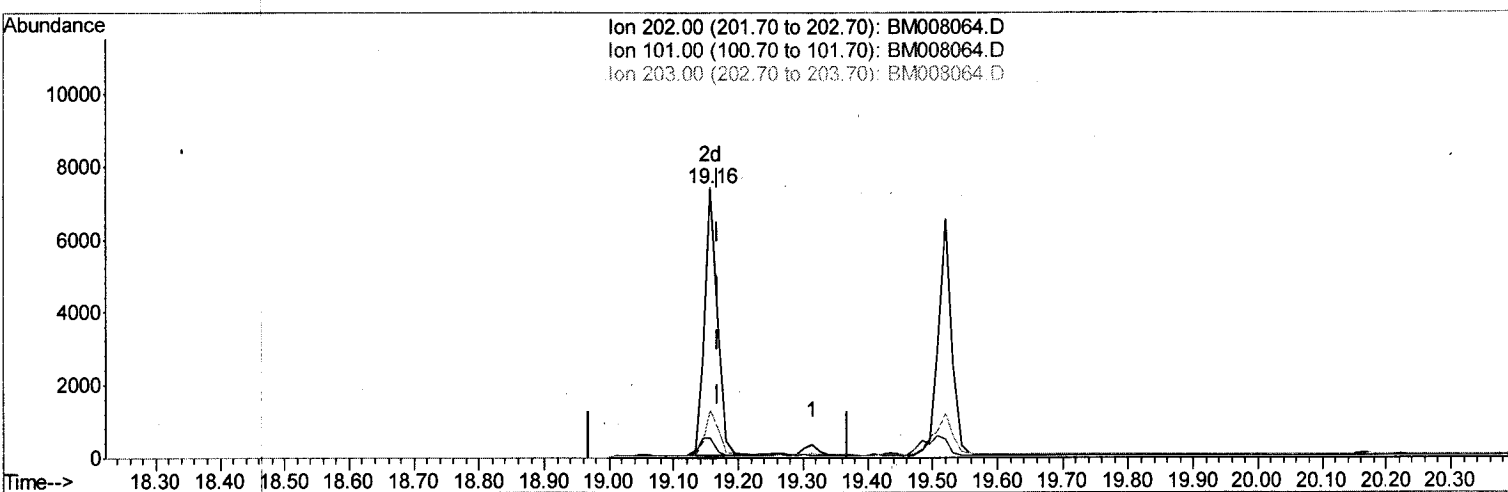

TIC: BM008064.D

(15) Fluoranthene (C)

19.157min (-0.012) 0.88ng/ul m

```
response 10159
```

Ion	Exp%	Act%
-----	------	------

202.00	100	100
--------	-----	-----

101.00	10.30	7.18
--------	-------	------

203.00	19.50	17.61
--------	-------	-------

0.00 0.00 0.00

$$n > \frac{S.J.}{112916}$$

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Quant Time: Nov 28 10:45:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

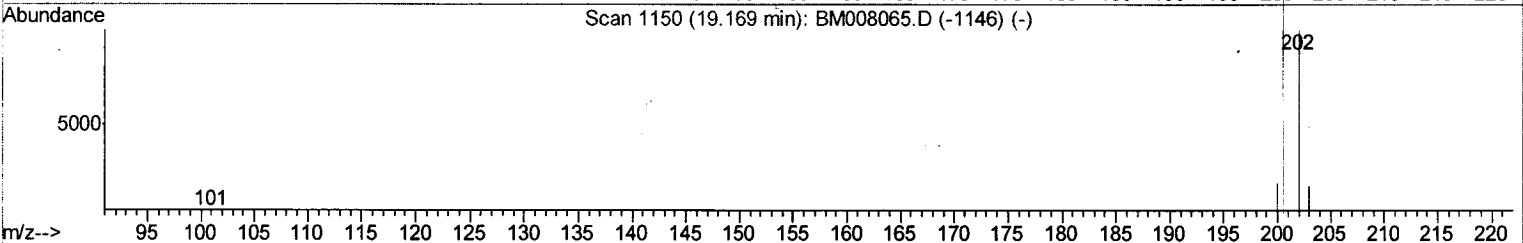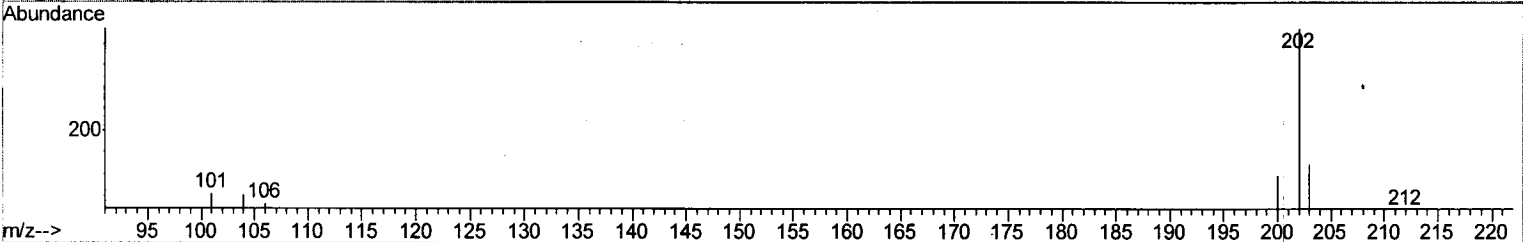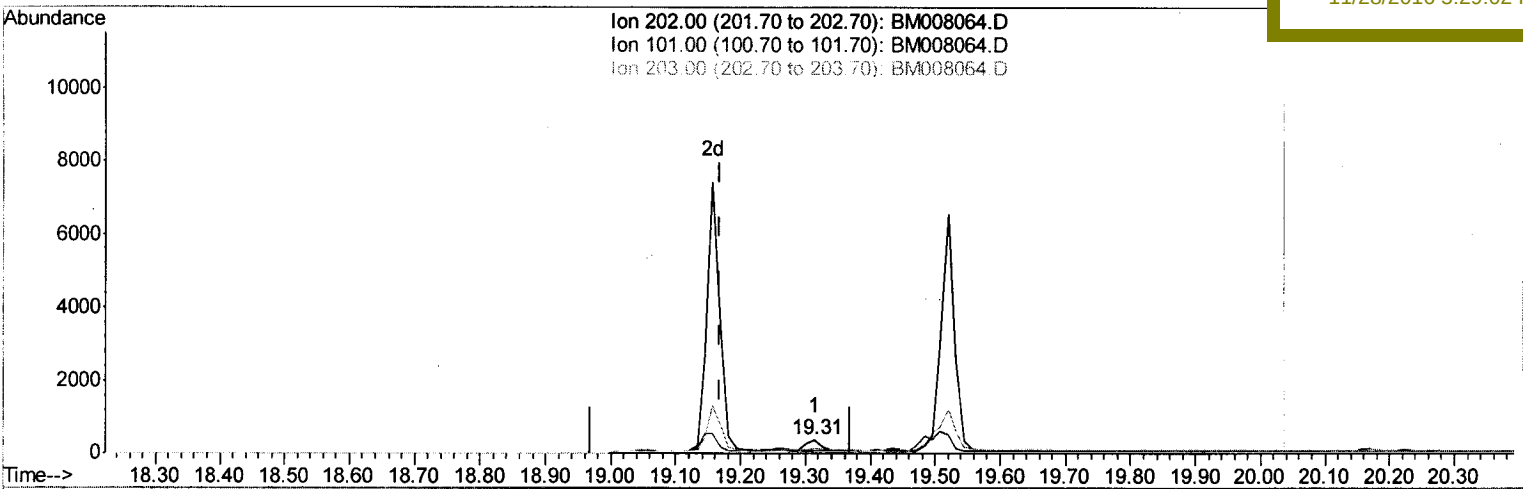

TIC: BM008064.D

(15) Fluoranthene (C)

19.314min (+0.145) 0.04ng/ul

response 502

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	21.59
203.00	19.50	35.73
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Quant Time: Nov 28 10:44:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

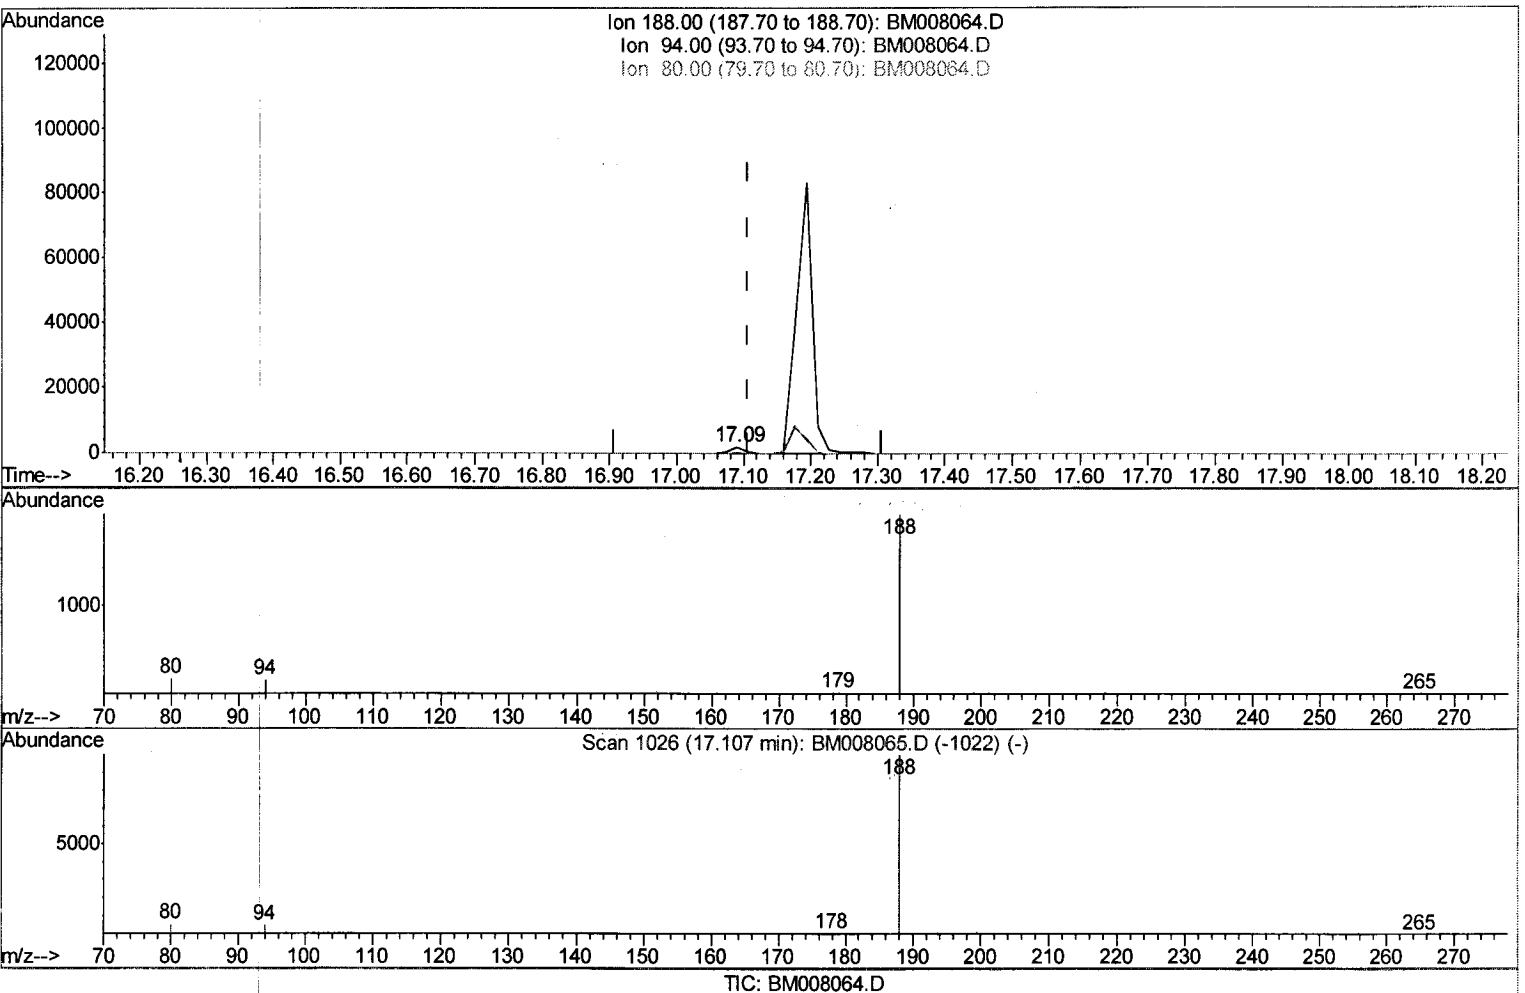

(10) Phenanthrene-d10 (I)

17.090min (-0.017) 0.40ng/ul m

response 2882

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.08
80.00	11.80	10.73
0.00	0.00	0.00

S. J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 28 10:44:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

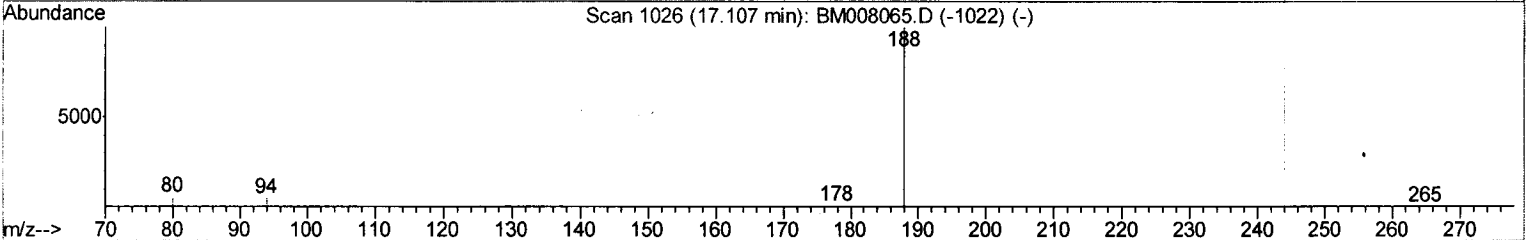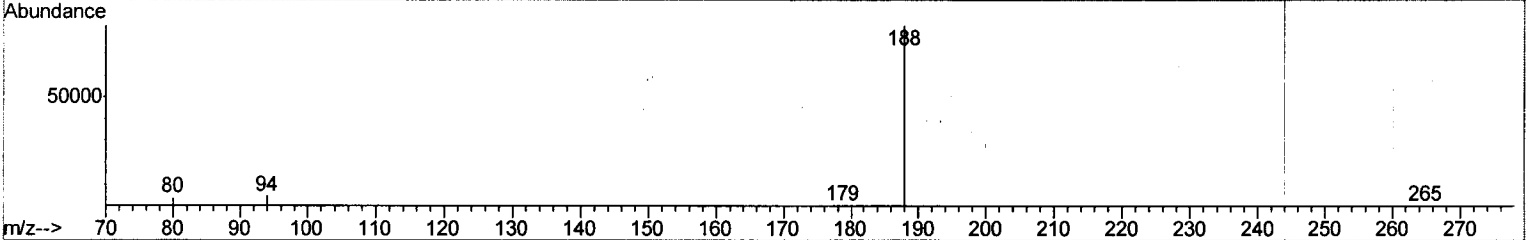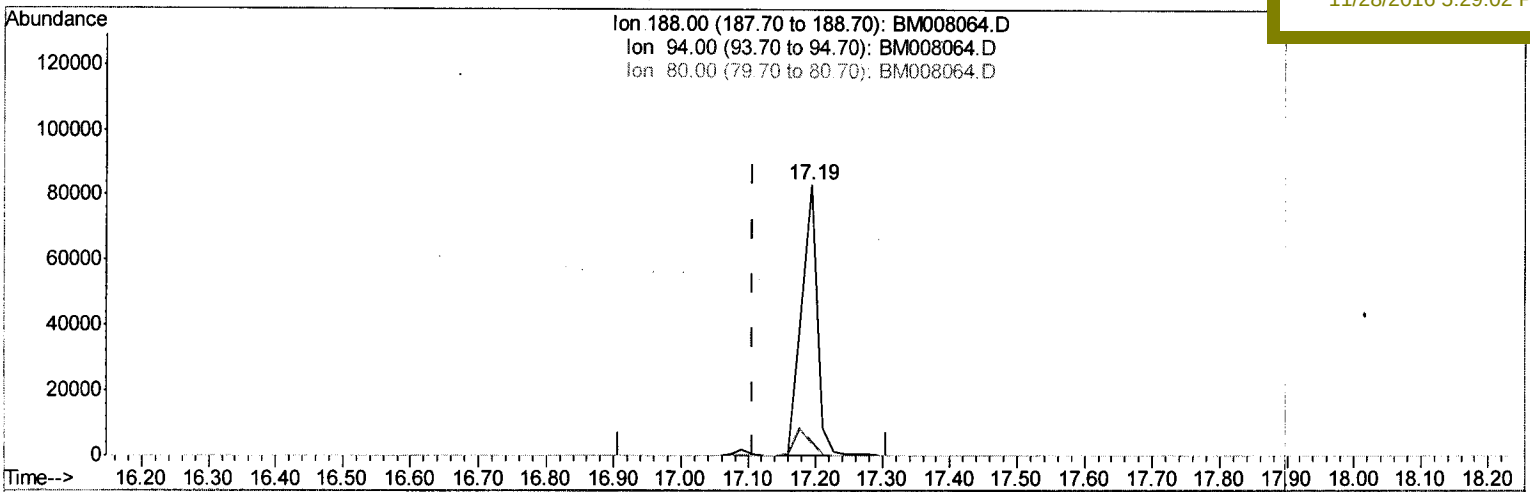

TIC: BM008064.D

(10) Phenanthrene-d10 (I)

17.193min (+0.086) 0.40ng/ul

response 134736

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.40#
80.00	11.80	4.45#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008064.D
 Acq On : 24 Nov 2016 09:08
 Operator : UM/SJ
 Sample : H5701-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WG4

Quant Time: Nov 28 10:49:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:29:02 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	718	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	2465	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.35	164	1511	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	2882m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.29	240	2877	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	2437m	0.40	ng/ul	-0.01

S.S.
 11/29/16

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.10	152	712	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	1728	0.21	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.06	152	869	0.13	ng/ul#	89
9) Fluorene	15.39	166	123	0.02	ng/ul#	67
12) Phenanthrene	17.12	178	2839	0.32	ng/ul	99
13) Anthracene	17.23	178	715	0.08	ng/ul#	80
15) Fluoranthene	19.16	202	10159m	0.88	ng/ul	
17) Pyrene	19.52	202	9228	0.92	ng/ul	97
18) Benzo(a)anthracene	21.27	228	4417	0.50	ng/ul	97
19) Chrysene	21.32	228	4836	0.44	ng/ul	96
21) Benzo(b)fluoranthene	22.86	252	6044m	0.62	ng/ul	
22) Benzo(k)fluoranthene	22.88	252	2352m	0.23	ng/ul	
23) Benzo(a)pyrene	23.42	252	3975m	0.44	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.78	276	2855m	0.25	ng/ul	
25) Dibenzo(a,h)anthracene	25.78	278	892m	0.10	ng/ul	
26) Benzo(g,h,i)perylene	26.46	276	2297m	0.23	ng/ul	

S.S.
 11/29/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed