

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:16:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

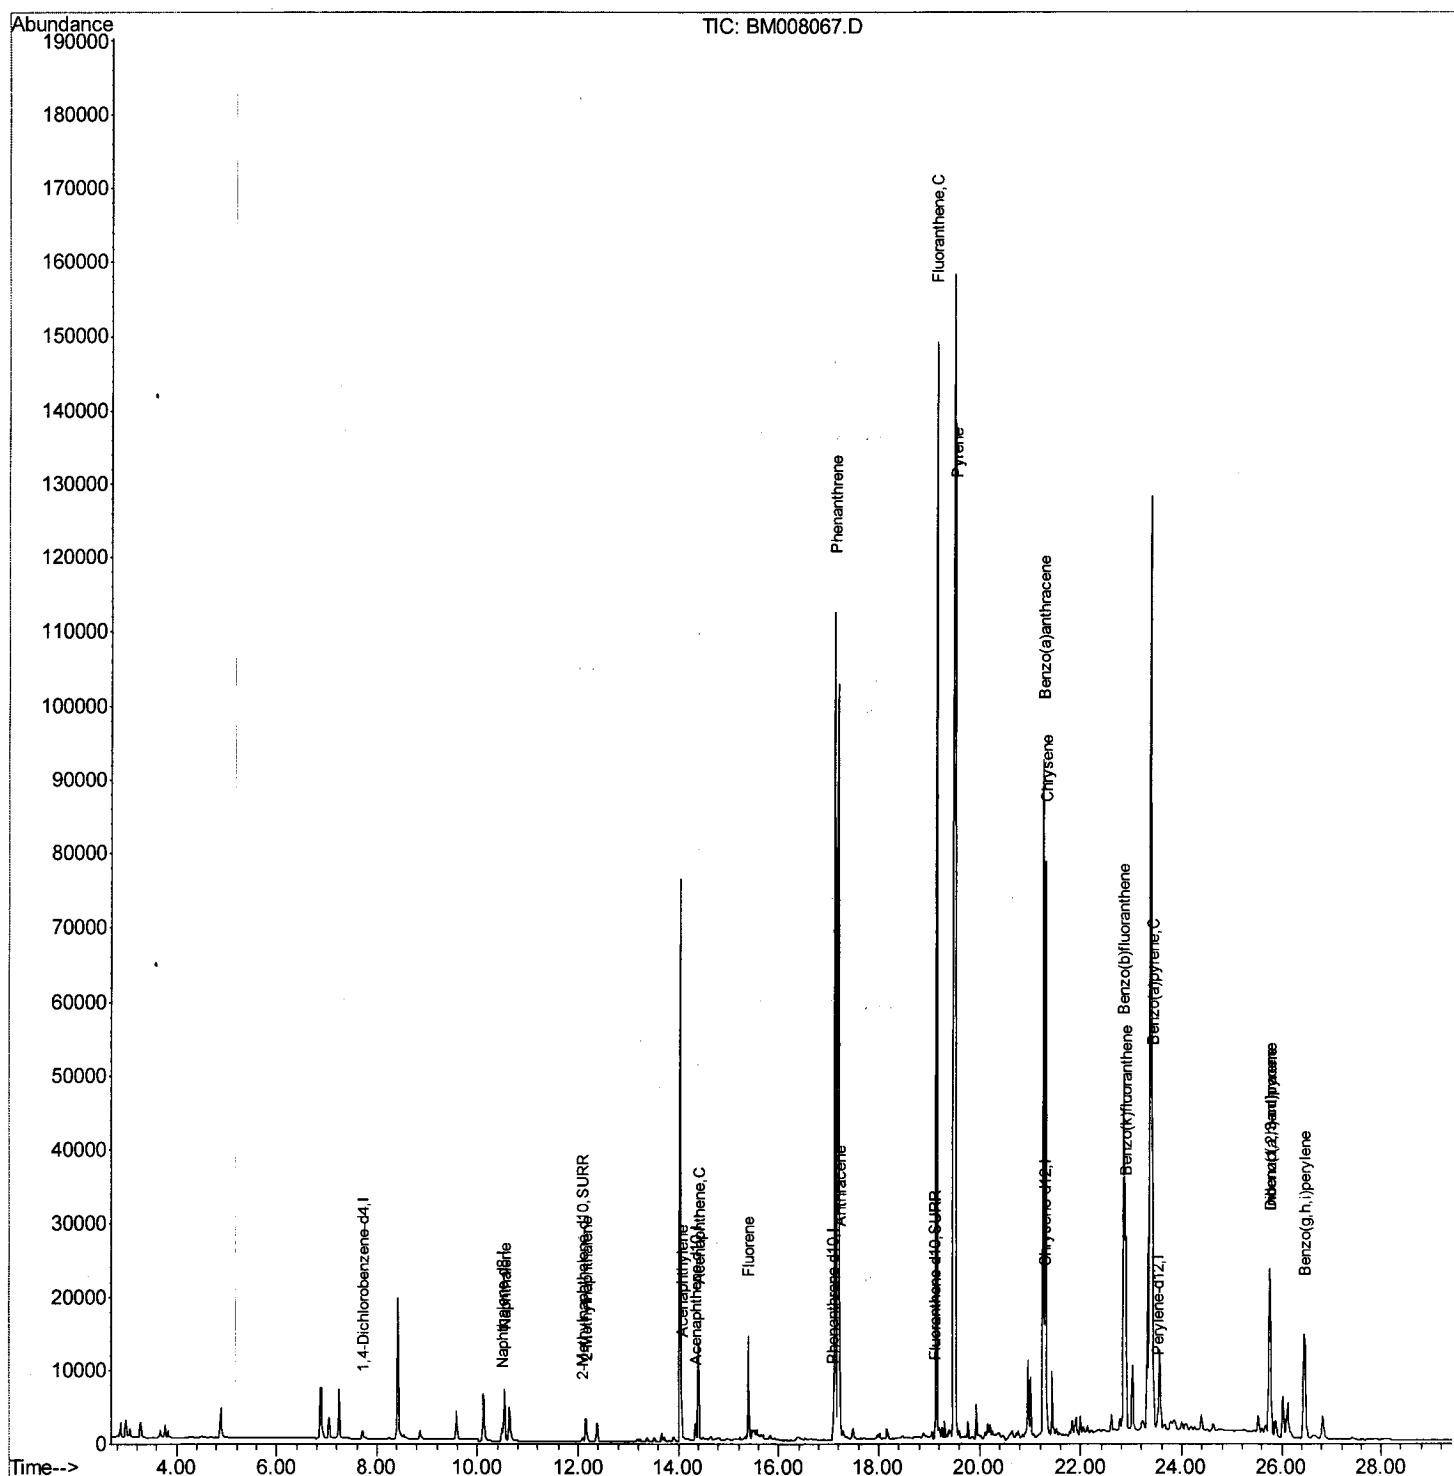

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 A4WD7

Quant Time: Nov 25 01:29:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

Umangi
 11/28/2016 5:30:01 PM

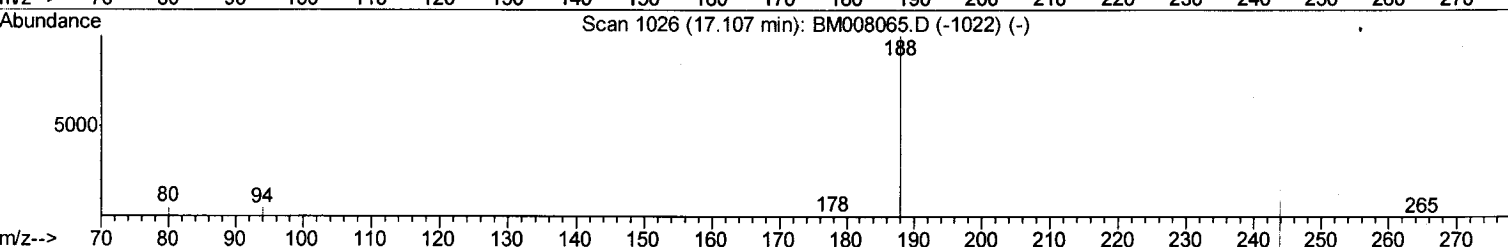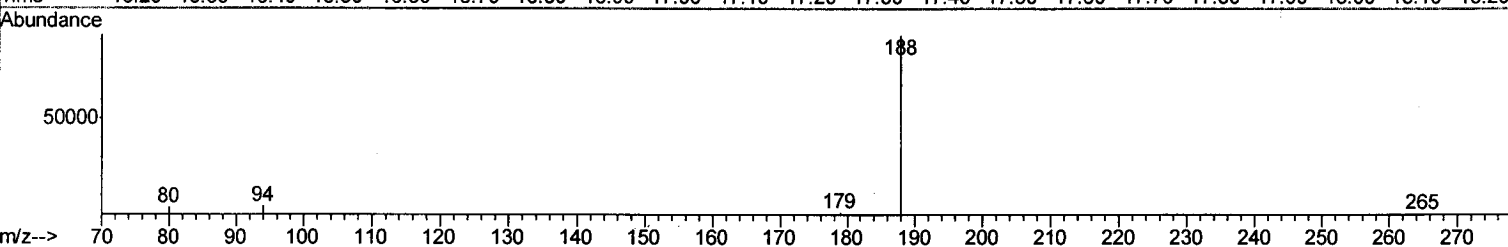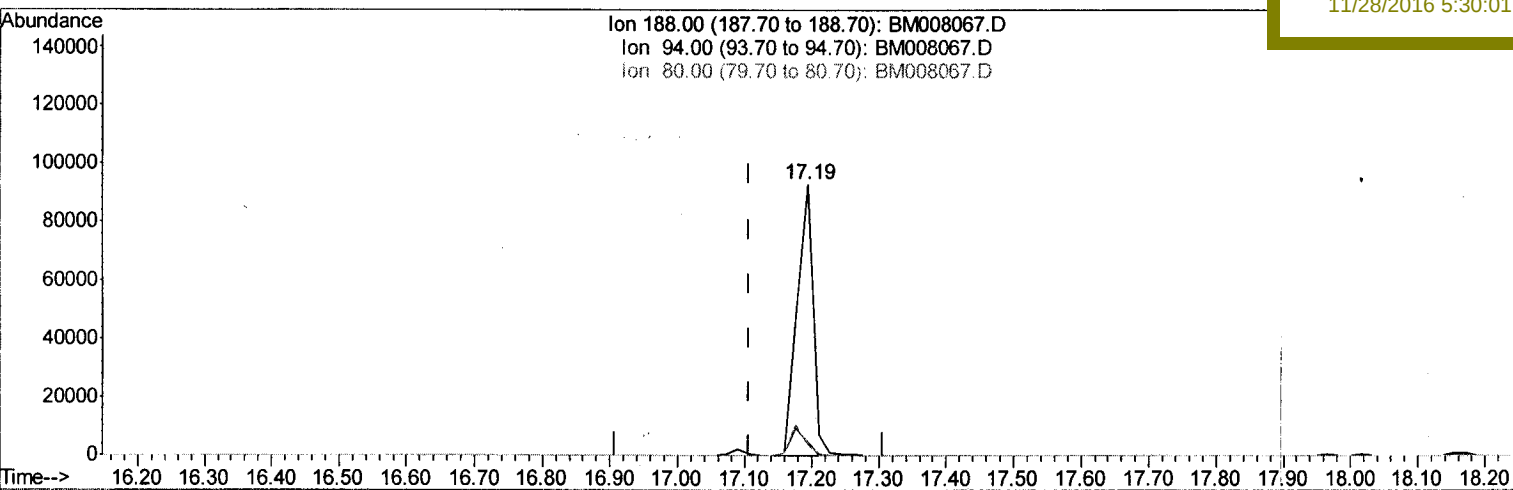

TIC: BM008067.D

(10) Phenanthrene-d10 (I)

17.193min (+0.086) 0.40ng/ul

response 153080

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	4.84#
80.00	11.80	3.95#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 01:29:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

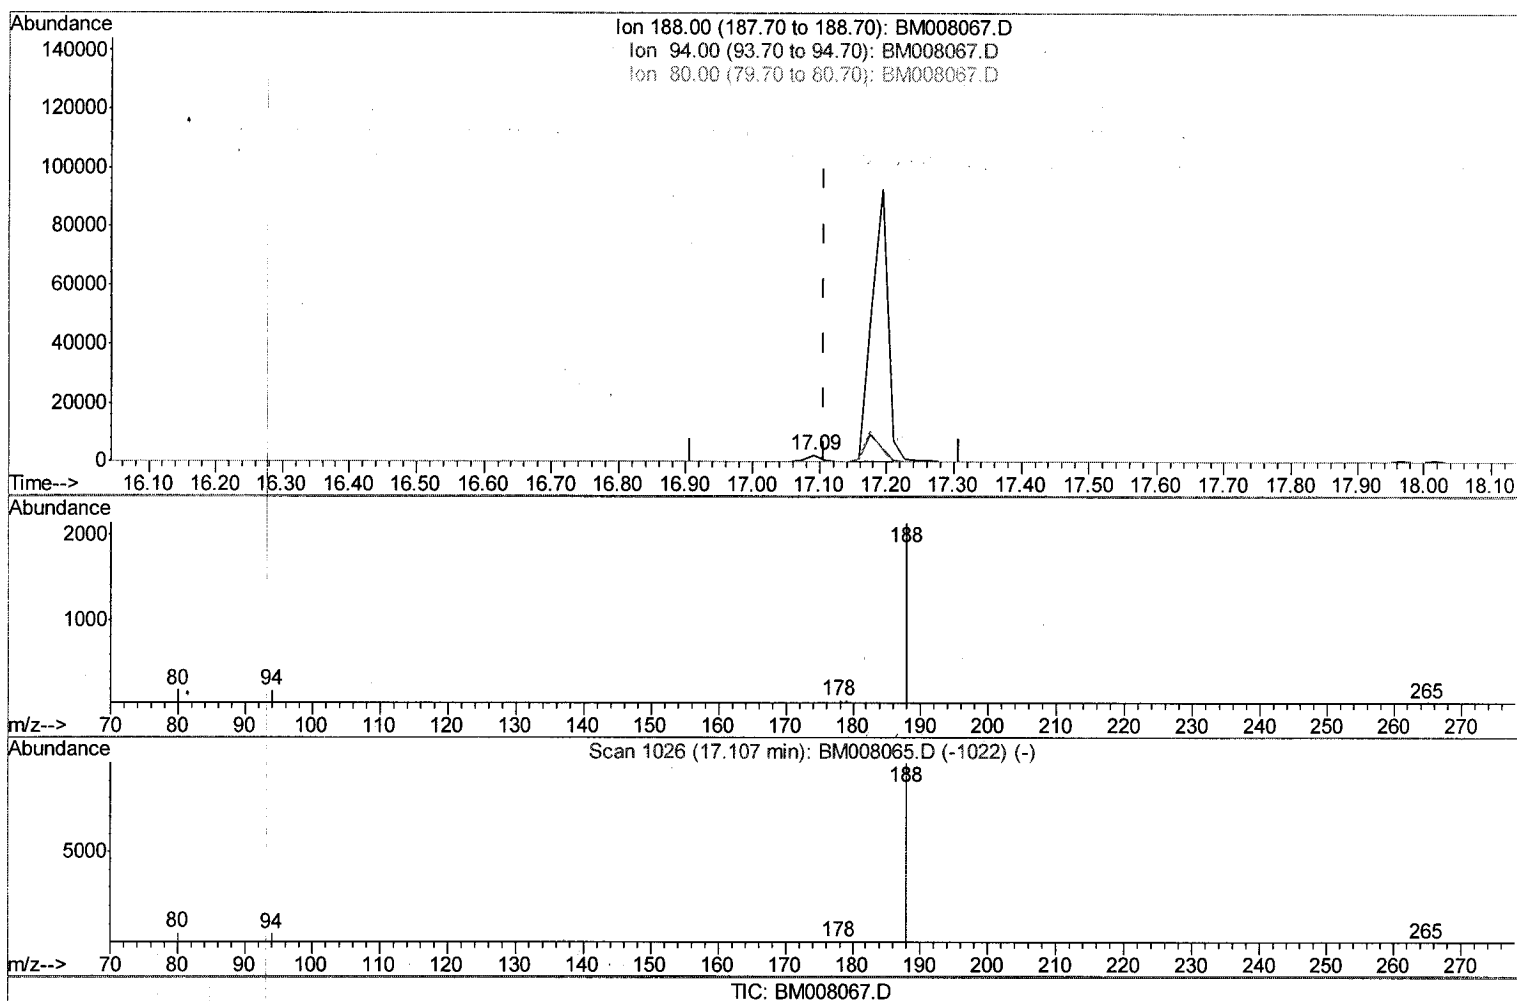

TIC: BM008067.D

(10) Phenanthrene-d10 (I)

17.090min (-0.017) 0.40ng/ul m

response 3198

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.04
80.00	11.80	9.41#
0.00	0.00	0.00

S.J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Nov 25 01:29:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

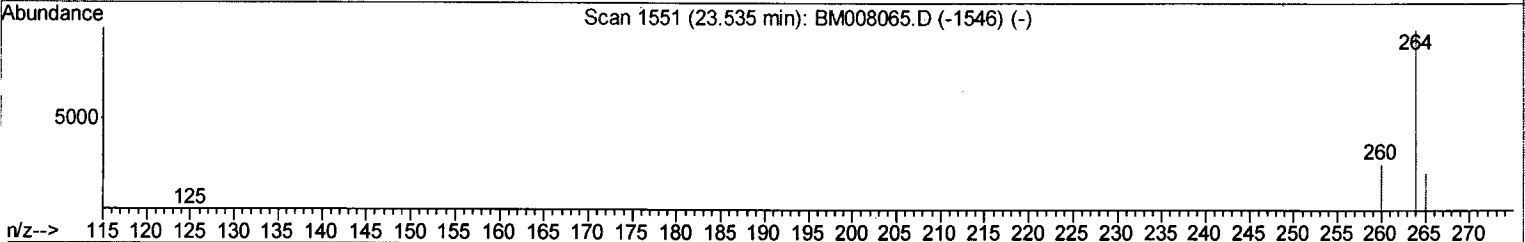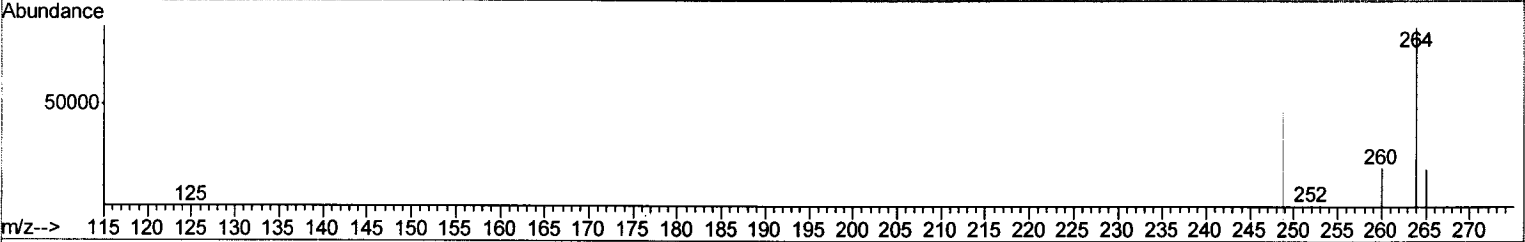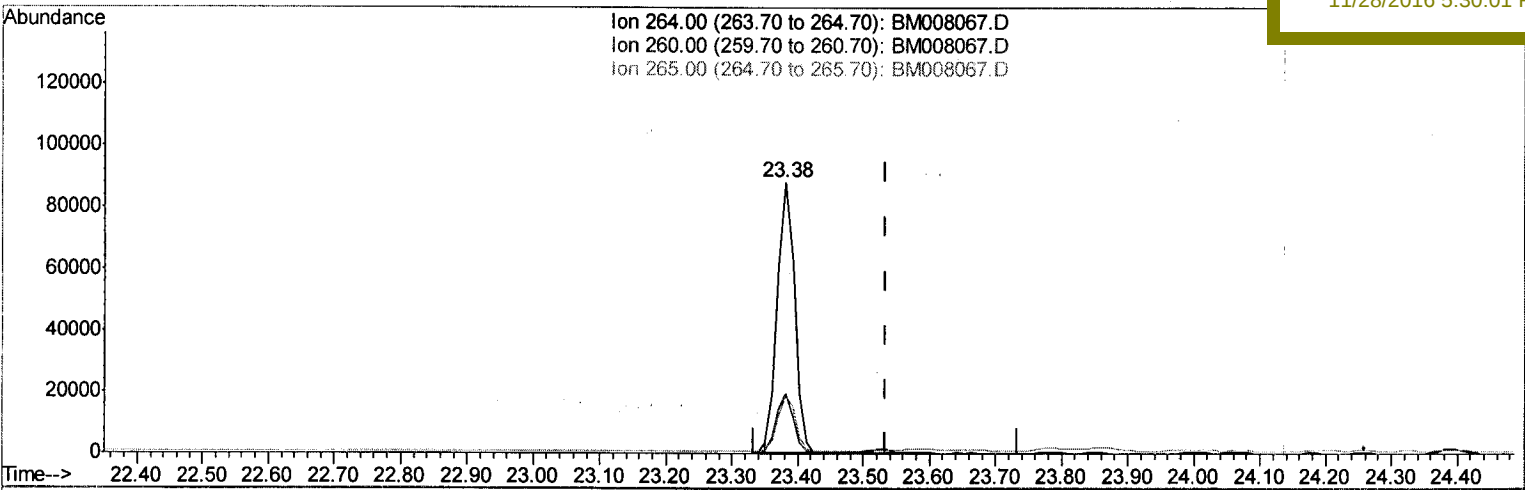

TIC: BM008067.D

(20) Perylene-d12 (I)

23.382min (-0.153) 0.40ng/ul

response 158570

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.22#
265.00	103.50	21.49#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 01:29:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

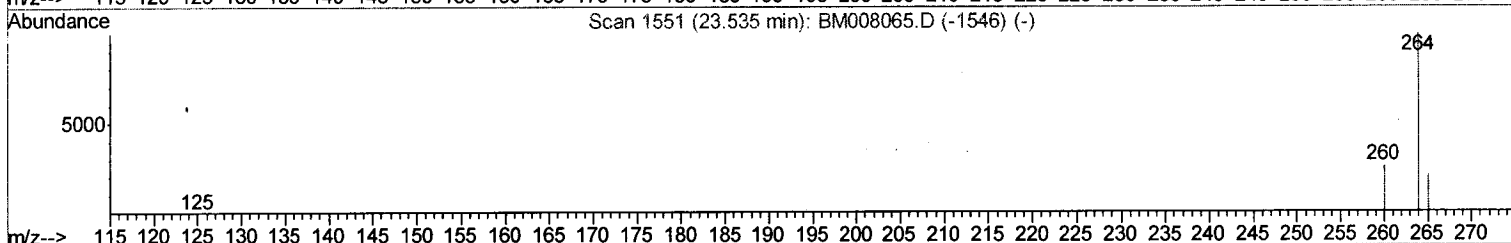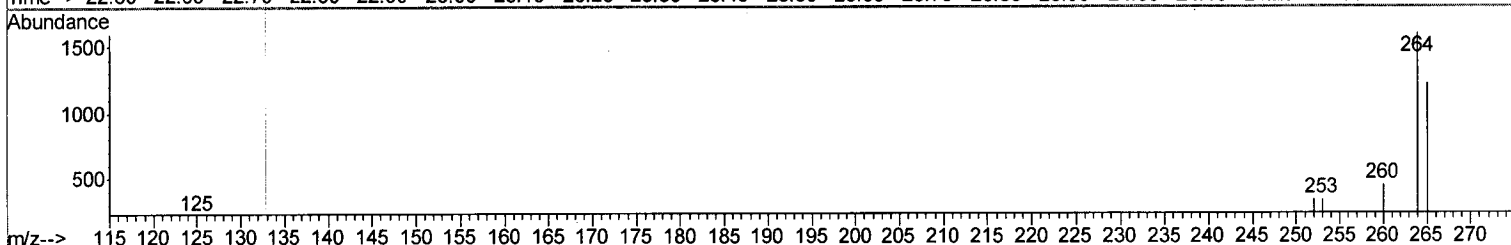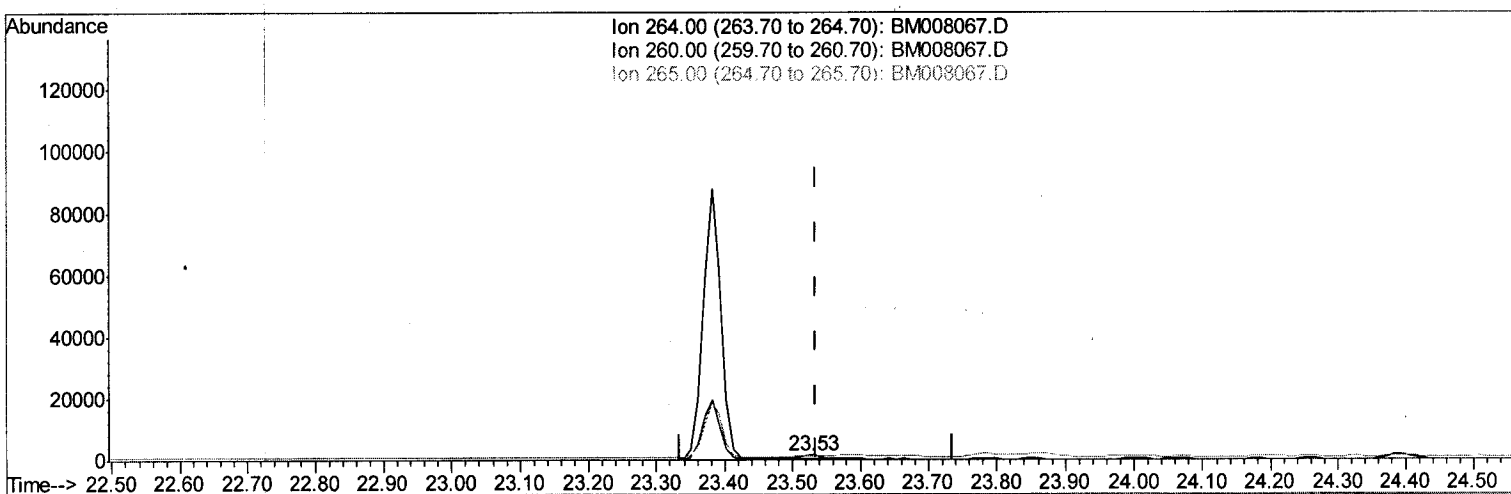

TIC: BM008067.D

(20) Perylene-d12 (I)

23.528min (-0.007) 0.40ng/ul m

response 2418

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.16
265.00	103.50	76.62#
0.00	0.00	0.00

S.J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

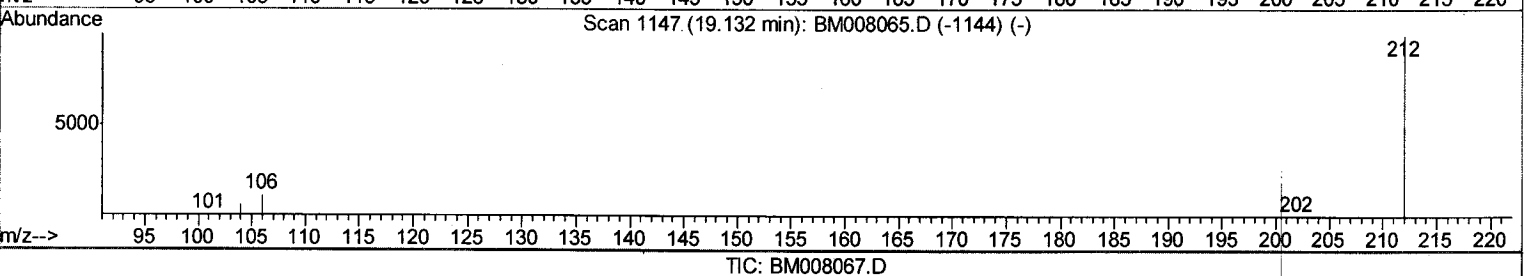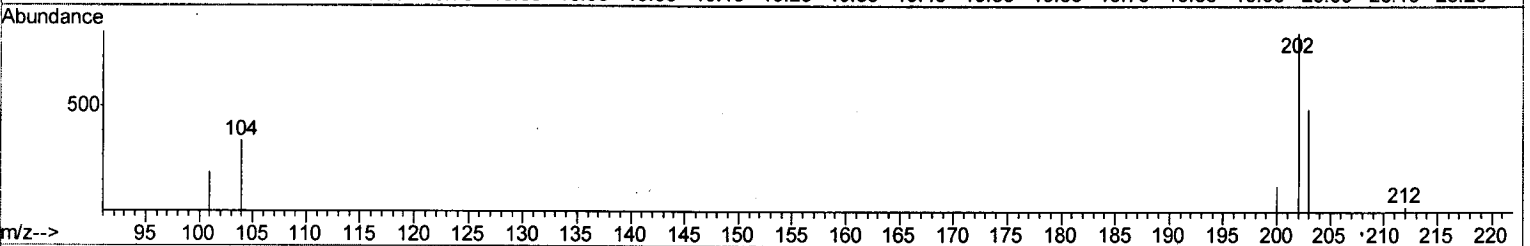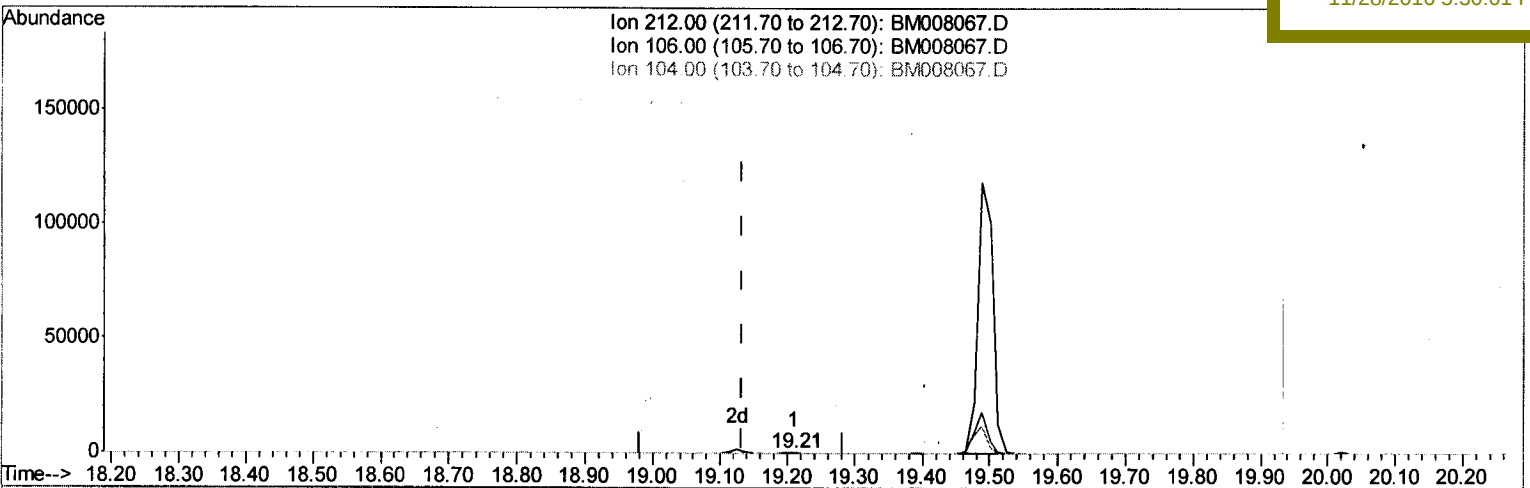

(14) Fluoranthene-d10 (SURR)

19.210min (+0.078) 0.01ng/ul

response 79

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	51.90#
104.00	15.60	874.68#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

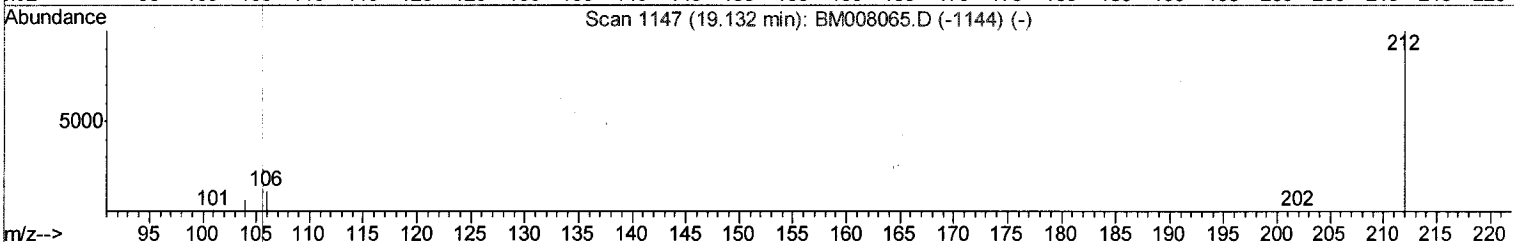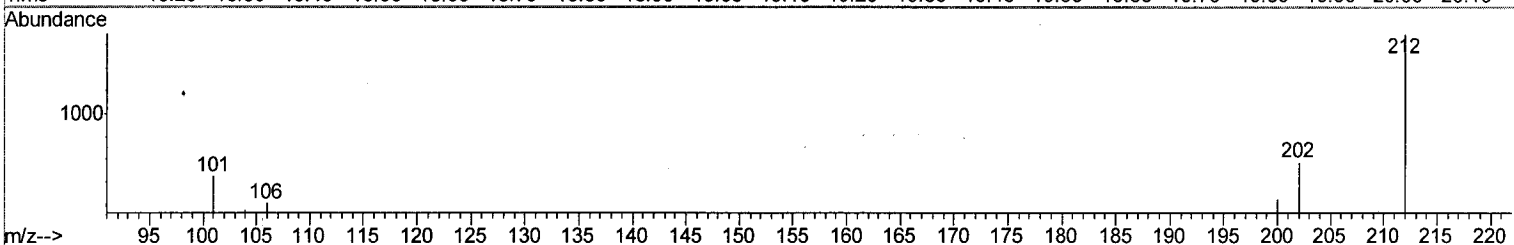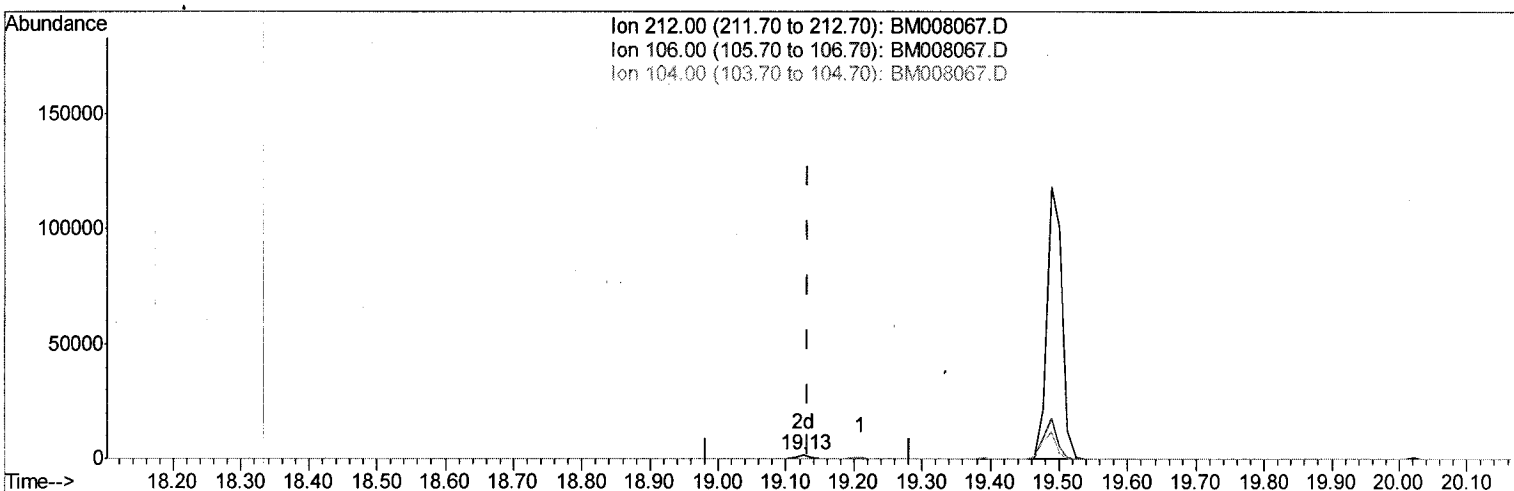

TIC: BM008067.D

(14) Fluoranthene-d10 (SURR)

19.126min (-0.007) 0.27ng/ul m

response 2454

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	1.67#
104.00	15.60	28.16#
0.00	0.00	0.00

S.J
 11/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

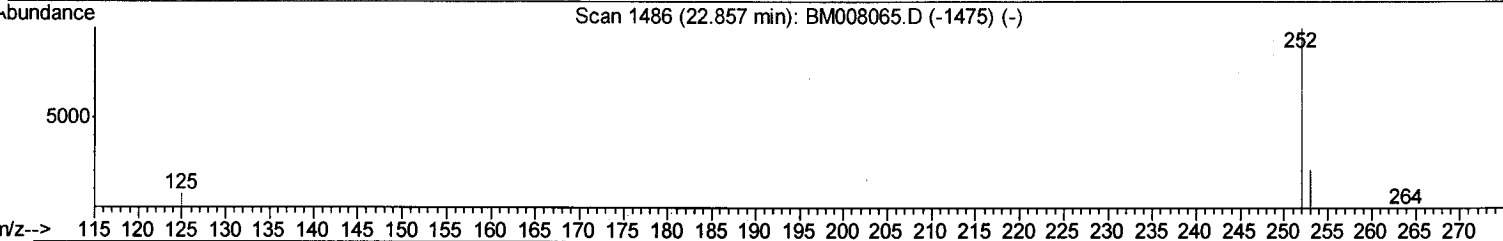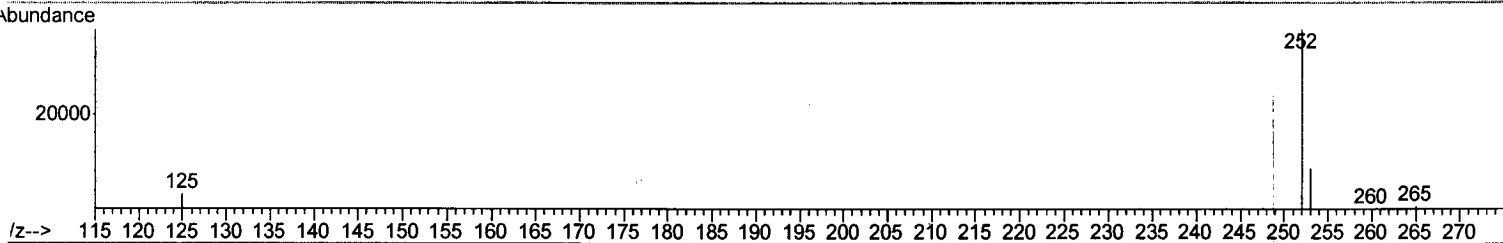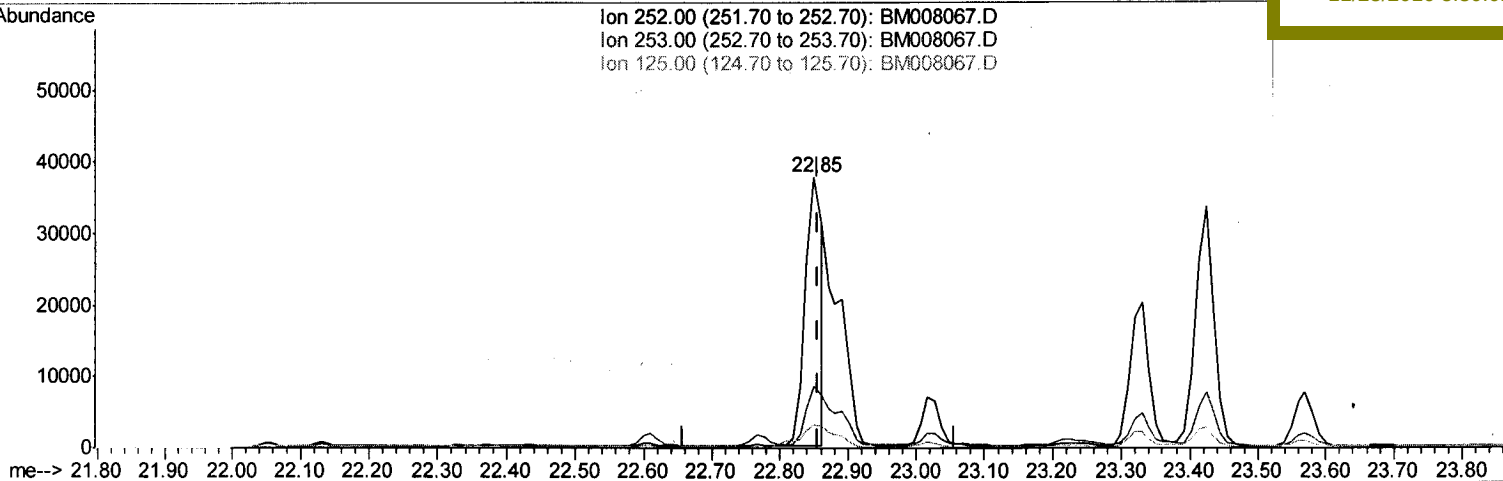

(21) Benzo(b)fluoranthene
 22.850min (-0.007) 6.72ng/ui
 response 64814

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.69
125.00	17.50	8.55
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

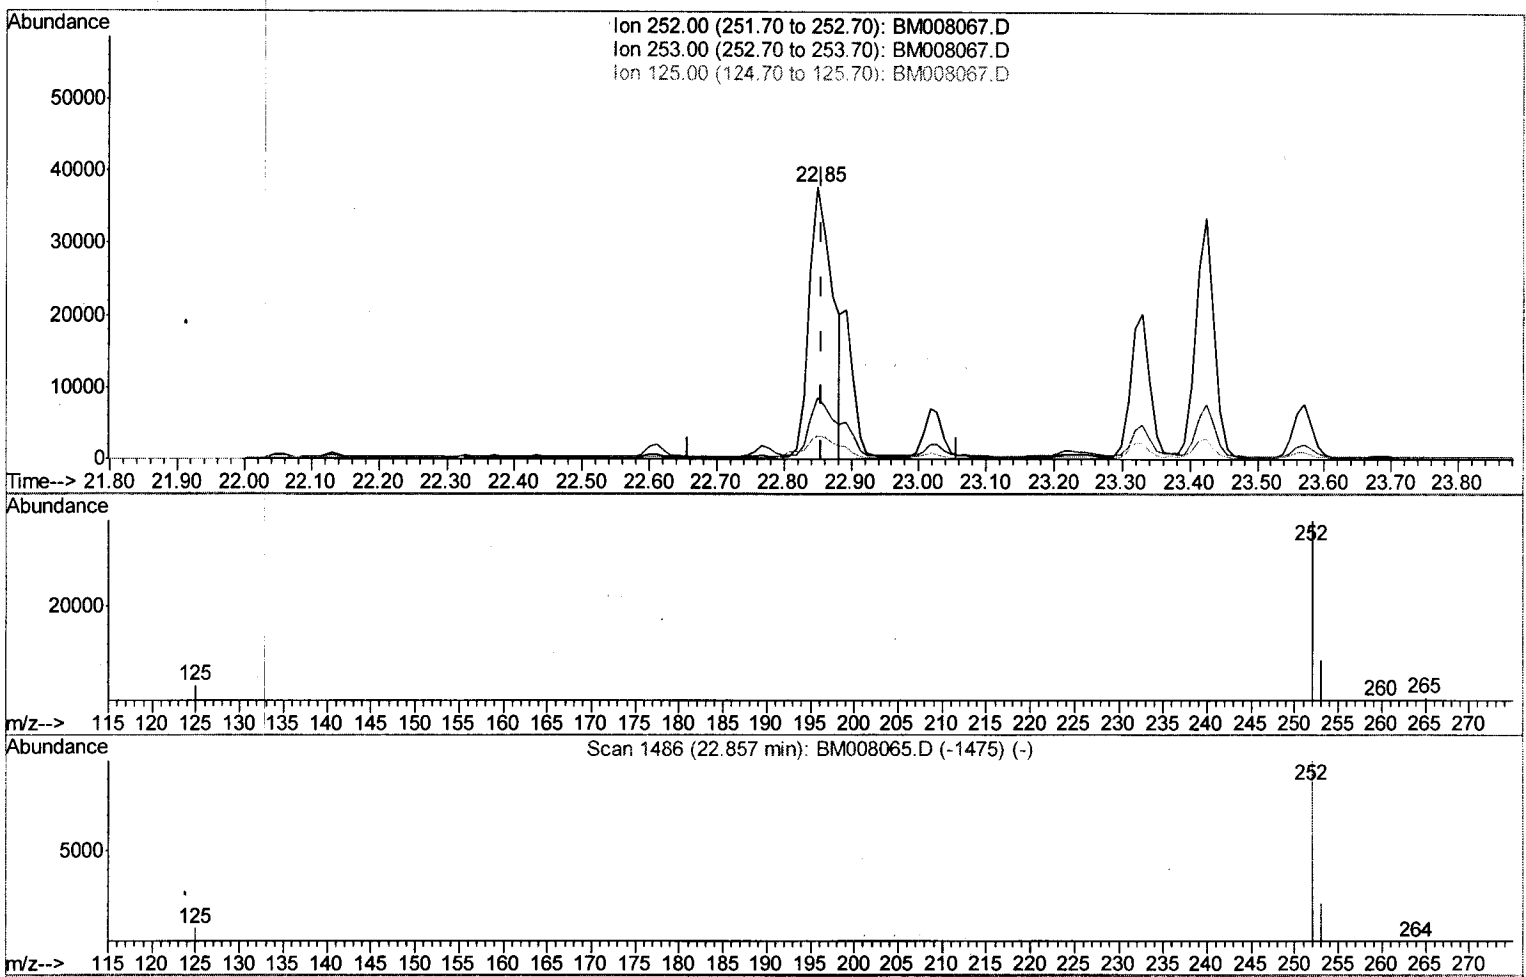

(21) Benzo(b)fluoranthene

22.850min (-0.007) 9.60ng/ul m

response 92625

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.69
125.00	17.50	8.55
0.00	0.00	0.00

S.J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

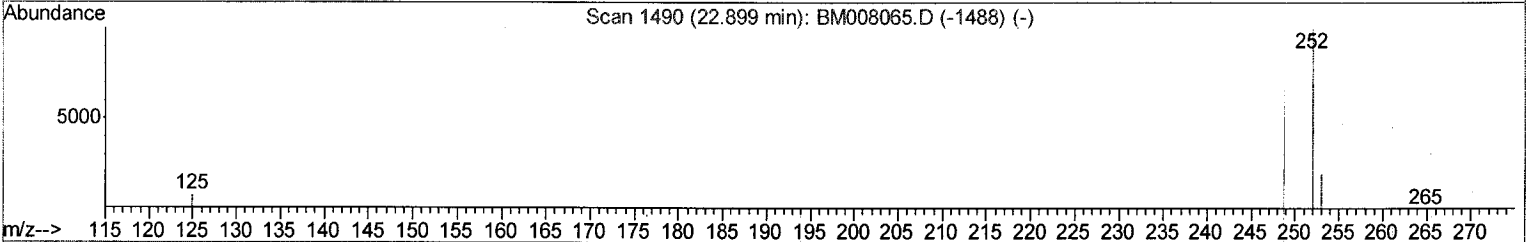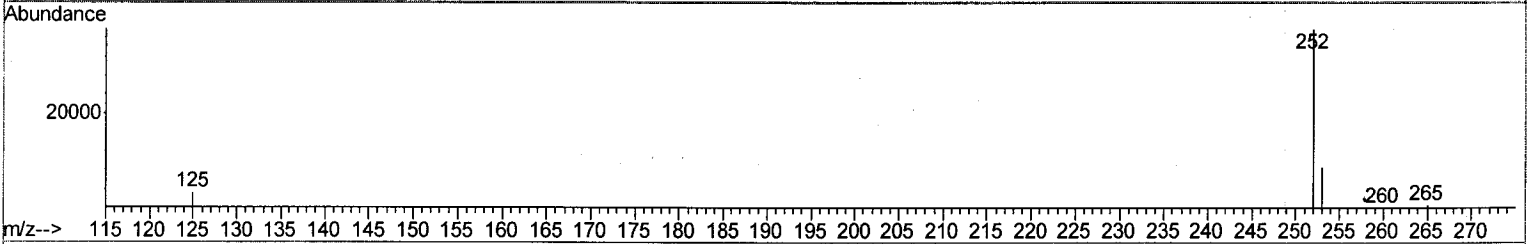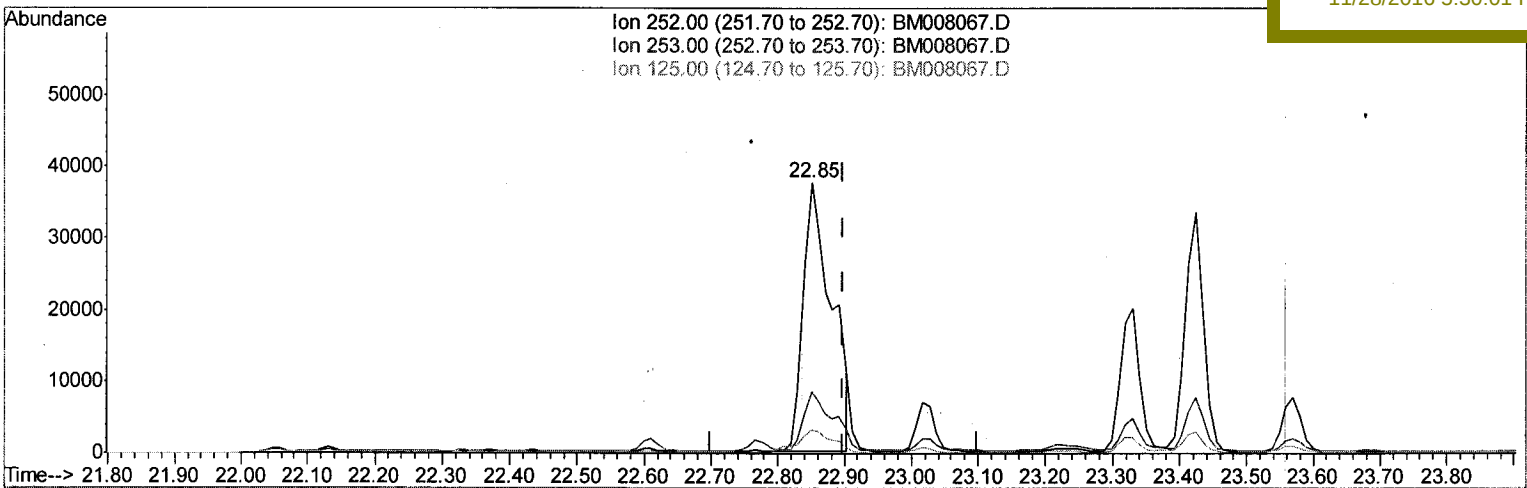

TIC: BM008067.D

(22) Benzo(k)fluoranthene

22.850min (-0.049) 11.14ng/ul

response 110864

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	22.69#
125.00	17.10	8.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

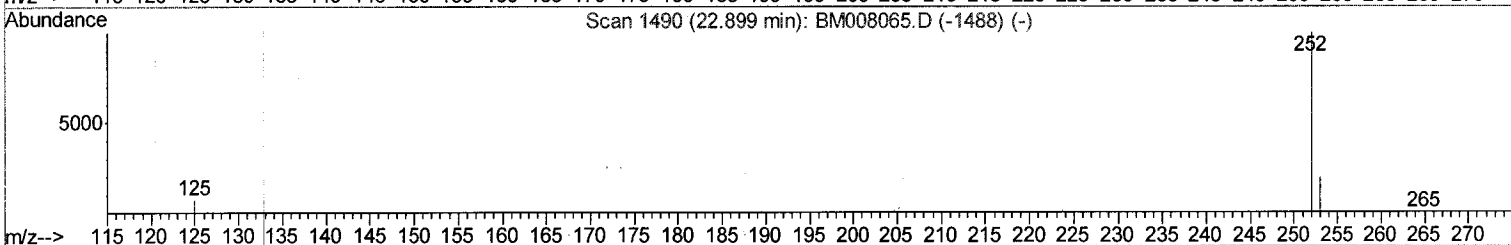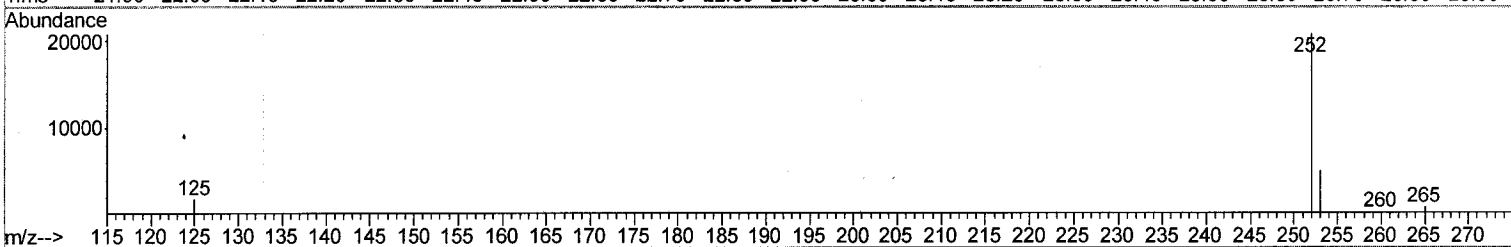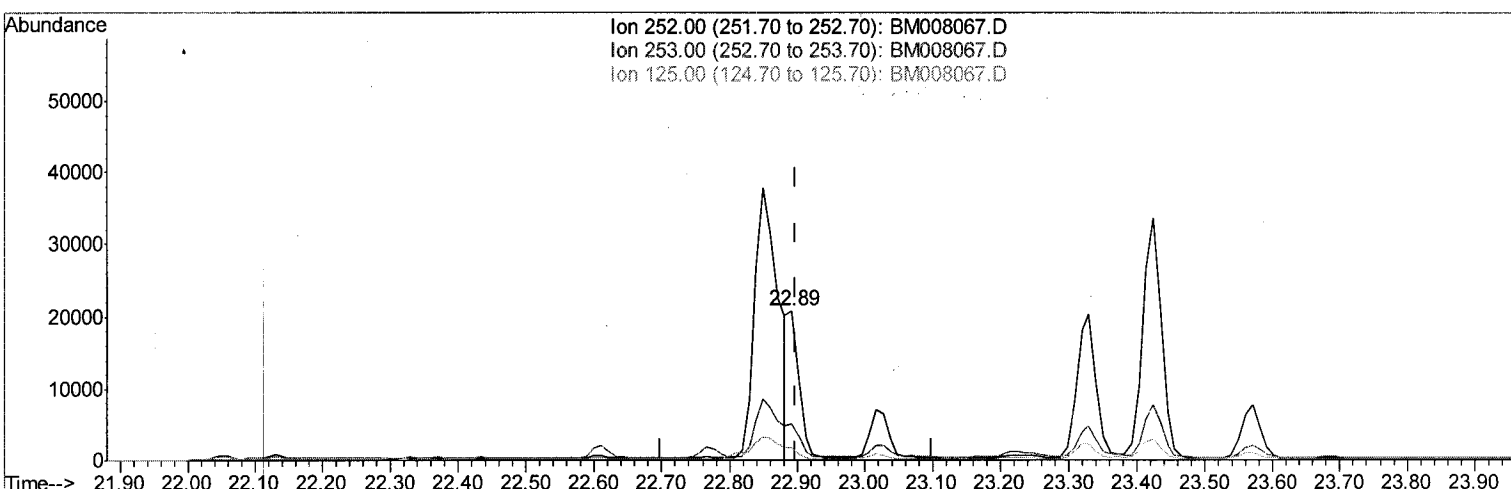

TIC: BM008067.D

(22) Benzo(k)fluoranthene

22.892min (-0.007) 2.35ng/ul m

response 23377

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.45#
125.00	17.10	8.32#
0.00	0.00	0.00

S. J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

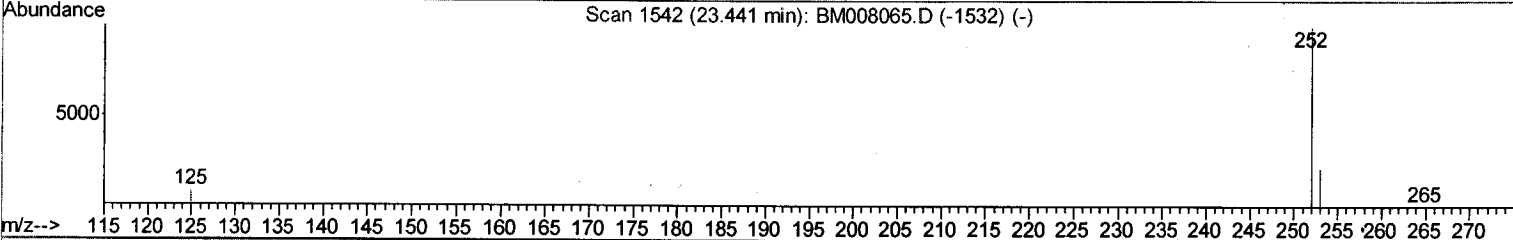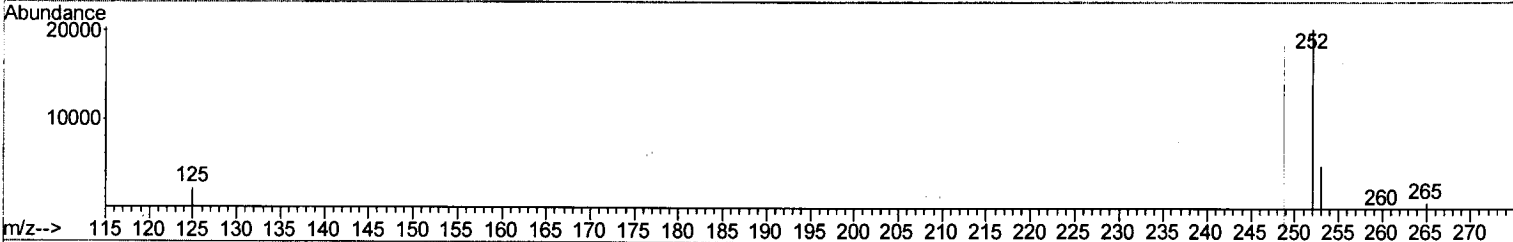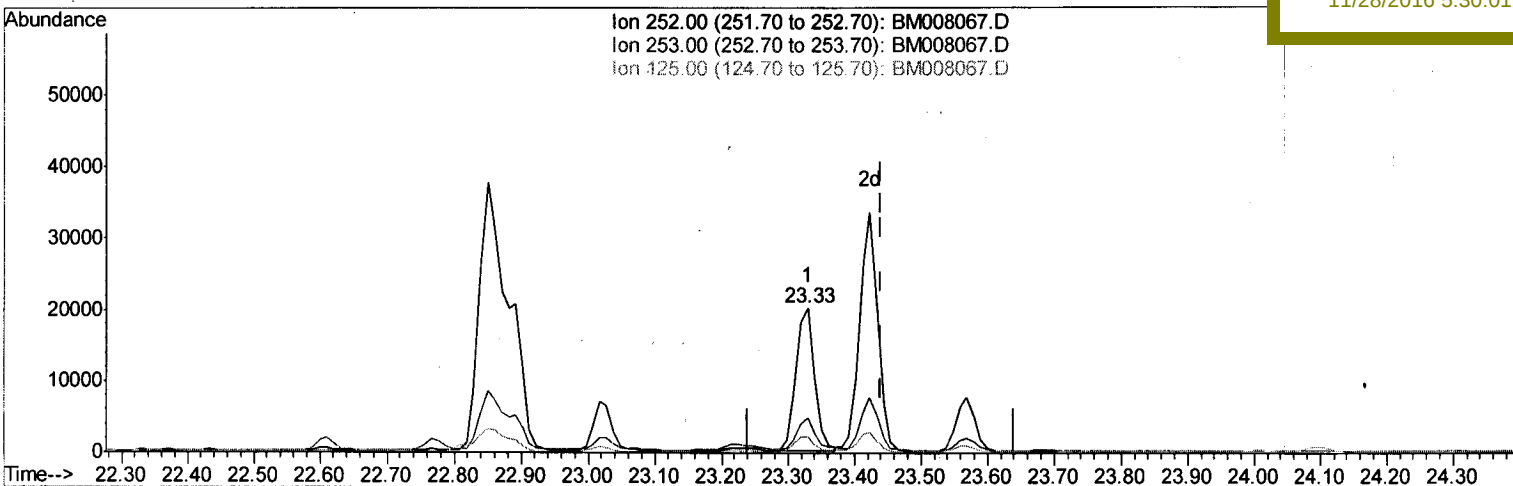

TIC: BM008067.D

(23) Benzo(a)pyrene (C)

23.330min (-0.111) 4.28ng/ul

response 38702

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.67#
125.00	22.60	11.02#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

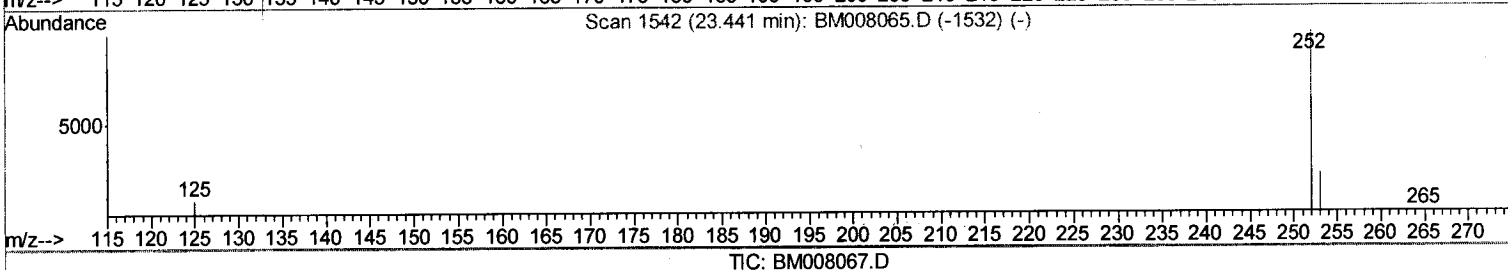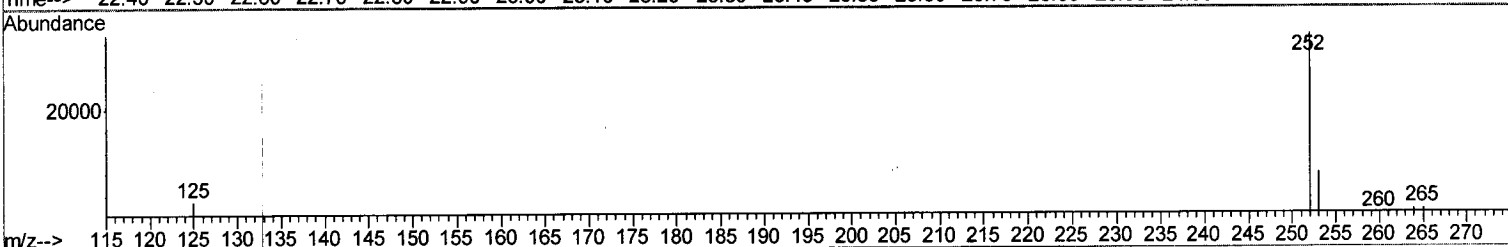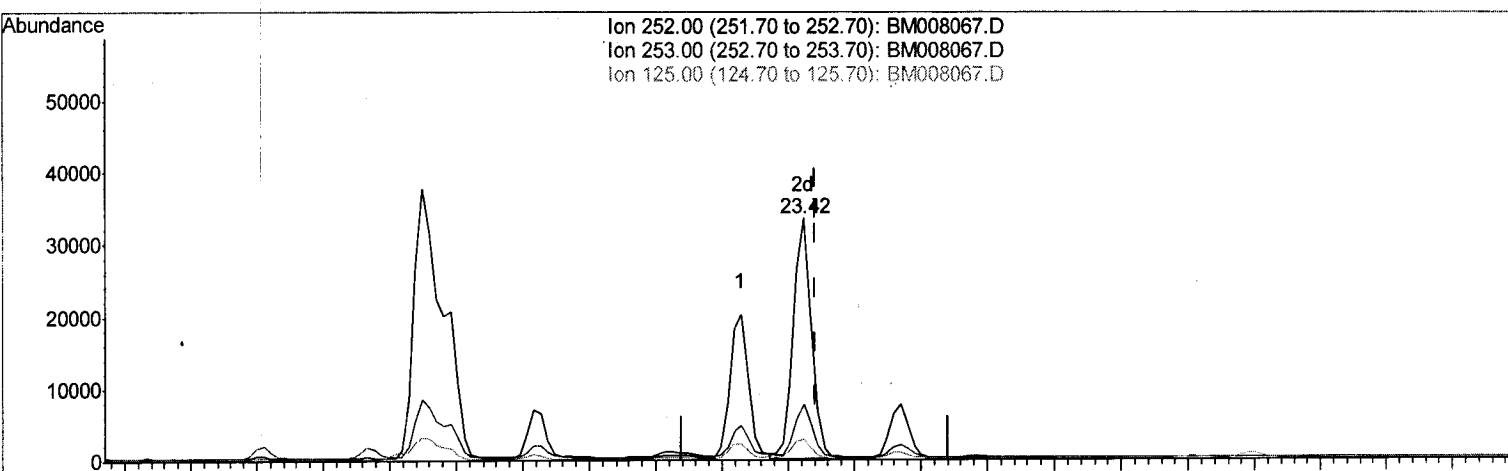

(23) Benzo(a)pyrene (C)

23.423min (-0.017) 7.03ng/ul m

response 63529

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.16#
125.00	22.60	8.47#
0.00	0.00	0.00

S.J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

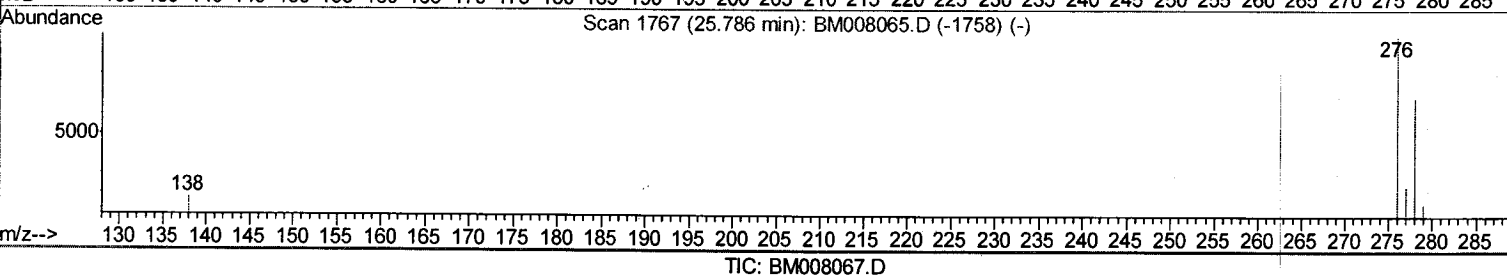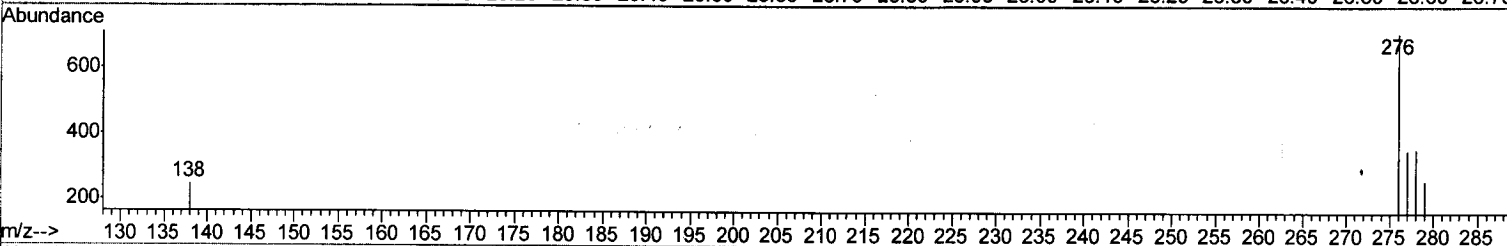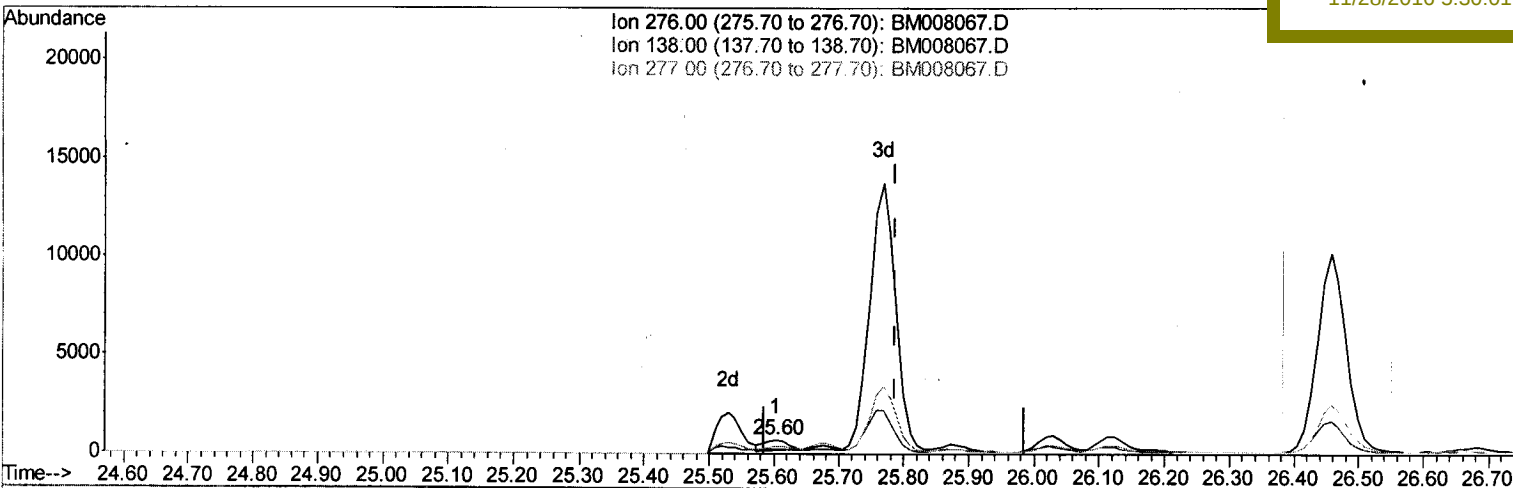

(24) Indeno(1,2,3-cd)pyrene

25.602min (-0.184) 0.12ng/ul

response 1295

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	15.52#
277.00	24.50	34.21#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

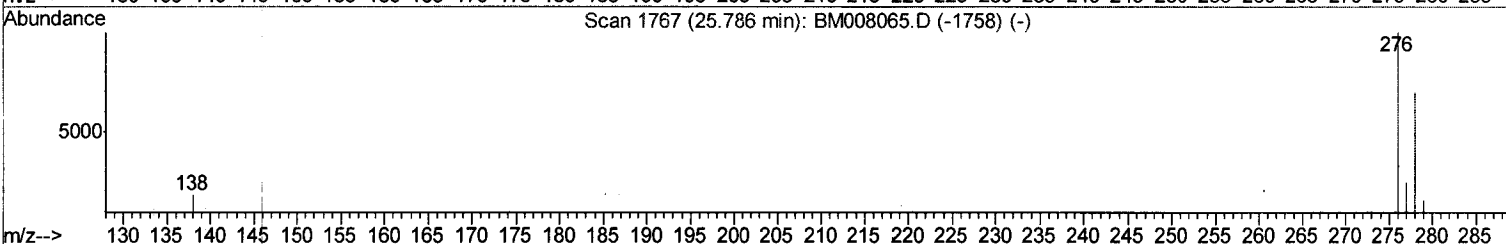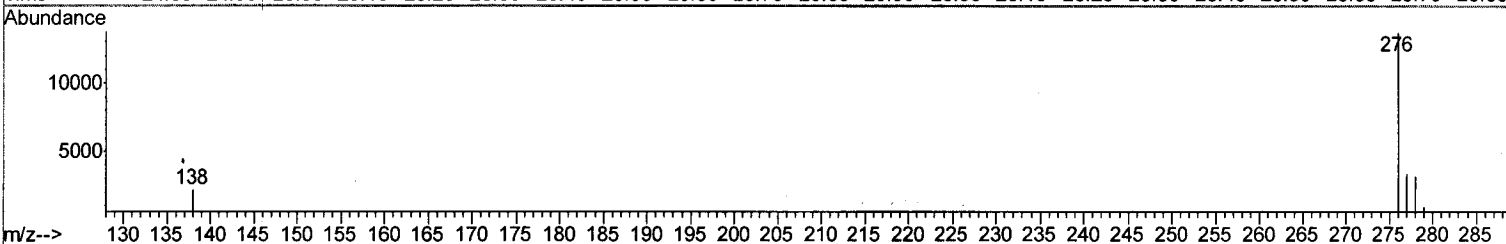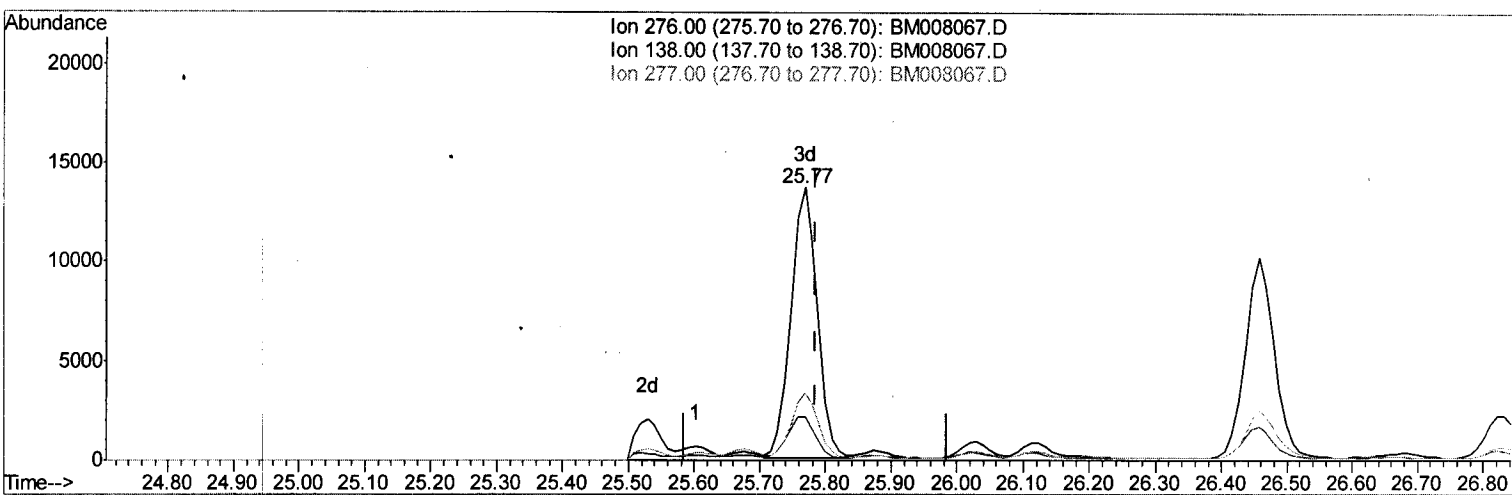

TIC: BM008067.D

(24) Indeno(1,2,3-cd)pyrene

25.769min (-0.017) 3.41ng/ul m

response 38106

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.53#
277.00	24.50	1.16#
0.00	0.00	0.00

> S.J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

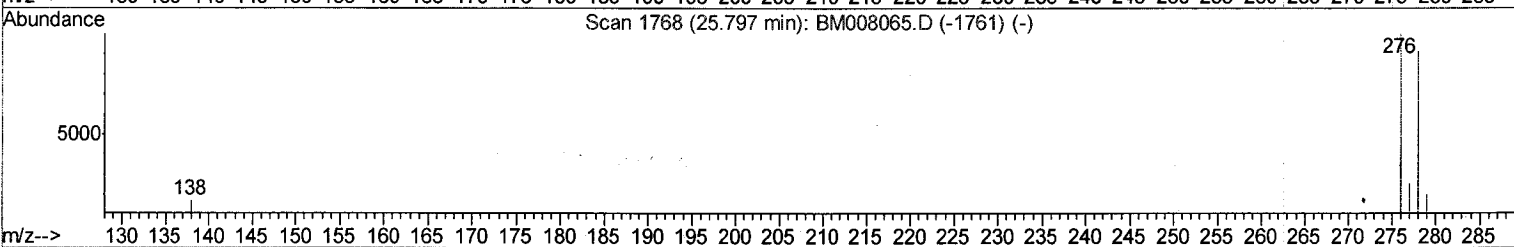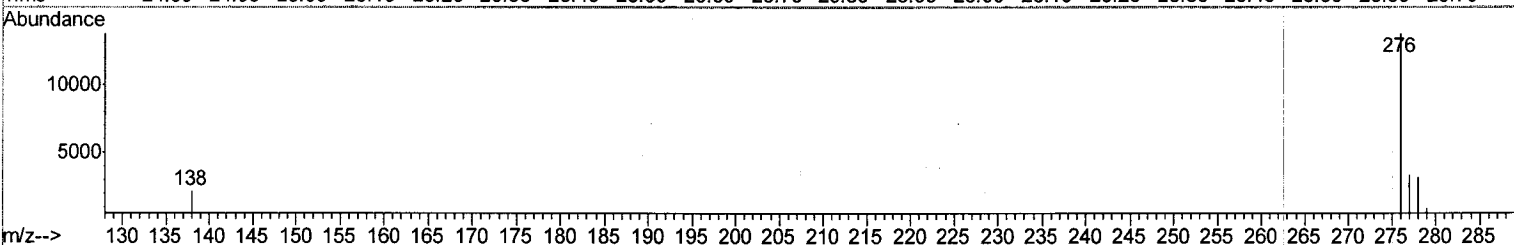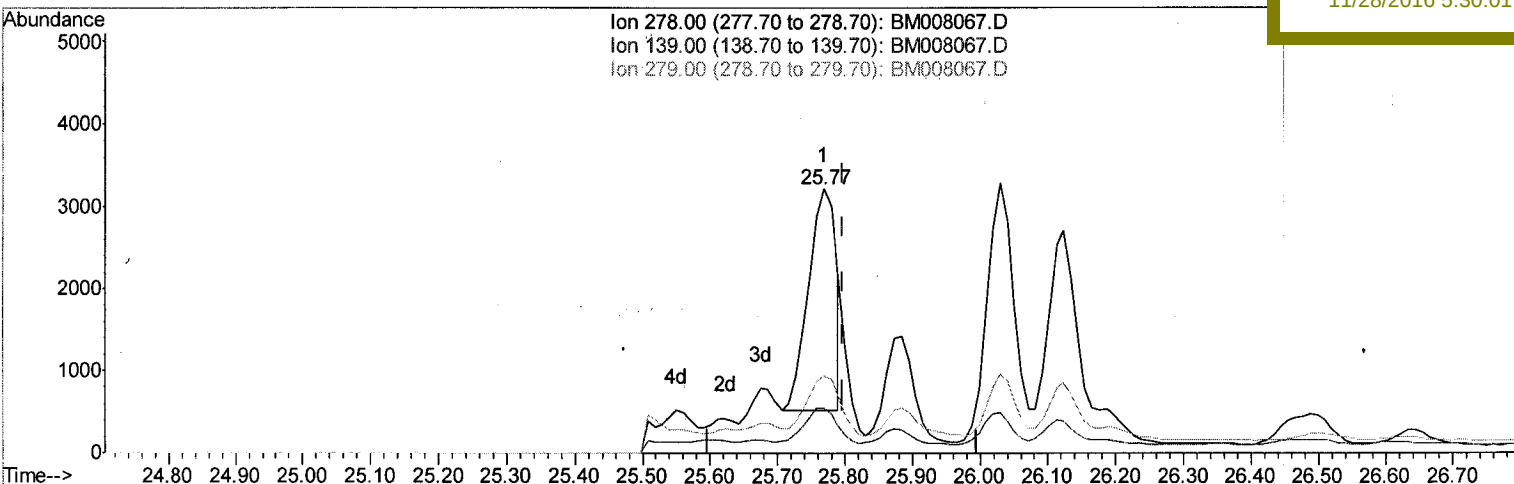

TIC: BM008067.D

(25) Dibenzo(a,h)anthracene

25.769min (-0.028) 0.87ng/ul

response 7769

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	17.38
279.00	32.40	29.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

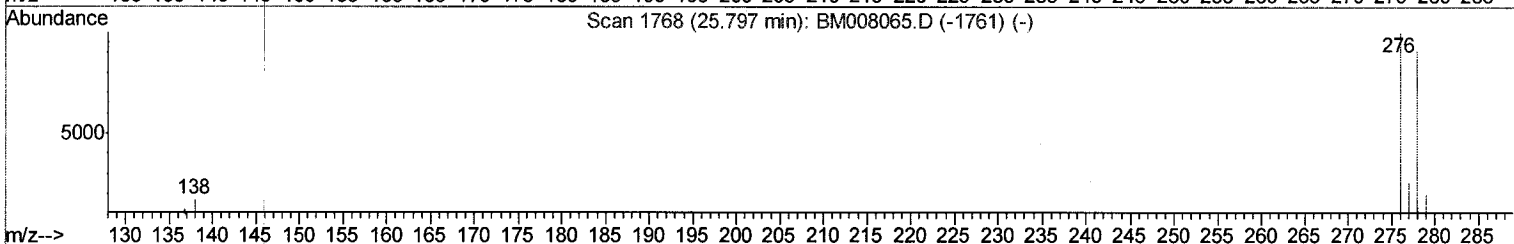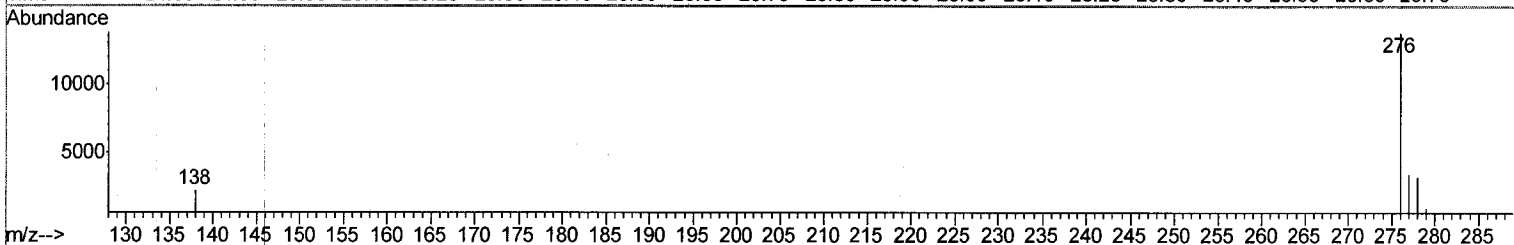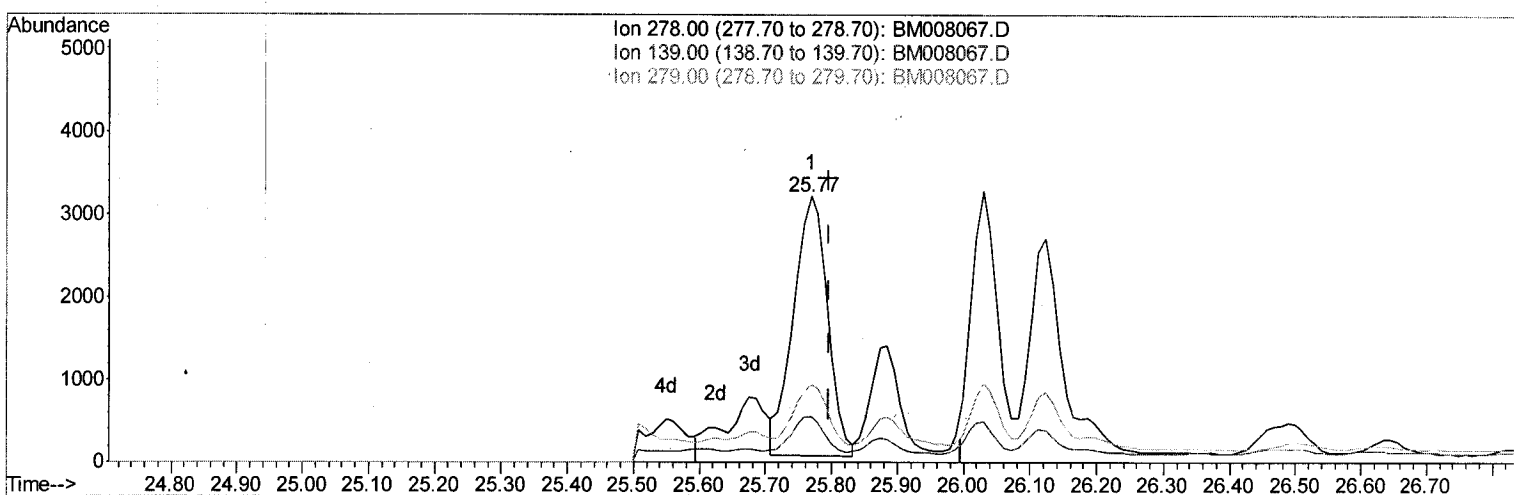

TIC: BM008067.D

(25) Dibenzo(a,h)anthracene

25.769min (-0.028) 1.25ng/ul m

response 11229

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	17.38
279.00	32.40	29.34
0.00	0.00	0.00

S. J
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

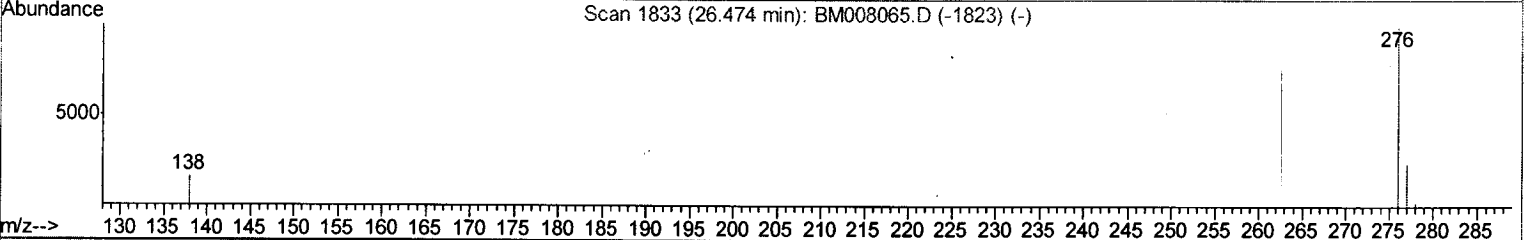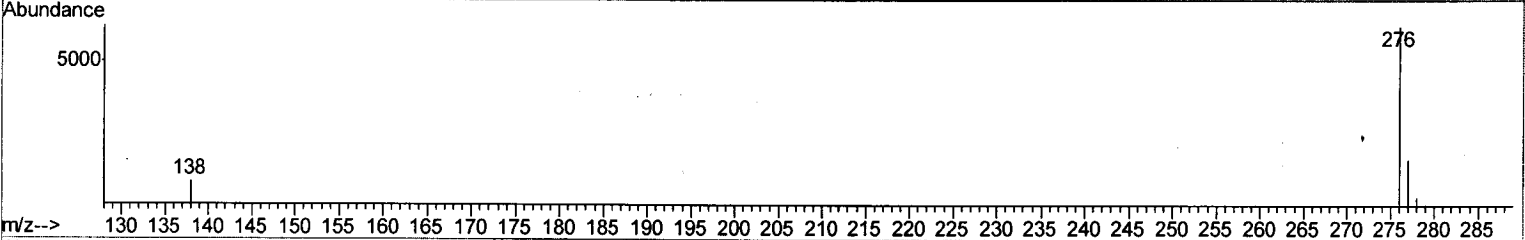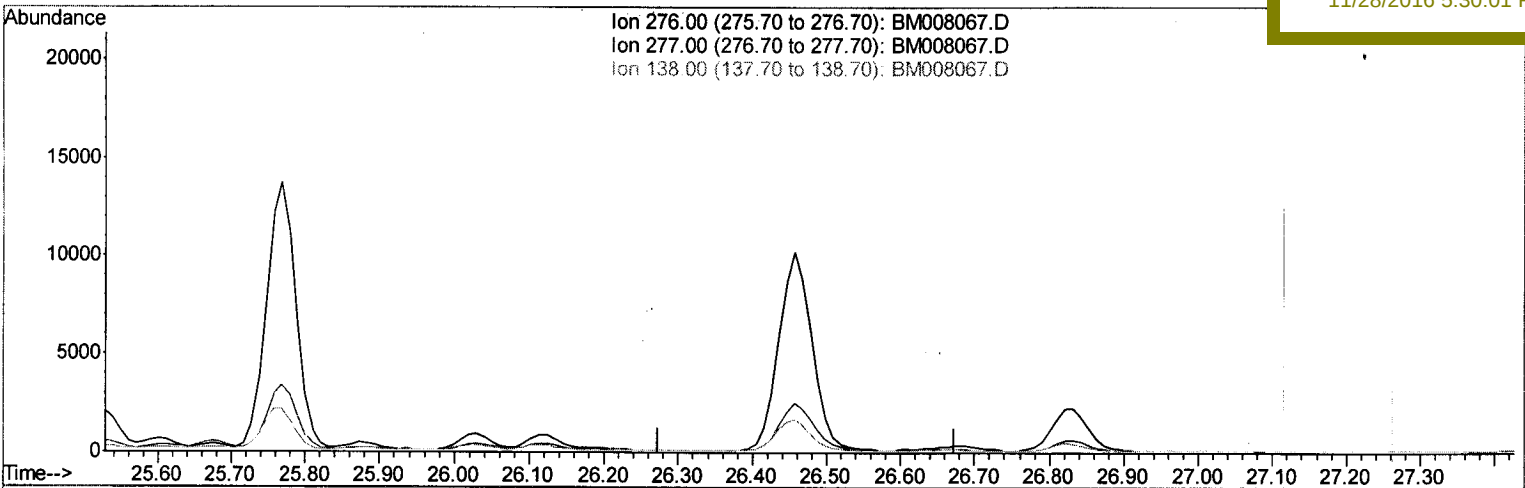

TIC: BM008067.D

(26) Benzo(g,h,i)perylene

26.474min (-26.474) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:14:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

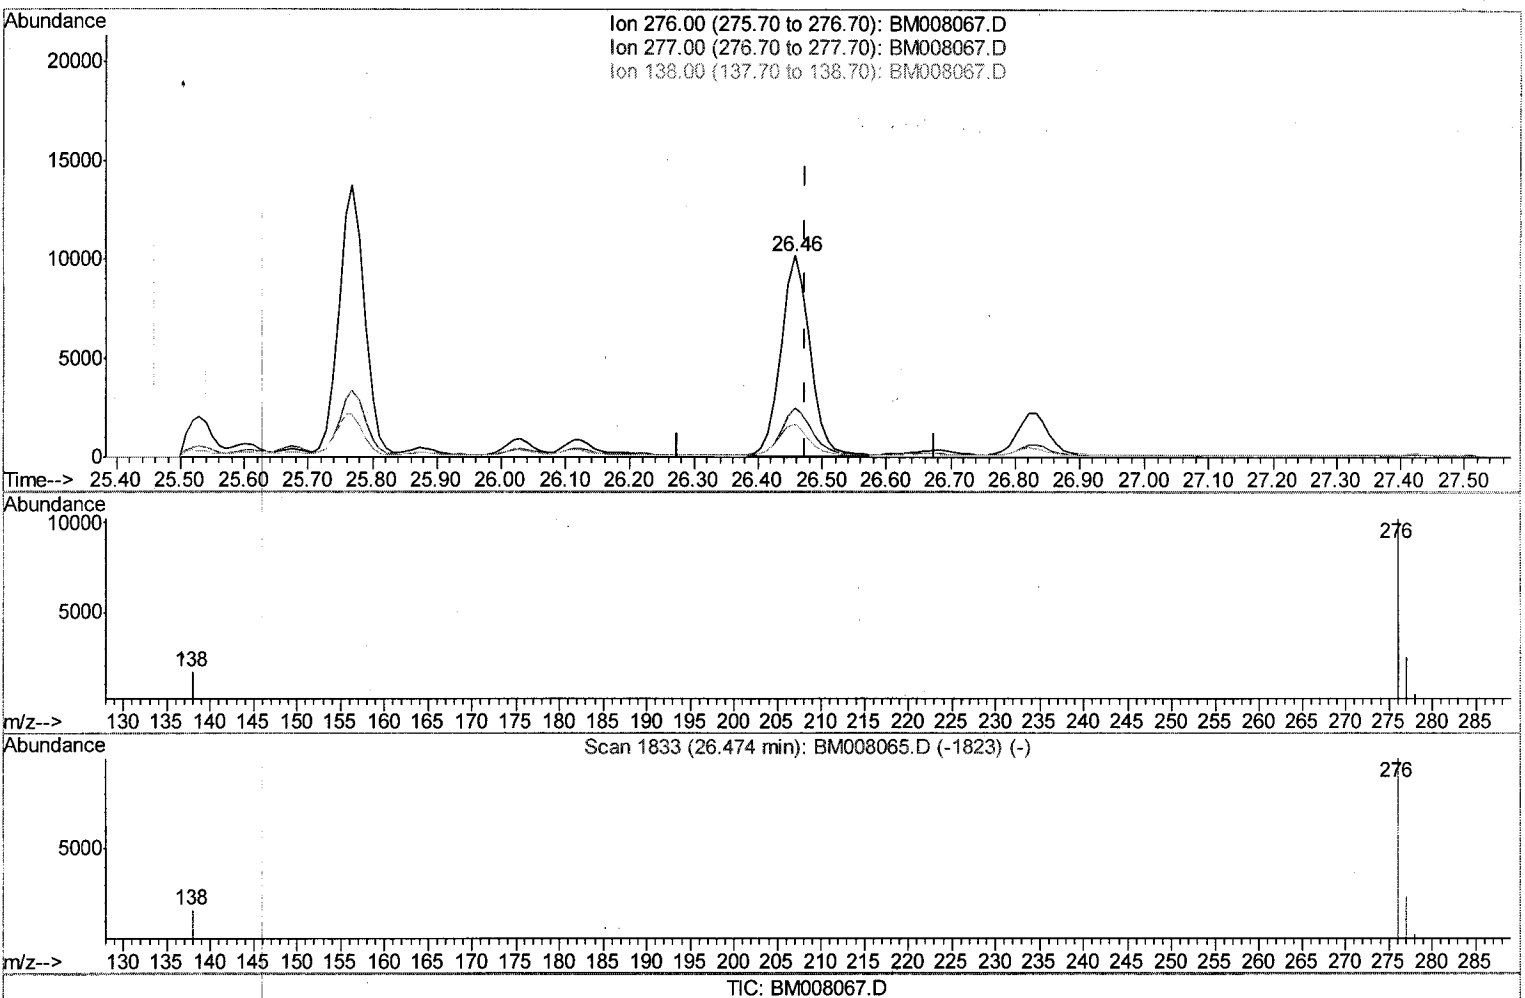

(26) Benzo(g,h,i)perylene

26.457min (-0.017) 3.22ng/ul m

response 31887

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	24.59
138.00	25.60	16.64#
0.00	0.00	0.00

> S.J
 11/29/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112316\
 Data File : BM008067.D
 Acq On : 24 Nov 2016 10:55
 Operator : UM/SJ
 Sample : H5701-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WD7

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:01 PM

Quant Time: Nov 25 02:16:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	736	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	2529	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.35	164	1560	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	3198m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.29	240	3236	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	2418m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.09	152	823	0.23	ng/ul	-0.01
14) Fluoranthene-d10	19.13	212	2454m	0.27	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.54	128	10401	1.47	ng/ul	94
5) 2-Methylnaphthalene	12.16	142	2781	0.61	ng/ul	99
7) Acenaphthylene	14.06	152	3318	0.47	ng/ul	99
8) Acenaphthene	14.40	153	8037	1.50	ng/ul	97
9) Fluorene	15.39	166	11023	1.79	ng/ul#	84
12) Phenanthrene	17.12	178	124063	12.46	ng/ul	94
13) Anthracene	17.23	178	32283	3.45	ng/ul#	92
15) Fluoranthene	19.15	202	164794	12.82	ng/ul	94
17) Pyrene	19.52	202	144659	12.88	ng/ul#	94
18) Benzo(a)anthracene	21.27	228	81128	8.17	ng/ul	98
19) Chrysene	21.32	228	71367	5.78	ng/ul	98
21) Benzo(b)fluoranthene	22.85	252	92625m	9.60	ng/ul	
22) Benzo(k)fluoranthene	22.89	252	23377m	2.35	ng/ul	
23) Benzo(a)pyrene	23.42	252	63529m	7.03	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.77	276	38106m	3.41	ng/ul	
25) Dibenzo(a,h)anthracene	25.77	278	11229m	1.25	ng/ul	
26) Benzo(g,h,i)perylene	26.46	276	31887m	3.22	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed