

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:48:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

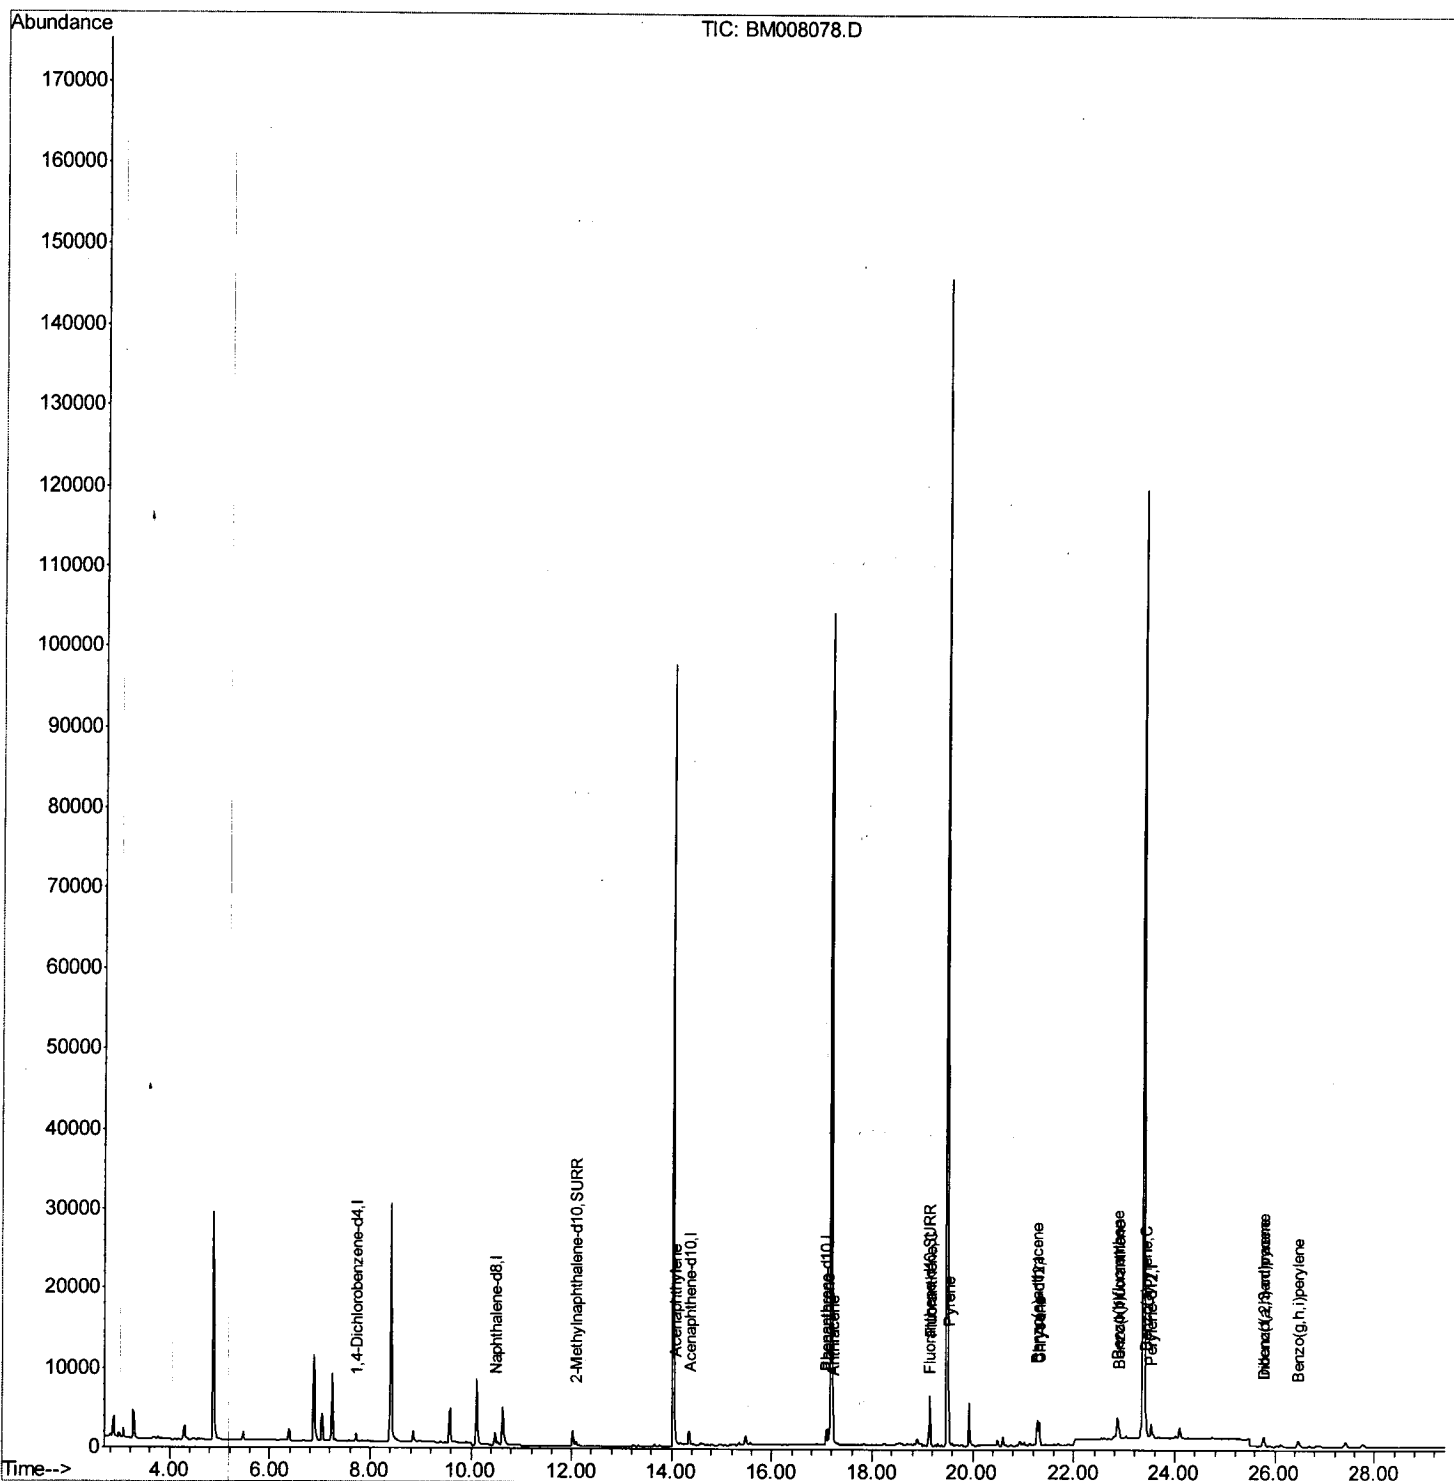

Quantitation Report (Qedit)


Data Path: Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File: BM008078.D
 Acq On: 24 Nov 2016 17:27
 Operator: UM/SJ
 Sample: H5701-17
 Misc:
 ALS Vial: 44 Sample Multiplier: 1

Instrument:
 BNA_M
 Client Sample ID:
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method: Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title: ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update: Fri Nov 25 01:27:01 2016
 Response via: Initial Calibration

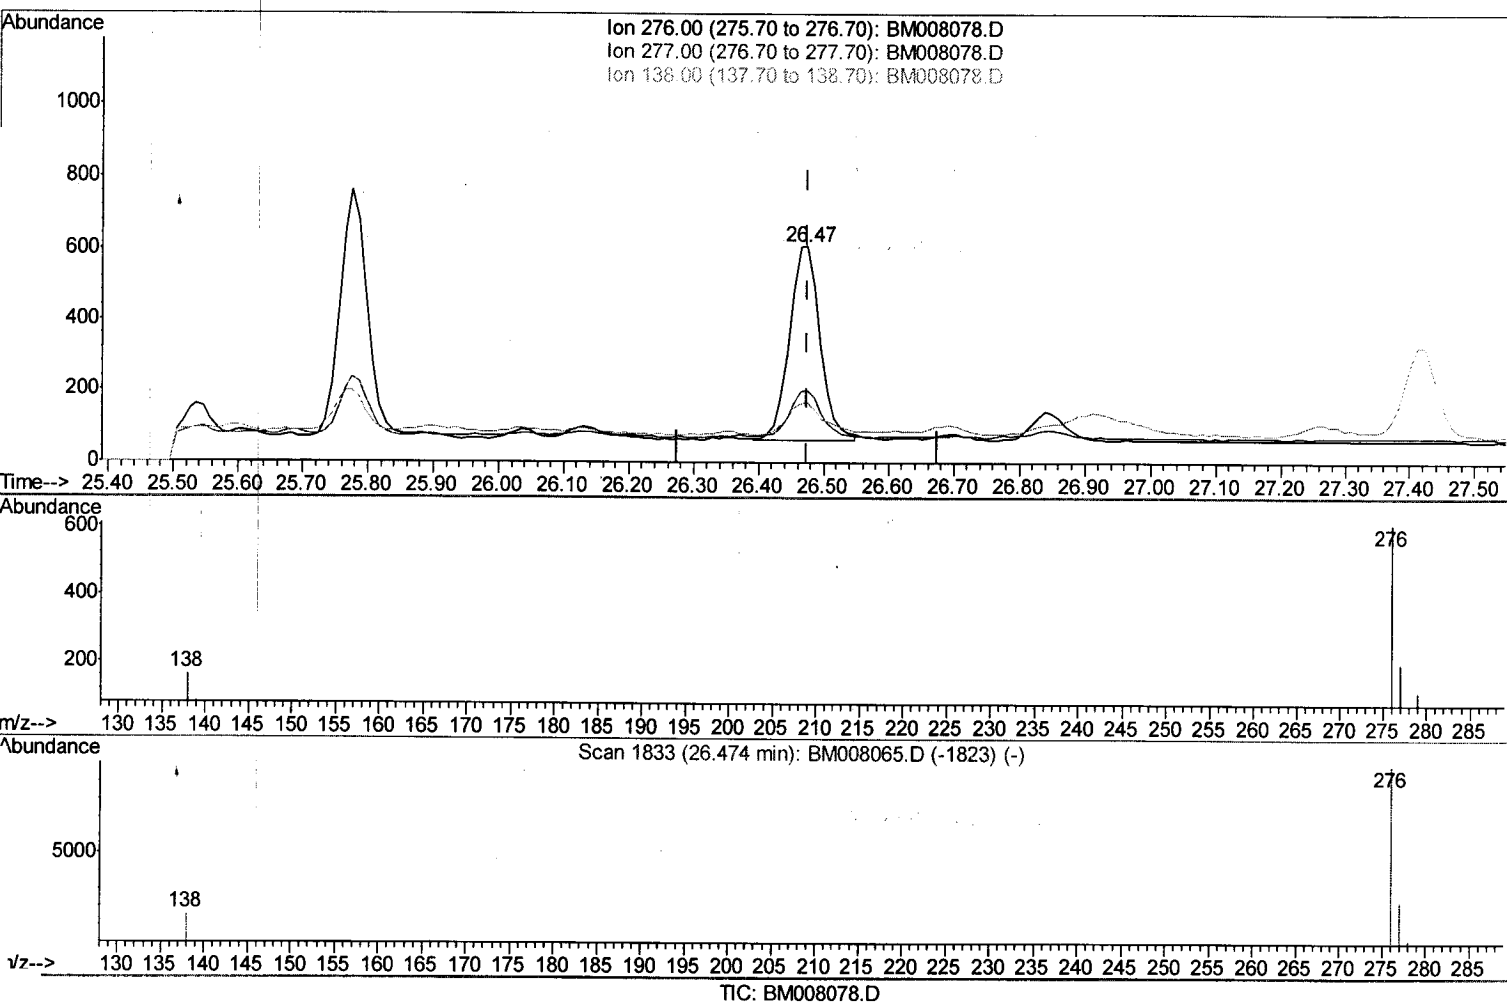

(26) Benzo(g,h,i)perylene

26.474min (+0.000) 0.20ng/ul m > S.J.
 response 1783
 11/29/16

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	33.06#
138.00	25.60	27.14
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

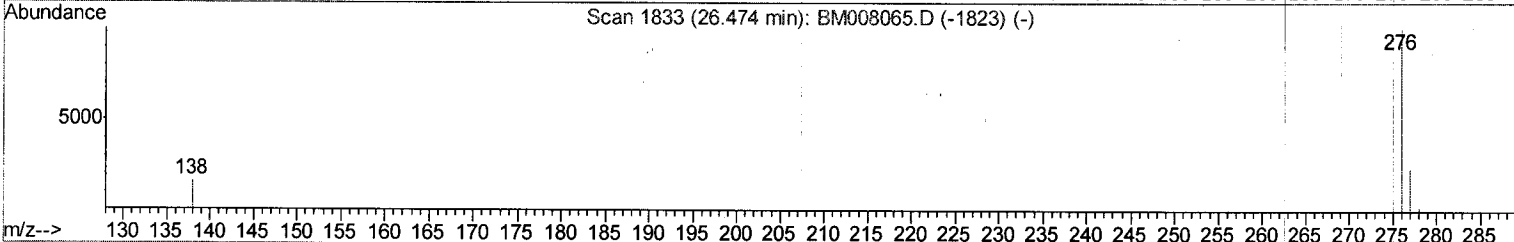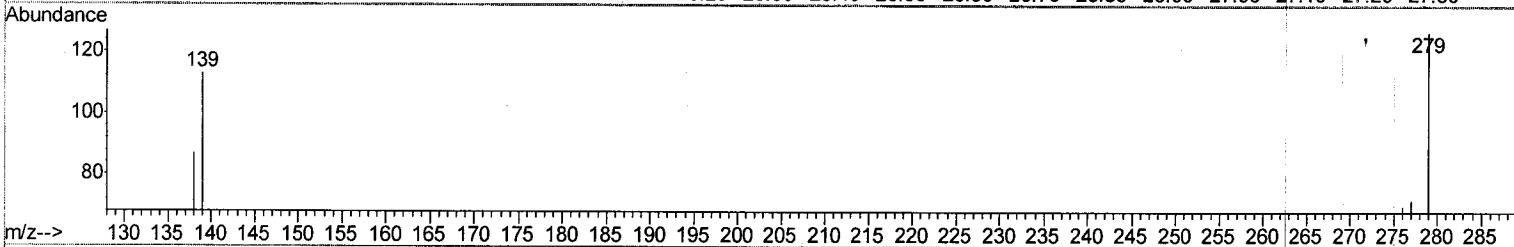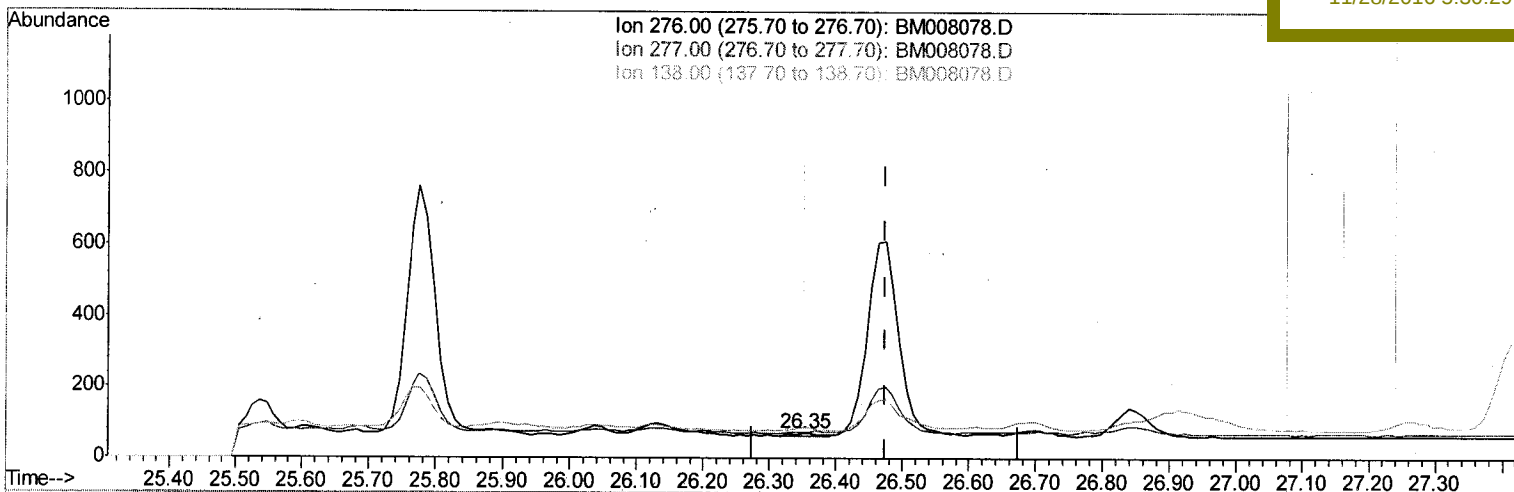

TIC: BM008078.D

(26) Benzo(g,h,i)perylene

26.349min (-0.125) 0.00ng/ul

response 16

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	102.86#
138.00	25.60	124.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

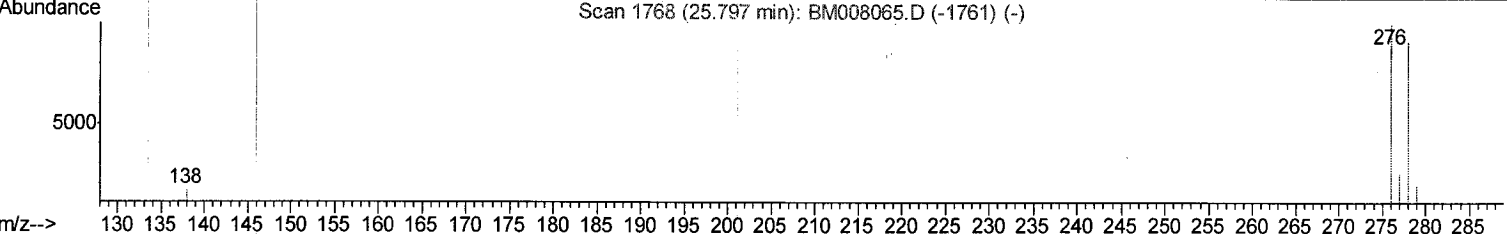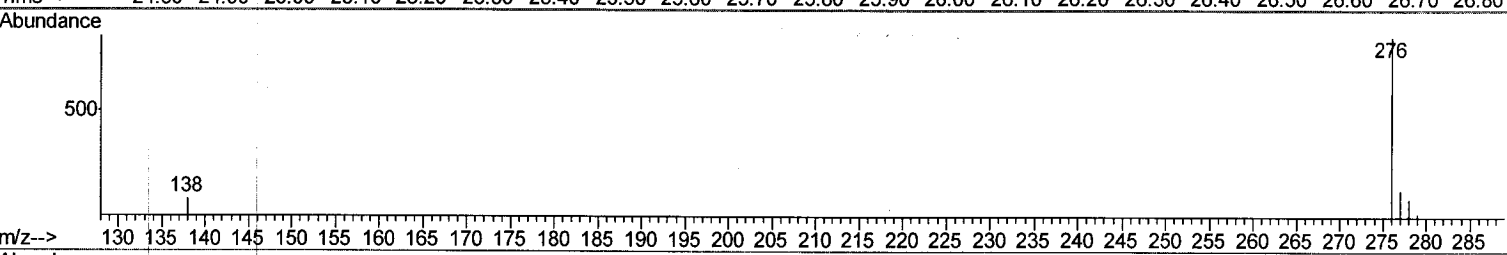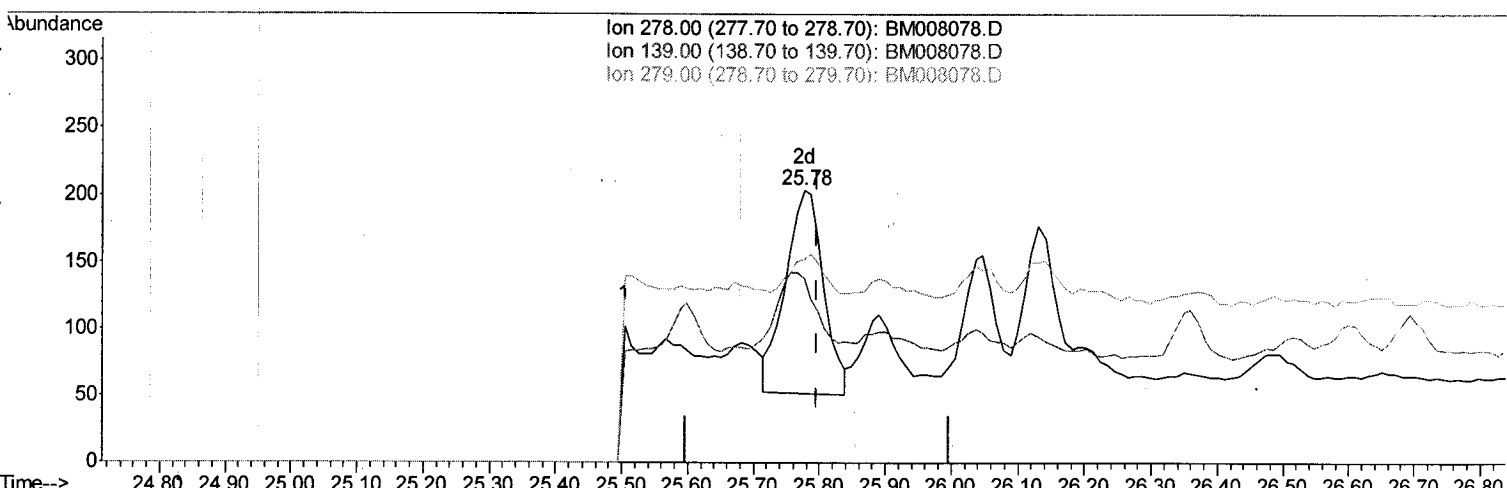

TIC: BM008078.D

(25) Dibenzo(a,h)anthracene

25.776min (-0.021) 0.08ng/ul m

response 612

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	67.65#
279.00	32.40	75.00#
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

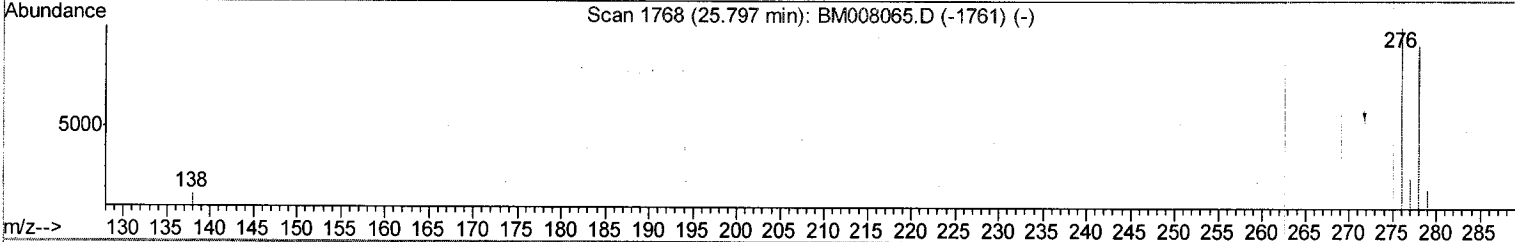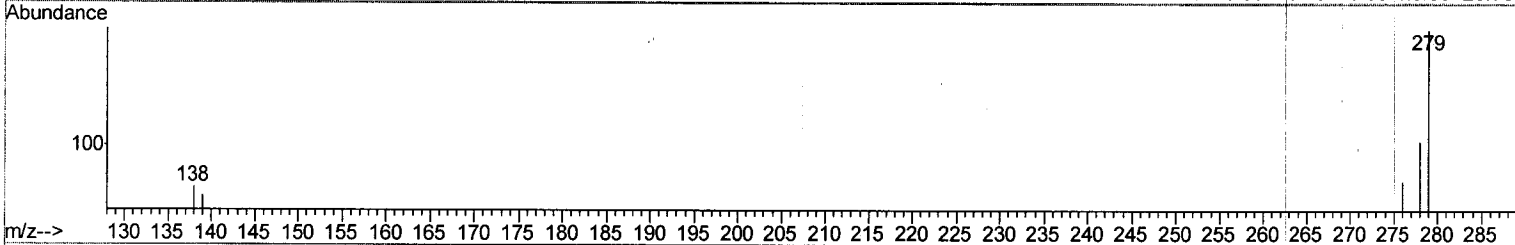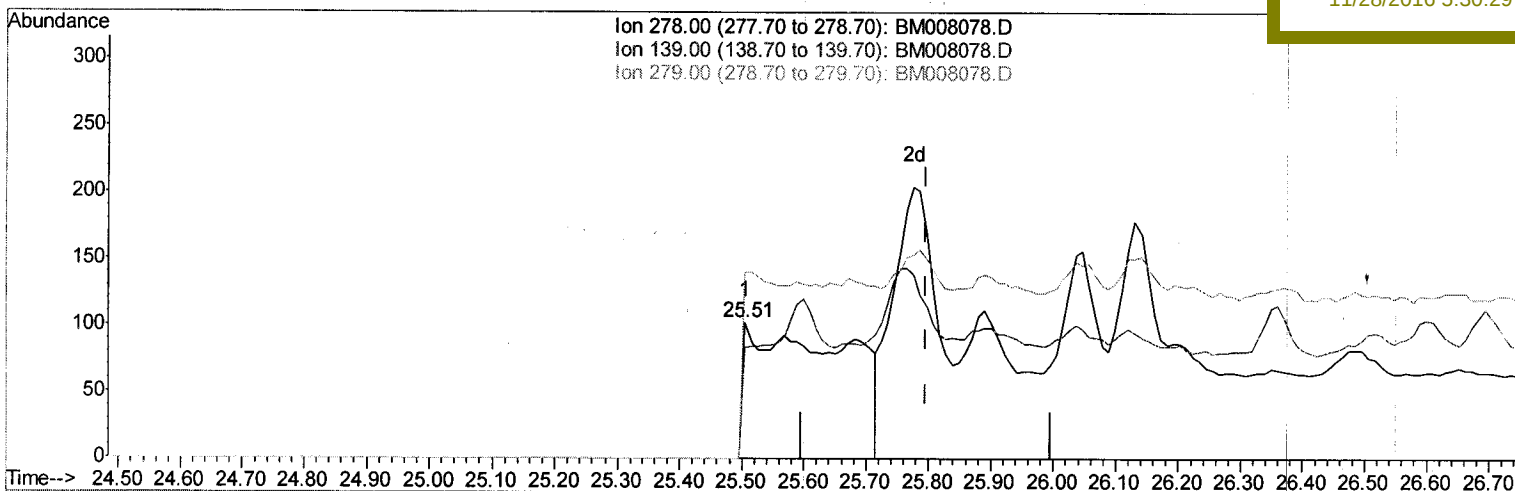

TIC: BM008078.D

(25) Dibenzo(a,h)anthracene

25.505min (-0.292) 0.14ng/ul

response 1116

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	81.37#
279.00	32.40	137.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

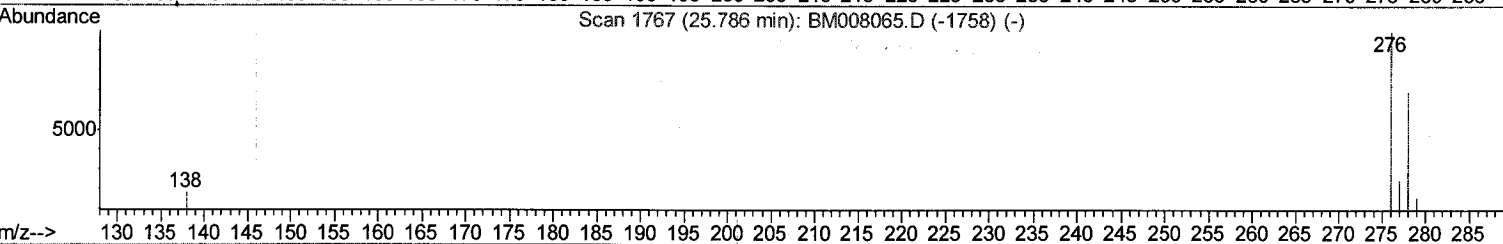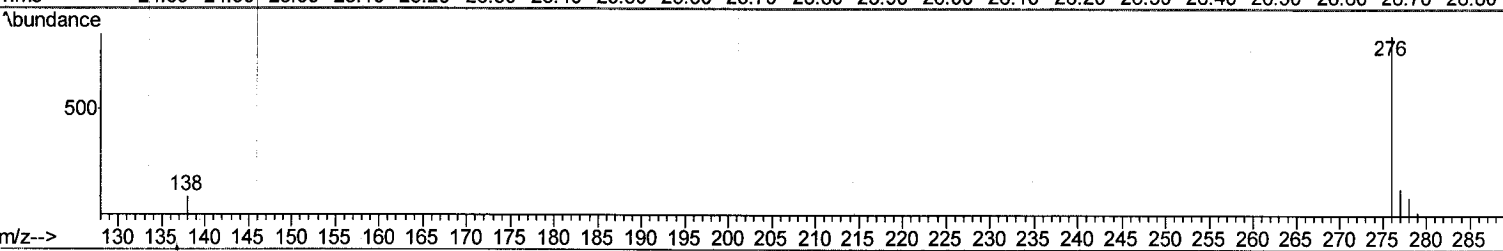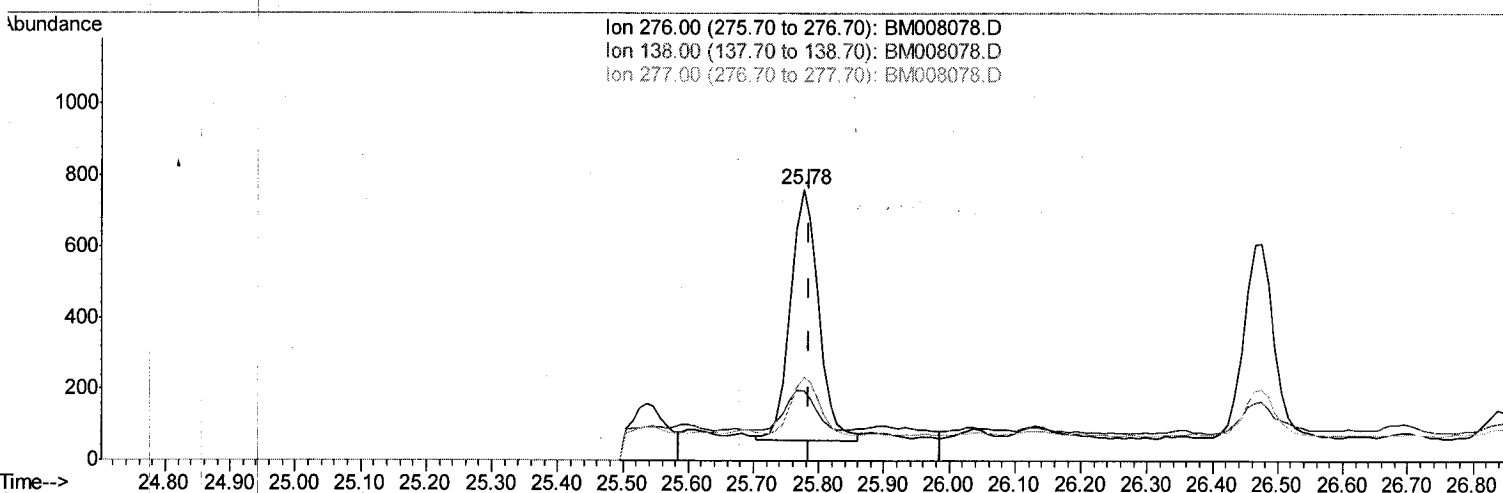

TIC: BM008078.D

(24) Indeno(1,2,3-cd)pyrene

25.776min (-0.010) 0.21ng/ul m

response 2098

Ion Exp% Act%

276.00 100 100

138.00 23.90 0.00#

277.00 24.50 53.86#

0.00 0.00 0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

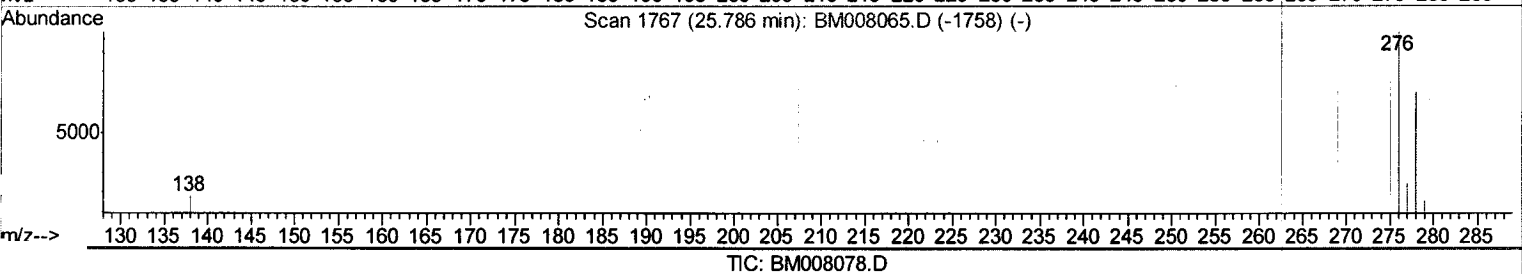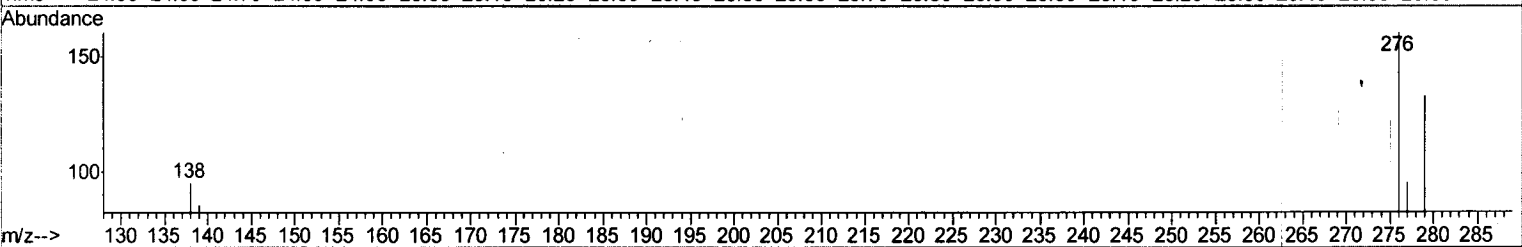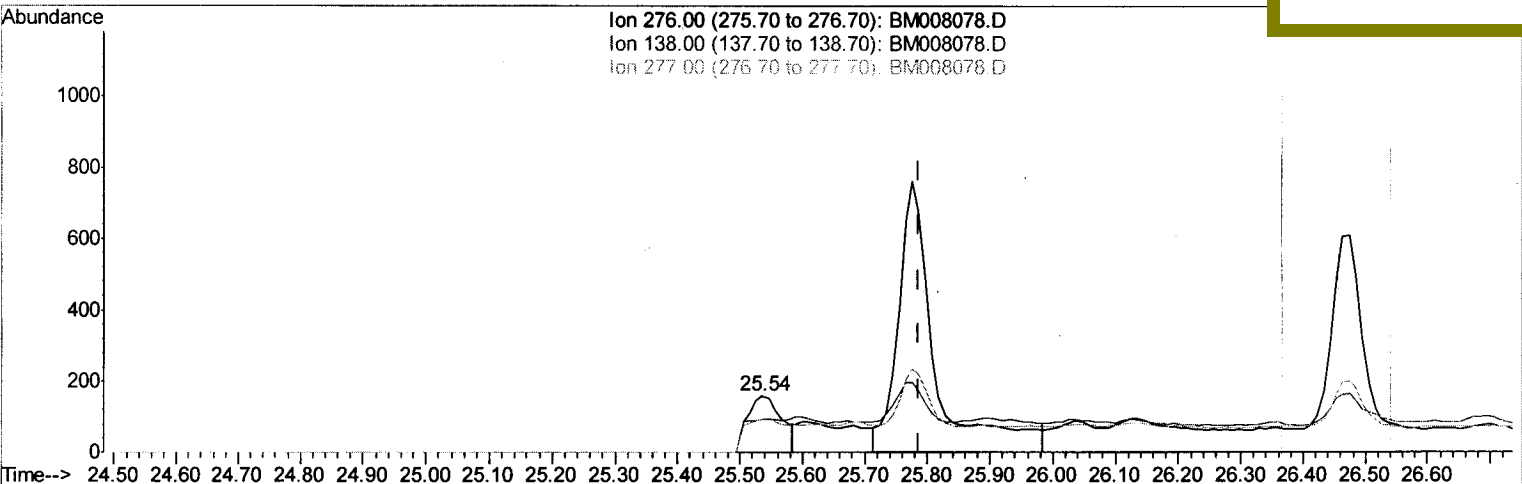

(24) Indeno(1,2,3-cd)pyrene

25.536min (-0.250) 0.12ng/ul

response 1210

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	93.39#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

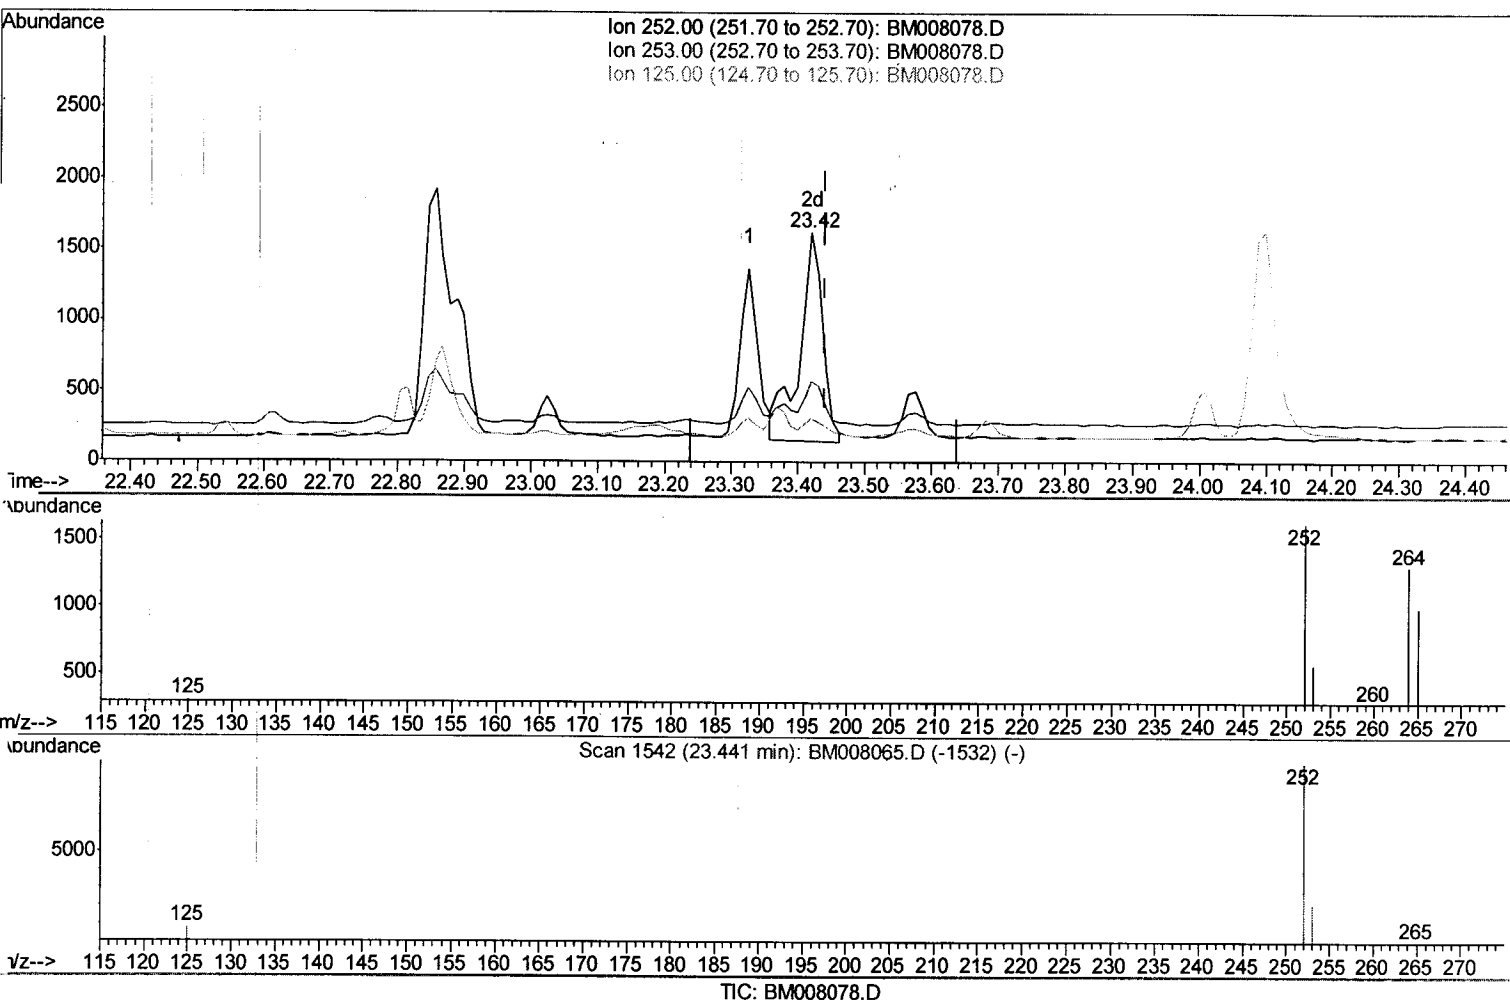

(23) Benzo(a)pyrene (C)

23.420min (-0.021) 0.44ng/ul m

response 3592

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	35.16
125.00	22.60	18.68
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

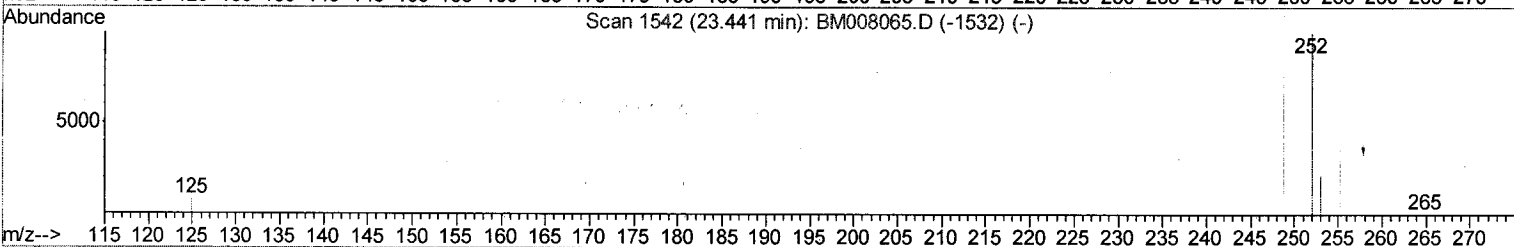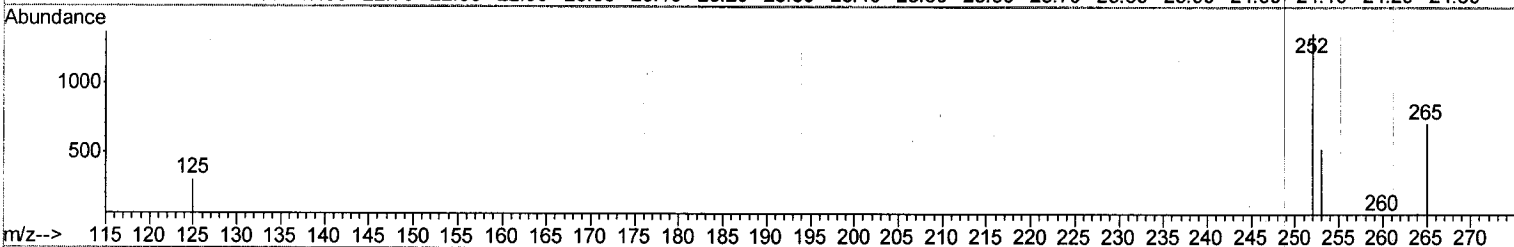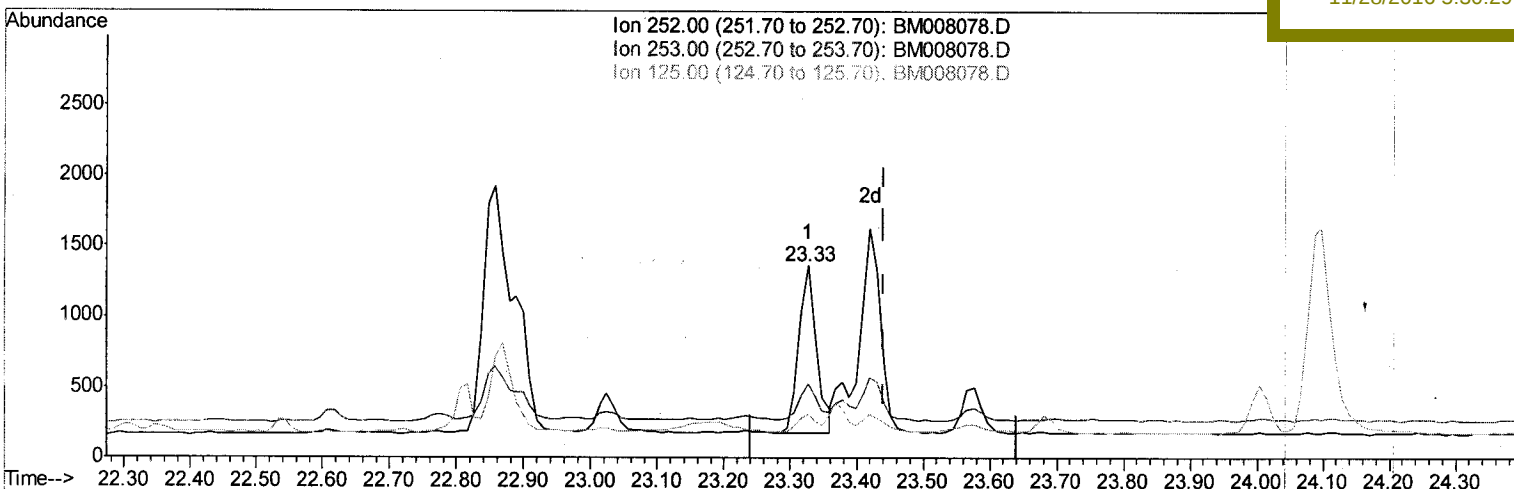

TIC: BM008078.D

(23) Benzo(a)pyrene (C)

23.326min (-0.114) 0.27ng/ul

response 2200

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	38.80
125.00	22.60	22.26
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

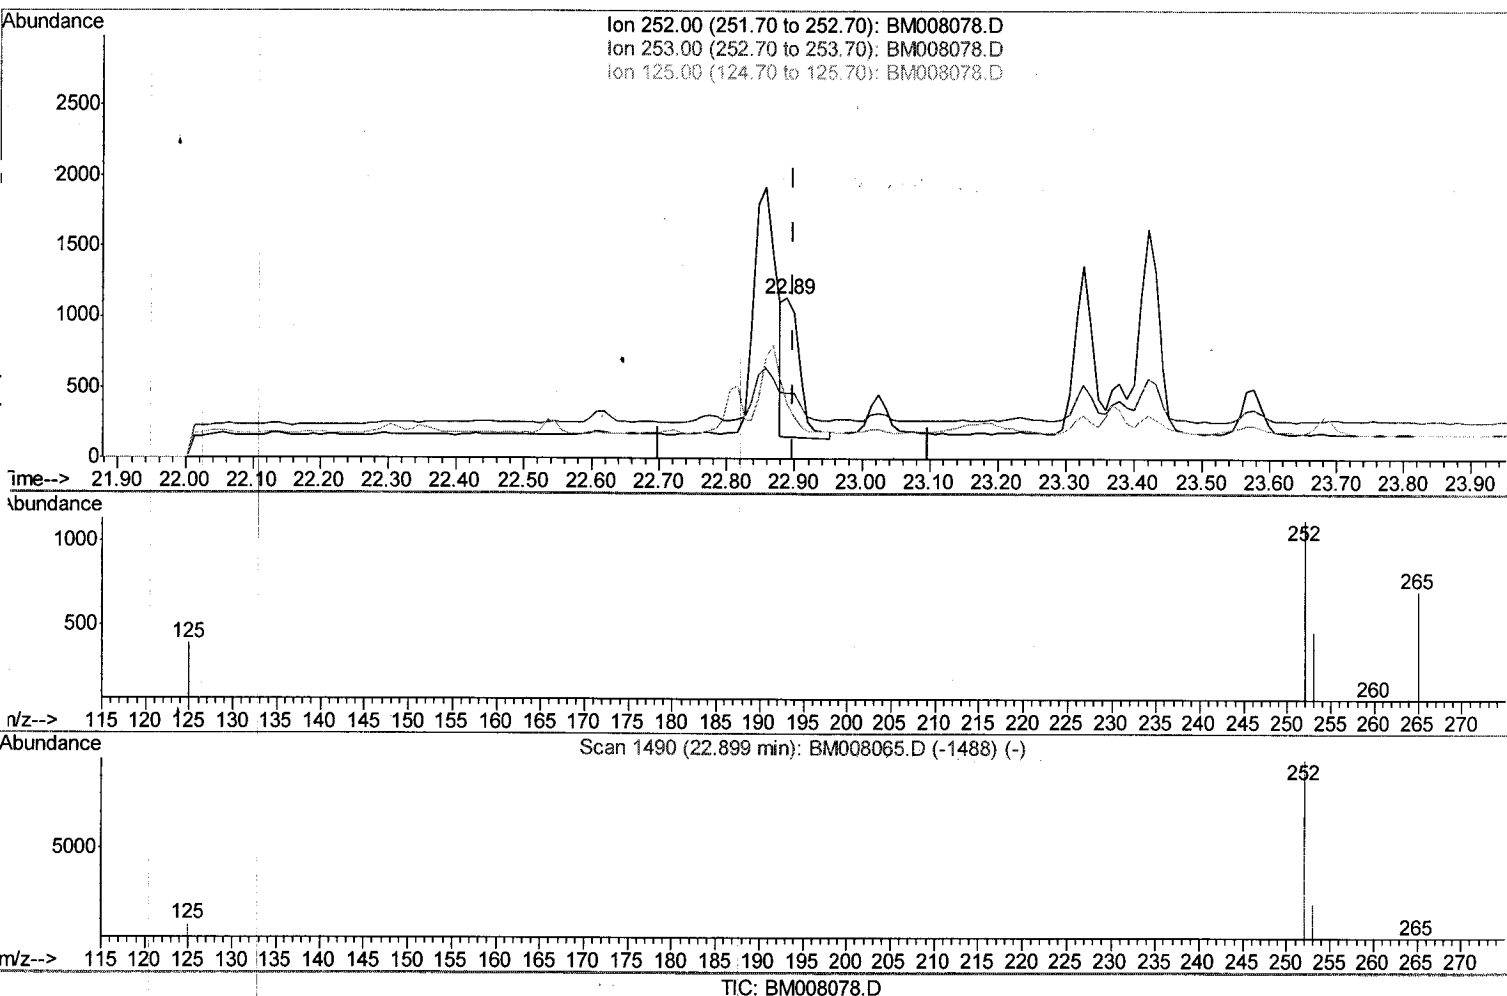

(22) Benzo(k)fluoranthene

22.889min (-0.010) 0.18ng/ul m

response 1588

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	41.18#
125.00	17.10	34.30#
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

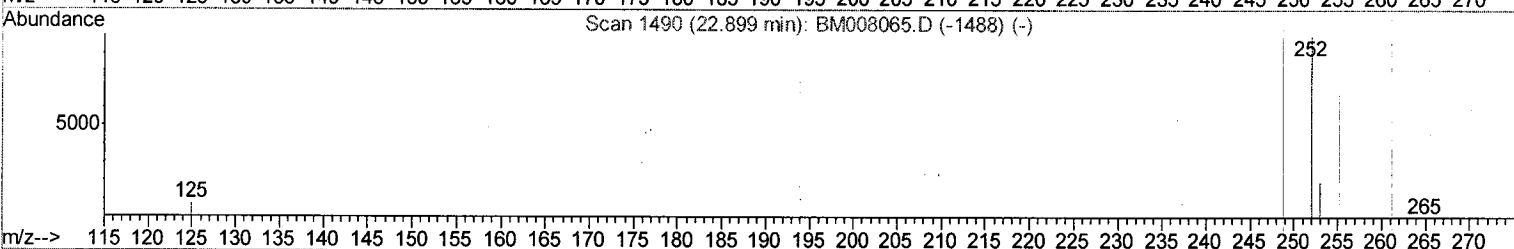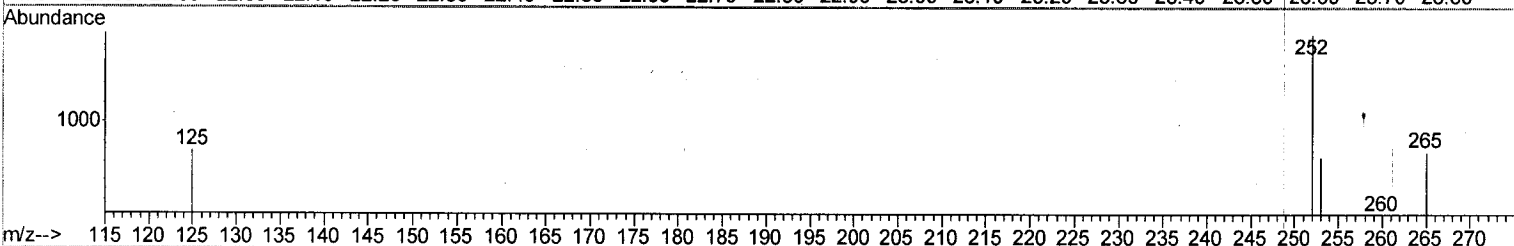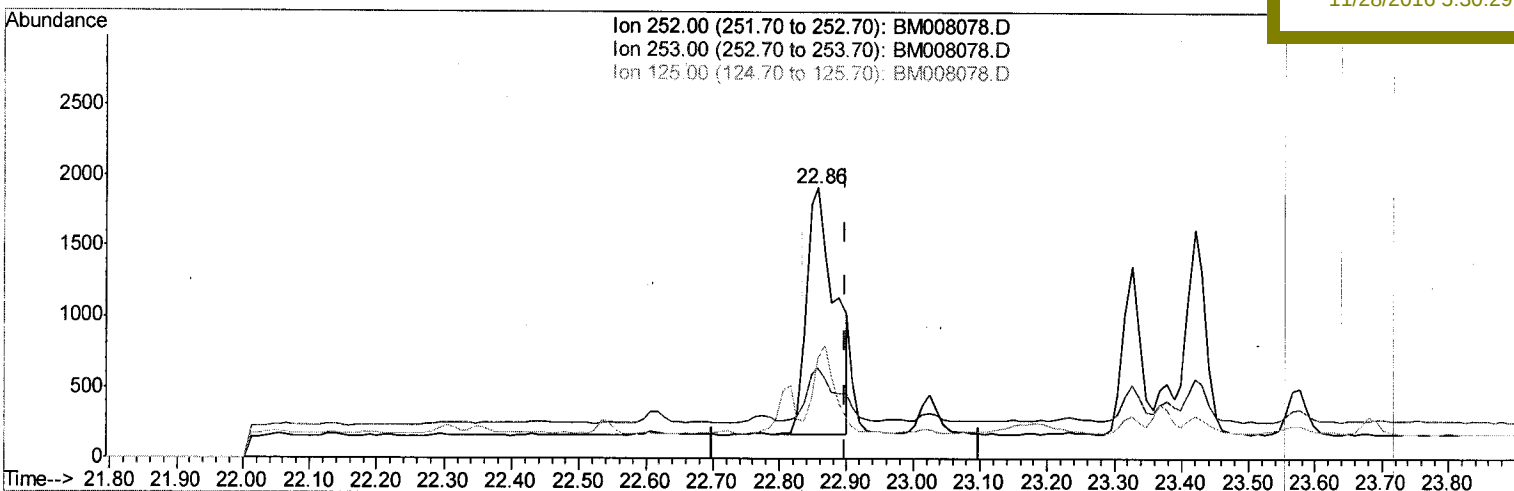

TIC: BM008078.D

(22) Benzo(k)fluoranthene

22.857min (-0.041) 0.57ng/ul

response 5158

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	33.73
125.00	17.10	36.70#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

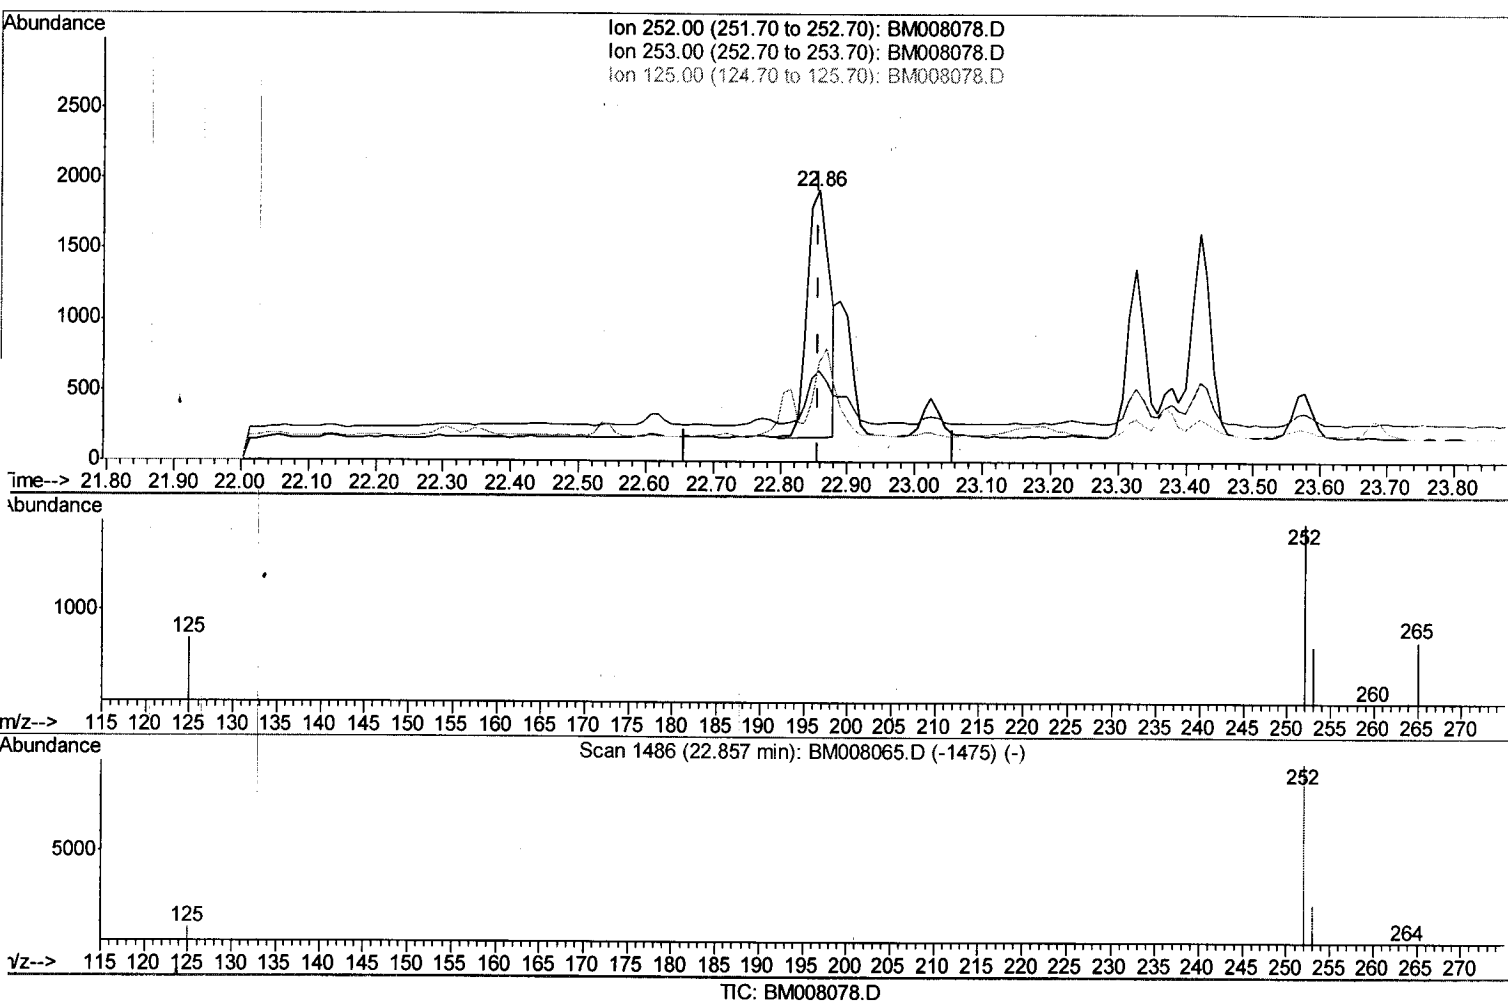

(21) Benzo(b)fluoranthene

22.857min (+0.000) 0.46ng/ul m) S. J.
 response 4029 11/29/16

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	33.73
125.00	17.50	36.70#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4WE8

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

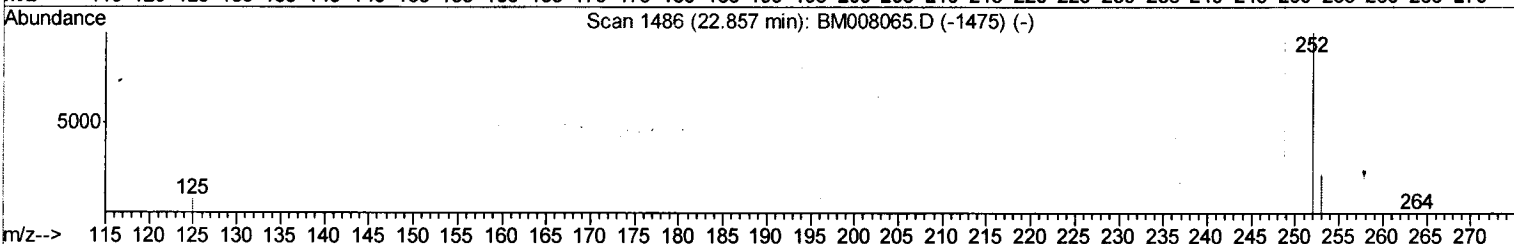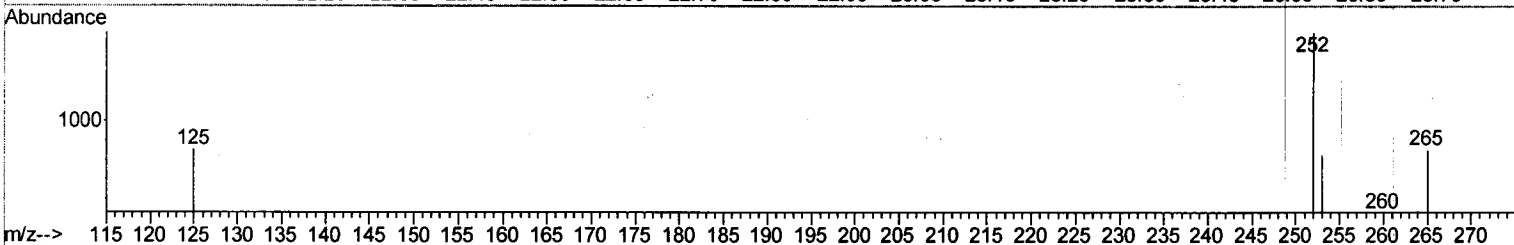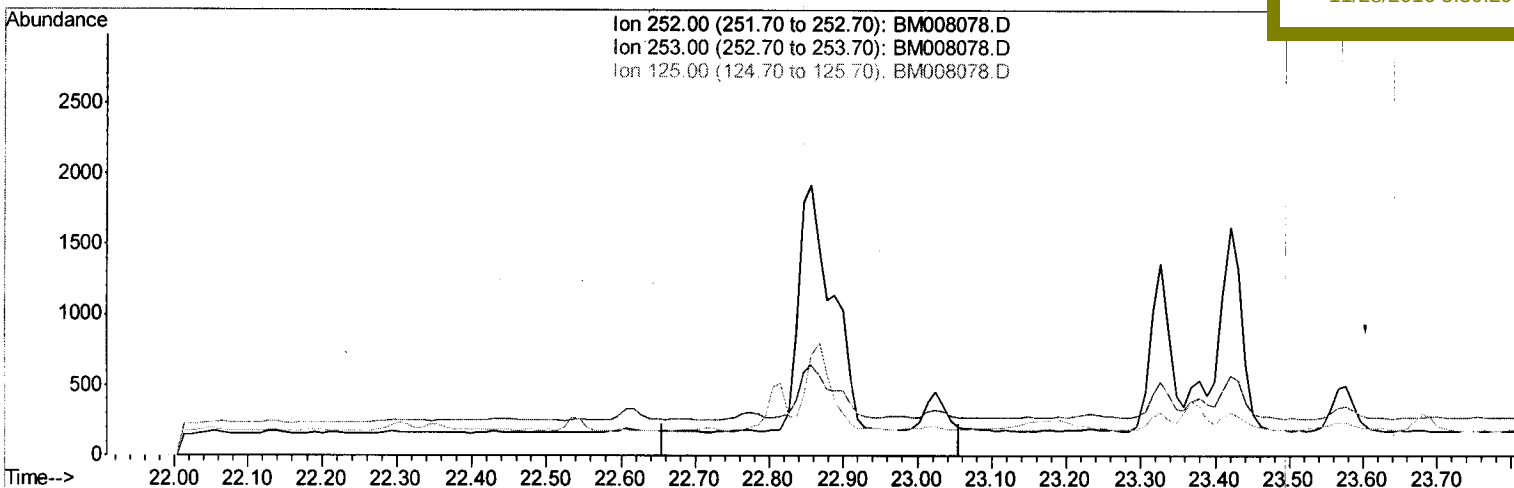

TIC: BM008078.D

(21) Benzo(b)fluoranthene

22.857min (-22.857) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	32.10	0.00
125.00	17.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

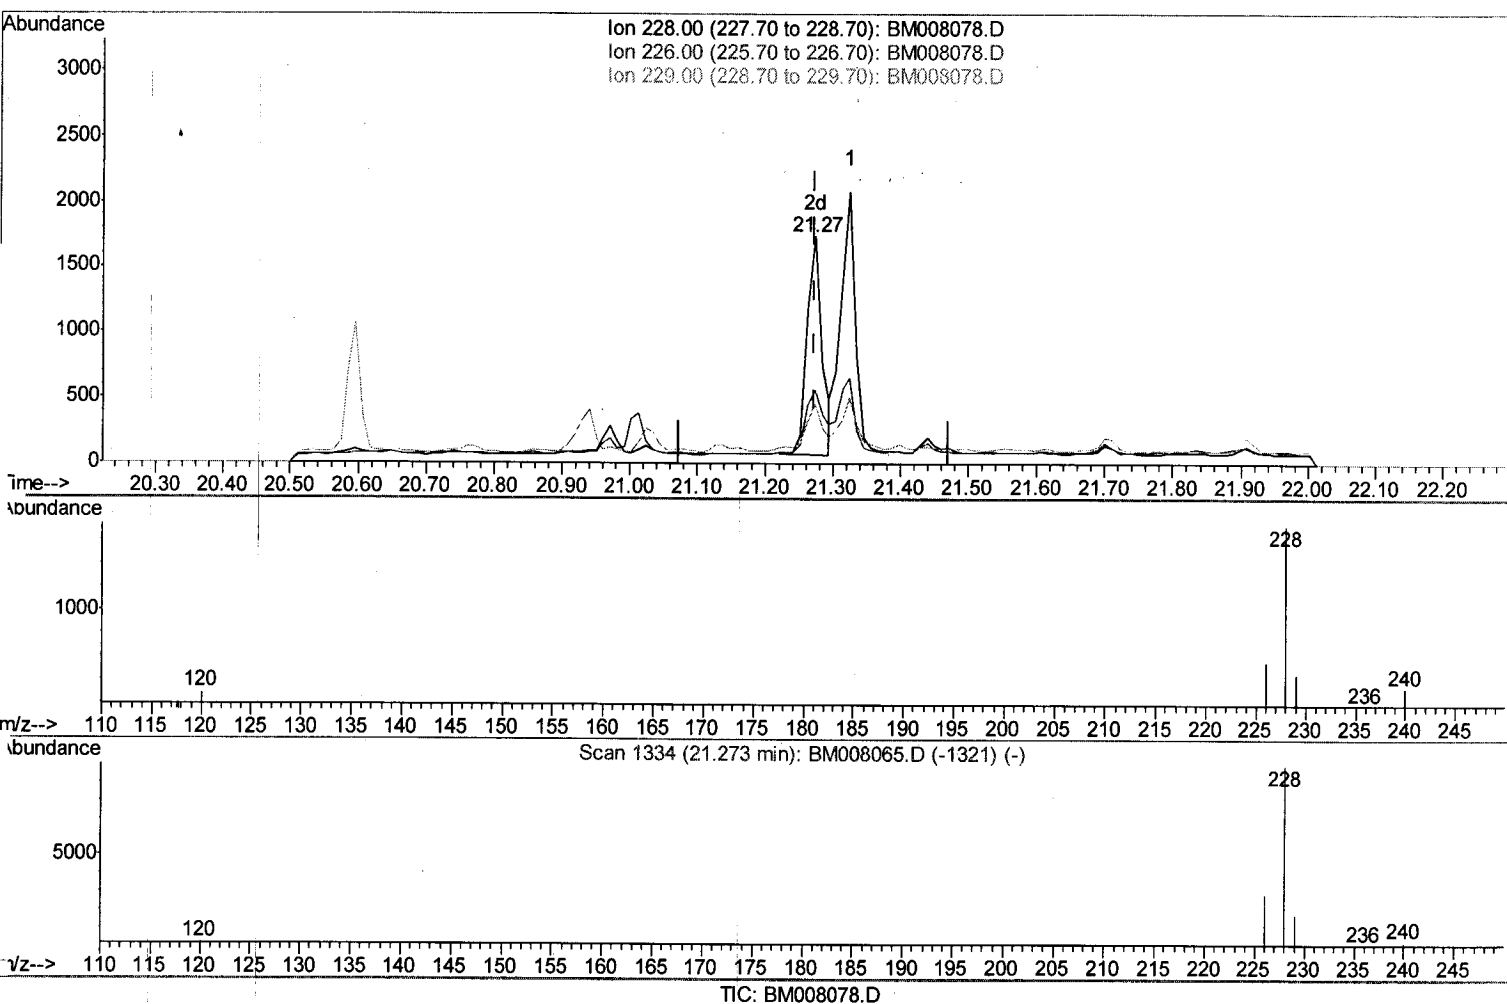

(18) Benzo(a)anthracene

21.273min (+0.000) 0.30ng/ul m

response 2536

Ion	Exp%	Act%
228.00	100	100
226.00	28.50	32.17
229.00	21.30	26.25#
0.00	0.00	0.00

S.J.
 11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 03:46:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

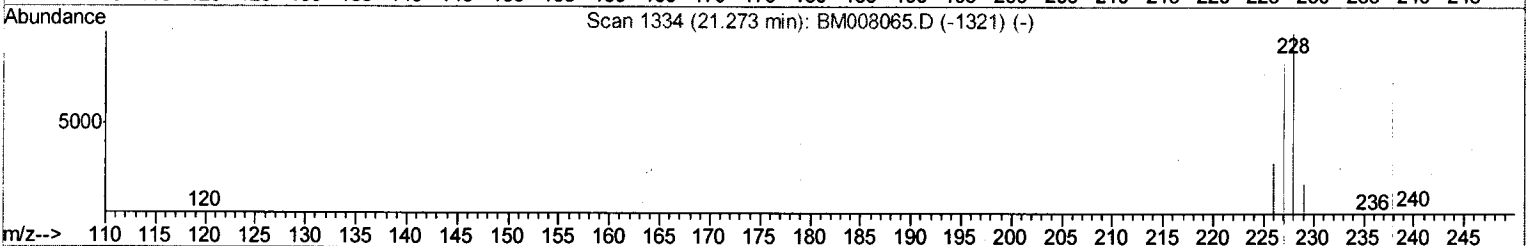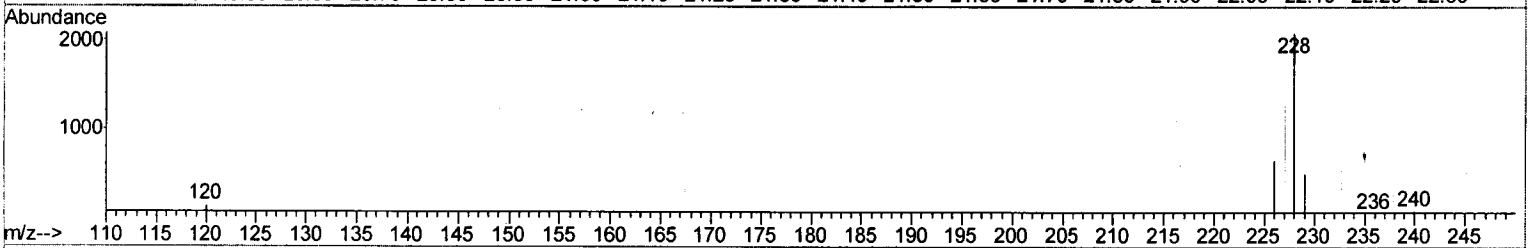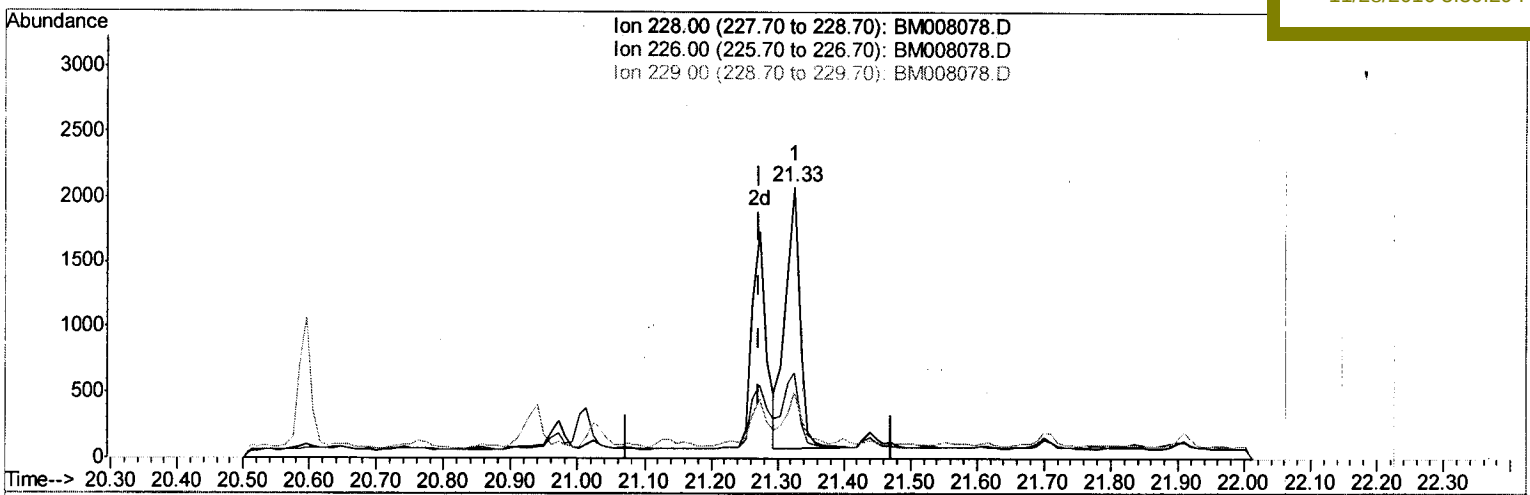

TIC: BM008078.D

(18) Benzo(a)anthracene

21.325min (+0.052) 0.37ng/ul

response 3056

Ion	Exp%	Act%
228.00	100	100
226.00	28.50	31.41
229.00	21.30	24.16
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 01:30:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

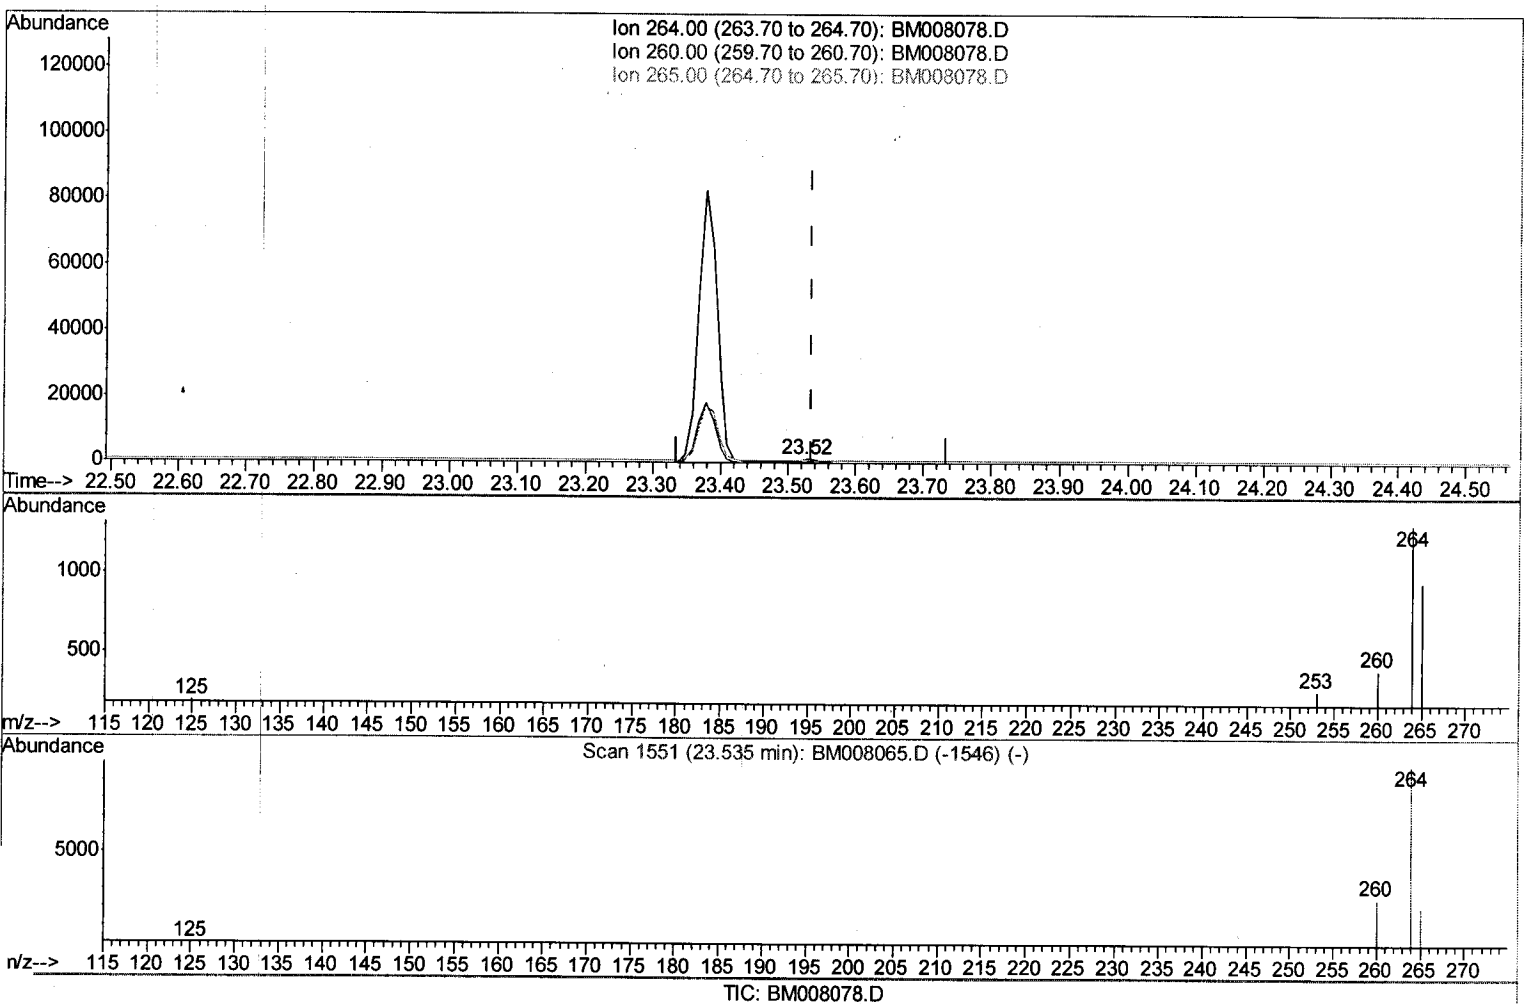

(20) Perylene-d12 (I)

23.524min (-0.010) 0.40ng/ul m > S-J.

response 2180

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.19
265.00	103.50	72.23#
0.00	0.00	0.00

11/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 01:30:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

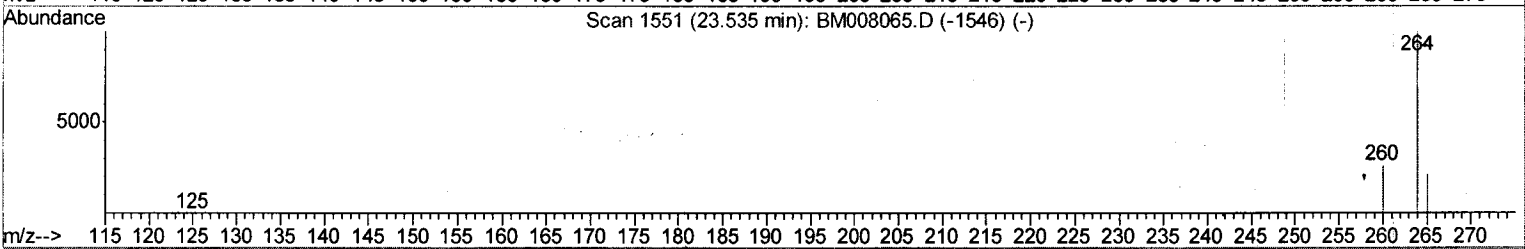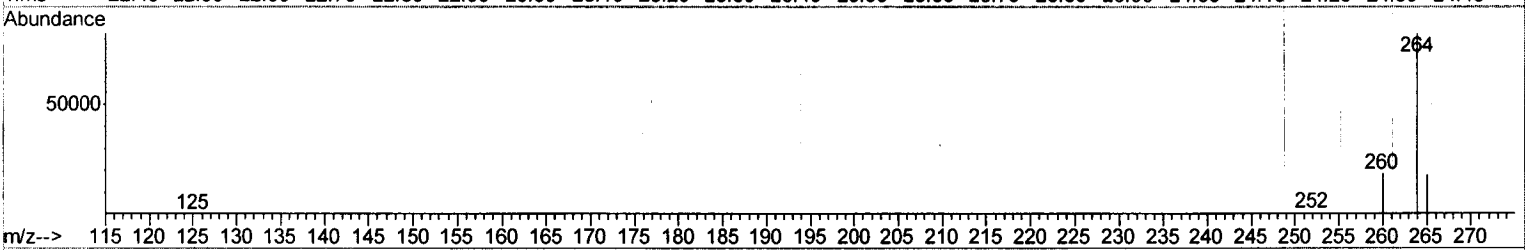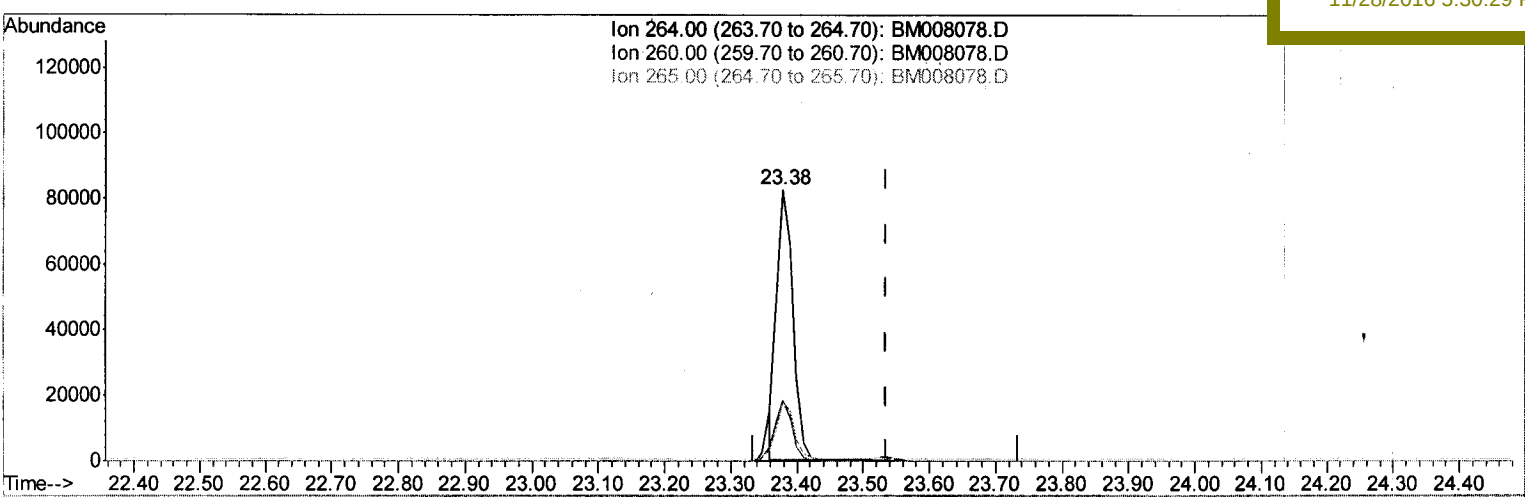

TIC: BM008078.D

(20) Perylene-d12 (I)
 23.378min (-0.156) 0.40ng/ul
 response 144405

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.24#
265.00	103.50	21.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Quant Time: Nov 25 01:30:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

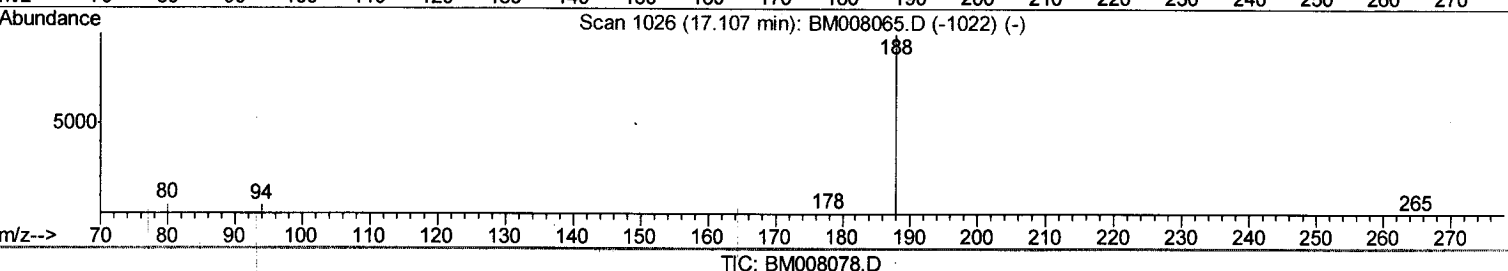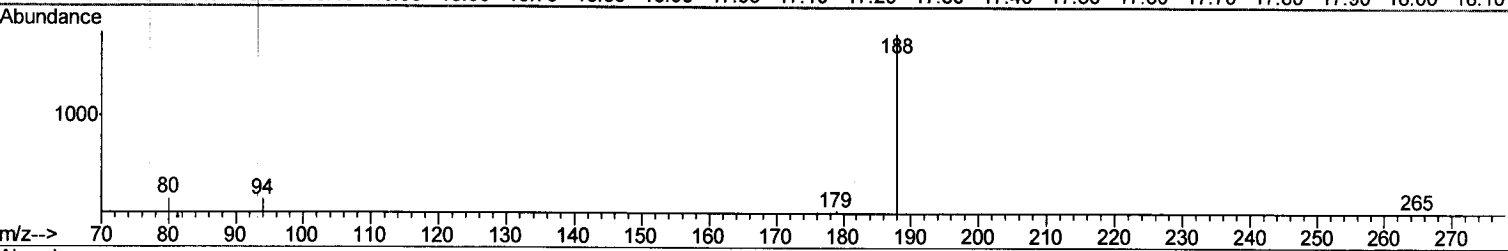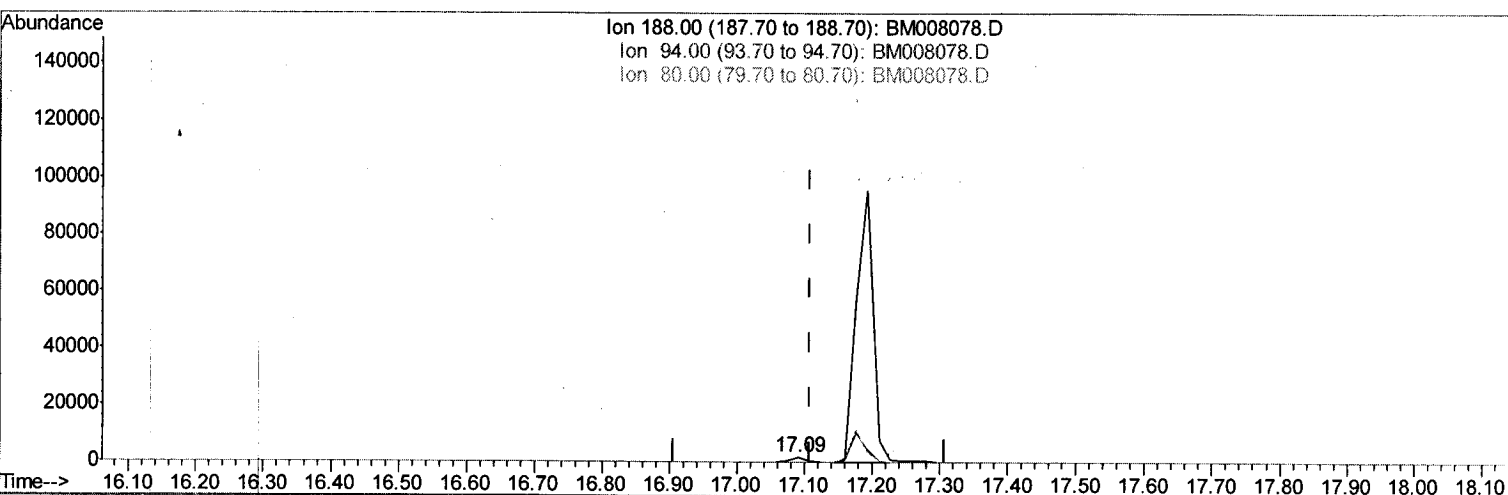

TIC: BM008078.D

(10) Phenanthrene-d10 (I)

17.090min (-0.017) 0.40ng/ul m > S.J.

response 2835

11/29/16

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.75
80.00	11.80	10.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 A4WE8

Quant Time: Nov 25 01:30:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

Umangi
 11/28/2016 5:30:29 PM

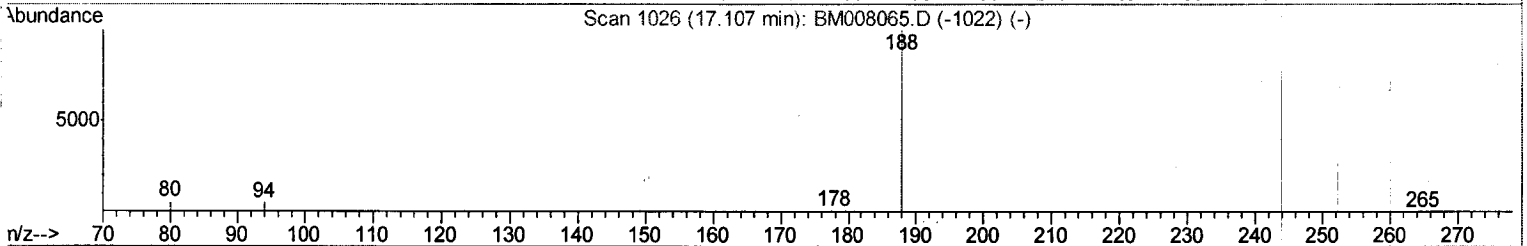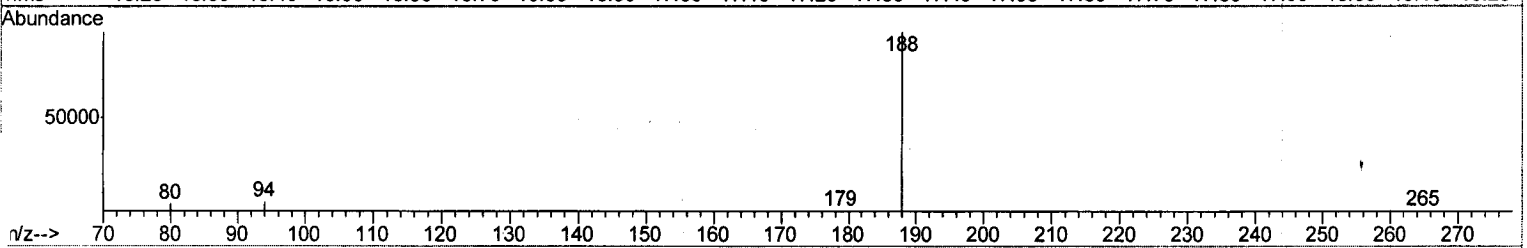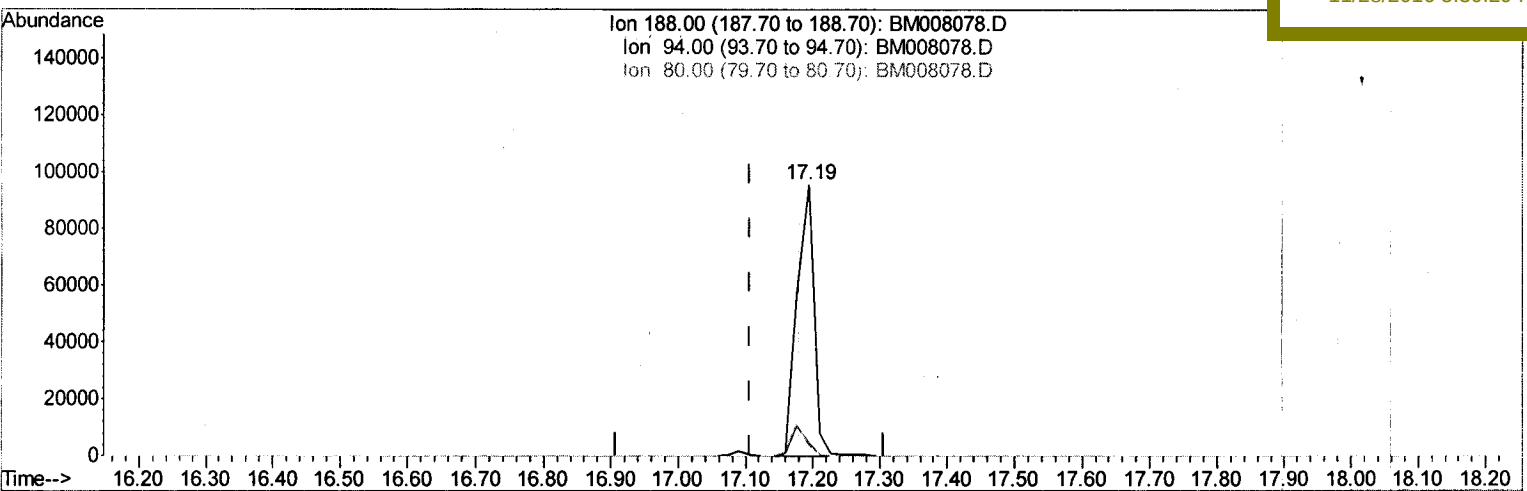

TIC: BM008078.D

(10) Phenanthrene-d10 (I)

17.193min (+0.086) 0.40ng/ul

response 167196

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	4.90#
80.00	11.80	4.01#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM112316\
 Data File : BM008078.D
 Acq On : 24 Nov 2016 17:27
 Operator : UM/SJ
 Sample : H5701-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WE8

Quant Time: Nov 25 03:48:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 25 01:27:01 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Umangi
 11/28/2016 5:30:29 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	636	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.49	136	2179	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.35	164	1377	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	2835m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.29	240	2710	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	2180m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	962	0.31	ng/ul	-0.01
14) Fluoranthene-d10	19.13	212	2120	0.26	ng/ul	0.00
Target Compounds				Qvalue		
7) Acenaphthylene	14.06	152	619	0.10	ng/ul#	81
12) Phenanthrene	17.12	178	2228	0.25	ng/ul	98
13) Anthracene	17.23	178	361	0.04	ng/ul#	62
15) Fluoranthene	19.16	202	5972	0.52	ng/ul	95
17) Pyrene	19.52	202	5935	0.63	ng/ul	98
18) Benzo(a)anthracene	21.27	228	2536m	0.30	ng/ul	
19) Chrysene	21.33	228	3053	0.30	ng/ul	96
21) Benzo(b)fluoranthene	22.86	252	4029m	0.46	ng/ul	
22) Benzo(k)fluoranthene	22.89	252	1588m	0.18	ng/ul	
23) Benzo(a)pyrene	23.42	252	3592m	0.44	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.78	276	2098m	0.21	ng/ul	
25) Dibenzo(a,h)anthracene	25.78	278	612m	0.08	ng/ul	
26) Benzo(g,h,i)perylene	26.47	276	1783m	0.20	ng/ul	

S.J.
 11/29/16

S.J.
 11/29/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed