

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112415\
 Data File : BM003286.D
 Acq On : 24 Nov 2015 14:31
 Operator : UM/IZ
 Sample : G4400-05MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YA232MS

Quant Time: Nov 25 04:07:54 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 25 04:04:01 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	5179	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	18810	0.40	ng/ul	0.01
5) Acenaphthene-d10	14.38	164	8232	0.40	ng/ul	0.00
6) Phenanthrene-d10	17.12	188	16703	0.40	ng/ul	0.00
7) Chrysene-d12	21.33	240	14288	0.40	ng/ul	0.00
8) Perylene-d12	23.58	264	13187	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.20	96	9994	1.98	ng/uL	0.00
Target Compounds						
3) 1,4-Dioxane	3.23	88	7902	1.31	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112415\
Data File : BM003286.D
Acq On : 24 Nov 2015 14:31
Operator : UM/IZ
Sample : G4400-05MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YA232MS

Quant Time: Nov 25 04:07:54 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 25 04:04:01 2015
Response via : Initial Calibration

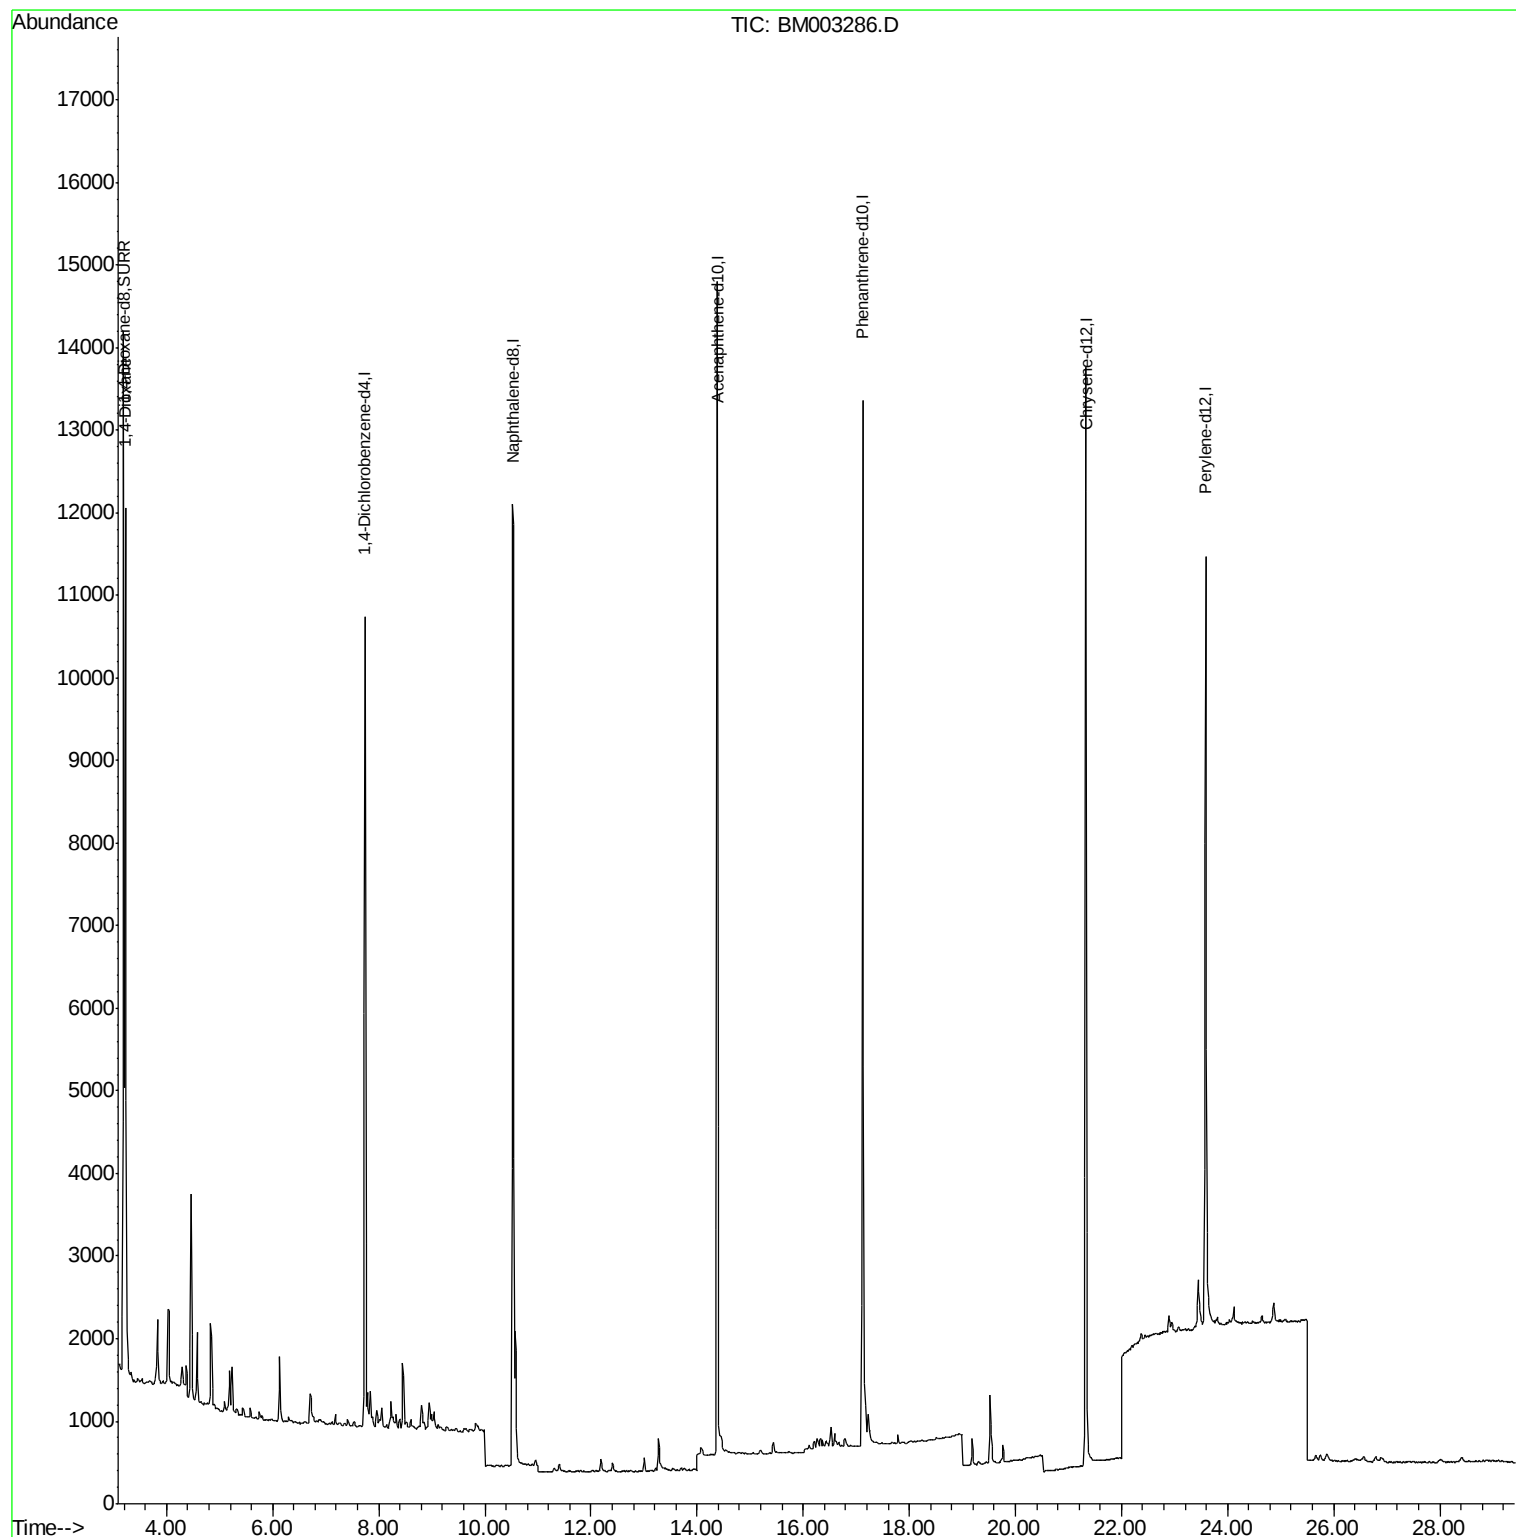


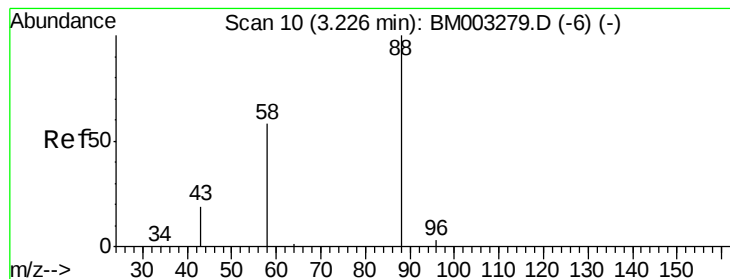

#3
 1,4-Dioxane
 Concen: 1.31 ng/ul
 RT: 3.23 min Scan# 10
 Delta R.T. -0.00 min
 Lab File: BM003286.D
 Acq: 24 Nov 2015 14:31

Instrument :
 BNA_M
 ClientSampleId :
 YA232MS

Tgt Ion: 88 Resp: 7902
 Ion Ratio Lower Upper
 88 100
 58 58.6 54.8 82.2
 43 21.7 22.6 33.8#

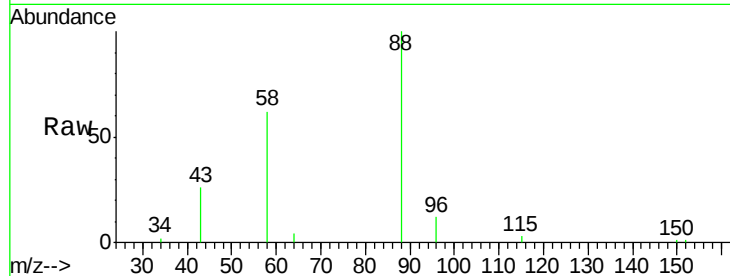

Abundance Ion 88.00 (87.70 to 88.70): BM0
 Ion 58.00 (57.70 to 58.70): BM0
 Ion 43.00 (42.70 to 43.70): BM0

