

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112415\
 Data File : BM003290.D
 Acq On : 24 Nov 2015 16:55
 Operator : UM/IZ
 Sample : PB86653BS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS53

Quant Time: Nov 25 04:18:18 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 25 04:16:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	5605	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	20290	0.40	ng/ul	0.00
5) Acenaphthene-d10	14.38	164	8889	0.40	ng/ul	0.00
6) Phenanthrene-d10	17.12	188	18081	0.40	ng/ul	0.00
7) Chrysene-d12	21.33	240	15671	0.40	ng/ul	0.00
8) Perylene-d12	23.59	264	14065	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.20	96	7480	1.37	ng/uL	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) 1,4-Dioxane	3.23	88	2402	0.37	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112415\
Data File : BM003290.D
Acq On : 24 Nov 2015 16:55
Operator : UM/IZ
Sample : PB86653BS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS53

Quant Time: Nov 25 04:18:18 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 25 04:16:44 2015
Response via : Initial Calibration

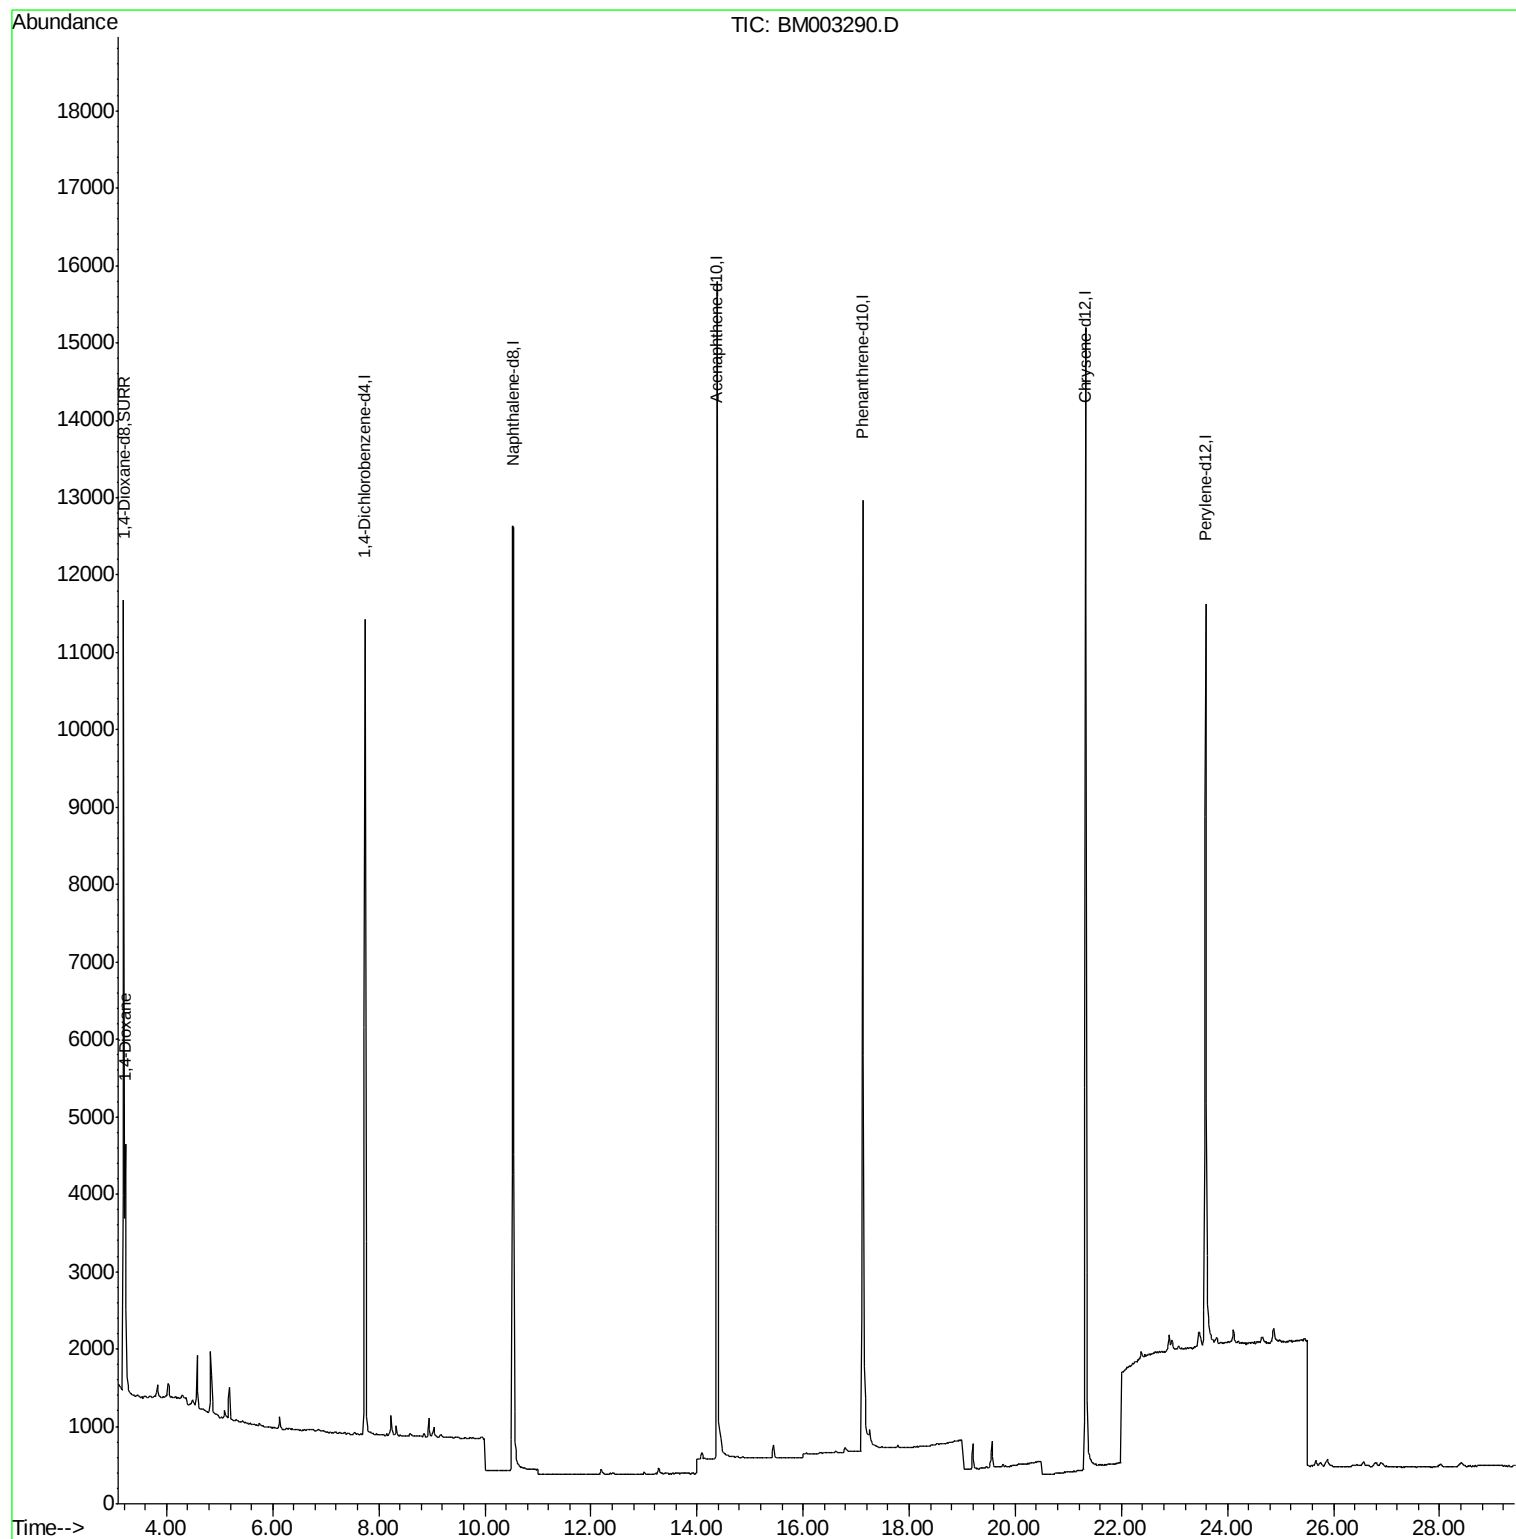

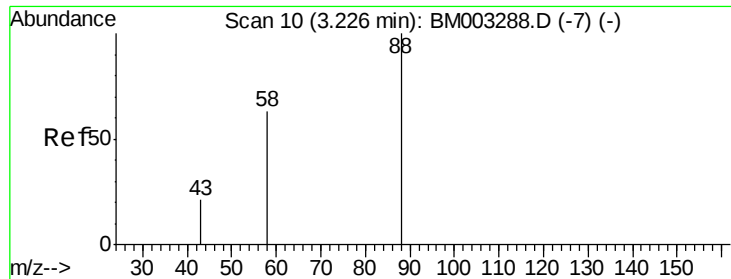

#3

1,4-Dioxane

Concen: 0.37 ng/ul

RT: 3.23 min Scan# 10

Delta R.T. 0.00 min

Lab File: BM003290.D

Acq: 24 Nov 2015 16:55

Instrument :

BNA_M

ClientSampleId :

SLCS53

Tot Ion: 88 Resp: 2402

Ion Ratio Lower Upper

88 100

58 55.7 54.8 82.2

43 21.7 22.6 33.8#

