


Data Path : Z:\HPCHEM1\BNA M\DATA\BM112415\
 Data File : BM003278.D
 Acq On : 24 Nov 2015 09:01
 Operator : UM/IZ
 Sample : DFTPP50
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP50

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 25 04:16:44 2015

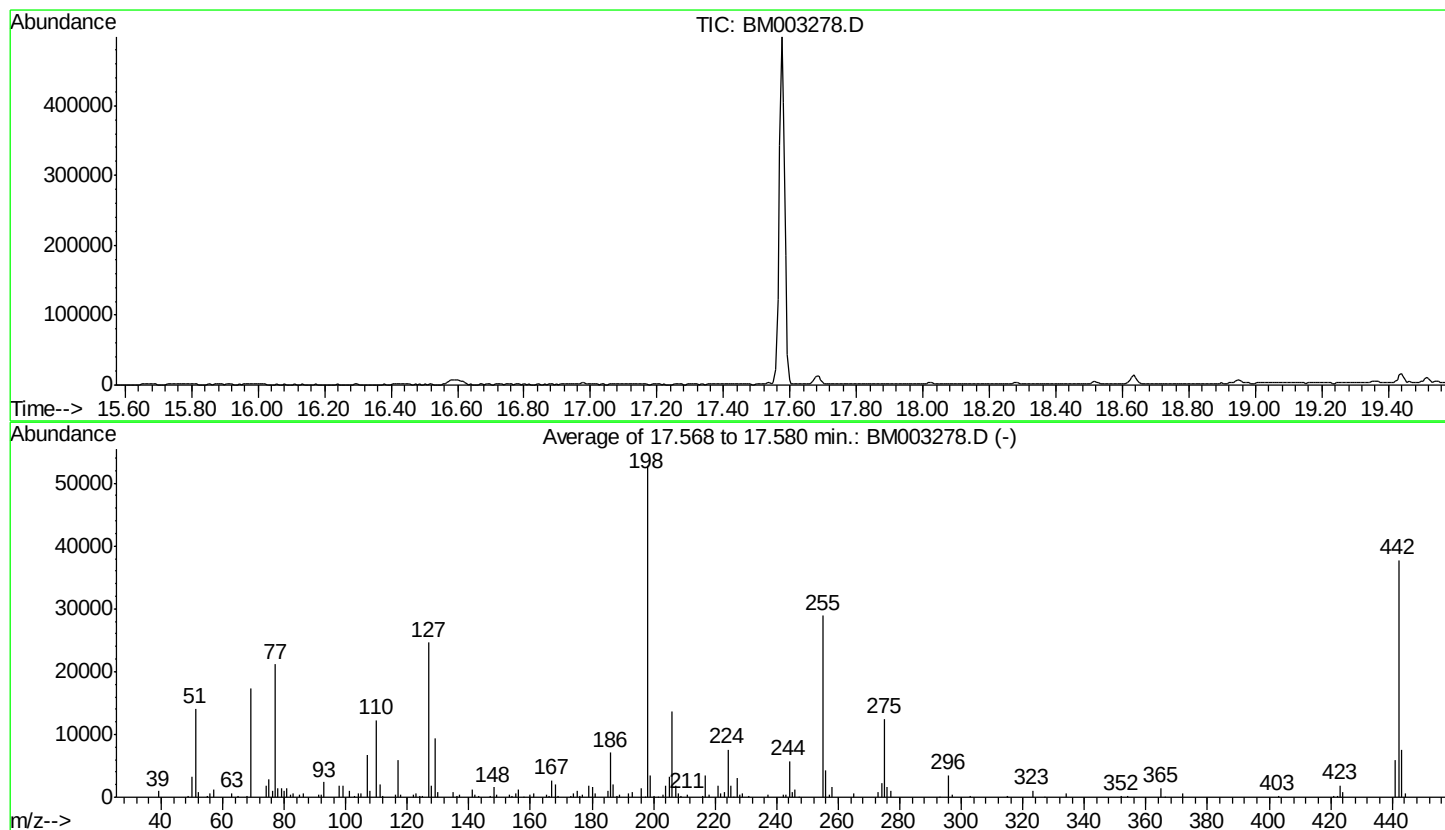

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	14083	PASS
68	69	0.00	2	1.3	231	PASS
69	198	0.00	100	32.9	17379	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	24642	PASS
197	198	0.00	1	0.2	106	PASS
198	198	100	100	100.0	52792	PASS
199	198	5	9	6.6	3464	PASS
275	198	10	60	23.7	12523	PASS
365	198	1	100	2.8	1471	PASS
441	443	0.01	100	78.1	5917	PASS
442	198	50	100	71.5	37768	PASS
443	442	15	24	20.1	7573	PASS

Scan 2456 (17.533 min): BM003278.D
DFTPP50

m/z	Abundance
73.10	939.0
147.00	439.0
207.10	1169.0
221.10	312.0
281.10	333.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

m/z	Abundance
39.00	943.0
48.90	335.0
50.10	3198.0
51.10	13902.0
52.00	748.0
56.00	511.0
57.00	1079.0
63.00	571.0
65.00	366.0
68.00	313.0
69.00	16816.0
73.00	412.0
74.00	1663.0
75.00	2797.0
76.10	910.0
77.10	20424.0
78.10	1323.0
79.00	1330.0
80.00	1116.0
81.00	1287.0
82.00	467.0
83.00	487.0
85.00	379.0
86.00	528.0
91.00	321.0
92.00	435.0
93.00	2241.0
98.00	1788.0
99.00	1857.0
101.00	807.0
104.00	454.0
105.00	541.0
107.00	6342.0
108.00	968.0
110.00	11426.0
111.00	1987.0
115.90	360.0
117.00	5325.0
118.00	435.0
121.90	370.0
122.90	673.0
127.00	22208.0
128.00	1811.0
129.00	8405.0
130.00	732.0
135.00	682.0
137.10	458.0
141.00	1127.0
141.90	381.0
147.10	657.0
148.00	1343.0
148.90	405.0
153.00	345.0
154.00	338.0
155.10	608.0
156.10	980.0
159.90	359.0
161.00	497.0
165.00	387.0
167.10	2331.0
168.00	2148.0
169.00	318.0
173.00	312.0
174.00	463.0
175.00	884.0
176.00	321.0
176.90	386.0
179.00	1516.0
180.00	1462.0
181.00	642.0
185.00	707.0
186.10	6090.0
187.00	1829.0
188.90	437.0
192.00	589.0
193.00	636.0
196.00	1119.0
198.00	43432.0
199.00	2964.0
202.90	344.0
204.10	1667.0
205.00	2598.0
206.10	11436.0
207.10	2637.0
208.00	613.0
209.00	309.0
211.10	405.0
217.00	2834.0
218.00	305.0
221.10	2015.0
221.90	489.0
223.00	719.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

224.10	5939.0
225.00	1499.0
227.10	2715.0
228.00	409.0
229.00	539.0
237.00	460.0
242.00	319.0
243.00	380.0
244.10	4786.0
245.10	647.0
246.00	699.0
255.10	22144.0
256.00	3532.0
257.00	356.0
258.00	1283.0
265.10	480.0
273.10	726.0
274.00	1603.0
275.10	9256.0
276.00	1369.0
277.00	838.0
296.00	2591.0
297.00	391.0
314.90	309.0
323.10	658.0
334.10	470.0
365.00	930.0
372.10	371.0
423.10	1259.0
424.10	567.0
441.10	3547.0
442.10	22480.0
443.10	4561.0
444.10	432.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

m/z	Abundance
39.10	1239.0
50.10	3912.0
51.10	16552.0
52.00	839.0
55.00	368.0
56.00	717.0
57.00	1255.0
63.00	709.0
65.00	422.0
68.00	381.0
69.00	20912.0
73.00	422.0
74.00	2102.0
75.00	3418.0
76.00	1147.0
77.10	25176.0
78.10	1781.0
79.00	1528.0
80.00	1235.0
81.00	1949.0
82.00	508.0
83.00	581.0
85.00	450.0
86.00	566.0
91.00	480.0
92.00	509.0
93.00	2734.0
98.00	2265.0
99.00	2088.0
101.00	1142.0
103.00	373.0
104.00	696.0
105.00	712.0
107.00	7781.0
108.00	1319.0
110.00	14730.0
111.00	2399.0
112.00	359.0
116.00	402.0
117.00	7149.0
118.00	638.0
122.00	496.0
123.00	871.0
124.00	378.0
125.00	389.0
127.00	29200.0
128.00	2249.0
129.00	11379.0
130.00	948.0
135.00	961.0
136.00	413.0
137.00	605.0
141.00	1496.0
142.00	517.0
143.00	357.0
147.10	869.0
148.00	1961.0
148.90	470.0
153.00	517.0
155.00	868.0
156.00	1404.0
157.90	324.0
160.00	525.0
161.00	725.0
165.00	632.0
166.00	444.0
167.00	3362.0
168.00	2496.0
169.10	357.0
173.00	394.0
174.00	663.0
175.00	1208.0
176.00	332.0
176.90	561.0
179.00	2252.0
180.00	1858.0
181.00	784.0
185.10	1225.0
186.10	8587.0
187.10	2429.0
188.00	386.0
189.00	604.0
192.00	609.0
193.00	929.0
196.00	1765.0
197.10	319.0
198.00	64176.0
199.00	4259.0
200.00	356.0
201.30	325.0
203.00	515.0
204.00	2285.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

205.10	3886.0
206.10	16440.0
207.10	3316.0
208.00	853.0
211.10	574.0
216.10	381.0
217.00	4051.0
218.00	458.0
221.10	2344.0
221.80	617.0
223.00	984.0
224.10	9316.0
225.10	2297.0
226.10	306.0
227.00	3479.0
228.00	577.0
229.10	900.0
231.10	383.0
237.00	473.0
242.00	435.0
243.10	401.0
244.10	6795.0
245.10	963.0
246.00	1438.0
255.10	34864.0
256.10	5049.0
257.10	479.0
258.00	1920.0
265.00	767.0
273.00	926.0
274.10	2728.0
275.10	14906.0
276.10	2204.0
277.00	1243.0
296.00	4043.0
297.00	639.0
303.00	425.0
315.10	464.0
323.10	1239.0
334.10	775.0
352.10	410.0
354.10	423.0
365.10	1618.0
366.10	304.0
372.10	710.0
403.00	393.0
421.10	440.0
423.10	2042.0
424.10	990.0
441.10	6855.0
442.10	43840.0
443.10	9008.0
444.10	864.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

m/z	Abundance
39.10	830.0
50.00	2849.0
51.10	11797.0
52.00	625.0
56.00	468.0
57.00	1052.0
63.00	595.0
69.00	14411.0
73.00	333.0
74.00	1627.0
75.00	2562.0
76.00	988.0
77.10	17984.0
78.00	1286.0
79.00	1164.0
80.00	913.0
81.00	1289.0
82.00	438.0
83.00	492.0
85.10	365.0
86.00	468.0
91.00	431.0
92.00	444.0
93.00	2120.0
98.00	1552.0
99.00	1706.0
101.00	824.0
104.00	533.0
105.00	554.0
107.00	6218.0
108.00	858.0
110.00	10550.0
111.00	1575.0
116.00	329.0
117.00	5243.0
118.00	449.0
122.00	399.0
123.00	589.0
124.00	331.0
125.00	307.0
127.00	22520.0
128.00	1724.0
129.00	8433.0
130.00	678.0
135.00	710.0
137.00	480.0
141.00	1053.0
142.10	320.0
147.00	586.0
148.00	1383.0
149.00	355.0
153.00	389.0
155.00	670.0
156.00	1044.0
160.00	353.0
161.00	649.0
165.10	464.0
165.90	379.0
167.00	2284.0
168.00	1790.0
174.00	592.0
175.00	927.0
177.00	435.0
179.00	1903.0
180.10	1315.0
181.00	592.0
185.00	930.0
186.10	6682.0
187.00	1941.0
189.00	371.0
192.00	635.0
193.00	664.0
196.00	1477.0
198.00	50768.0
199.00	3169.0
203.00	468.0
204.10	1658.0
205.00	3203.0
206.10	13322.0
207.10	2906.0
208.10	648.0
209.00	315.0
211.10	500.0
217.00	3478.0
218.00	466.0
221.10	2142.0
221.80	560.0
223.00	808.0
224.10	7470.0
225.10	1804.0
227.00	3056.0
228.00	396.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

229.00	605.0
237.10	324.0
242.00	380.0
243.00	416.0
244.10	5859.0
245.00	669.0
246.00	1276.0
247.00	320.0
255.10	29736.0
256.00	4402.0
257.00	398.0
258.00	1711.0
265.00	775.0
273.10	907.0
274.10	2167.0
275.10	13407.0
276.10	1623.0
277.00	1171.0
293.00	324.0
296.00	3895.0
297.00	503.0
303.10	368.0
315.00	418.0
323.10	1213.0
327.00	326.0
334.00	746.0
352.00	326.0
354.20	390.0
365.00	1867.0
372.10	628.0
403.10	374.0
421.10	355.0
422.10	333.0
423.10	2434.0
424.10	683.0
441.10	7351.0
442.10	46984.0
443.10	9150.0
444.10	751.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50