
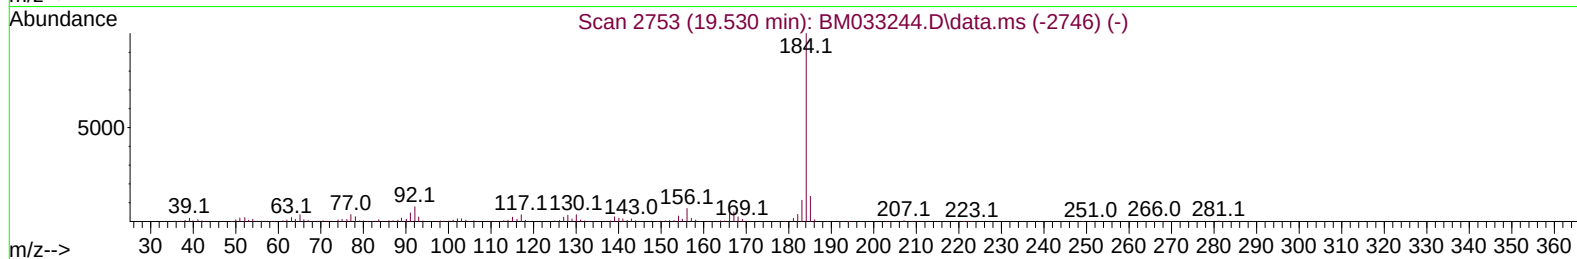
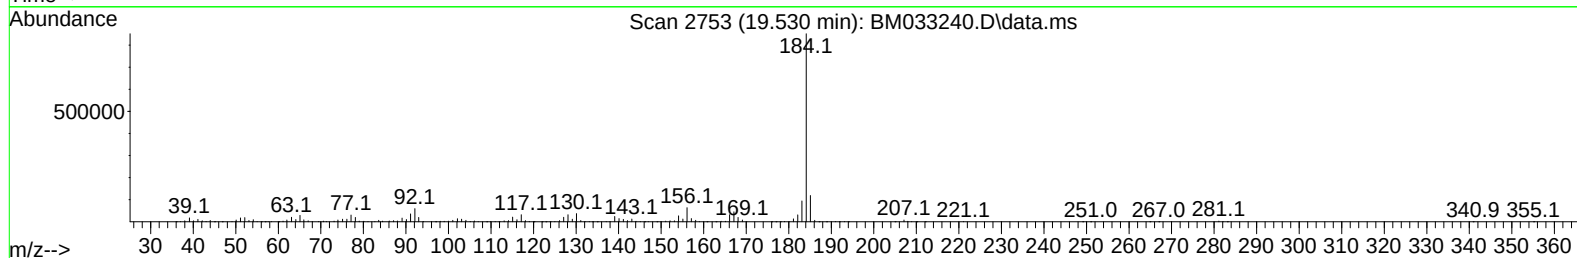


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
 Data File : BM033240.D
 Acq On : 24 Nov 2021 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 18:20:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

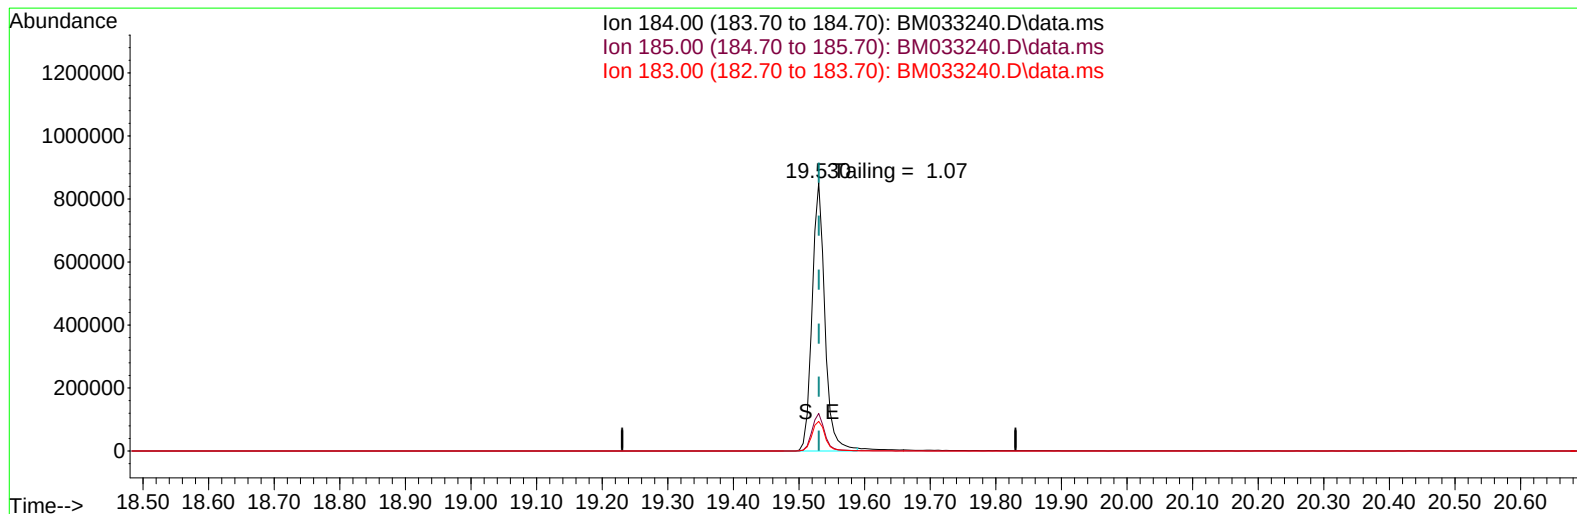

TIC: BM033240.D\data.ms

(77) Benzidine




19.530min (-0.000) 0.00 ng

response 1182164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.00
183.00	11.20	11.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
 Data File : BM033240.D
 Acq On : 24 Nov 2021 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 18:20:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

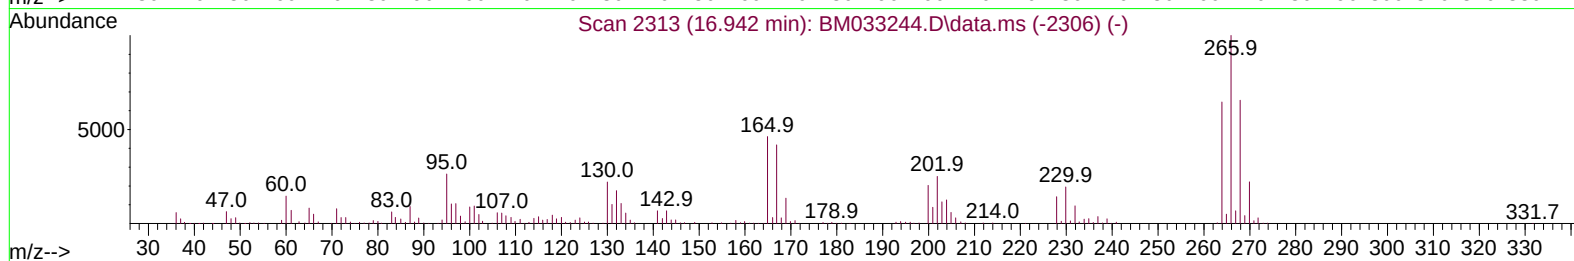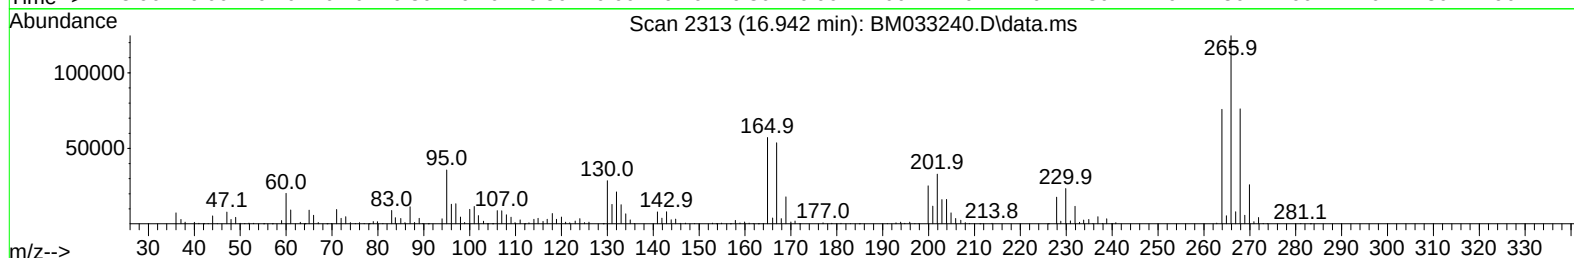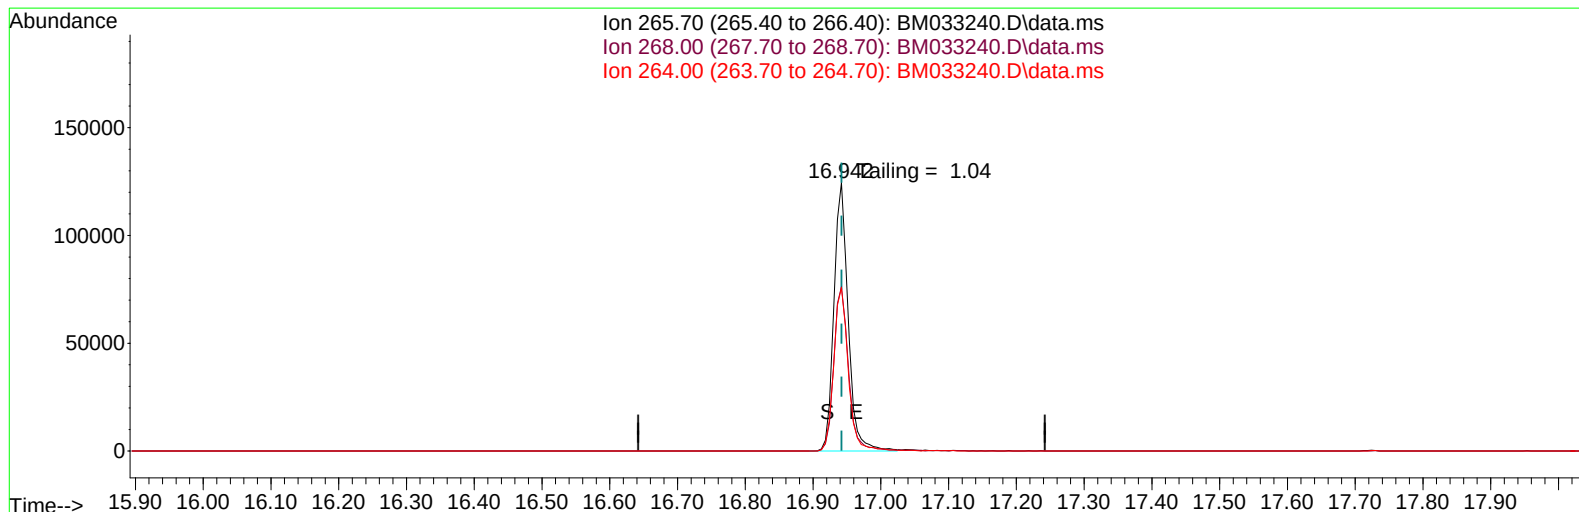

TIC: BM033240.D\data.ms

(70) Pentachlorophenol (C)

16.942min (-0.000) 0.00 ng

response 181495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.18
264.00	65.10	60.87
0.00	0.00	0.00