

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
 Data File : BM033249.D
 Acq On : 24 Nov 2021 16:24
 Operator : CG/JU
 Sample : PB140809BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB140809BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.507	363	369	384	rBV	1558743	2305742	38.20%	8.890%
2	7.096	629	639	655	rBV	1445016	2386491	39.54%	9.202%
3	7.937	776	782	791	rBV	437473	711823	11.79%	2.745%
4	9.095	971	979	989	rBV	1278861	2239852	37.11%	8.636%
5	10.731	1250	1257	1271	rBV	505470	912371	15.12%	3.518%
6	13.183	1666	1674	1685	rBV	2939910	4425265	73.31%	17.063%
7	14.560	1901	1908	1915	rBV	729750	1085979	17.99%	4.187%
8	16.042	2154	2160	2173	rBV	1335941	1932628	32.02%	7.452%
9	17.295	2367	2373	2383	rBV	848522	1205569	19.97%	4.648%
10	19.901	2810	2816	2823	rBV	4636550	6035981	100.00%	23.273%
11	21.453	3075	3080	3090	rBV	1040610	1359800	22.53%	5.243%
12	23.789	3471	3477	3489	rVB2	664702	1333824	22.10%	5.143%




Sum of corrected areas: 25935325

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
Data File : BM033249.D
Acq On : 24 Nov 2021 16:24
Operator : CG/JU
Sample : PB140809BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140809BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

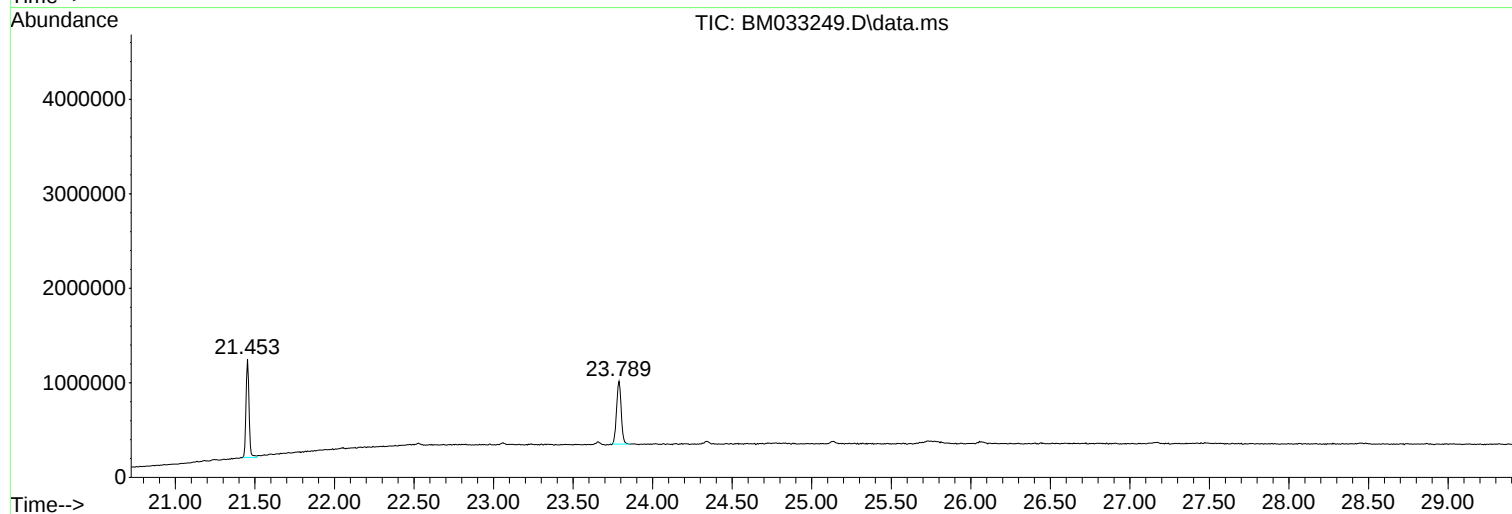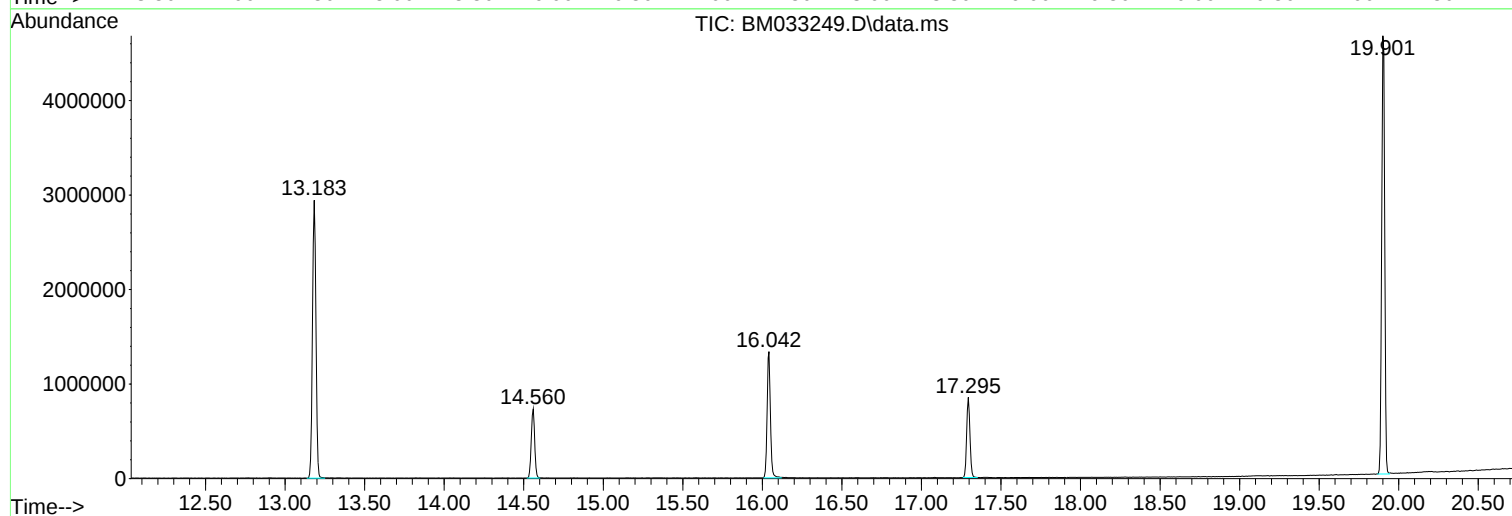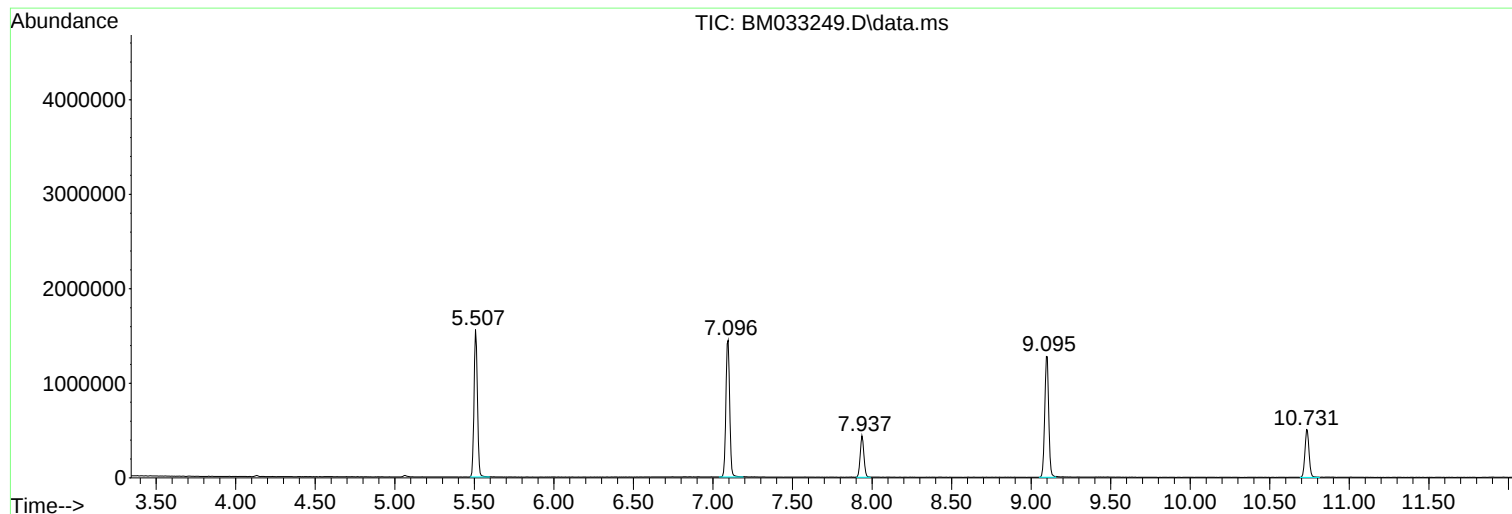

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
Data File : BM033249.D
Acq On : 24 Nov 2021 16:24
Operator : CG/JU
Sample : PB140809BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140809BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
Data File : BM033249.D
Acq On : 24 Nov 2021 16:24
Operator : CG/JU
Sample : PB140809BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140809BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------