
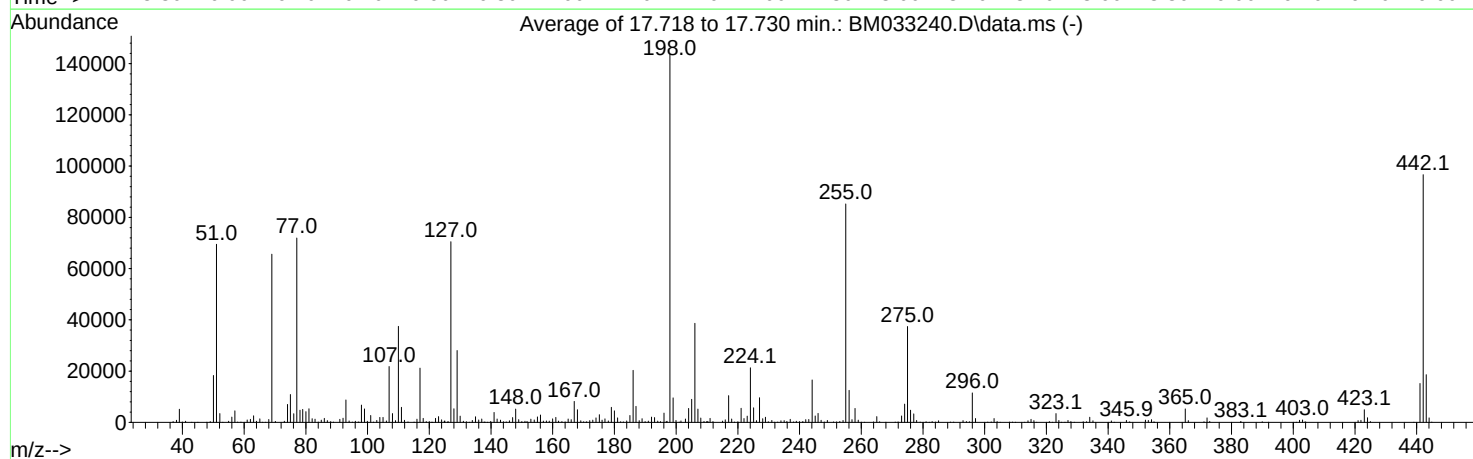


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
 Data File : BM033240.D
 Acq On : 24 Nov 2021 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 24 15:16:33 2021

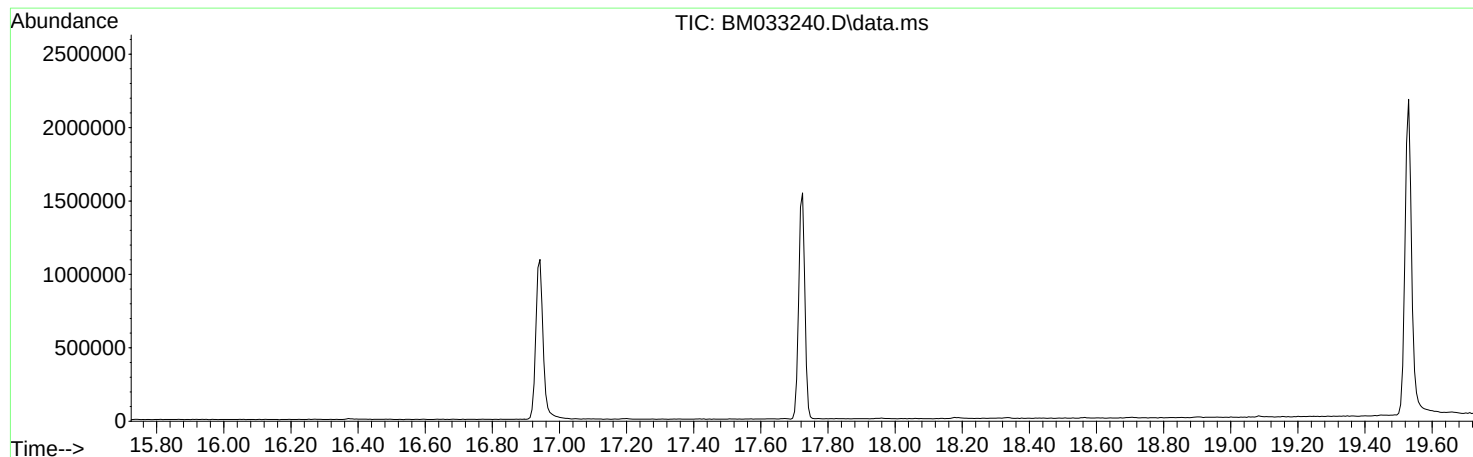

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	69493	PASS
68	69	0.00	2	1.7	1126	PASS
69	198	0.00	100	45.7	65635	PASS
70	69	0.00	2	0.6	375	PASS
127	198	10	80	49.1	70523	PASS
197	198	0.00	2	0.3	417	PASS
198	198	100	100	100.0	143544	PASS
199	198	5	9	6.7	9591	PASS
275	198	10	60	26.0	37392	PASS
365	198	1	100	3.6	5236	PASS
441	198	0.01	100	10.6	15169	PASS
442	442	50	100	100.0	96680	PASS
443	442	15	24	19.2	18589	PASS

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/24/2021	BNA_M	<u>BM033240.D</u>
Compound Name	Response	Retention Time
DDT	547879	20.75
DDD	2512	20.31
DDE	59	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2571	550450	0.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
Data File : BM033240.D
Acq On : 24 Nov 2021 09:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 24 18:20:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

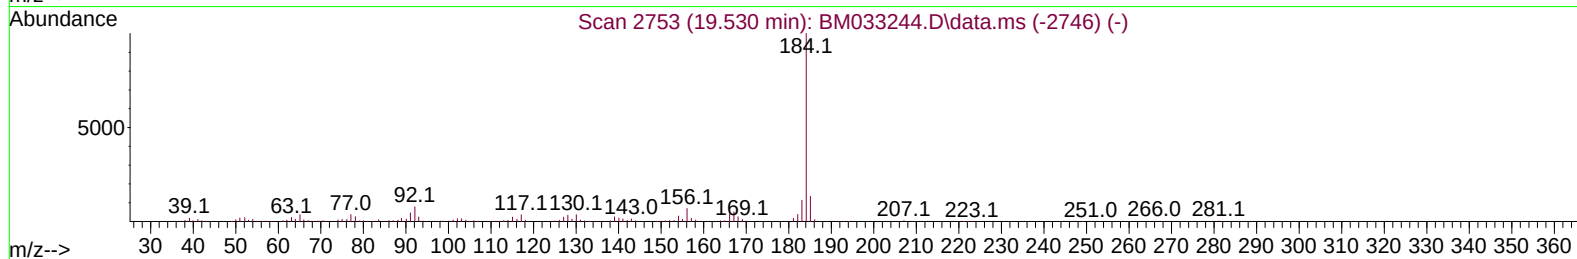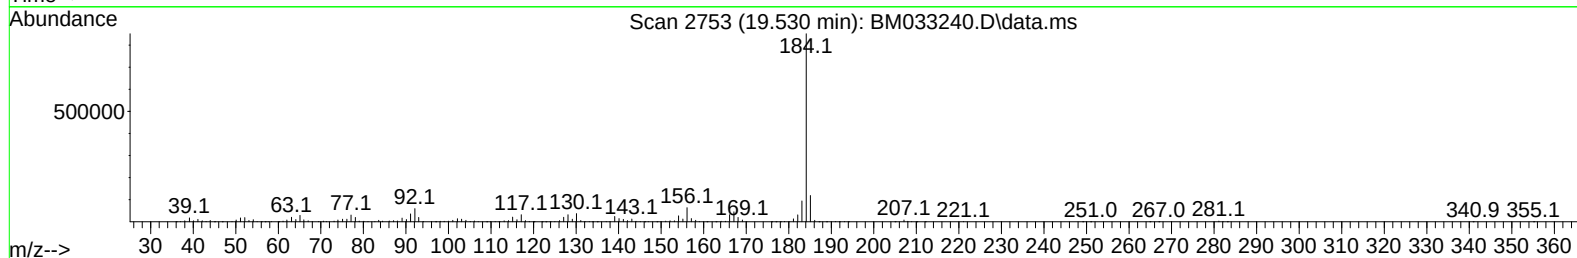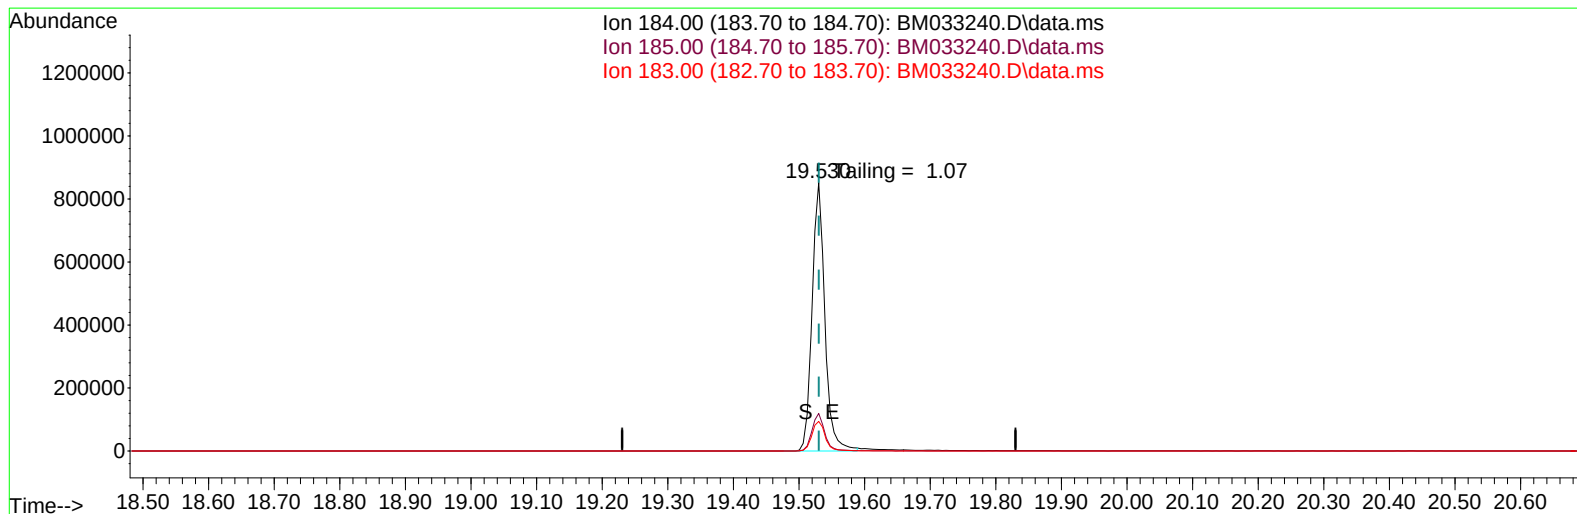

TIC: BM033240.D\data.ms

(77) Benzidine

19.530min (-0.000) 0.00 ng




response 1182164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.00
183.00	11.20	11.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112421\
 Data File : BM033240.D
 Acq On : 24 Nov 2021 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Nov 24 18:20:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

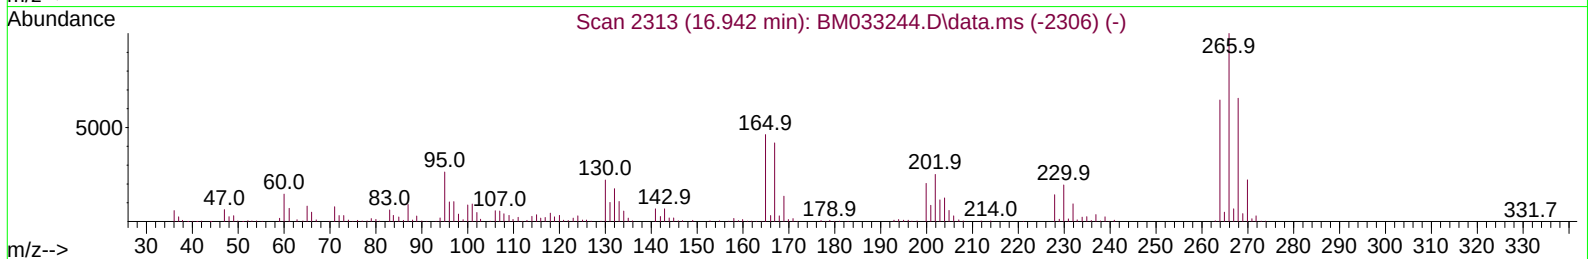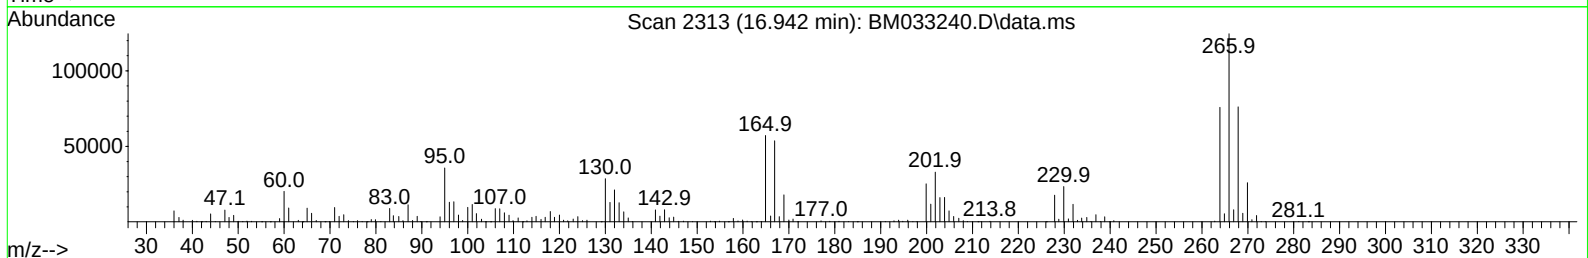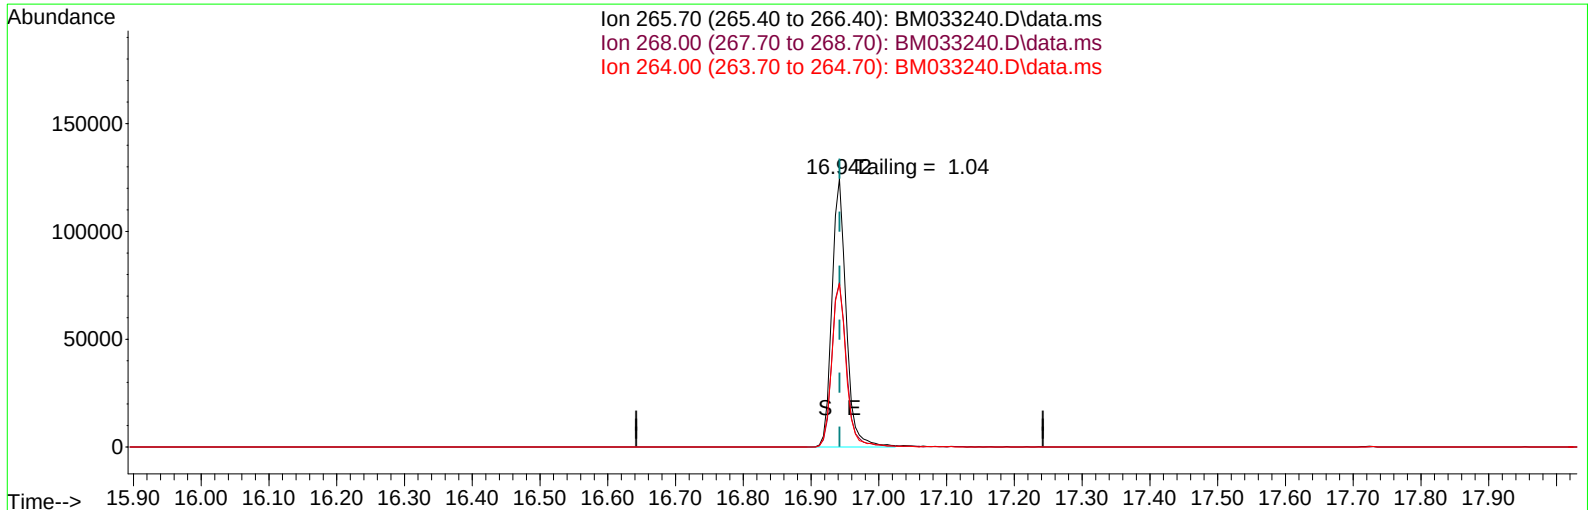

TIC: BM033240.D\data.ms

(70) Pentachlorophenol (C)

16.942min (-0.000) 0.00 ng

response 181495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.18
264.00	65.10	60.87
0.00	0.00	0.00