

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112515\
 Data File : BM003298.D
 Acq On : 25 Nov 2015 16:33
 Operator : UM/IZ
 Sample : SSTDCCC002EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD00267

Quant Time: Nov 26 00:10:52 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 26 00:09:17 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	7232	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	25777	0.40	ng/ul	0.00
5) Acenaphthene-d10	14.38	164	11069	0.40	ng/ul	0.00
6) Phenanthrene-d10	17.13	188	22386	0.40	ng/ul	0.00
7) Chrysene-d12	21.34	240	22483	0.40	ng/ul	0.01
8) Perylene-d12	23.59	264	19534	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.20	96	13588	1.92	ng/uL	0.00
Target Compounds						
3) 1,4-Dioxane	3.23	88	16070	1.91	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112515\
Data File : BM003298.D
Acq On : 25 Nov 2015 16:33
Operator : UM/IZ
Sample : SSTDCCC002EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD00267

Quant Time: Nov 26 00:10:52 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 26 00:09:17 2015
Response via : Initial Calibration

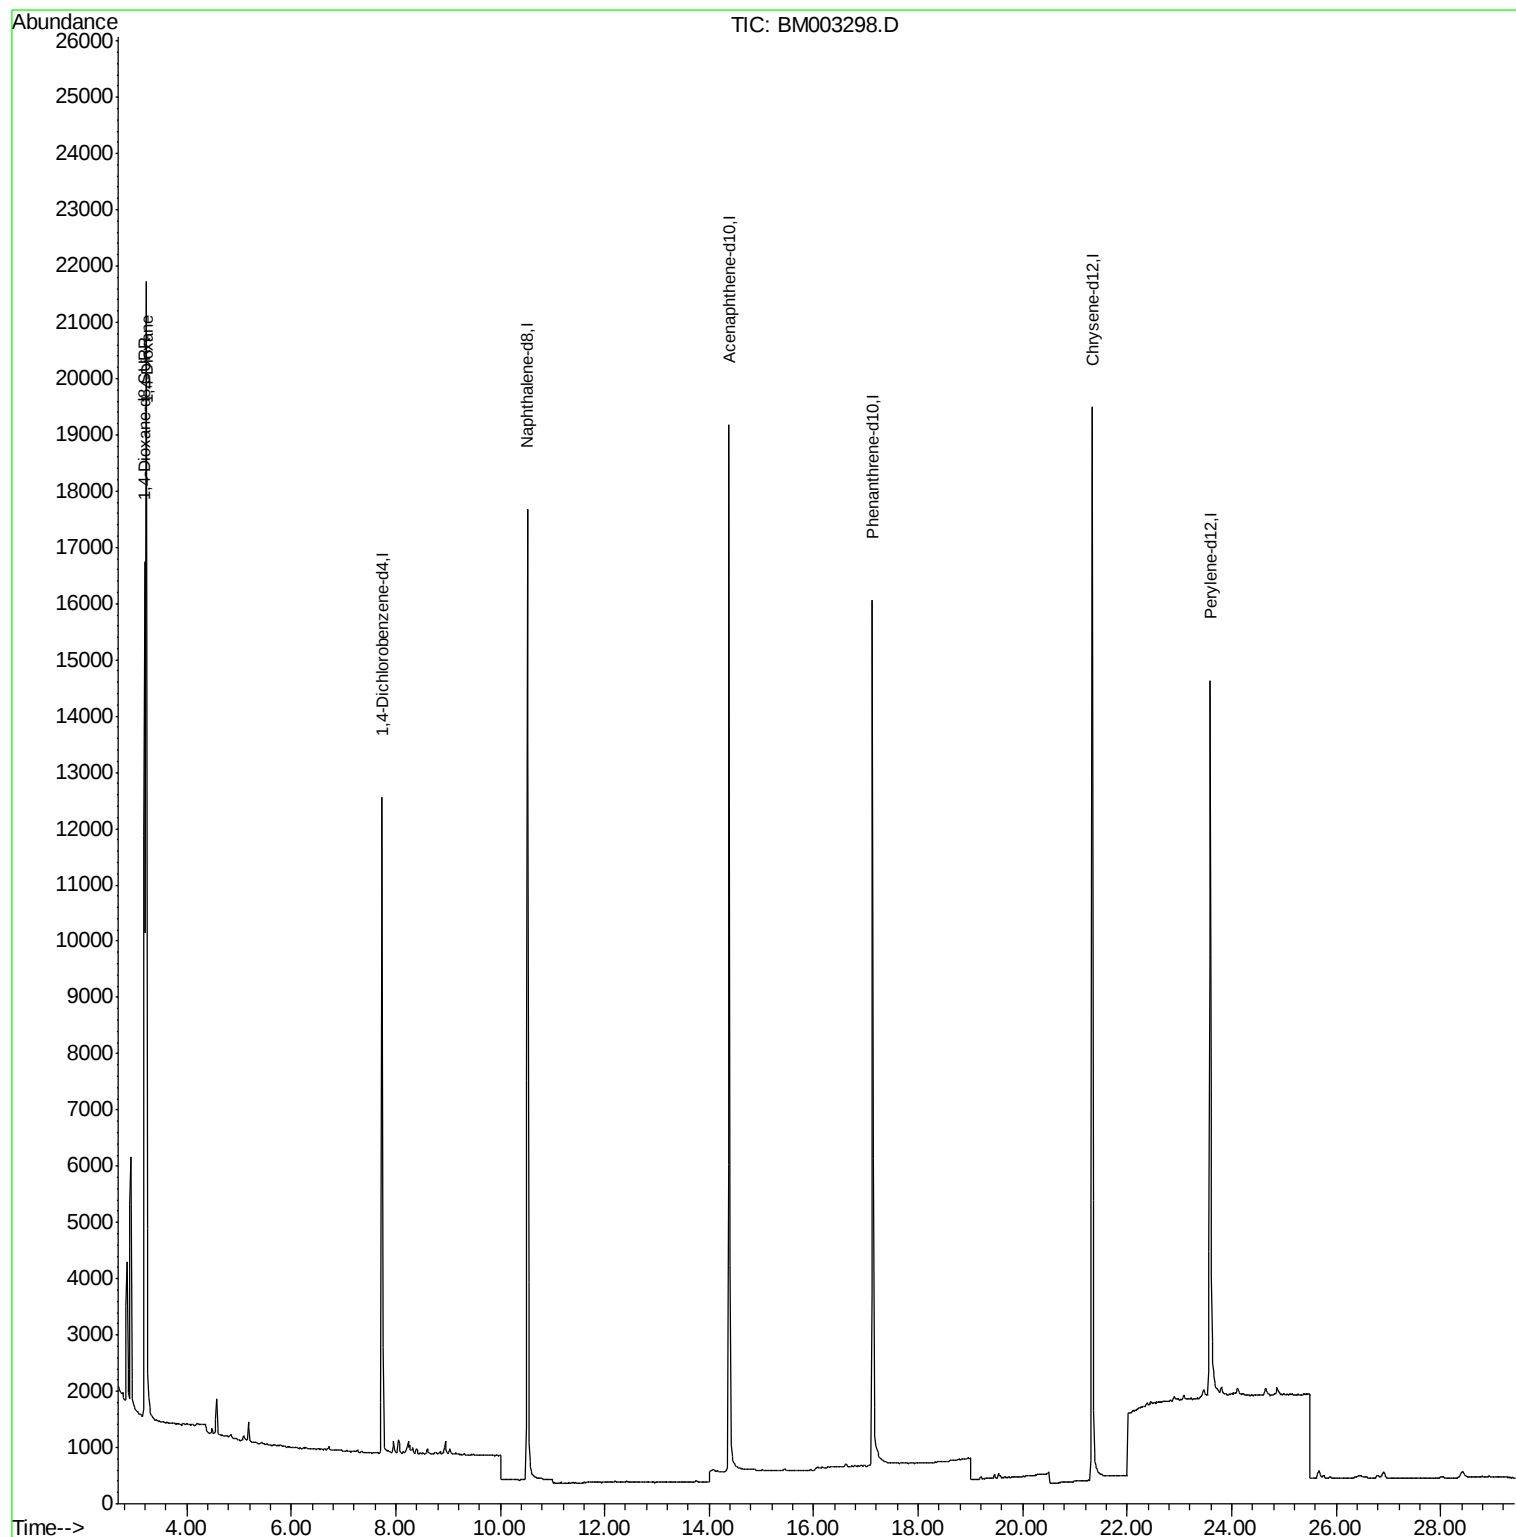

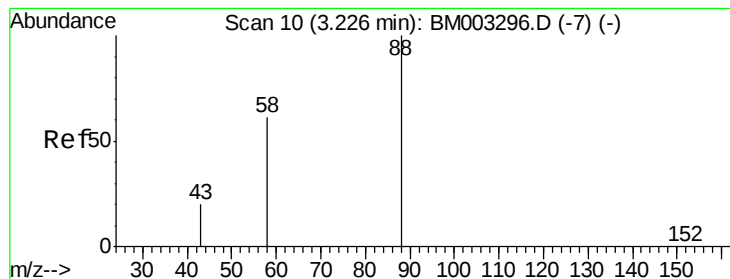

#3

1,4-Dioxane

Concen: 1.91 ng/ul

RT: 3.23 min Scan# 36

Delta R.T. 0.00 min

Lab File: BM003298.D

Acq: 25 Nov 2015 16:33

Instrument :

BNA_M

ClientSampleId :

SSTD00267


Tgt Ion: 88 Resp: 16070

Ion Ratio Lower Upper

88 100

58 58.7 54.8 82.2

43 21.4 22.6 33.8#

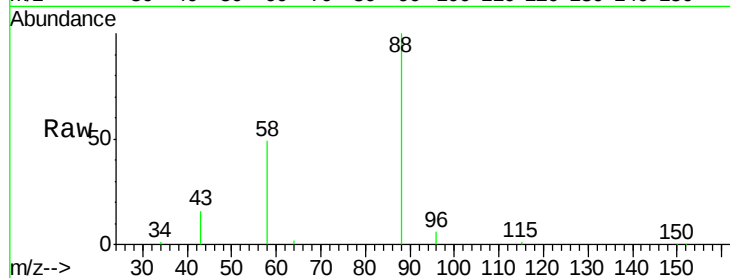

Abundance Ion 88.00 (87.70 to 88.70): BM003298.D (-23) (-)

