

Data Path : Z:\HPCHEM1\BNA_M\Data\BM112515\
 Data File : BM003296.D
 Acq On : 25 Nov 2015 10:43
 Operator : UM/IZ
 Sample : SSTDCCC002
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP51

Quant Time: Nov 26 00:08:34 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 25 04:16:44 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	5586	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	20500	0.40	ng/ul	-0.01
5) Acenaphthene-d10	14.38	164	9670	0.40	ng/ul	0.00
6) Phenanthrene-d10	17.12	188	20727	0.40	ng/ul	0.00
7) Chrysene-d12	21.32	240	20605	0.40	ng/ul	0.00
8) Perylene-d12	23.58	264	17510	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.20	96	10857	1.99	ng/uL	0.00
Target Compounds						
3) 1,4-Dioxane	3.23	88	13059	2.01	ng/ul#	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM112515\
Data File : BM003296.D
Acq On : 25 Nov 2015 10:43
Operator : UM/IZ
Sample : SSTDCCC002
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP51

Quant Time: Nov 26 00:08:34 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 25 04:16:44 2015
Response via : Initial Calibration

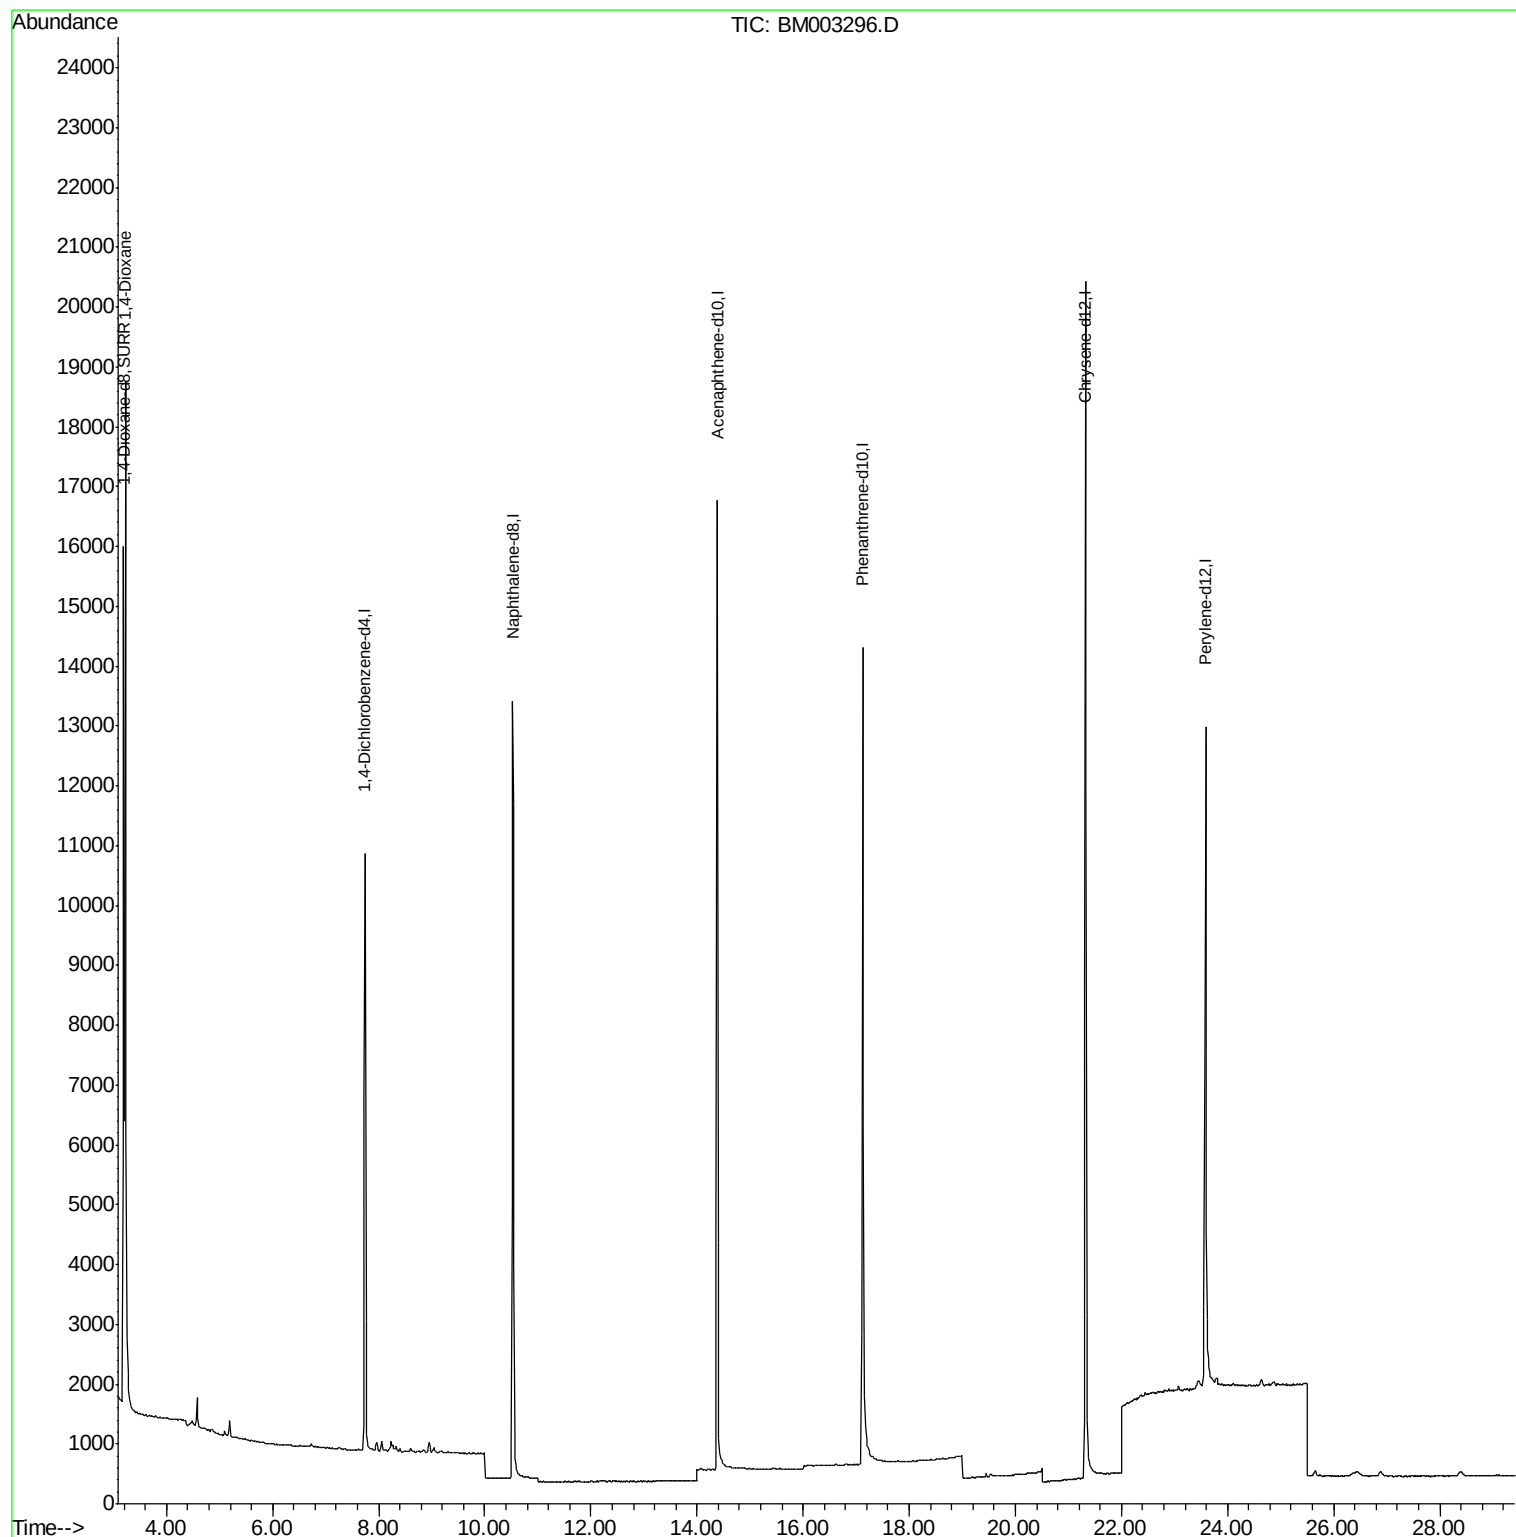

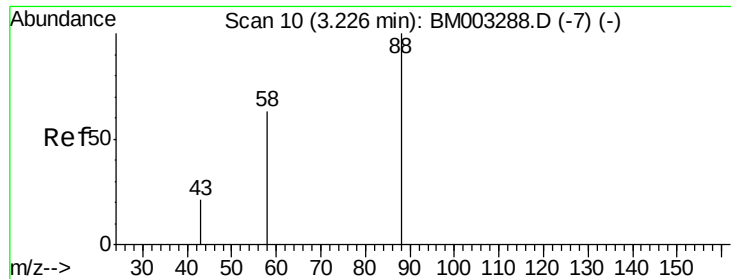

#3
 1,4-Dioxane
 Concen: 2.01 ng/ul
 RT: 3.23 min Scan# 10
 Delta R.T. 0.00 min
 Lab File: BM003296.D
 Acq: 25 Nov 2015 10:43

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP51

Tgt Ion: 88 Resp: 13059
 Ion Ratio Lower Upper
 88 100
 58 58.0 54.8 82.2
 43 20.9 22.6 33.8#

