


Data Path : Z:\HPCHEM1\BNA M\DATA\BM112515\
 Data File : BM003295.D
 Acq On : 25 Nov 2015 10:07
 Operator : UM/IZ
 Sample : DFTPP51
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP51

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 26 00:09:17 2015

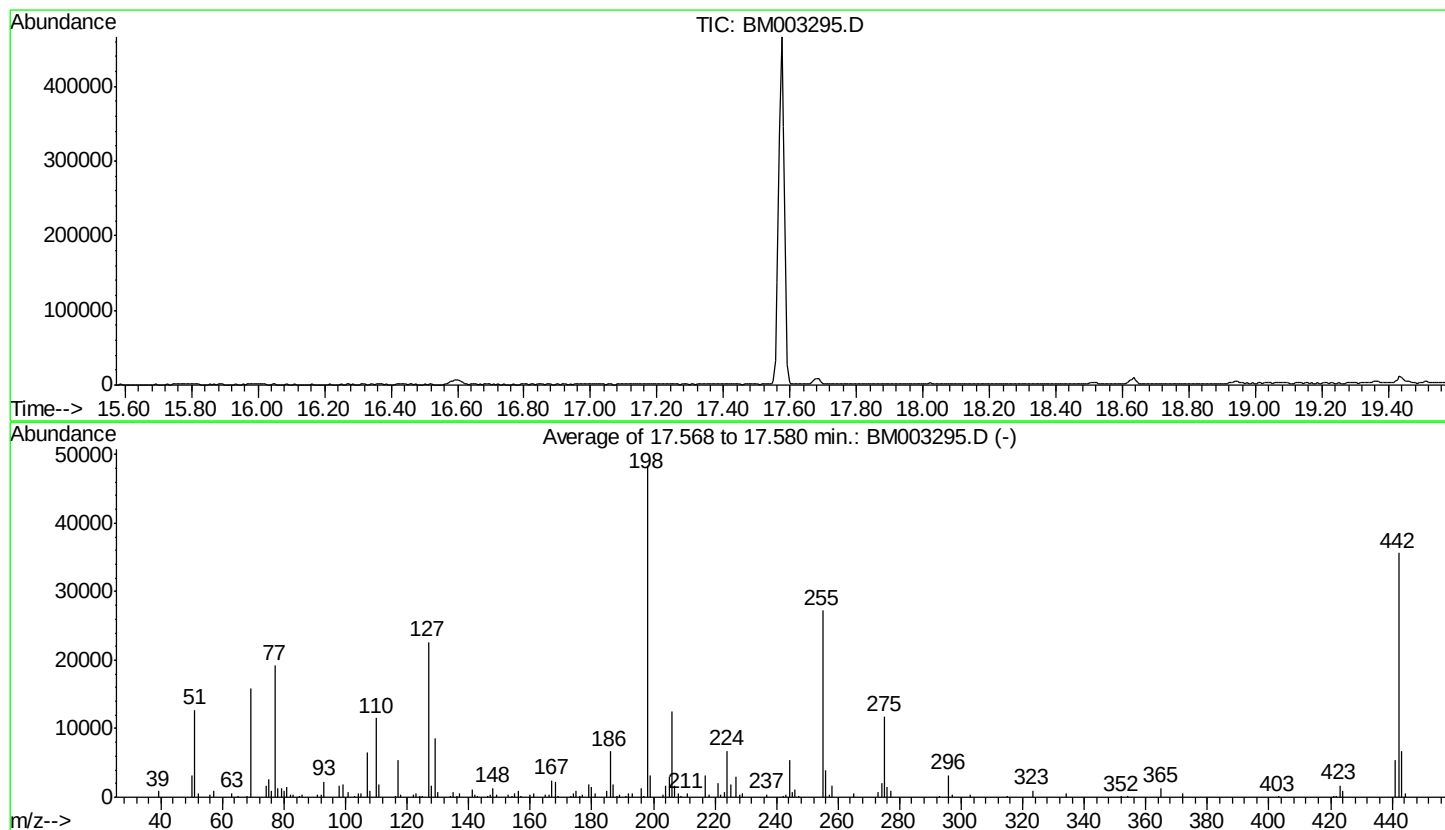

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	12749	PASS
68	69	0.00	2	0.8	125	PASS
69	198	0.00	100	32.9	15918	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	22674	PASS
197	198	0.00	1	0.3	138	PASS
198	198	100	100	100.0	48381	PASS
199	198	5	9	6.6	3198	PASS
275	198	10	60	24.3	11751	PASS
365	198	1	100	2.7	1317	PASS
441	443	0.01	100	79.9	5398	PASS
442	198	50	100	73.6	35621	PASS
443	442	15	24	19.0	6754	PASS

Scan 2456 (17.533 min): BM003295.D
DFTPP51

m/z	Abundance
73.00	597.0
147.10	321.0
207.00	1083.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
39.10	873.0
50.10	3363.0
51.10	12862.0
52.00	630.0
56.00	417.0
57.00	922.0
63.00	594.0
69.00	16013.0
73.00	371.0
74.00	1642.0
75.00	2677.0
76.00	954.0
77.10	19152.0
78.00	1465.0
79.00	1258.0
80.00	922.0
81.00	1443.0
81.90	381.0
82.90	358.0
86.00	369.0
91.00	380.0
92.00	407.0
93.00	2195.0
98.00	1797.0
99.00	2095.0
100.90	827.0
103.90	528.0
105.00	541.0
107.00	6369.0
108.00	900.0
110.00	11641.0
111.00	1854.0
116.00	367.0
117.00	5150.0
118.00	437.0
122.00	361.0
123.00	608.0
124.00	306.0
127.00	21792.0
128.00	1726.0
129.00	8112.0
130.00	711.0
134.90	642.0
136.00	313.0
137.00	580.0
141.00	1109.0
141.90	355.0
147.00	624.0
148.00	1271.0
149.00	440.0
153.00	335.0
154.00	311.0
155.00	641.0
156.00	867.0
160.00	318.0
161.00	524.0
164.90	364.0
166.00	312.0
167.00	2260.0
168.00	2434.0
174.10	436.0
175.00	861.0
177.00	427.0
179.00	1642.0
180.00	1394.0
181.00	562.0
185.00	773.0
186.00	6304.0
187.00	1723.0
189.00	443.0
191.10	303.0
192.00	475.0
193.00	592.0
196.10	1180.0
198.00	43320.0
199.00	3068.0
203.00	308.0
204.10	1523.0
205.10	2590.0
206.10	10969.0
207.00	2646.0
208.00	601.0
210.90	489.0
217.00	2614.0
218.00	379.0
221.10	1530.0
221.90	333.0
223.00	644.0
224.10	5898.0
225.10	1555.0
227.00	2467.0
228.10	337.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

229.00	608.0
237.00	450.0
243.00	313.0
244.10	4598.0
245.10	607.0
245.90	1006.0
255.00	22536.0
256.10	3298.0
258.00	1433.0
265.00	489.0
273.00	604.0
274.10	1838.0
275.10	9573.0
276.00	1364.0
277.00	765.0
296.10	2517.0
297.00	352.0
323.10	877.0
334.00	504.0
365.00	915.0
372.10	420.0
423.00	1171.0
424.10	853.0
441.10	3502.0
442.10	23480.0
443.10	4565.0
444.20	447.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
39.10	1114.0
50.10	3816.0
51.10	15282.0
52.00	854.0
56.00	494.0
57.00	1263.0
63.00	709.0
65.10	423.0
68.00	376.0
69.00	19376.0
73.00	337.0
74.00	1950.0
75.00	3205.0
76.00	1190.0
77.10	23792.0
78.10	1615.0
79.00	1618.0
80.00	1272.0
81.00	1699.0
82.00	435.0
83.00	498.0
85.00	349.0
86.00	399.0
91.00	378.0
92.00	546.0
93.00	2963.0
98.00	2026.0
99.00	2322.0
101.00	930.0
103.00	349.0
104.00	591.0
104.90	640.0
107.00	7797.0
108.00	1155.0
110.00	13473.0
111.00	2209.0
116.00	347.0
117.00	6446.0
117.90	437.0
122.00	586.0
123.00	805.0
124.00	425.0
125.00	391.0
127.00	27472.0
128.00	2187.0
129.00	10823.0
130.00	891.0
133.90	304.0
135.00	796.0
136.00	330.0
137.00	562.0
141.00	1403.0
142.00	466.0
143.00	361.0
146.00	304.0
147.00	658.0
148.00	1696.0
149.00	502.0
153.00	467.0
154.00	371.0
155.00	733.0
156.00	1265.0
157.00	348.0
160.00	492.0
161.00	710.0
165.00	594.0
166.00	385.0
167.00	3047.0
168.00	2378.0
169.00	315.0
173.10	326.0
174.00	728.0
175.00	1060.0
176.00	388.0
177.00	573.0
179.00	2294.0
180.00	1720.0
181.00	669.0
185.00	1098.0
186.00	7825.0
187.00	2440.0
188.10	337.0
188.90	490.0
191.00	418.0
192.00	622.0
193.00	715.0
196.00	1671.0
196.80	414.0
198.00	58112.0
199.00	3745.0
203.00	376.0
204.10	2121.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

205.10	3734.0
206.10	15353.0
207.10	3034.0
208.10	733.0
209.00	332.0
210.90	585.0
217.00	3847.0
218.00	556.0
221.10	2716.0
221.80	544.0
223.00	931.0
224.10	8182.0
225.10	2202.0
227.00	3714.0
227.90	466.0
229.00	764.0
237.00	577.0
242.00	394.0
243.00	465.0
244.10	6756.0
245.00	852.0
246.00	1323.0
247.00	301.0
255.10	32832.0
256.00	4713.0
257.00	571.0
258.00	1883.0
265.00	712.0
273.00	1055.0
274.10	2373.0
275.10	14161.0
276.10	1859.0
277.00	1219.0
293.00	358.0
296.00	3924.0
297.00	534.0
303.10	487.0
315.10	324.0
323.10	1157.0
334.10	669.0
352.10	454.0
354.10	372.0
365.00	1592.0
372.10	632.0
403.10	326.0
421.00	357.0
422.00	306.0
423.10	2048.0
424.10	1022.0
441.10	6487.0
442.10	41632.0
443.10	8037.0
444.10	704.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
39.00	652.0
50.00	2547.0
51.10	10104.0
52.00	474.0
56.00	347.0
57.00	801.0
63.00	456.0
69.00	12366.0
73.00	310.0
74.00	1350.0
75.00	2174.0
76.00	689.0
77.10	14599.0
78.00	1046.0
79.00	985.0
80.00	820.0
81.00	1205.0
82.00	317.0
83.00	352.0
85.90	307.0
91.00	323.0
92.00	326.0
93.00	1839.0
98.00	1463.0
99.00	1411.0
101.00	685.0
104.00	382.0
105.00	396.0
107.00	5444.0
108.00	646.0
110.00	9473.0
111.00	1517.0
117.00	4510.0
118.00	437.0
122.00	312.0
123.00	508.0
127.00	18760.0
128.00	1359.0
129.00	7124.0
130.00	609.0
135.00	606.0
137.00	418.0
141.00	869.0
142.00	363.0
147.00	589.0
148.00	1062.0
149.00	328.0
153.00	307.0
155.10	534.0
156.10	782.0
160.00	362.0
160.90	445.0
165.00	385.0
166.00	337.0
167.00	2223.0
168.00	1799.0
173.00	306.0
174.00	416.0
175.00	840.0
176.00	305.0
177.00	405.0
179.00	1501.0
180.00	1302.0
181.00	428.0
185.00	689.0
186.10	5904.0
187.00	1645.0
189.00	420.0
192.00	479.0
193.00	659.0
196.10	1195.0
198.00	43712.0
199.00	2783.0
203.00	327.0
204.00	1633.0
205.00	2614.0
206.10	11356.0
207.00	2404.0
208.00	586.0
209.00	320.0
210.90	481.0
217.00	2956.0
218.10	351.0
221.10	1866.0
221.90	425.0
223.00	609.0
224.10	6336.0
225.00	1724.0
227.00	2585.0
228.00	366.0
229.00	479.0
237.00	382.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

242.10	346.0
243.00	371.0
244.10	4827.0
245.10	679.0
246.00	1010.0
255.10	26416.0
256.00	3589.0
257.00	336.0
258.00	1679.0
265.00	735.0
273.00	778.0
274.10	2055.0
275.10	11519.0
276.00	1444.0
277.00	1103.0
296.00	3272.0
296.90	452.0
303.10	375.0
315.00	352.0
323.10	1047.0
334.10	723.0
365.00	1445.0
372.10	445.0
422.00	354.0
423.10	2059.0
424.10	896.0
441.10	6205.0
442.10	41752.0
443.10	7661.0
444.10	692.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51