

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037726.D
 Acq On : 26 Nov 2022 10:36
 Operator : CG/JU
 Sample : N5592-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB1

Quant Time: Nov 27 21:26:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	191122	20.000	ng/ul	0.00
20) Naphthalene-d8	10.933	136	939365	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.739	164	587721	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	1193639	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1129411	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1047729	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	24433	5.302	ng/uL	0.00
4) Pyridine-d5	3.875	84	180744	12.049	ng/ul	0.00
7) Phenol-d5	7.257	99	164293	8.616	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	453200	35.631	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	378624	28.577	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	295984	19.507	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	264506	35.918	ng/ul	0.00
24) 2-Nitrophenol-d4	10.010	143	247396	34.094	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.545	165	427180	32.169	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	525997	23.871	ng/ul	-0.01
46) Dimethylphthalate-d6	14.139	166	1777483	42.698	ng/ul	0.00
49) Acenaphthylene-d8	14.433	160	1927742	39.232	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	80026	8.727	ng/ul	-0.01
60) Fluorene-d10	15.721	176	1504606	41.268	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.833	200	235100	36.614	ng/ul	0.00
73) Anthracene-d10	17.574	188	2613442	46.820	ng/ul	0.00
81) Pyrene-d10	19.850	212	3021731	52.649	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2604915	48.302	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.469	88	19875	3.923	ng/uL#	90
48) 2,6-Dinitrotoluene	14.145	165	14644	1.714	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037726.D
Acq On : 26 Nov 2022 10:36
Operator : CG/JU
Sample : N5592-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB1

Quant Time: Nov 27 21:26:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration




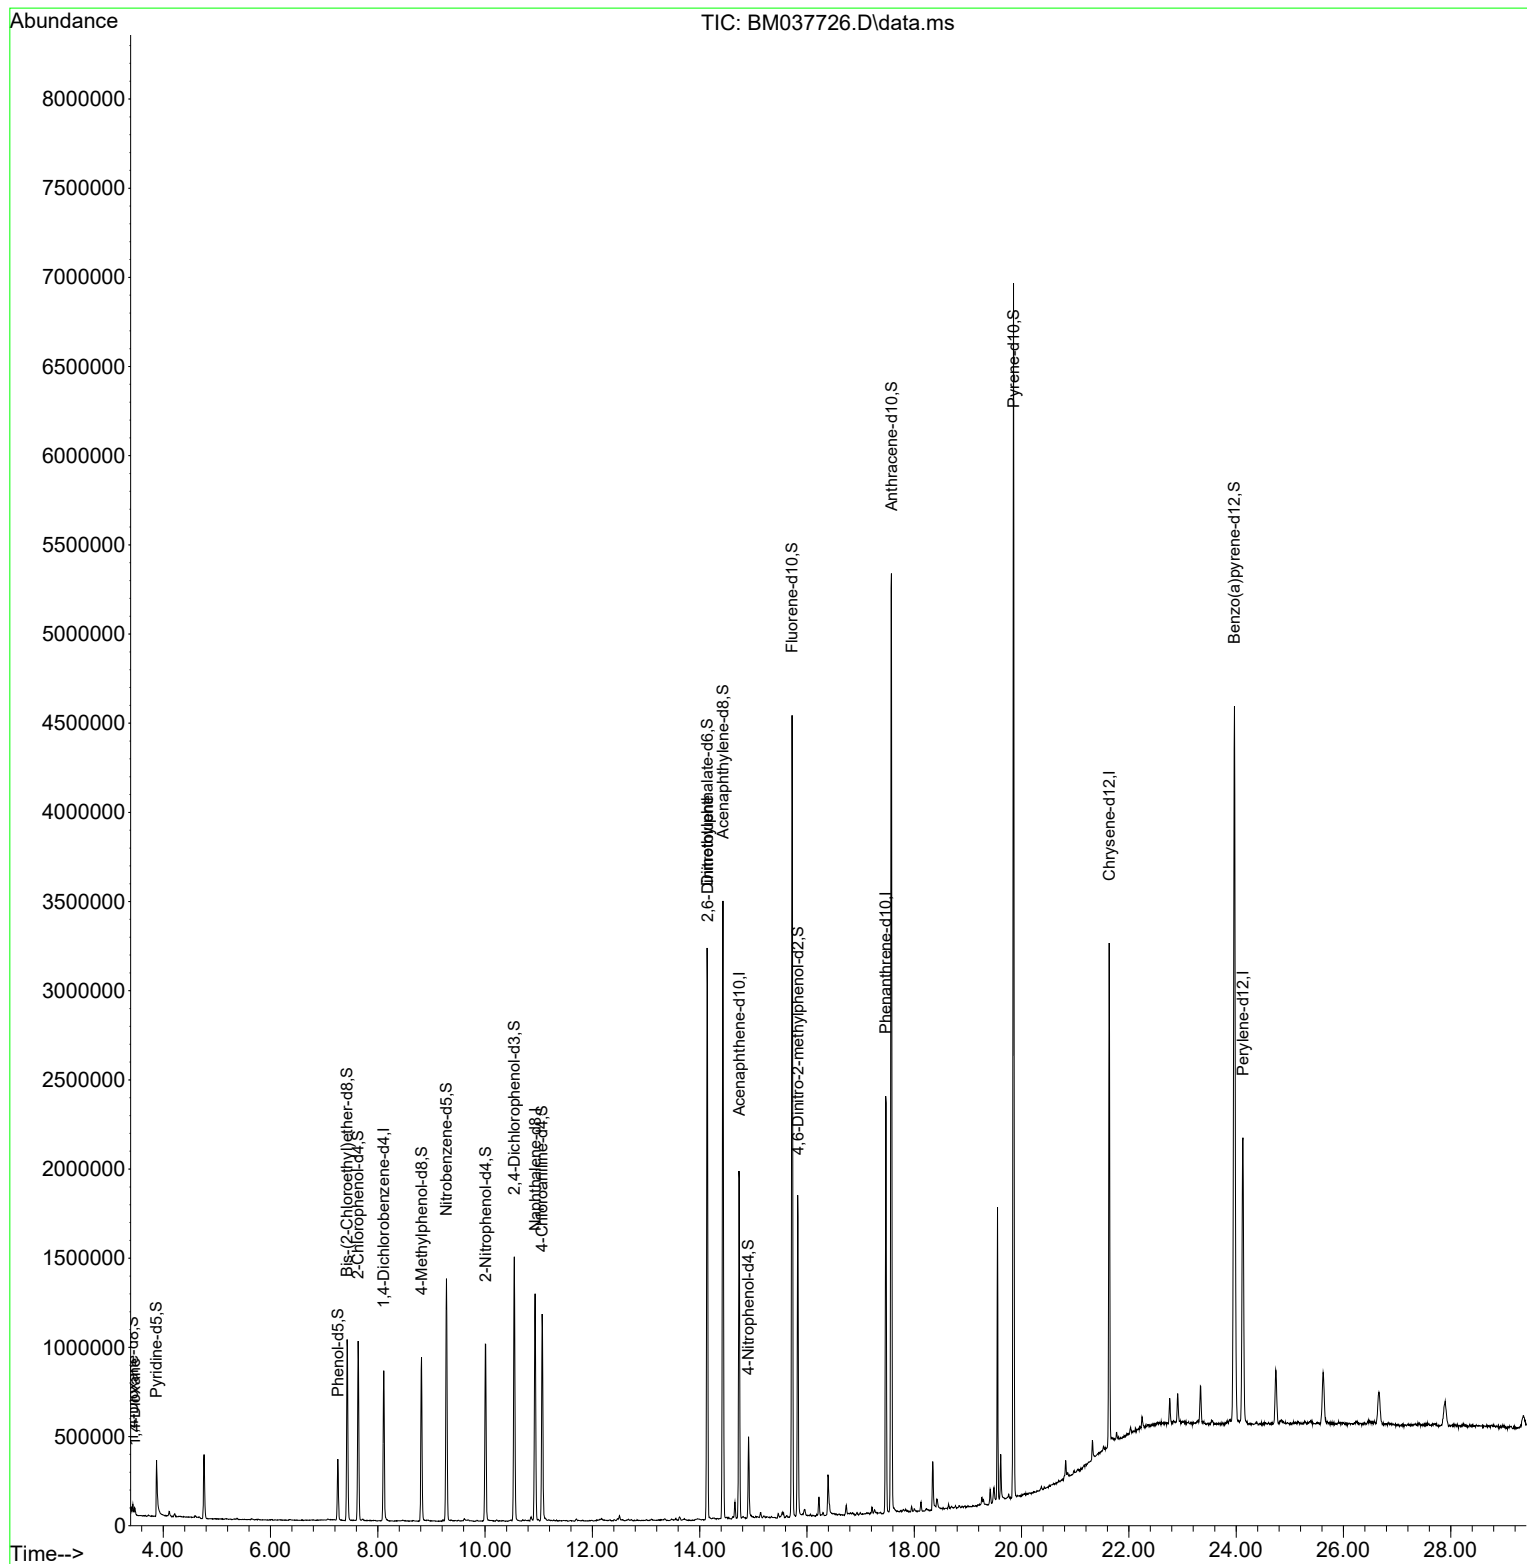


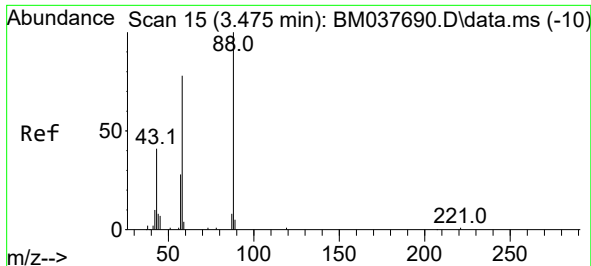

#2
1,4-Dioxane
Concen: 3.923 ng/uL
RT: 3.469 min Scan# 14
Delta R.T. -0.006 min
Lab File: BM037726.D
Acq: 26 Nov 2022 10:36

Instrument :
BNA_M
ClientSampleId :
H0AB1

Tgt Ion: 88 Resp: 19875
Ion Ratio Lower Upper
88 100
43 41.7 42.8 64.2#
58 83.2 62.6 94.0

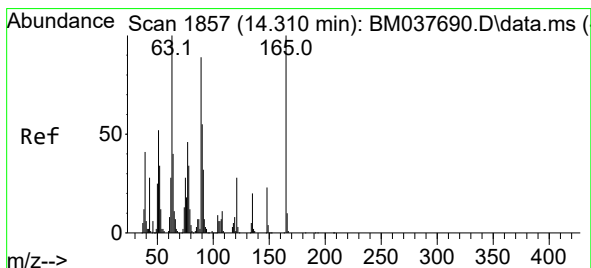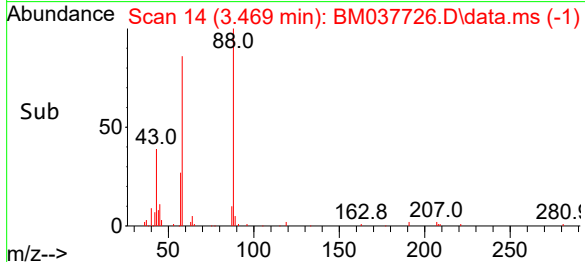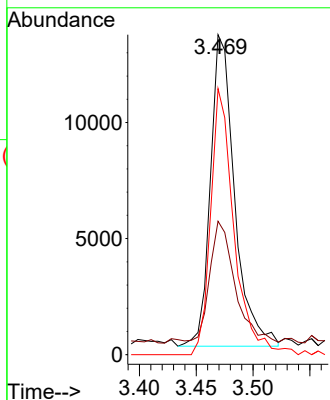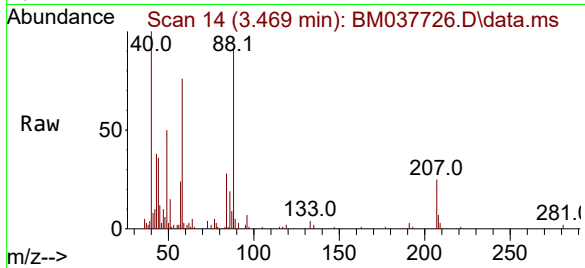

#48
2,6-Dinitrotoluene
Concen: 1.714 ng/uL
RT: 14.145 min Scan# 1829
Delta R.T. -0.171 min
Lab File: BM037726.D
Acq: 26 Nov 2022 10:36

Tgt Ion: 165 Resp: 14644
Ion Ratio Lower Upper
165 100
89 3.3 56.4 84.6#
121 31.9 18.9 28.3#

